


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
Data File : BN015517.D
Acq On : 13 Jul 2021 08:13
Operator : CG/JU
Sample : M2869-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGDY4

Manual Integrations
APPROVED

mohammad
7/13/2021 1:45:38 PM

Quant Time: Jul 13 08:53:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 11:02:52 2021
Response via : Initial Calibration

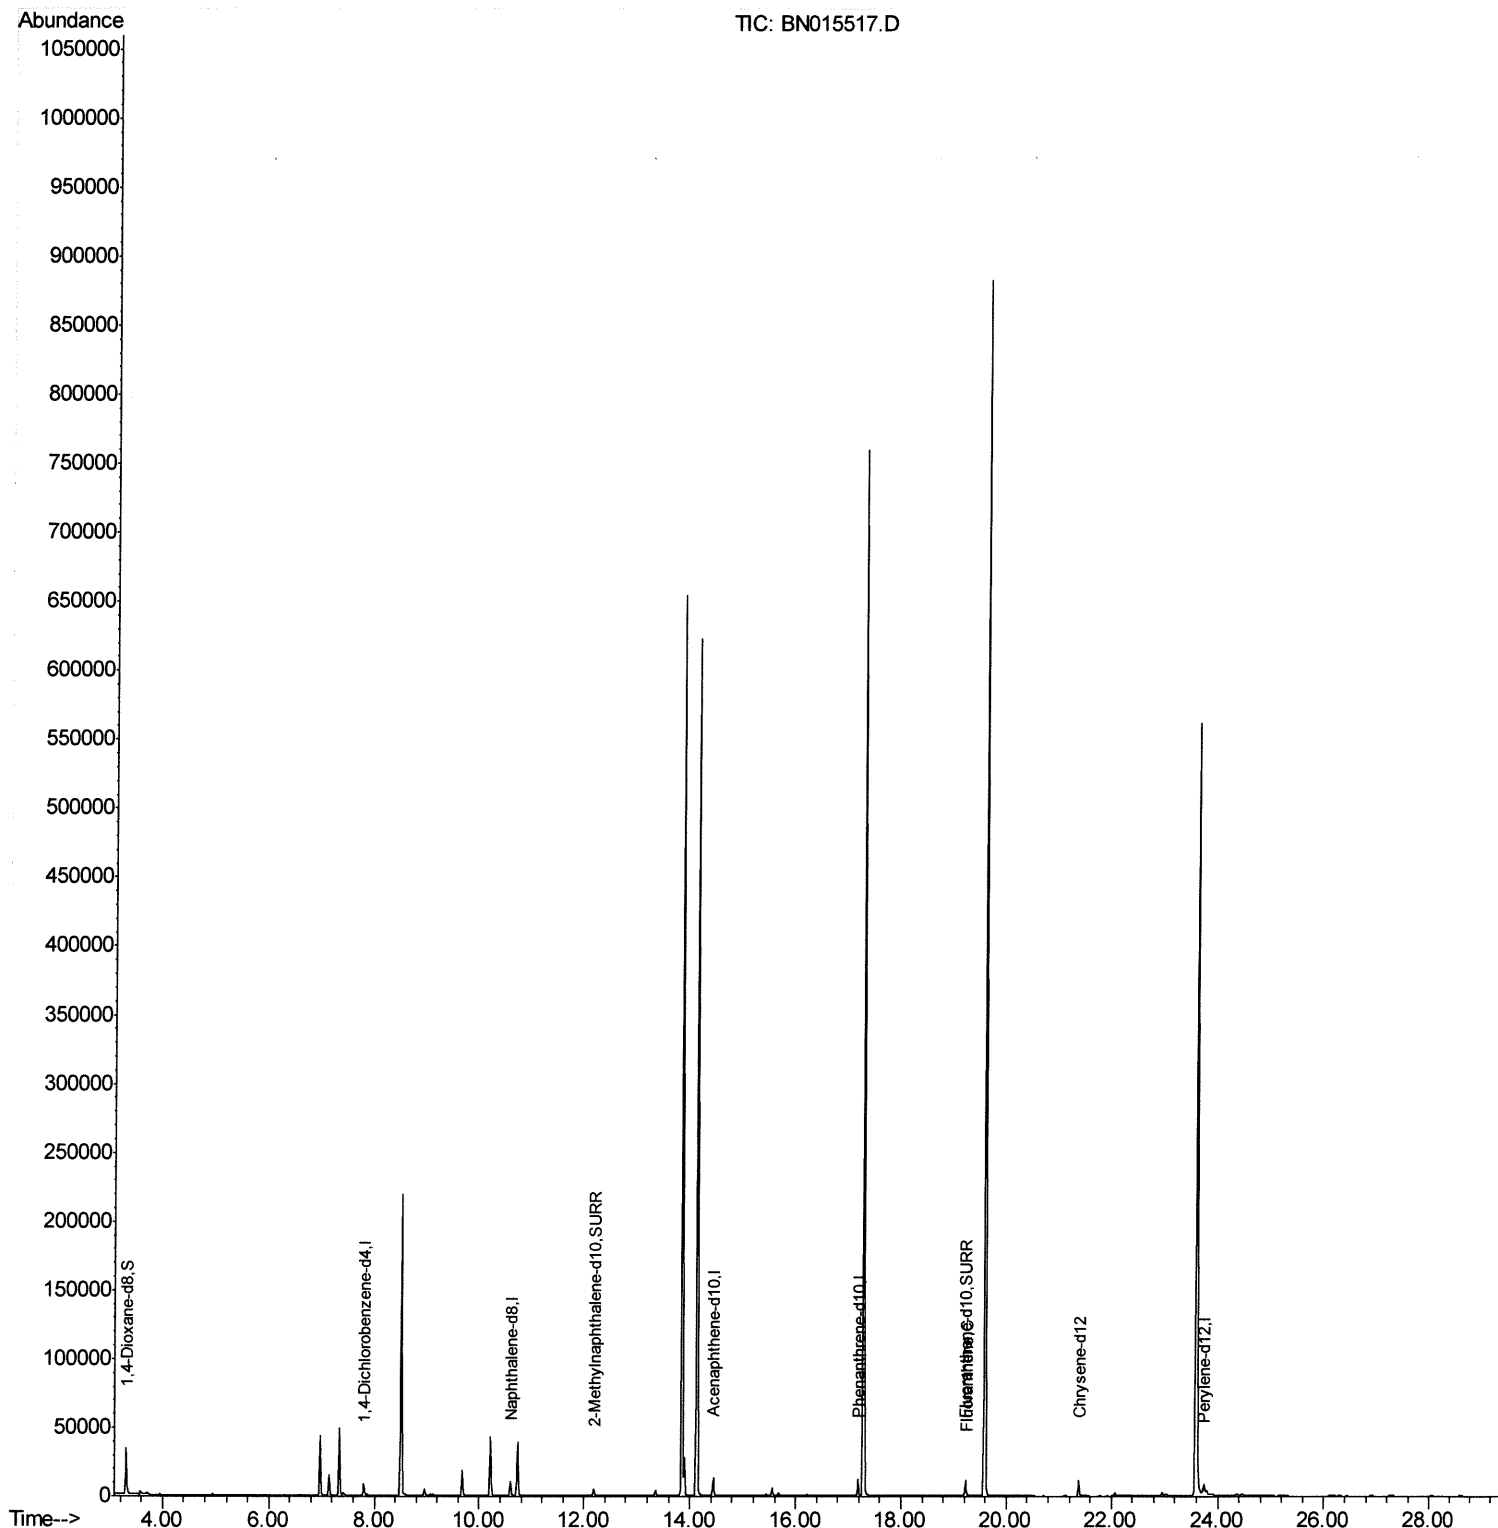



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015517.D
 Acq On : 13 Jul 2021 08:13
 Operator : CG/JU
 Sample : M2869-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDY4

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:45:38 PM

Quant Time: Jul 13 08:47:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

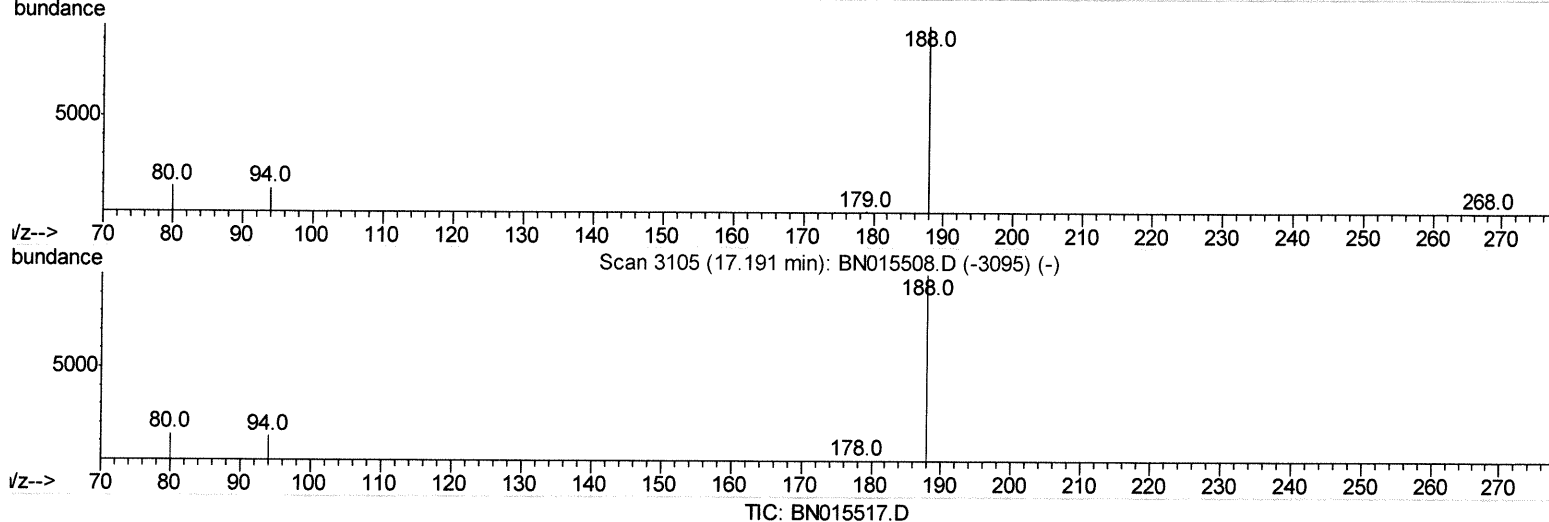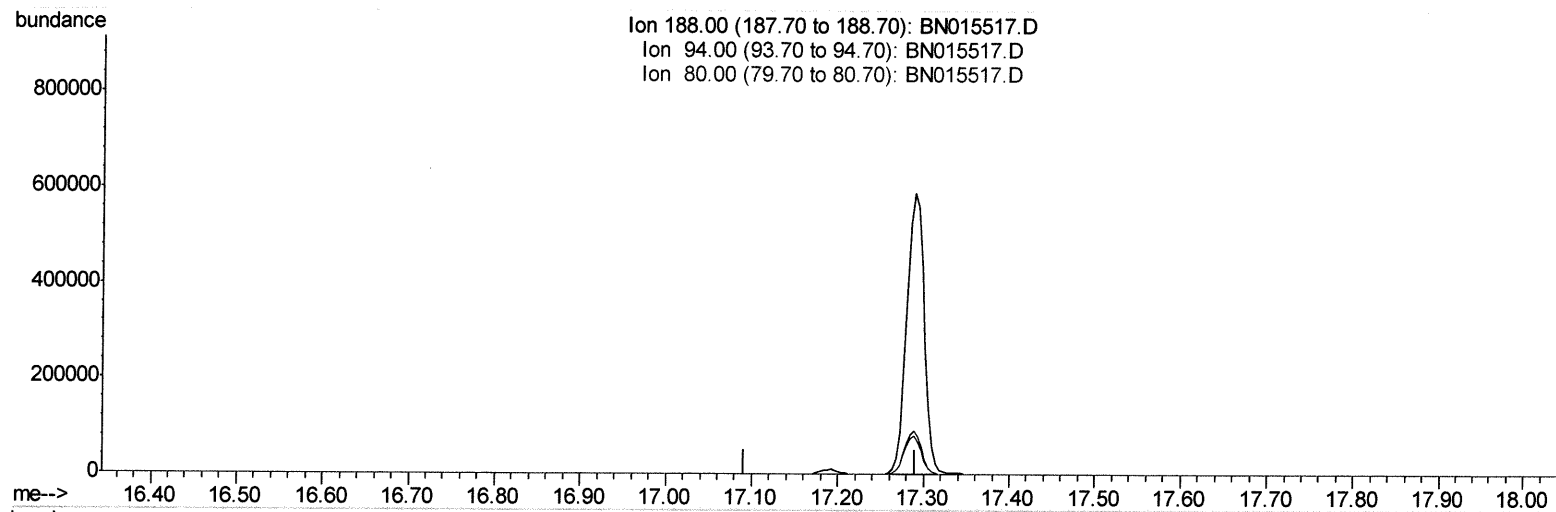

(13) Phenanthrene-d10 (I)

17.192min (-17.192) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	14.10	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015517.D
 Acq On : 13 Jul 2021 08:13
 Operator : CG/JU
 Sample : M2869-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDY4

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:45:38 PM

Quant Time: Jul 13 08:47:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

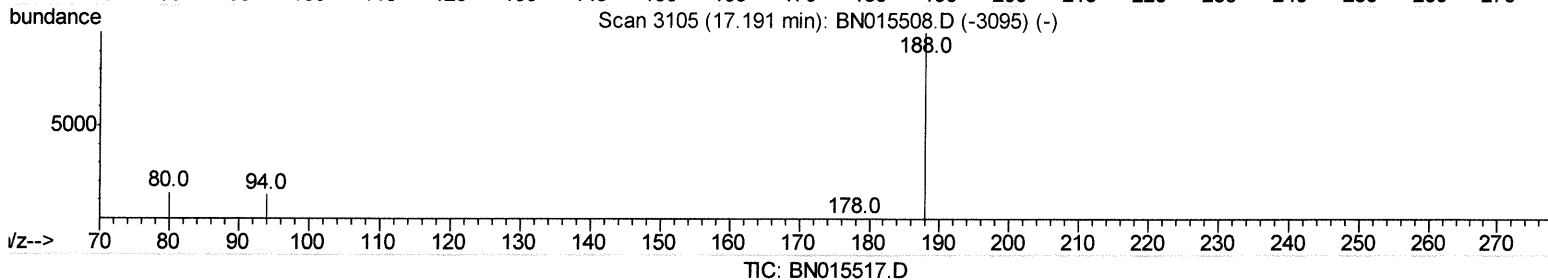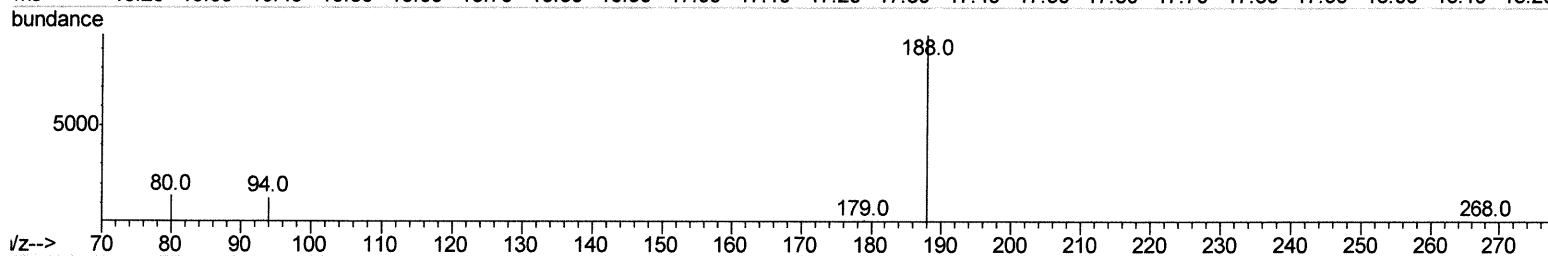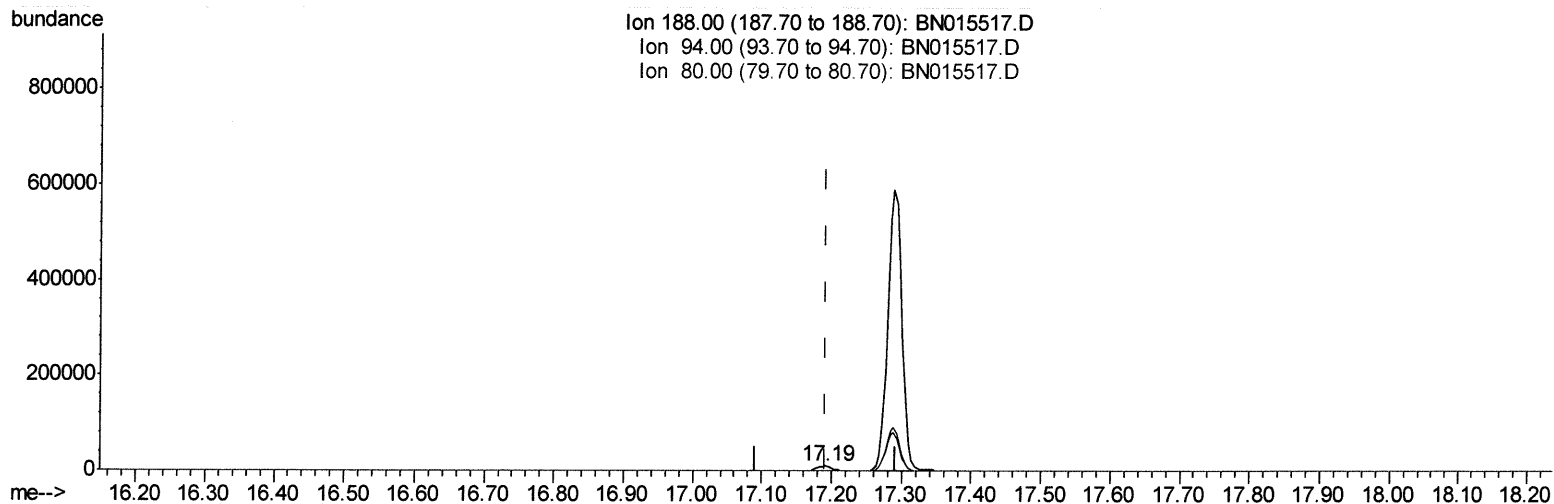

(13) Phenanthrene-d10 (I)

17.191min (-0.000) 0.40ng/ul m

response 13561

Ion	Exp%	Act%
188.00	100	100
94.00	14.10	12.90
80.00	14.40	14.06
0.00	0.00	0.00

Jy 7/14/21

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015517.D
 Acq On : 13 Jul 2021 08:13
 Operator : CG/JU
 Sample : M2869-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDY4

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:45:38 PM

Quant Time: Jul 13 08:53:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	3891	0.40	ng/ul	0.00
4) Naphthalene-d8	10.59	136	13223	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.44	164	7009	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.19	188	13561m>	0.40	ng/ul	> 0.00
17) Chrysene-d12	21.39	240	10565	0.40	ng/ul	0.00
23) Perylene-d12	23.74	264	10677	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.31	96	21925	5.00	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.19	152	6674	0.32	ng/ul	0.00
18) Fluoranthene-d10	19.22	212	12438	0.36	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.25	202	1031	0.021	ng/ul#	Ovalue 77

(#) = qualifier out of range (m) = manual integration (+) = signals summed