


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
Data File : BN015526.D
Acq On : 13 Jul 2021 13:38
Operator : CG/JU
Sample : PB137523BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK523

Manual Integrations
APPROVED

mohammad
7/13/2021 4:39:36 PM

Quant Time: Jul 13 14:09:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 11:02:52 2021
Response via : Initial Calibration

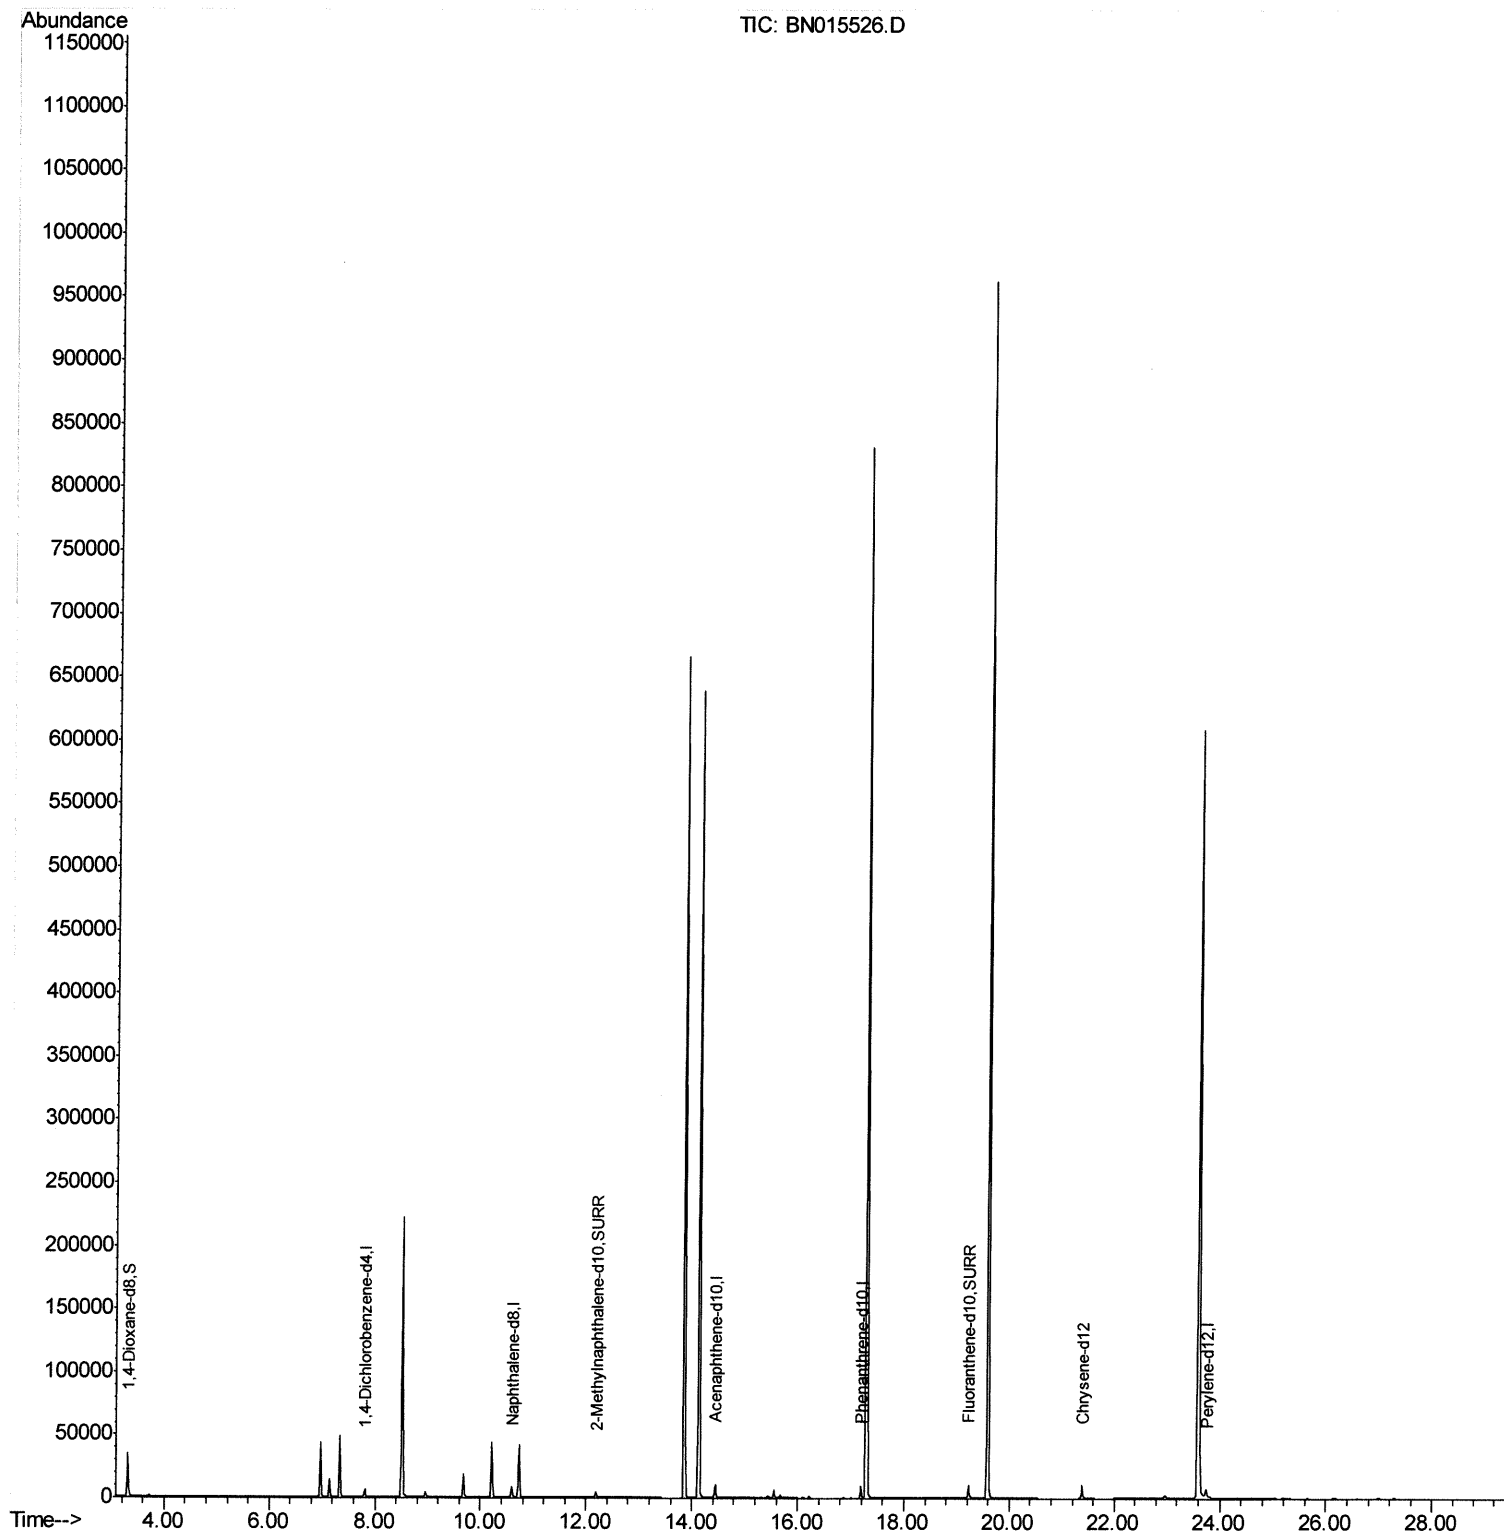




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015526.D
 Acq On : 13 Jul 2021 13:38
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/13/2021 4:39:36 PM

Quant Time: Jul 13 14:08:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

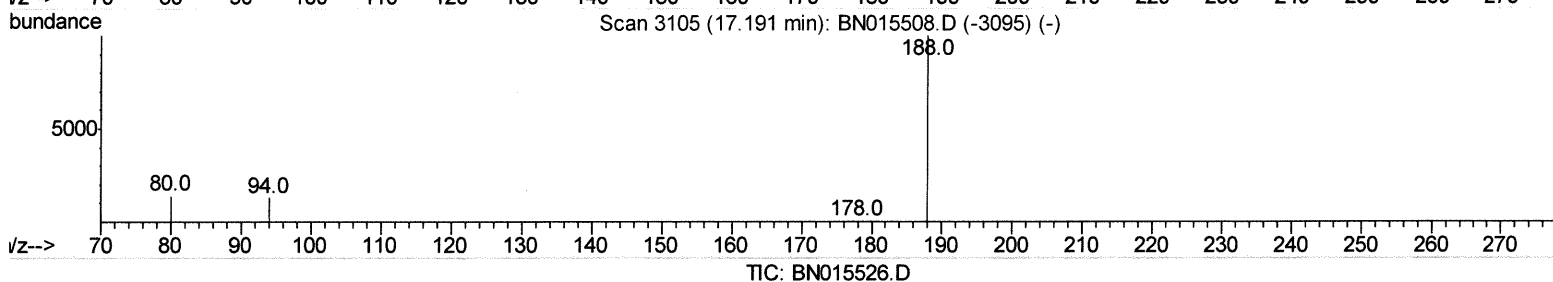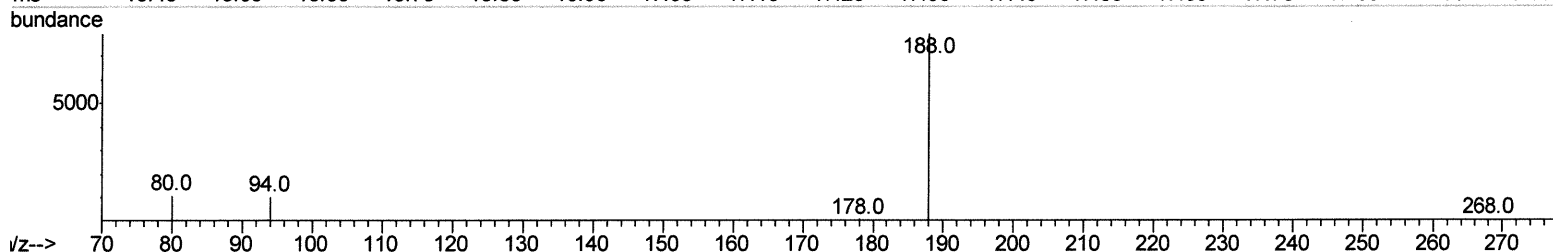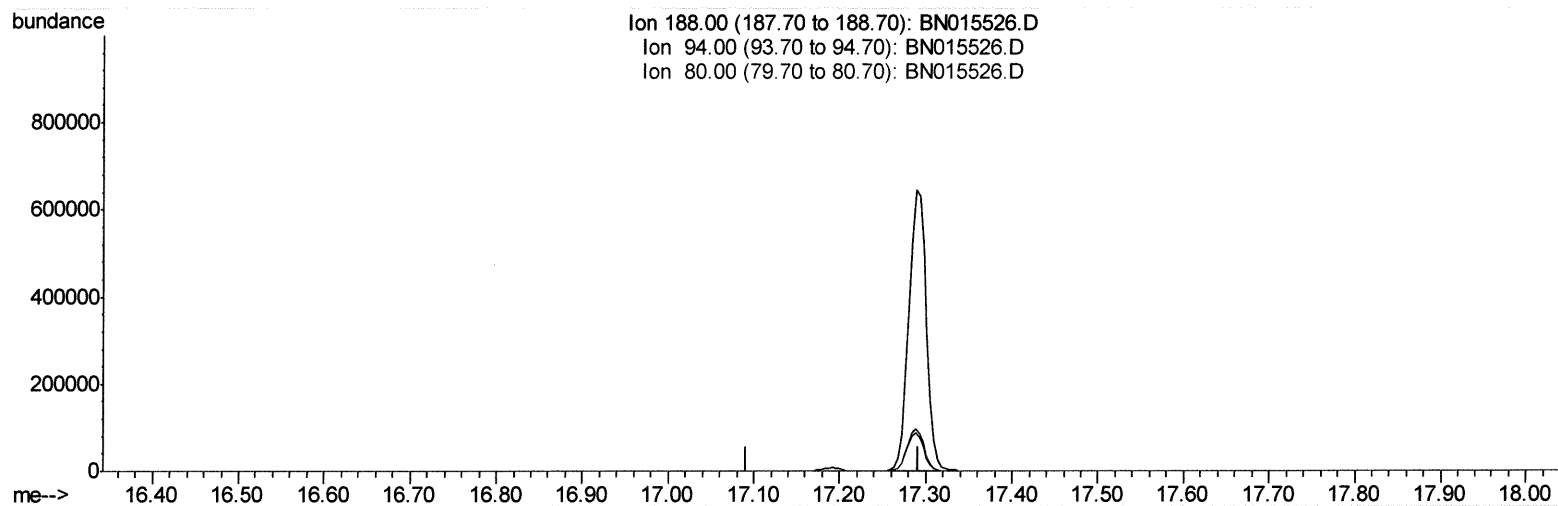

(13) Phenanthrene-d10 (I)

17.192min (-17.192) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	14.10	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015526.D
 Acq On : 13 Jul 2021 13:38
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/13/2021 4:39:36 PM

Quant Time: Jul 13 14:08:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

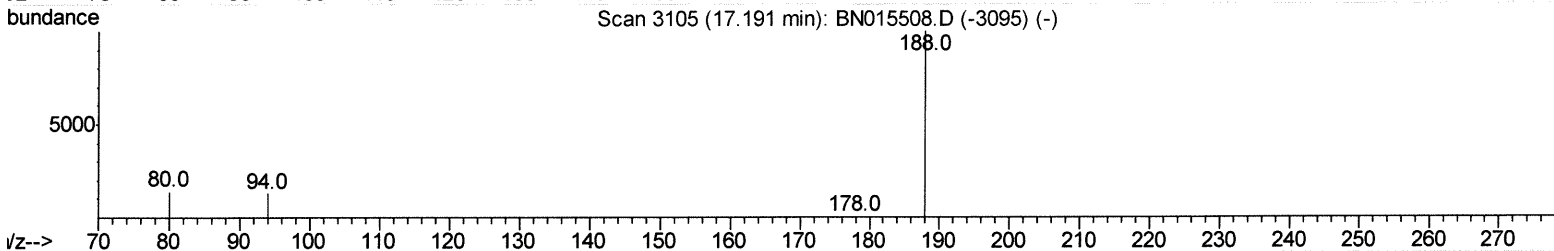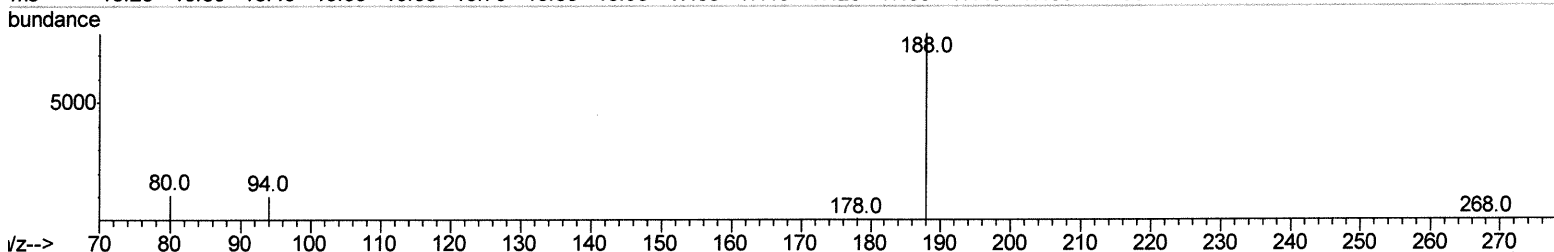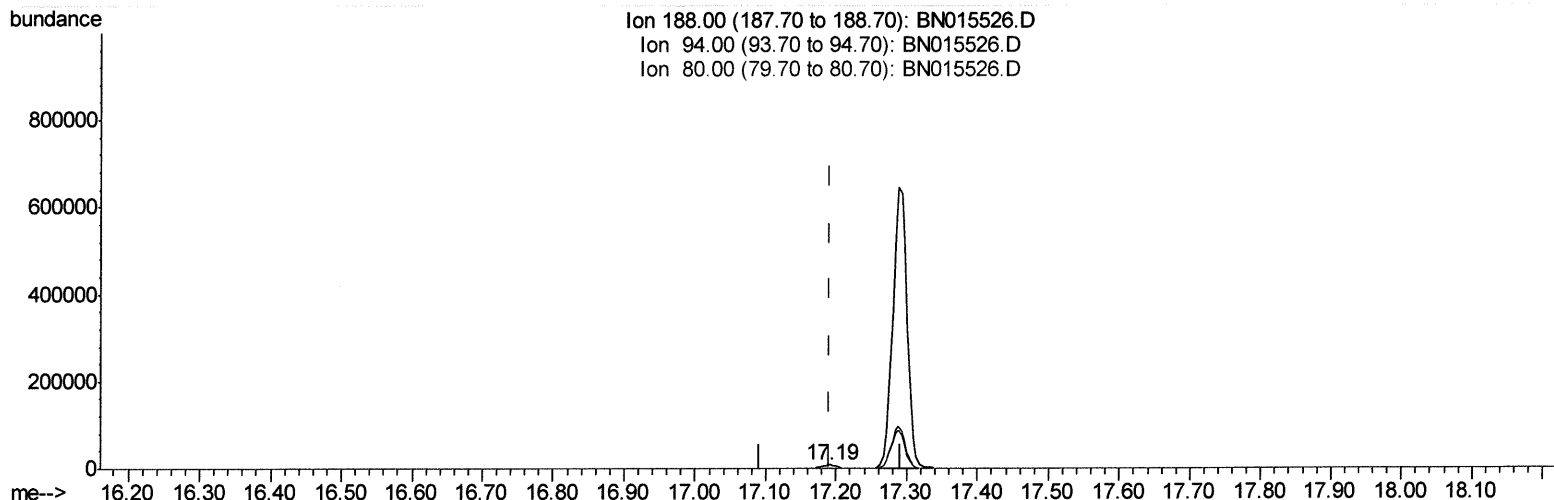

TIC: BN015526.D

(13) Phenanthrene-d10 (I)

17.191min (-0.000) 0.40ng/ul m

response 11259

347/14/21

Ion	Exp%	Act%
188.00	100	100
94.00	14.10	12.99
80.00	14.40	13.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015526.D
 Acq On : 13 Jul 2021 13:38
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/13/2021 4:39:36 PM

Quant Time: Jul 13 14:09:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	3000	0.40	ng/ul	0.00
4) Naphthalene-d8	10.59	136	10503	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.44	164	5815	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.19	188	11259m	0.40	ng/ul	0.00
17) Chrysene-d12	21.39	240	9032	0.40	ng/ul	0.00
23) Perylene-d12	23.74	264	9279	0.40	ng/ul	0.00

2/14/21

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	23106	6.83	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.19	152	5743	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.22	212	11389	0.38	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed