

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071221\
 Data File : BN015517.D
 Acq On : 13 Jul 2021 08:13
 Operator : CG/JU
 Sample : M2869-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDY4

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:45:38 PM

Quant Time: Jul 13 08:48:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 11:02:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.808	152	3891	0.400	ng/ul	0.00
4) Naphthalene-d8	10.595	136	13223	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.441	164	7009	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.191	188	13561m	0.400	ng/ul	0.00
17) Chrysene-d12	21.387	240	10565	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	10677	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	21925	4.999	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.190	152	6674	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.225	212	12438	0.358	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.253	202	1031	0.021	ng/ul#	Qvalue 77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071221\
Data File : BN015517.D
Acq On : 13 Jul 2021 08:13
Operator : CG/JU
Sample : M2869-14
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BGDY4

Manual Integrations
APPROVED

mohammad
7/13/2021 1:45:38 PM


Quant Time: Jul 13 08:48:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 11:02:52 2021
Response via : Initial Calibration

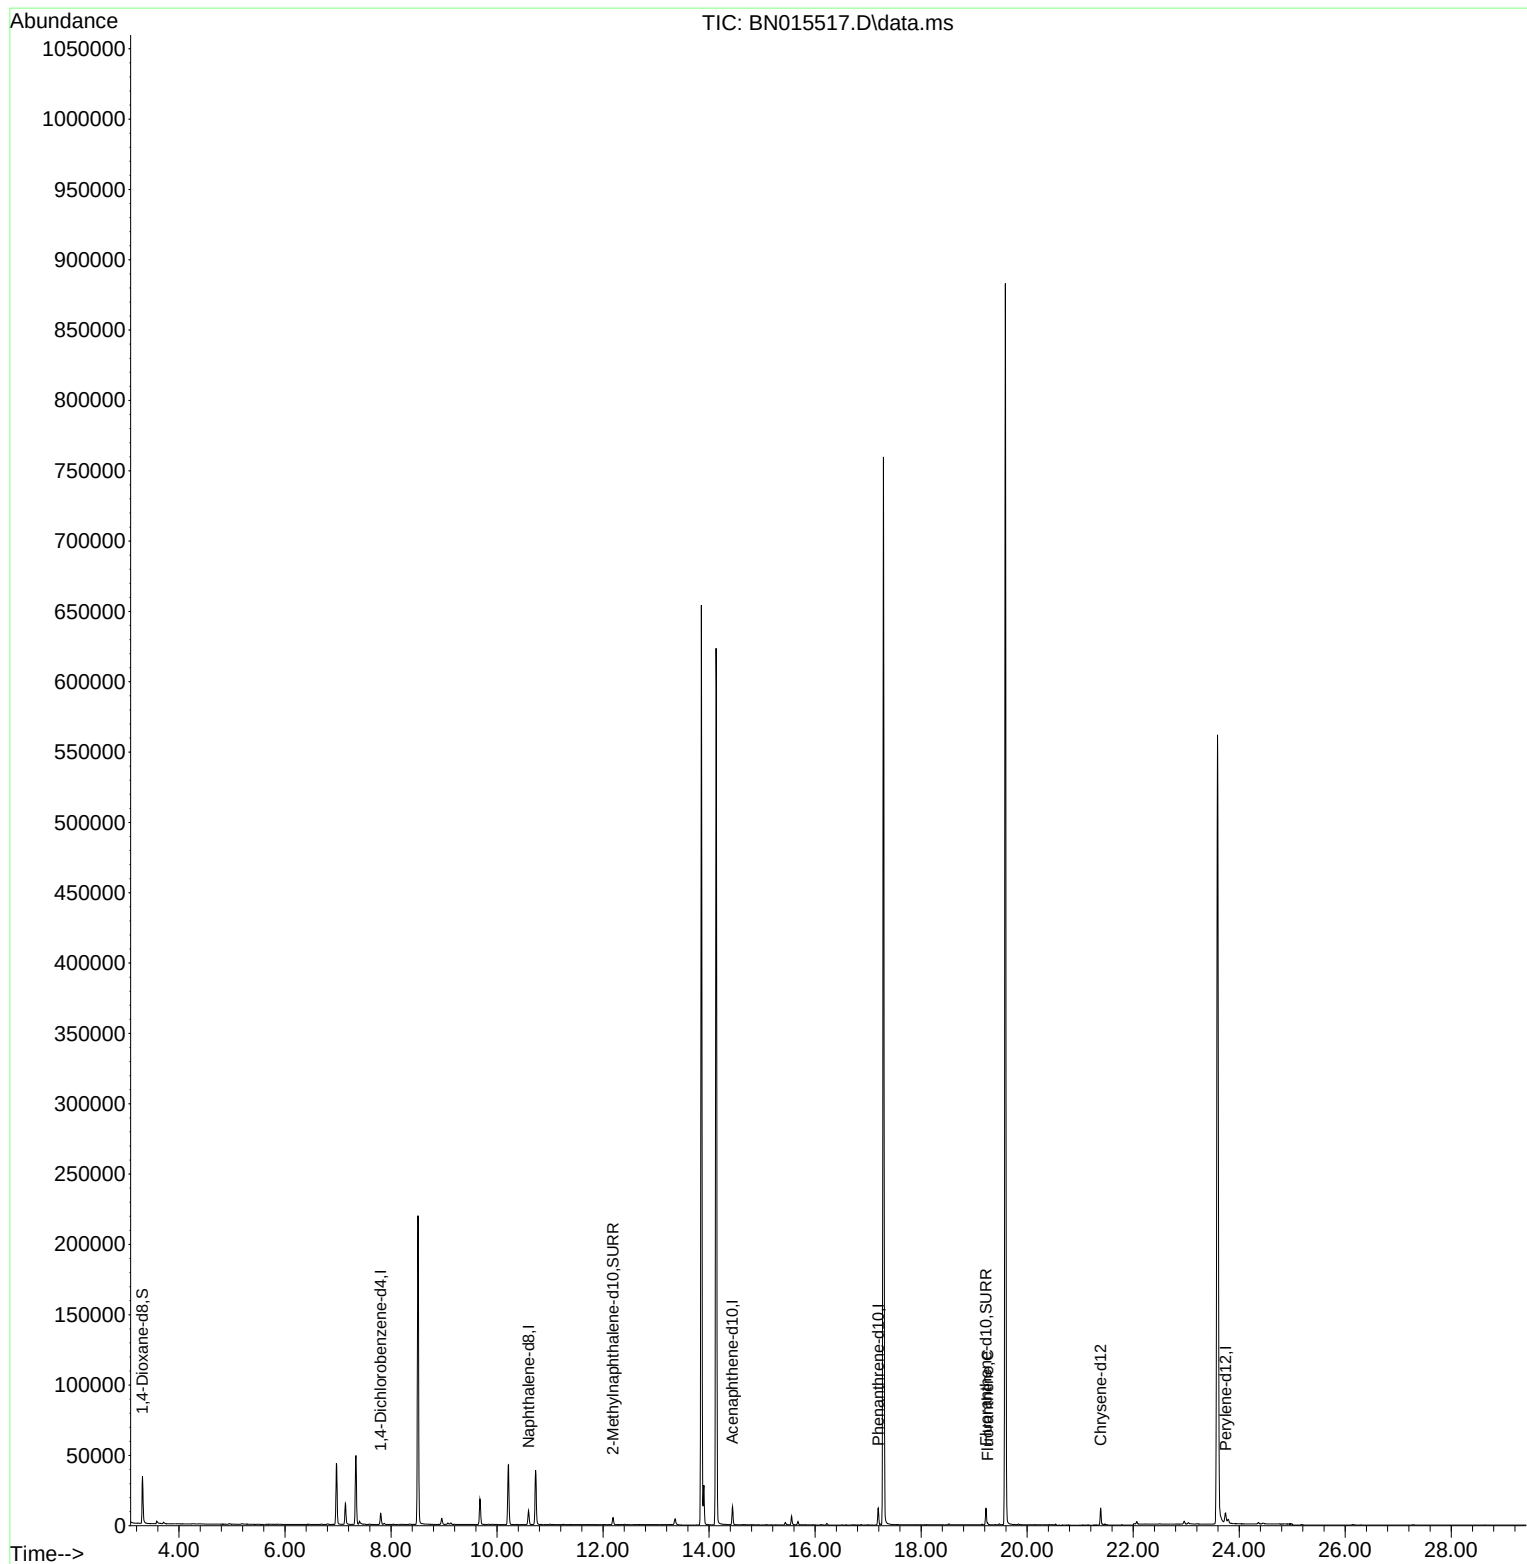

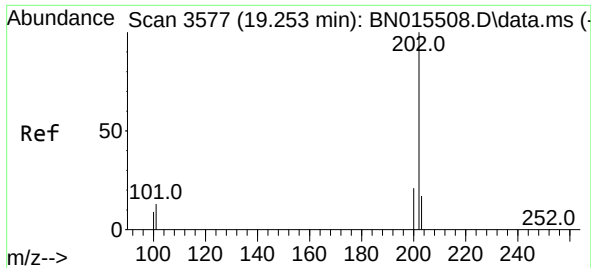

#19
Fluoranthene
Concen: 0.021 ng/ul
RT: 19.253 min Scan# 3577
Delta R.T. -0.005 min
Lab File: BN015517.D
Acq: 13 Jul 2021 08:13

Instrument :
BNA_N
ClientSampleId :
BGDY4

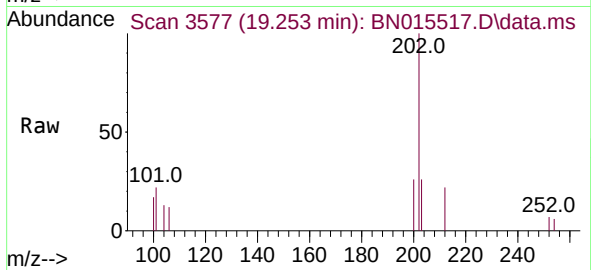

Tgt Ion	Ratio	Lower	Upper
202	100		
101	21.6	10.1	15.1#
100	17.4	7.4	11.0#

Manual Integrations
APPROVED

mohammad
7/13/2021 1:45:38 PM

