

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
 Data File : BN032634.D
 Acq On : 11 Jul 2024 14:06
 Operator : MA/JU
 Sample : PB161917BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK917

Quant Time: Jul 12 01:54:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 01:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.561	152	5794	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.327	136	19677	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.207	164	12875	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.062	188	1529189	0.400	ng/ul	0.07
17) Chrysene-d12	21.203	240	18728	0.400	ng/ul	0.00
23) Perylene-d12	23.383	264	29660	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	32242	4.634	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.971	152	6513	0.219	ng/ul	0.00
18) Fluoranthene-d10	19.008	212	17496	0.287	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.206	166	2428	0.049	ng/ul#	13
20) Pyrene	19.371	202	2523	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.231	252	5006	0.055	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032634.D
Acq On : 11 Jul 2024 14:06
Operator : MA/JU
Sample : PB161917BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK917

Quant Time: Jul 12 01:54:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration




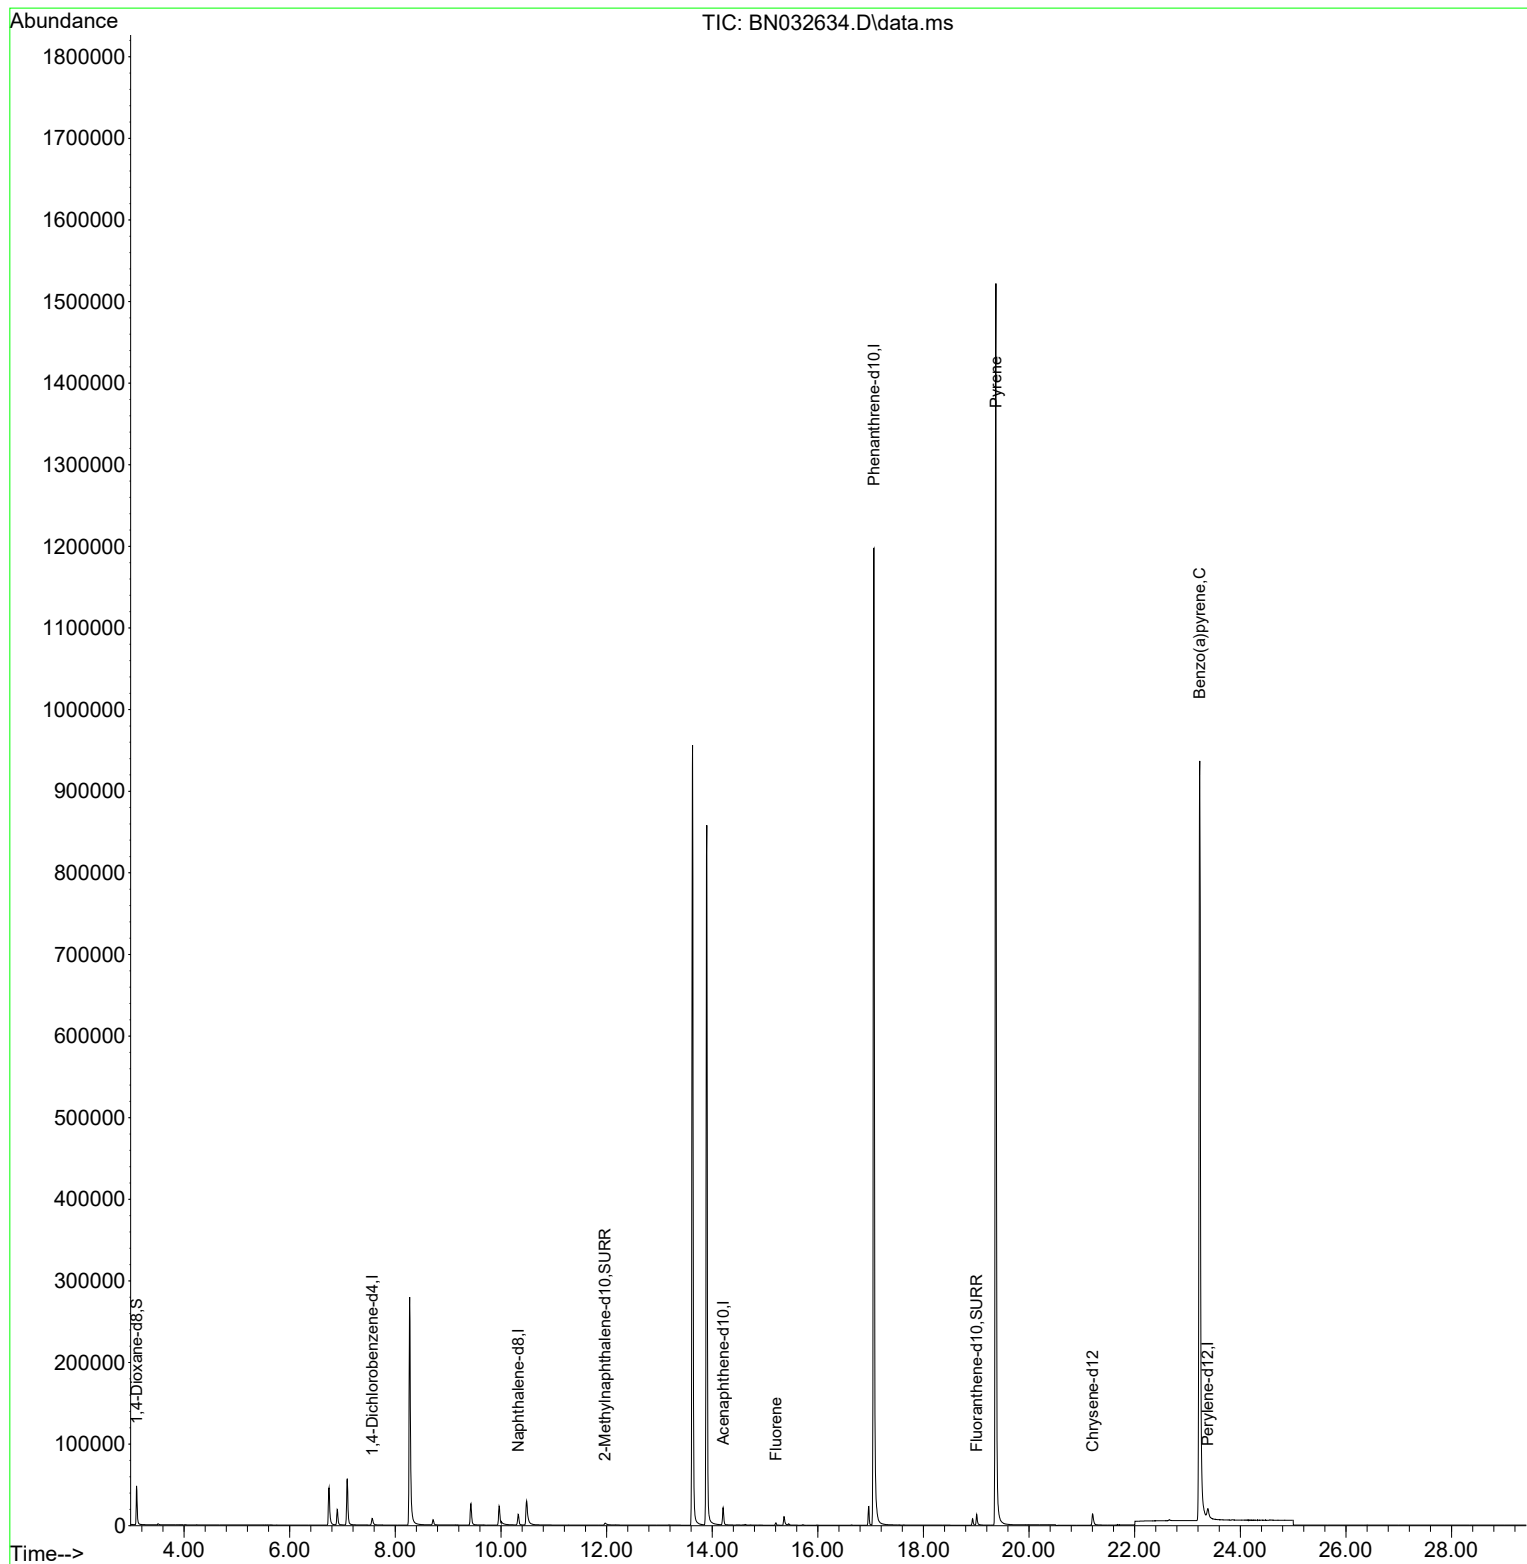


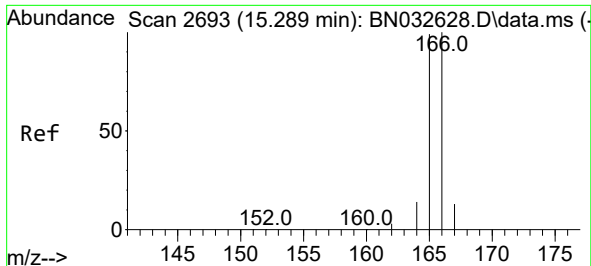

#12
Fluorene
Concen: 0.049 ng/ul
RT: 15.206 min Scan# 206
Delta R.T. -0.083 min
Lab File: BN032634.D
Acq: 11 Jul 2024 14:06




Instrument :
BNA_N
ClientSampleId :
SBLK917


Tgt Ion:166 Resp: 2428
Ion Ratio Lower Upper
166 100
165 7.3 79.7 119.5#
167 34.3 11.4 17.2#

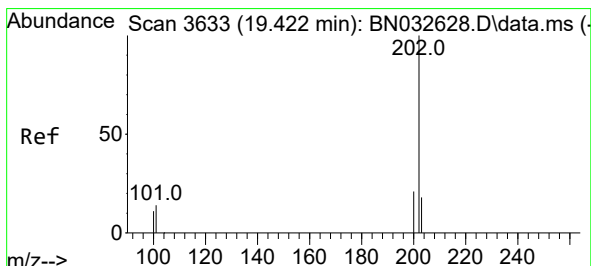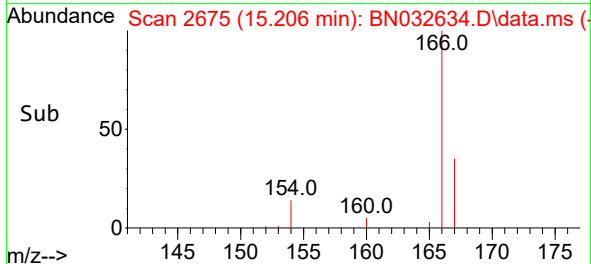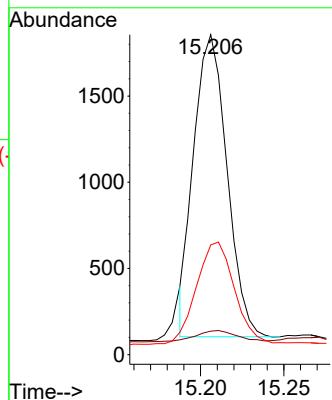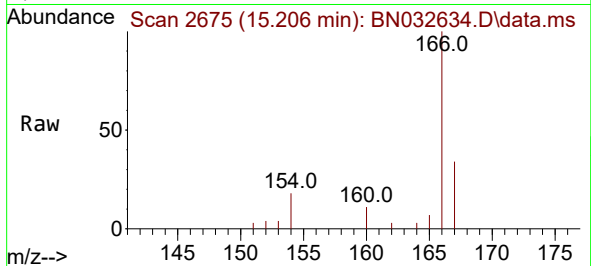

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.371 min Scan# 3622
Delta R.T. -0.051 min
Lab File: BN032634.D
Acq: 11 Jul 2024 14:06


Tgt Ion:202 Resp: 2523
Ion Ratio Lower Upper
202 100
101 151.0 11.8 17.6#
100 1078.5 9.6 14.4#

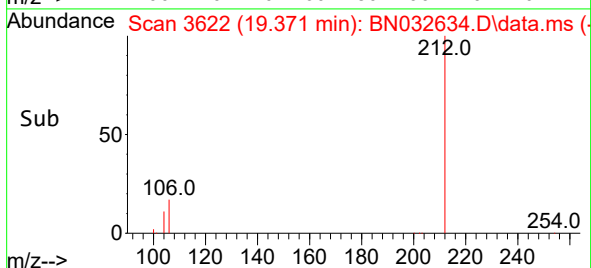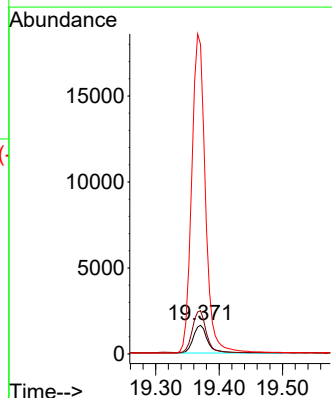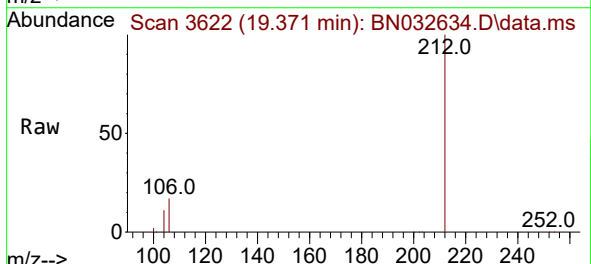

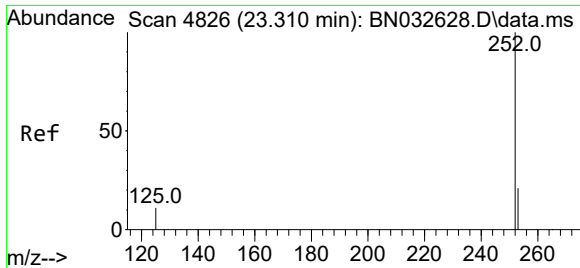

#26
Benzo(a)pyrene
Concen: 0.055 ng/ul
RT: 23.231 min Scan# 41
Delta R.T. -0.079 min
Lab File: BN032634.D
Acq: 11 Jul 2024 14:06

Instrument :
BNA_N
ClientSampleId :
SBLK917

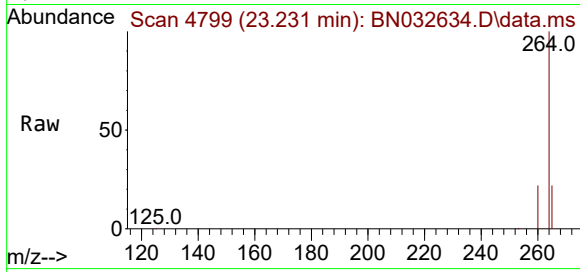

Tgt Ion:252 Resp: 5006
Ion Ratio Lower Upper
252 100
253 50.1 25.4 38.0#
125 54.0 20.6 30.8#

