

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
 Data File : BN032701.D
 Acq On : 13 Jul 2024 09:41
 Operator : MA/JU
 Sample : PB161929BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK929

Quant Time: Jul 15 08:55:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 01:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.548	152	5423	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.315	136	16036	0.400	ng/ul	-0.05
9) Acenaphthene-d10	14.196	164	8489	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.053	188	1130602	0.400	ng/ul	0.06
17) Chrysene-d12	21.184	240	9216	0.400	ng/ul	-0.01
23) Perylene-d12	23.367	264	21072	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	38978	5.986	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.942	152	6794	0.280	ng/ul	-0.03
18) Fluoranthene-d10	18.998	212	13040	0.434	ng/ul	-0.03
Target Compounds						
					Qvalue	
20) Pyrene	19.360	202	1845	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.221	252	4523	0.070	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032701.D
Acq On : 13 Jul 2024 09:41
Operator : MA/JU
Sample : PB161929BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK929

Quant Time: Jul 15 08:55:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

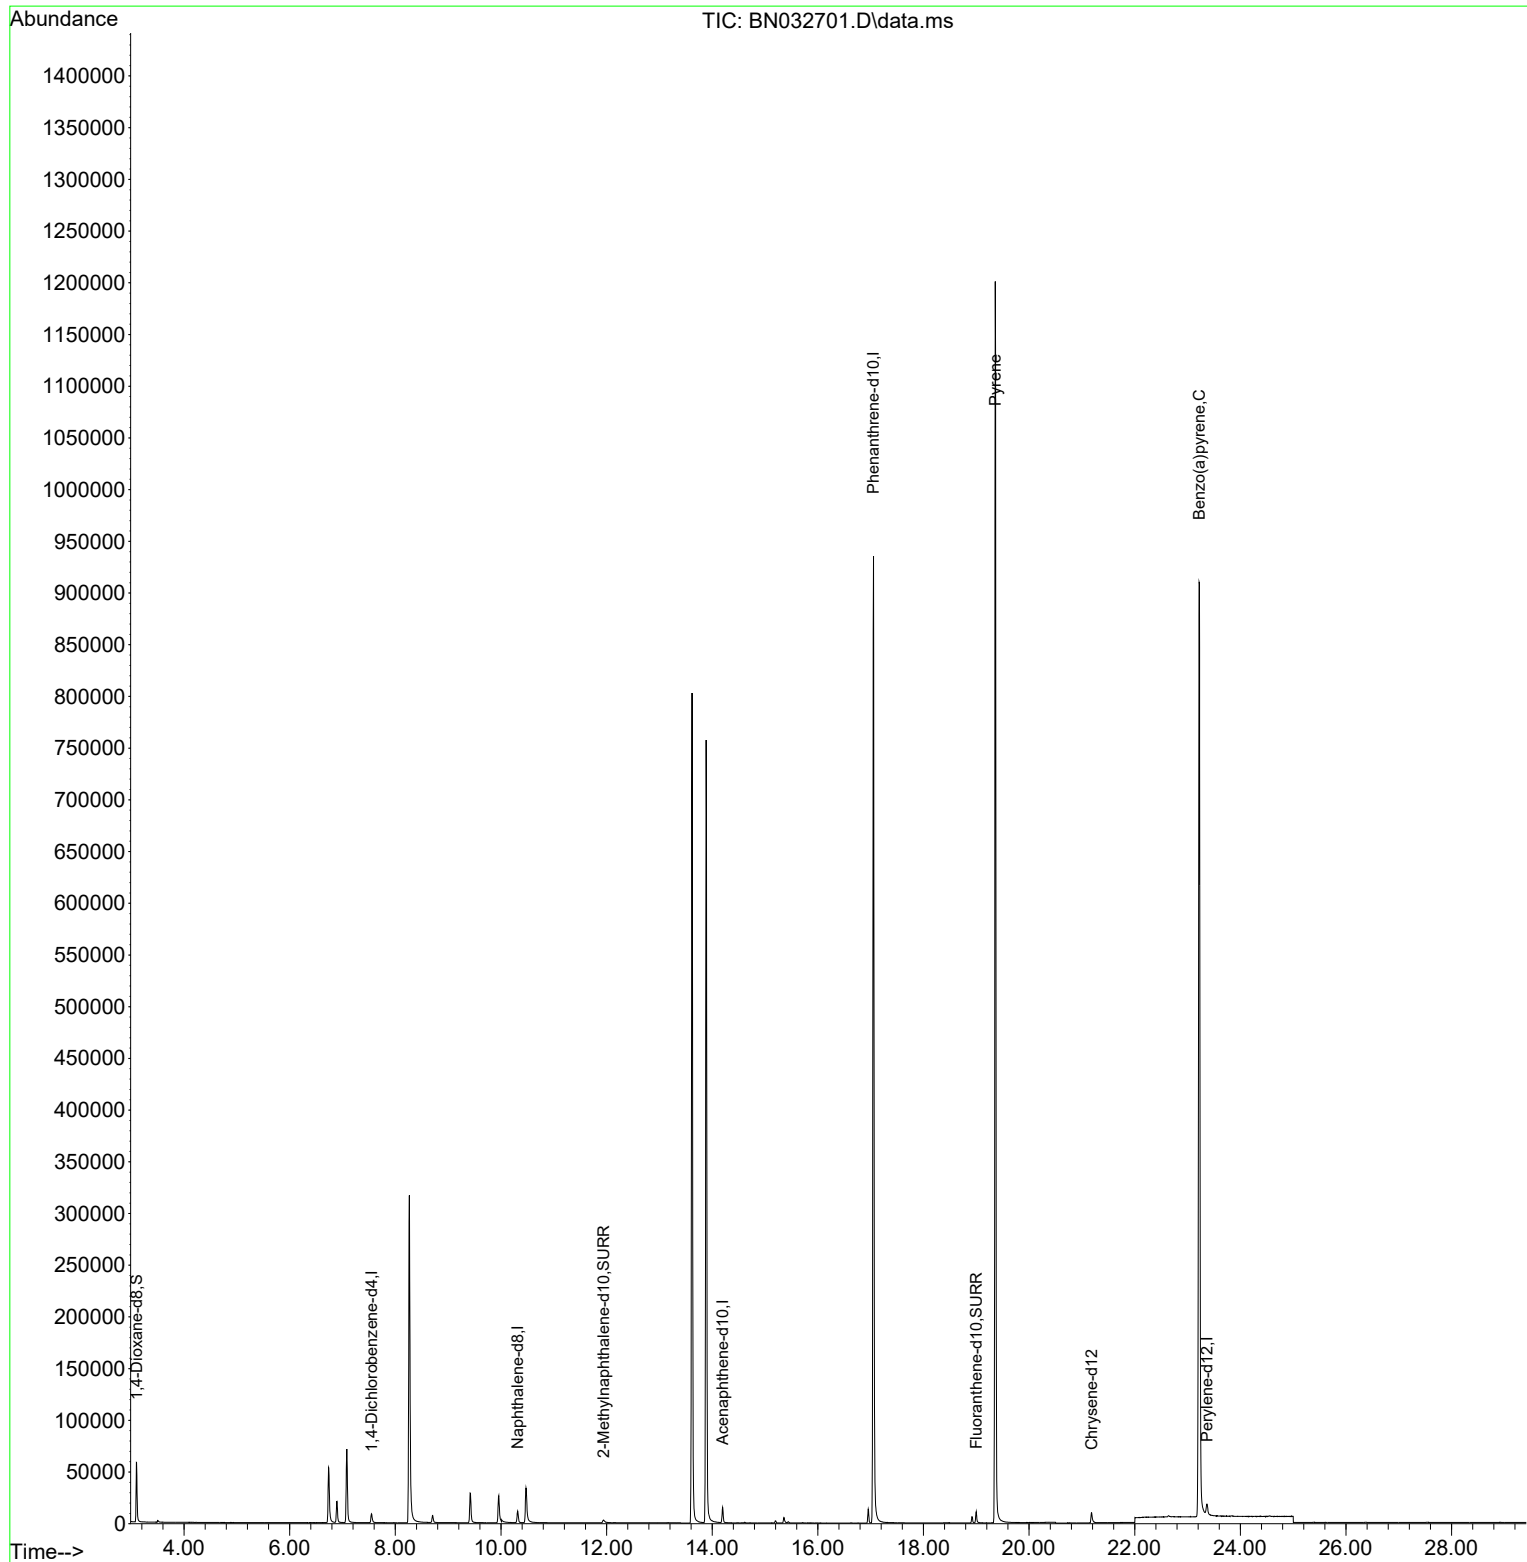

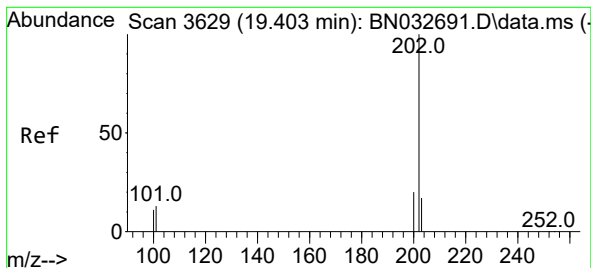

#20

Pyrene

Concen: 0.048 ng/ul

RT: 19.360 min Scan# 3

Delta R.T. -0.062 min

Lab File: BN032701.D

Acq: 13 Jul 2024 09:41

Instrument :

BNA_N

ClientSampleId :

SBLK929





Tgt Ion:202 Resp: 1845

Ion Ratio Lower Upper

202 100

101 151.0 11.8 17.6#

100 1102.9 9.6 14.4#

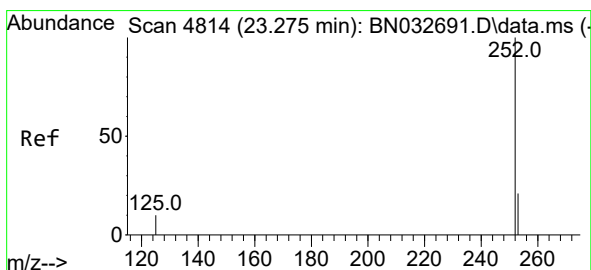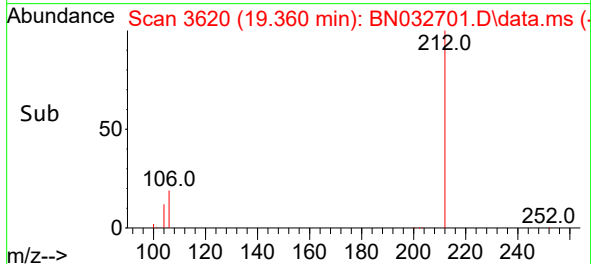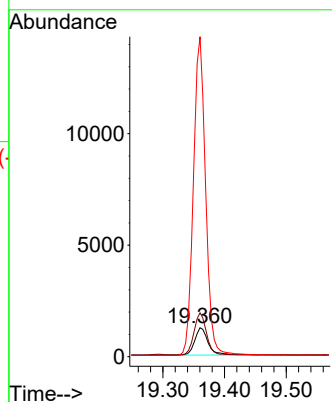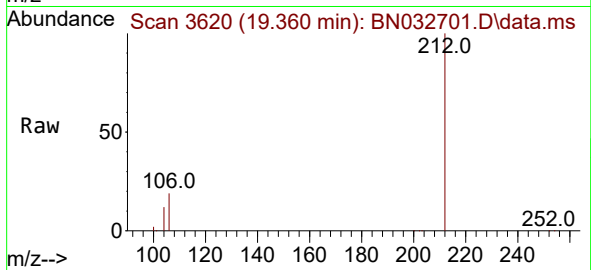

#26

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.221 min Scan# 4796

Delta R.T. -0.089 min

Lab File: BN032701.D

Acq: 13 Jul 2024 09:41

Tgt Ion:252 Resp: 4523

Ion Ratio Lower Upper

252 100

253 53.4 25.4 38.0#

125 57.3 20.6 30.8#

