




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

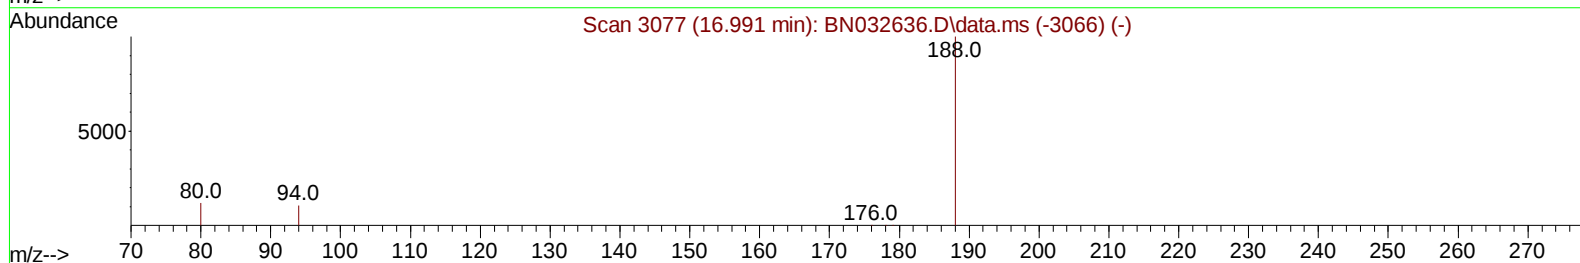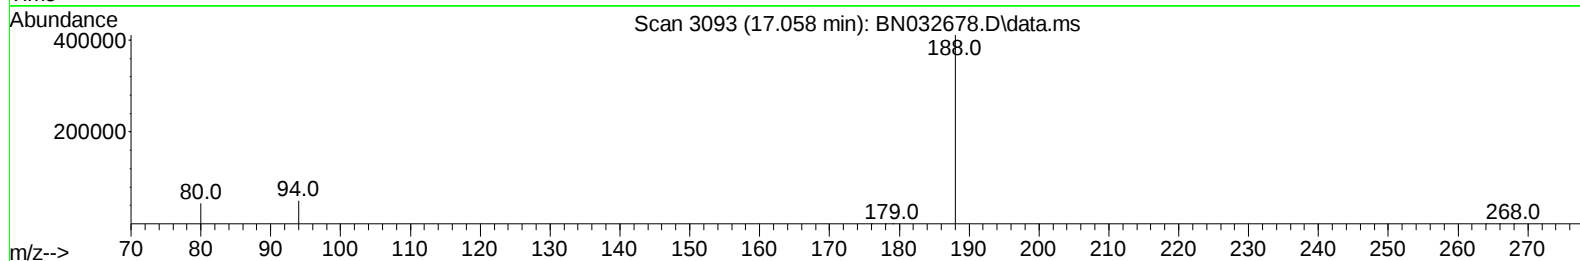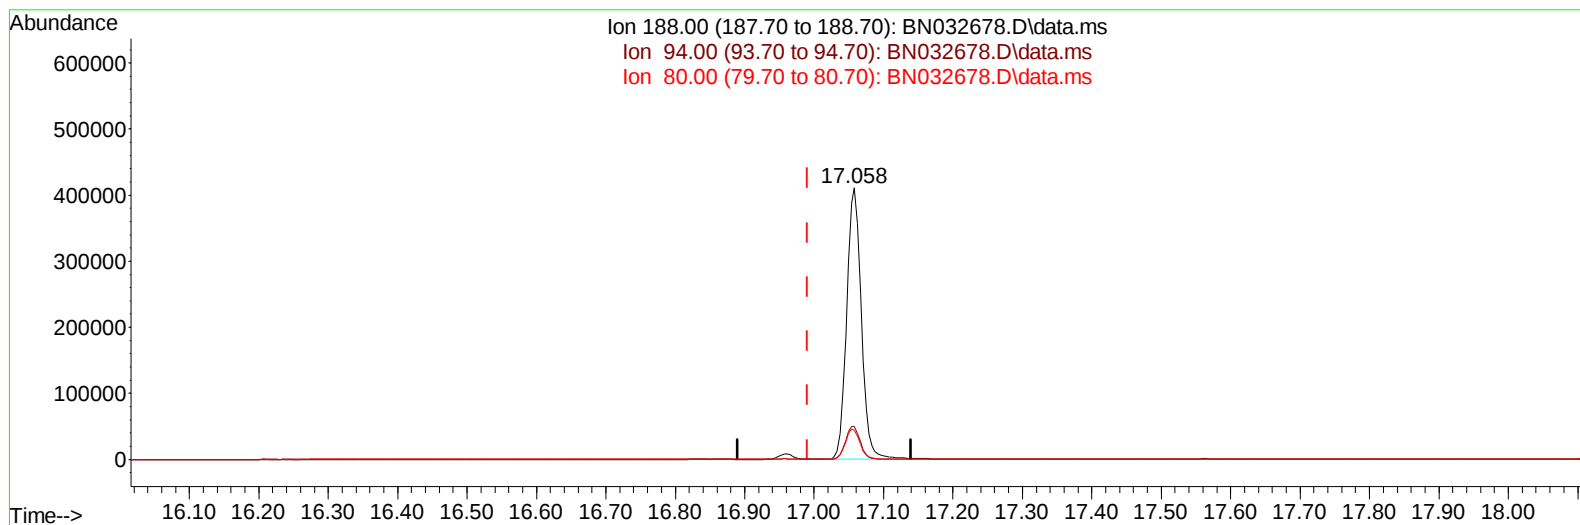

TIC: BN032678.D\data.ms

(13) Phenanthrene-d10 (I)

17.058min (+ 0.067) 0.40 ng/u1

response 599091

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	12.16
80.00	12.00	10.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

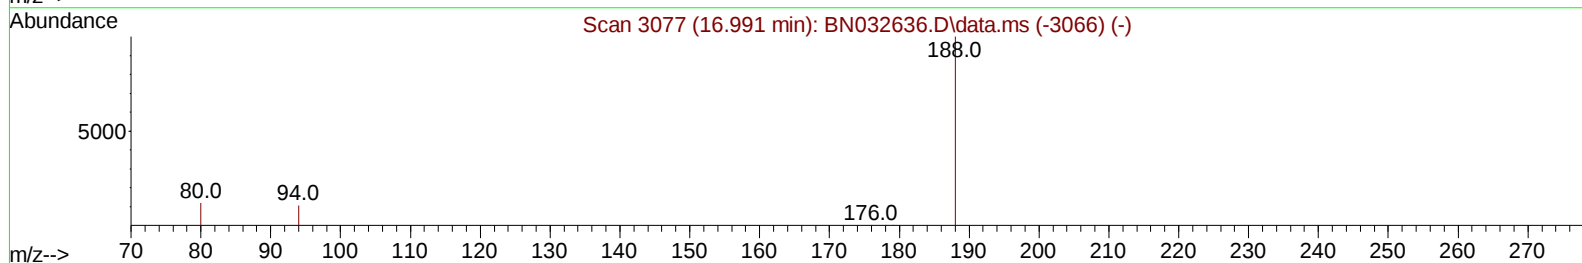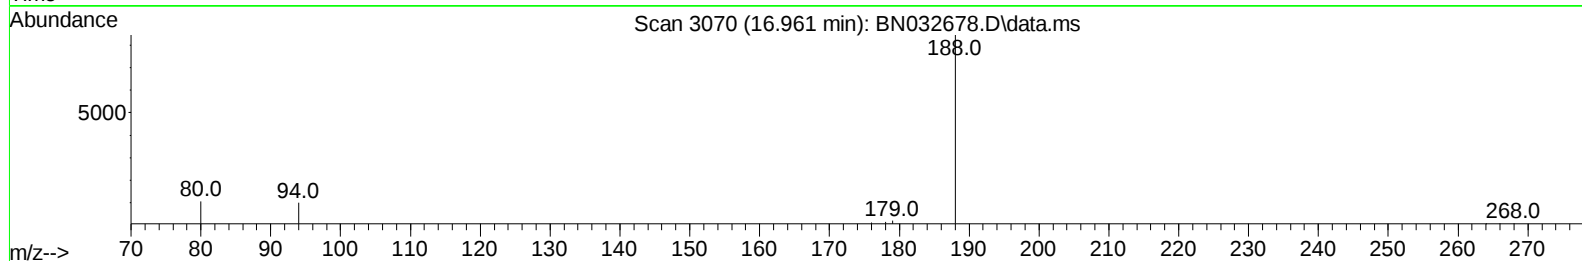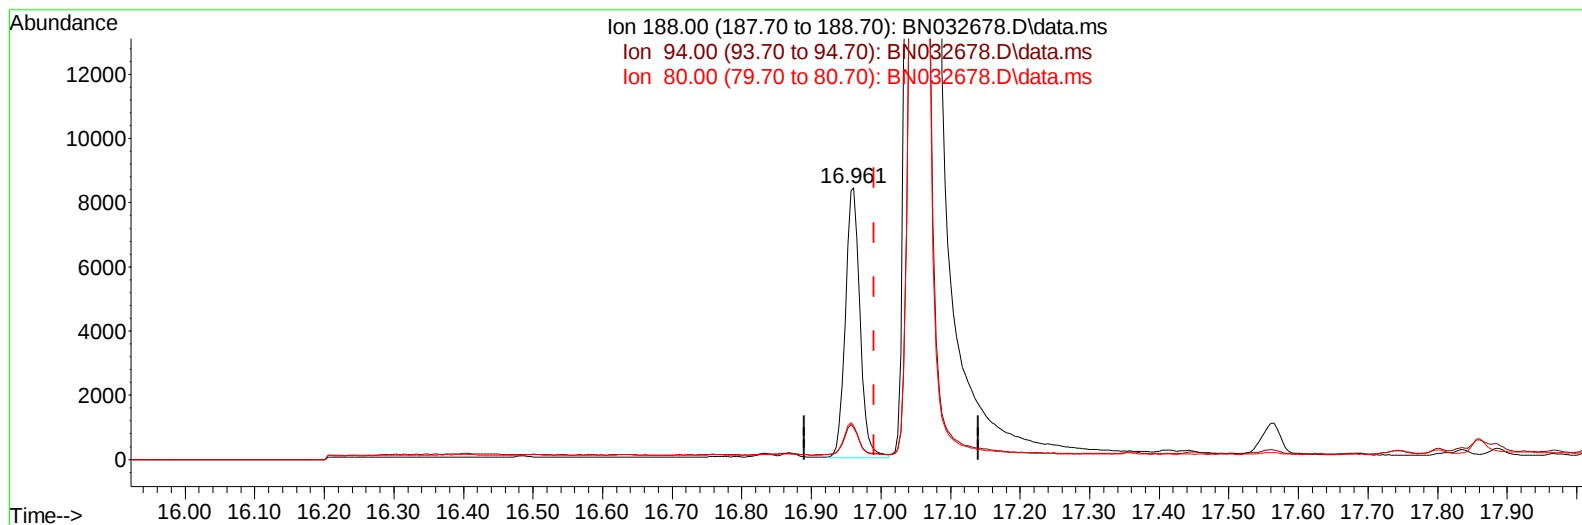

TIC: BN032678.D\data.ms

(13) Phenanthrene-d10 (I)

16.961min (-0.030) 0.40 ng/ul m

response 12231

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	11.73
80.00	12.00	12.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

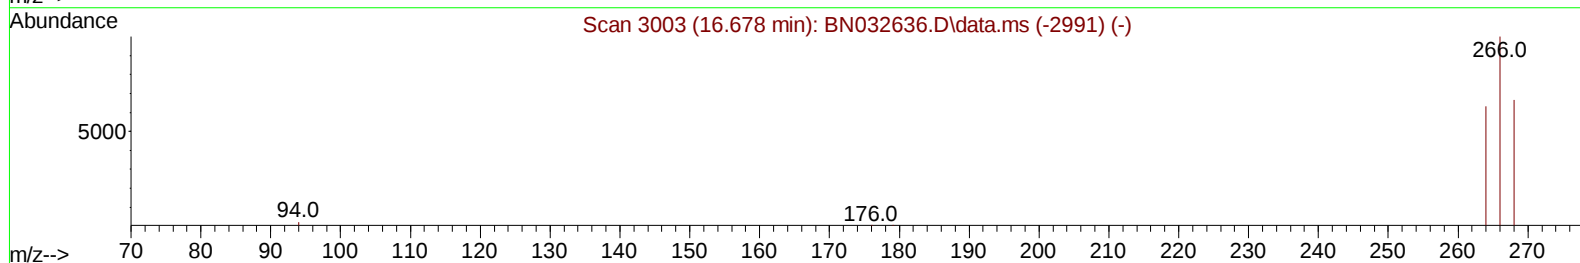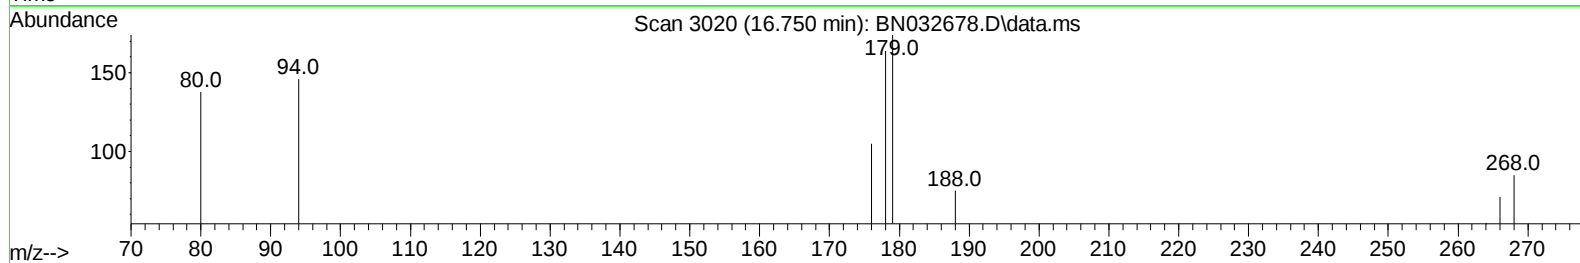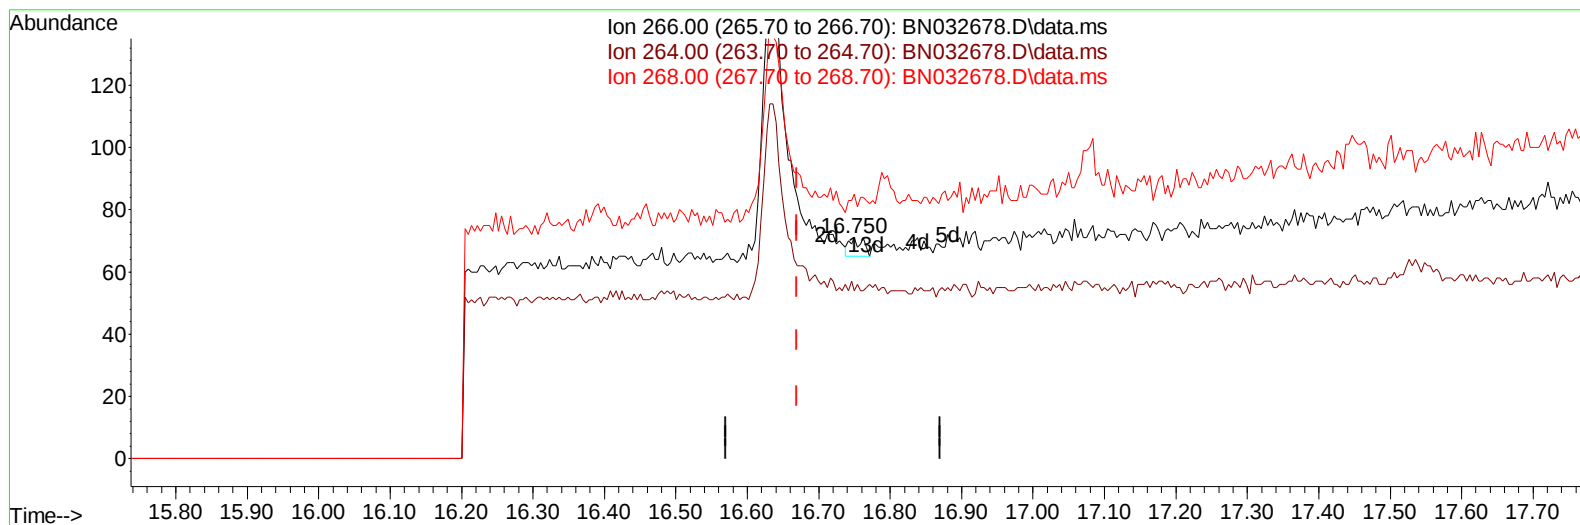

TIC: BN032678.D\data.ms

(14) Pentachloropheno1

16.750min (+ 0.080) 0.00 ng/u1

response 8

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.80	0.00#
268.00	64.50	50.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

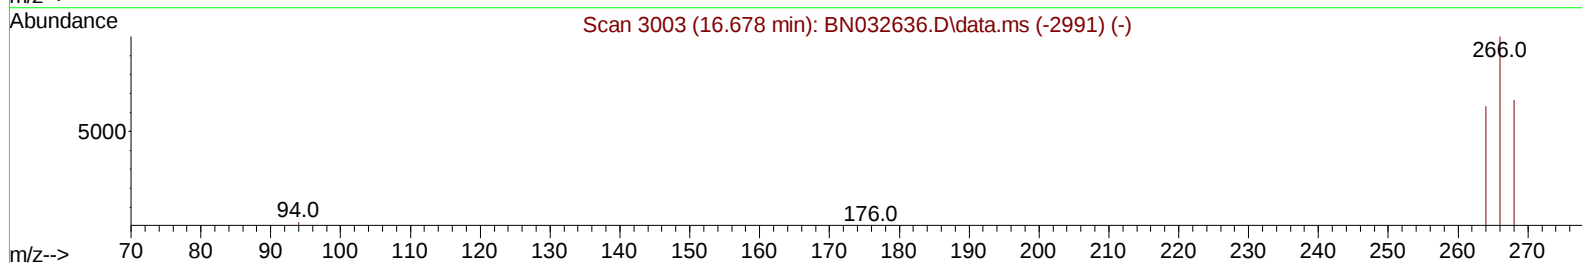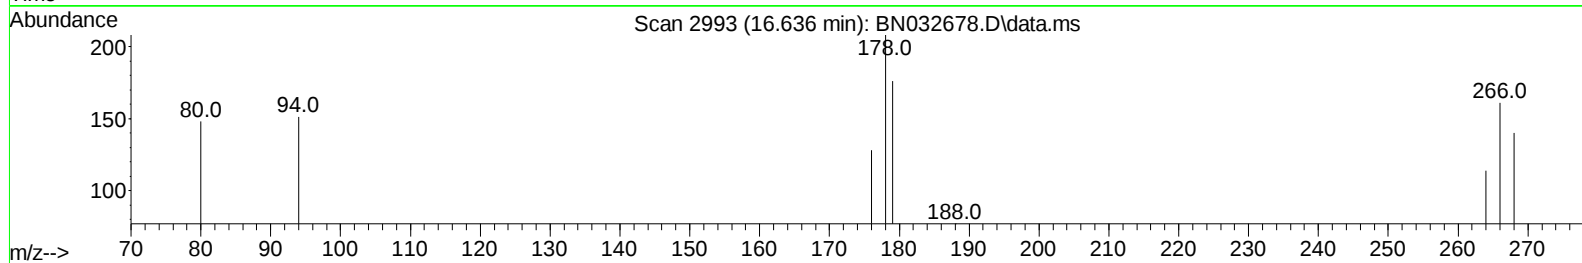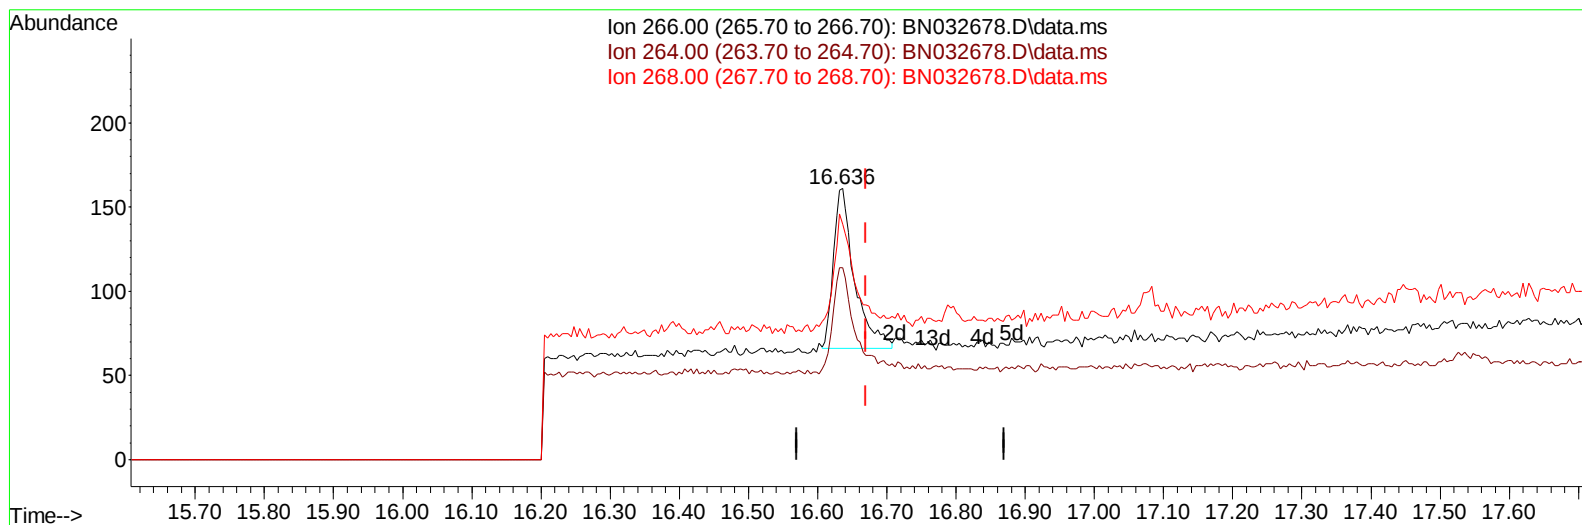

TIC: BN032678.D\data.ms

(14) Pentachloropheno1

16.636min (-0.034) 0.09 ng/ul m

response 202

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	61.80	0.00#
268.00	64.50	1.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

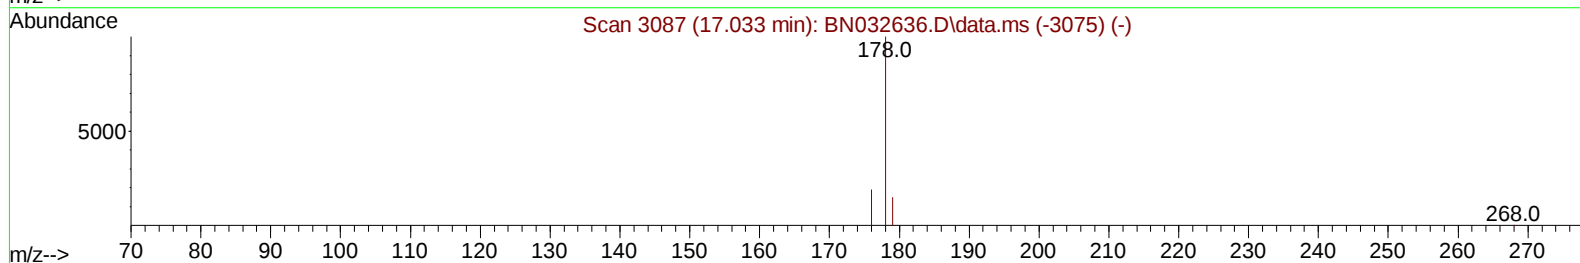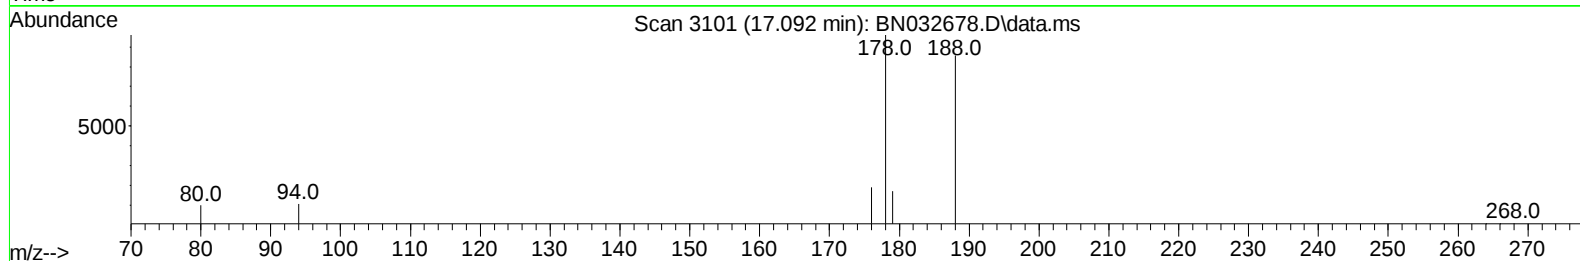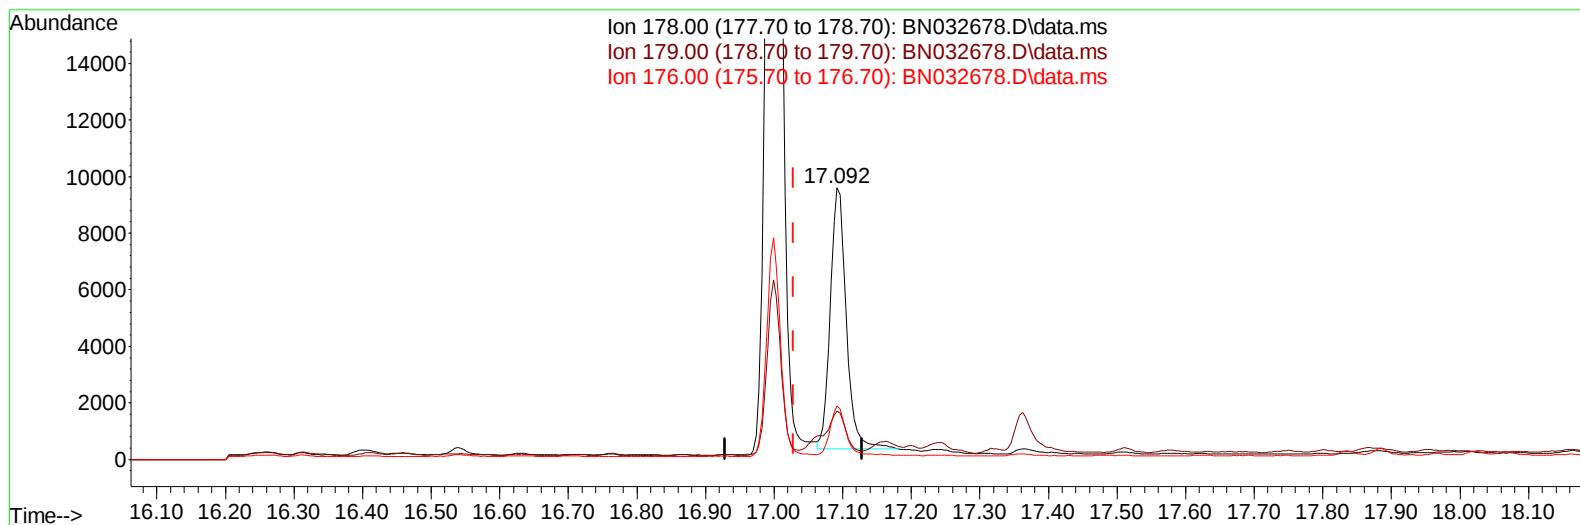

TIC: BN032678.D\data.ms

(15) Phenanthrene

17.092min (+ 0.063) 0.45 ng/u1

response 15065

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.20	17.72
176.00	19.50	19.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

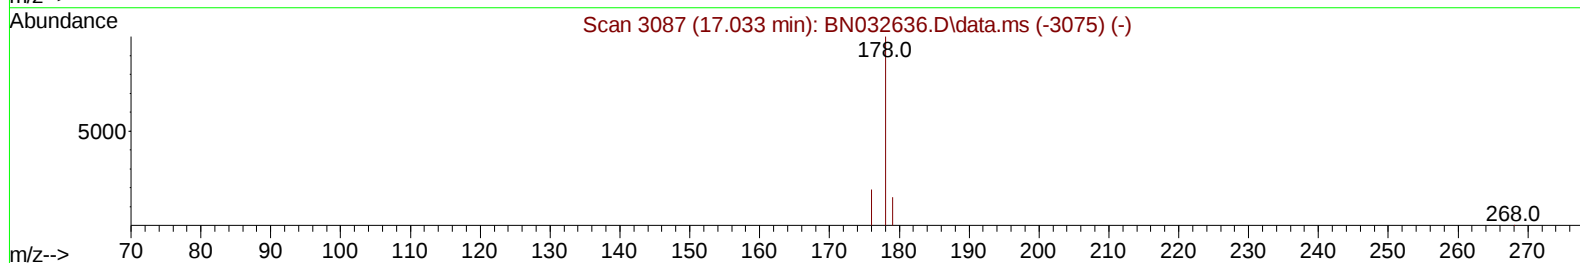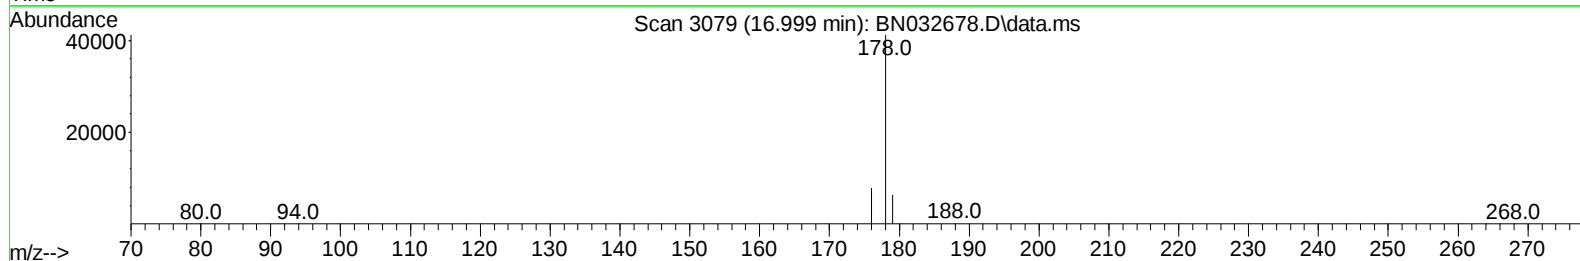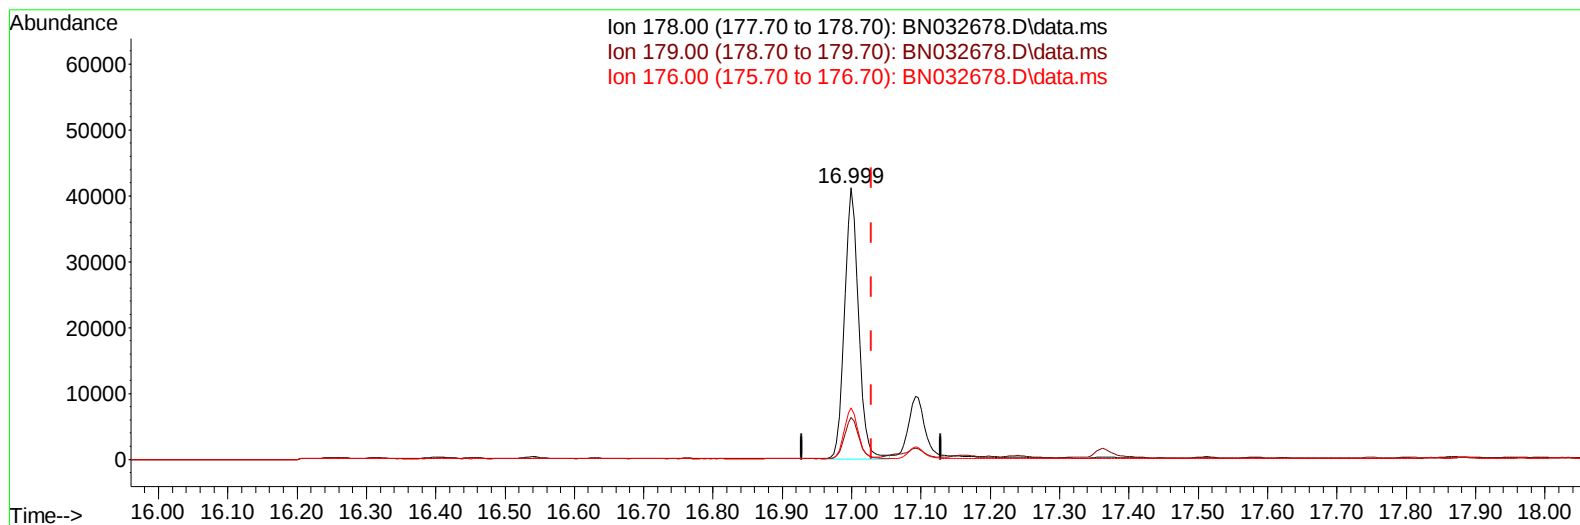

TIC: BN032678.D\data.ms

(15) Phenanthrene

16.999min (-0.030) 1.74 ng/ul m

response 57816

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.20	15.41
176.00	19.50	19.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

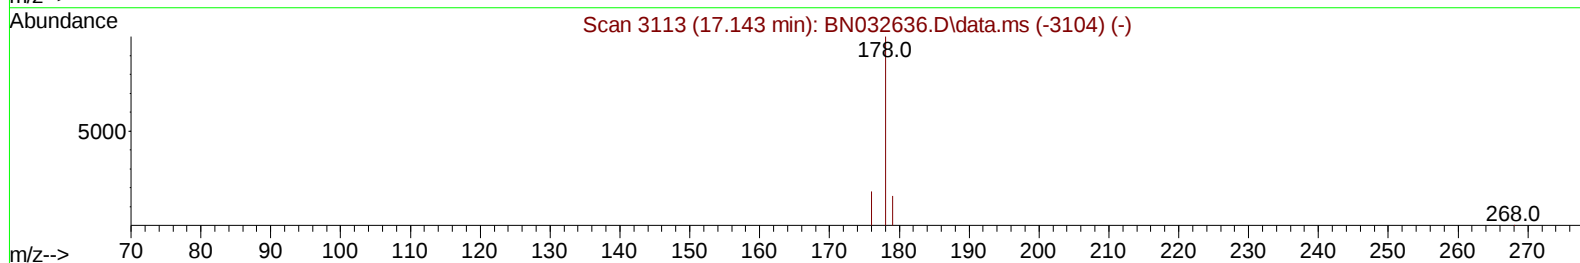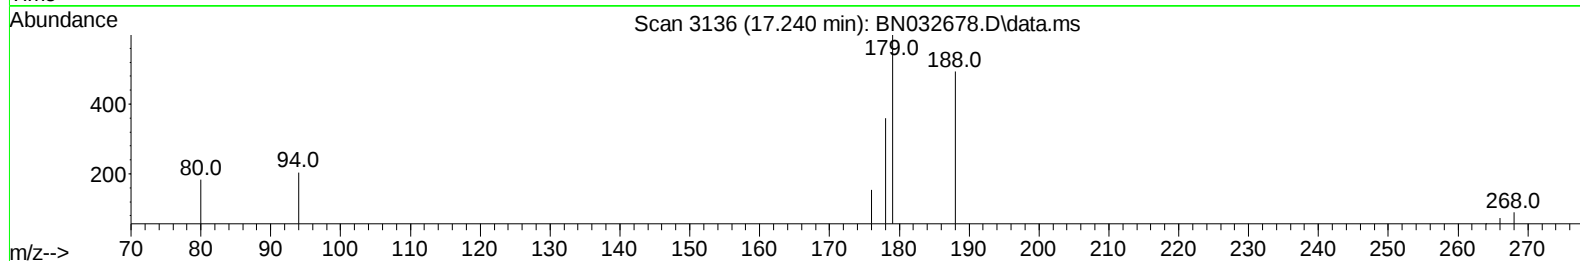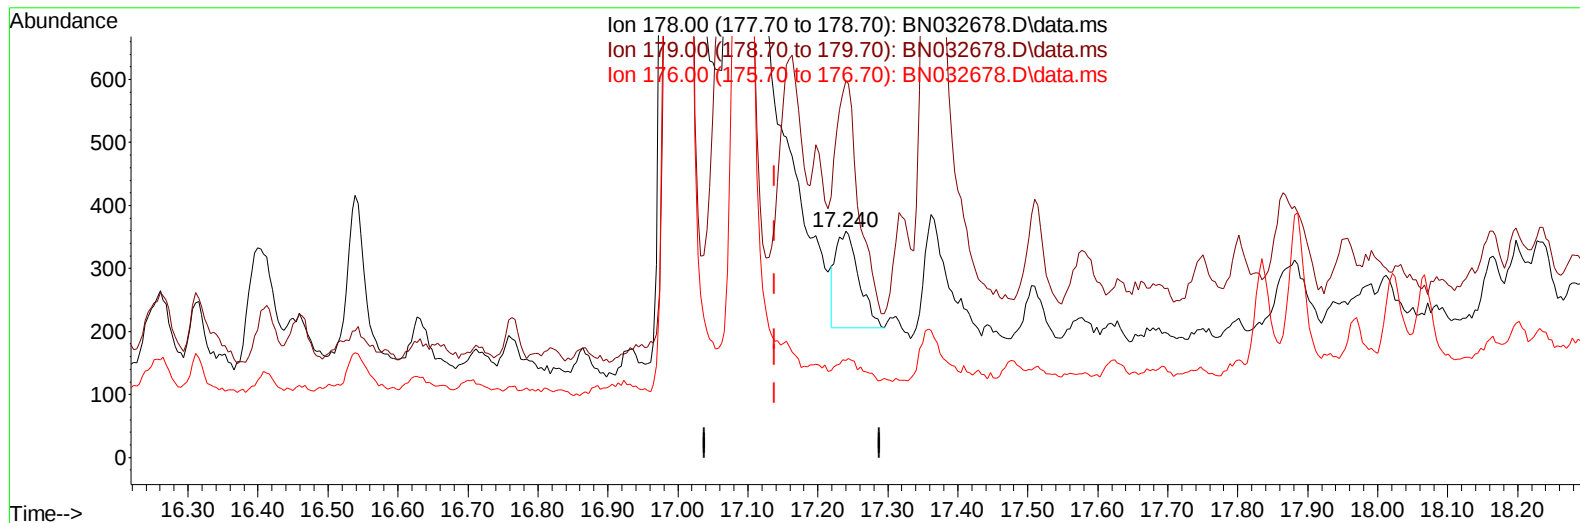

TIC: BN032678.D\data.ms

(16) Anthracene

17.240min (+ 0.101) 0.01 ng/u1

response 355

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.80	166.57#
176.00	19.20	42.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

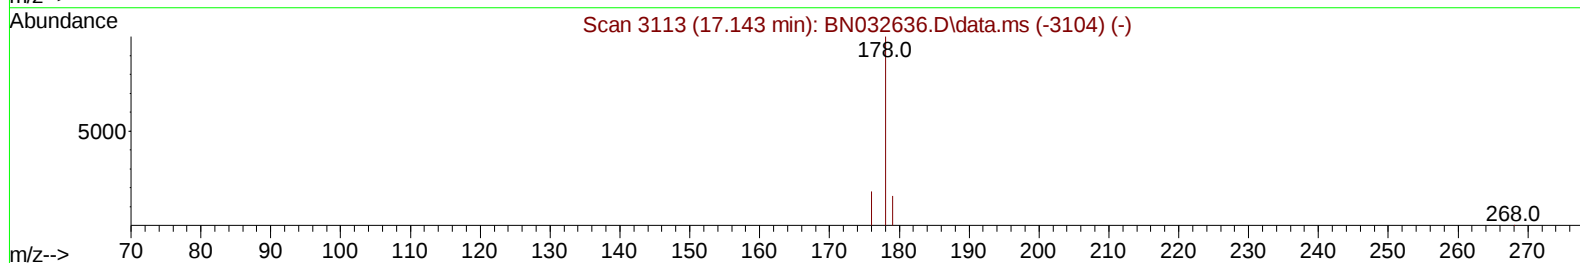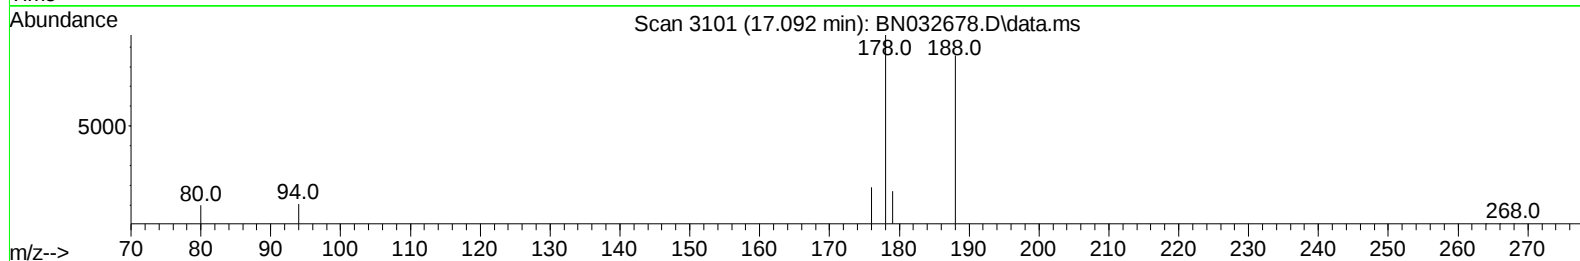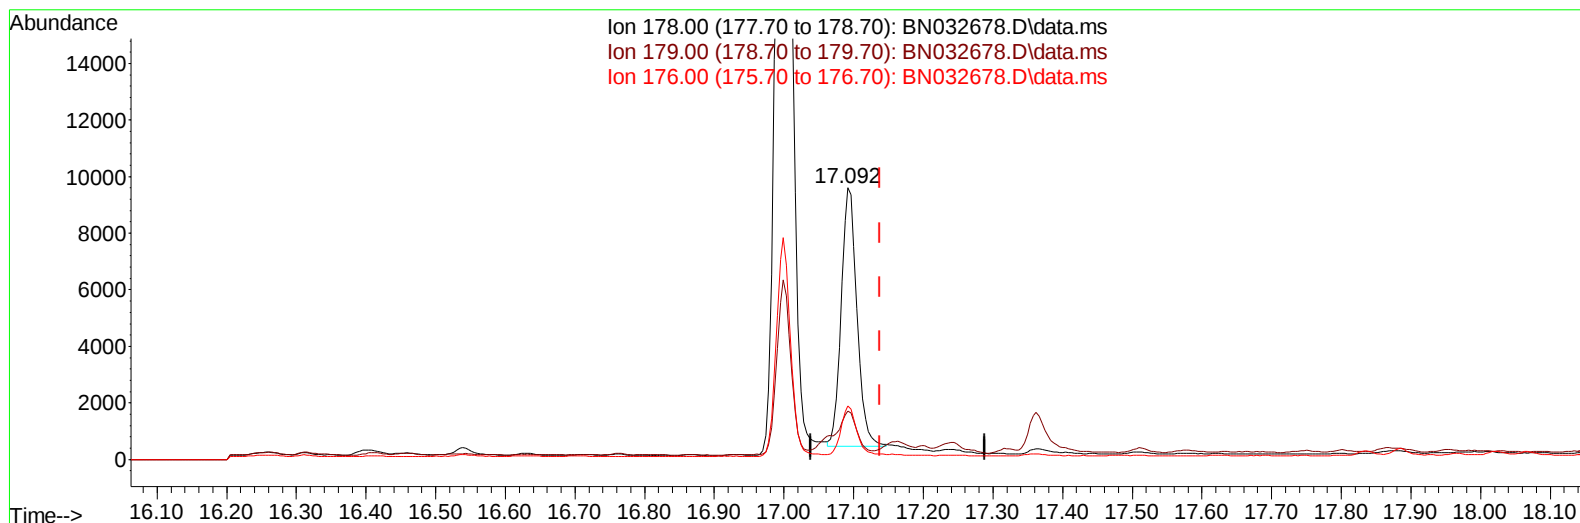

TIC: BN032678.D\data.ms

(16) Anthracene

17.092min (-0.047) 0.53 ng/u1 m

response 14344

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.80	17.72
176.00	19.20	19.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

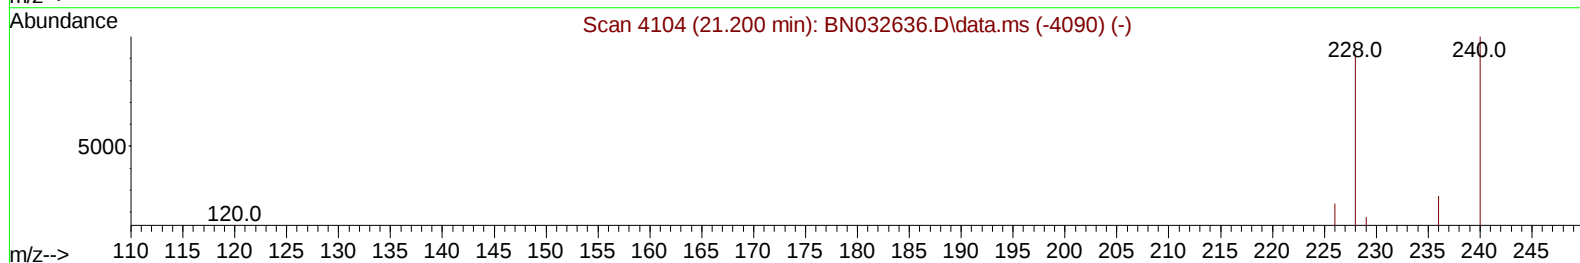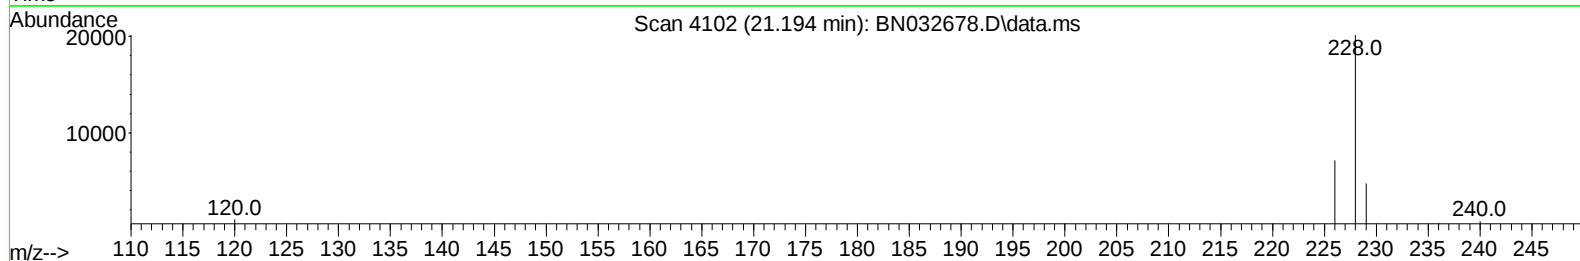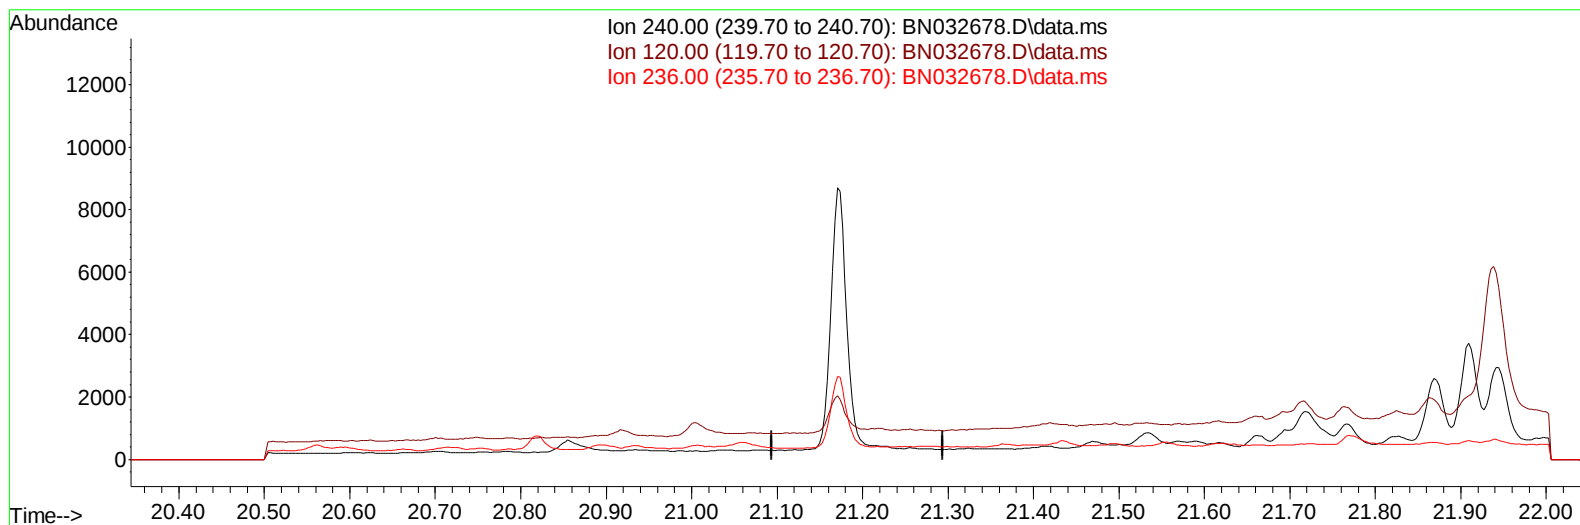

TIC: BN032678.D\data.ms

(17) Chrysene-d12

21.194min (-21.194) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	18.00	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

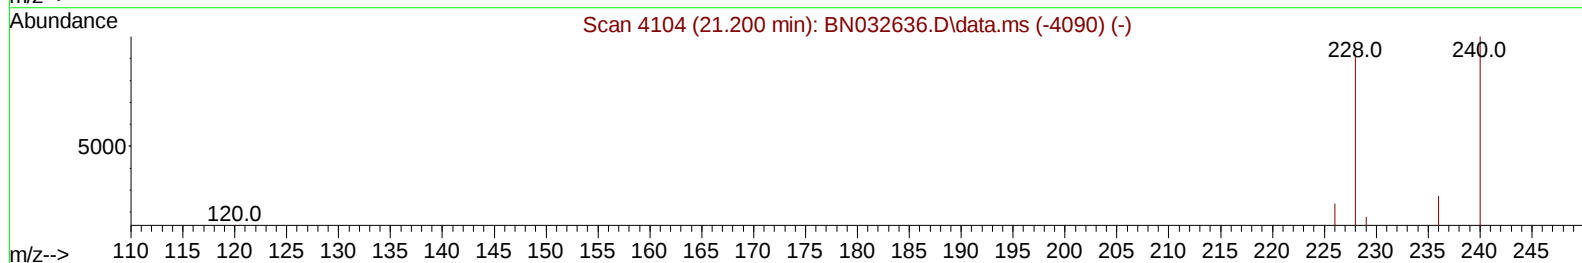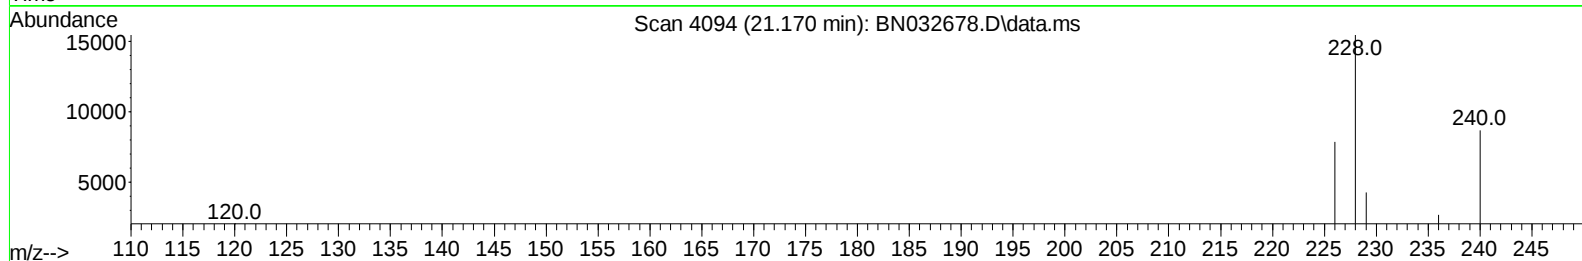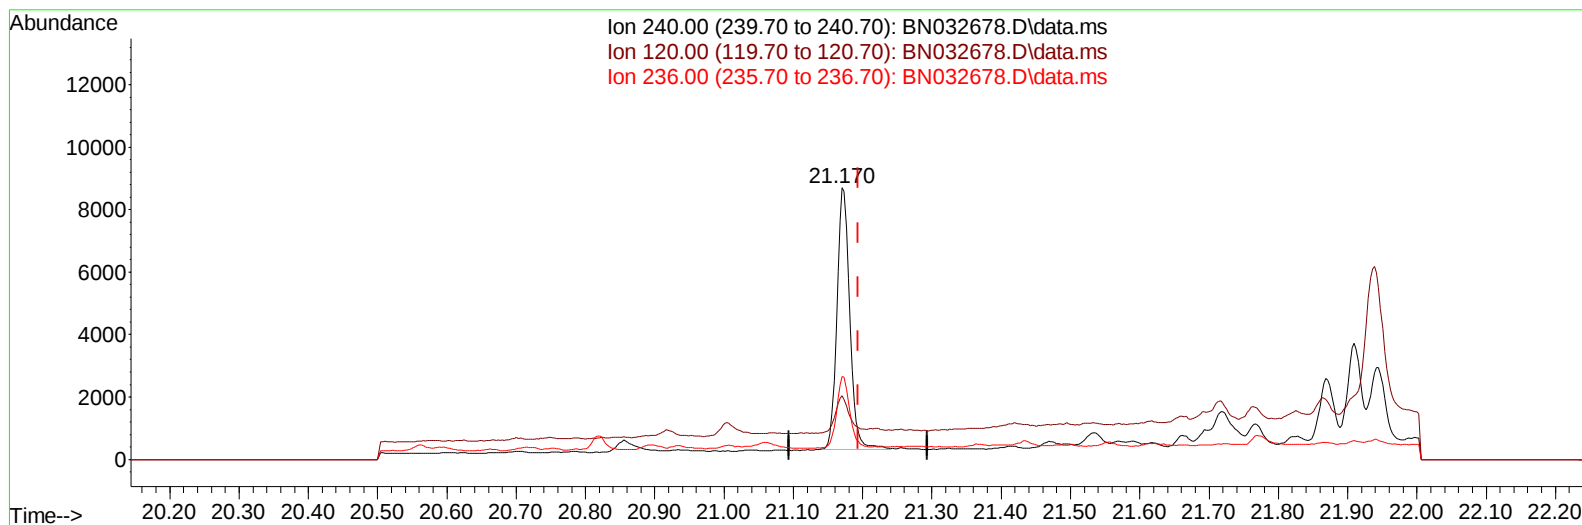

TIC: BN032678.D\data.ms

(17) Chrysene-d12

21.170min (-0.023) 0.40 ng/ul m

response 10738

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	18.00	23.47#
236.00	28.40	30.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

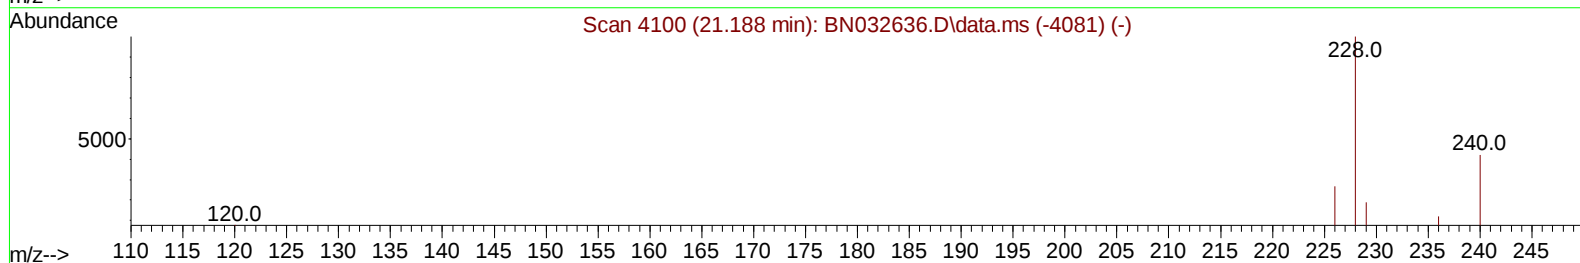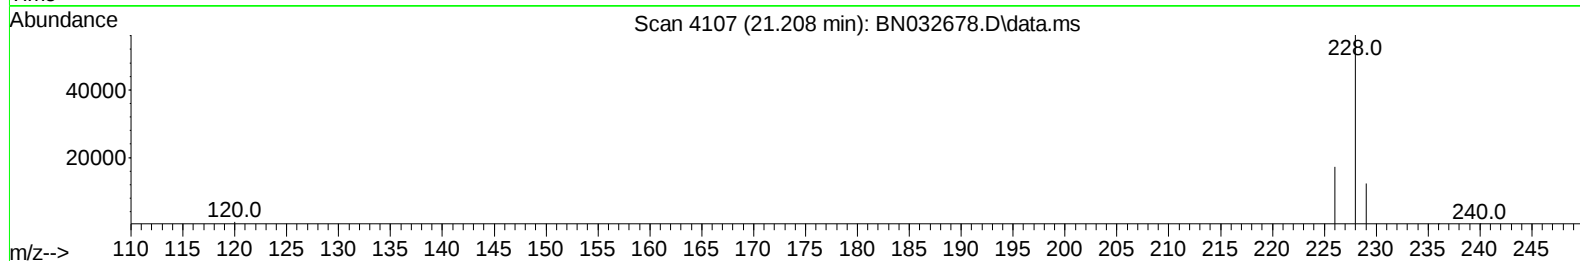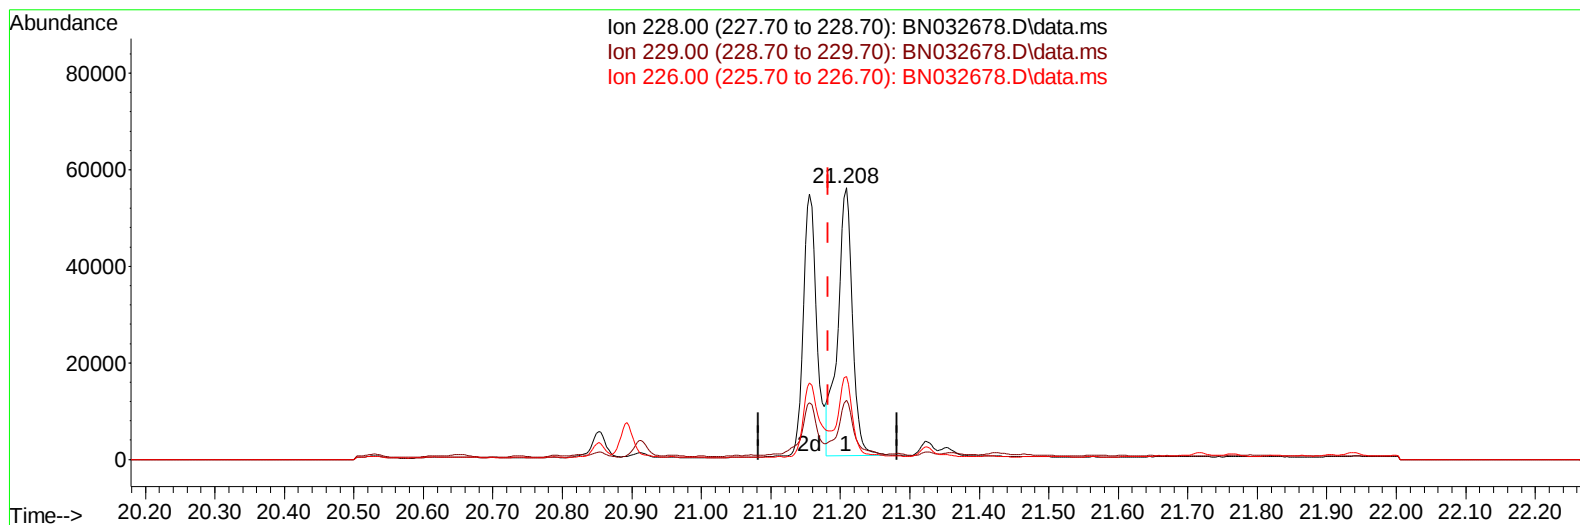

TIC: BN032678.D\data.ms

(21) Benzo(a)anthracene

21.208min (+ 0.026) 2.40 ng/u1

response 82181

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.10	21.92
226.00	27.40	30.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

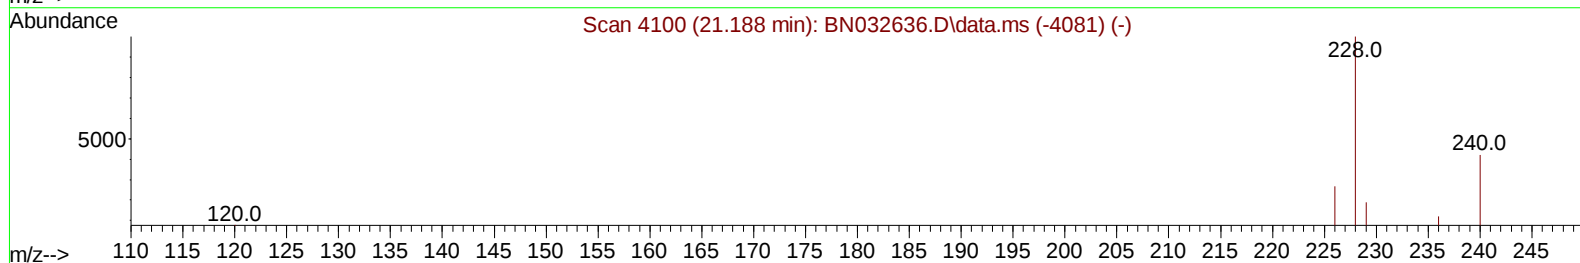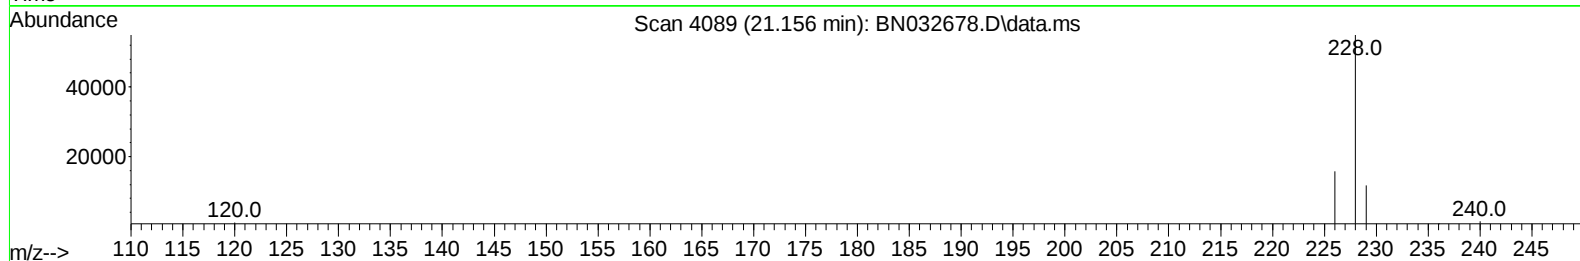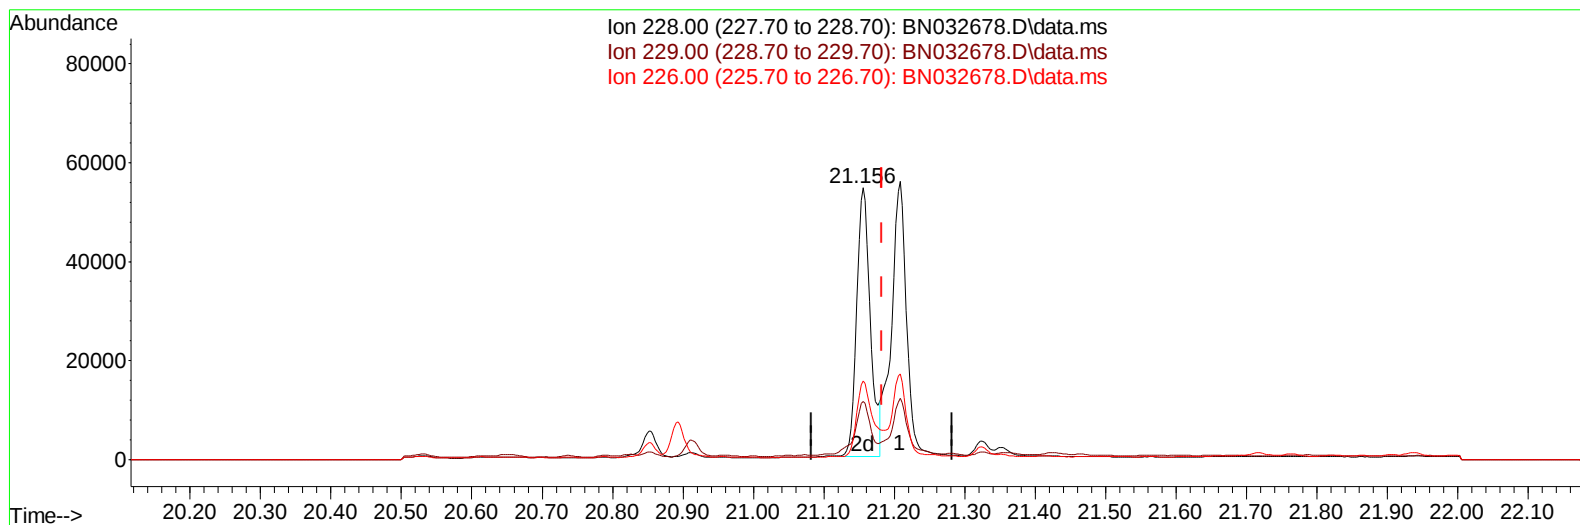

TIC: BN032678.D\data.ms

(21) Benzo(a)anthracene

21.156min (-0.026) 2.14 ng/u1 m

response 73236

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	20.10	21.42
226.00	27.40	28.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

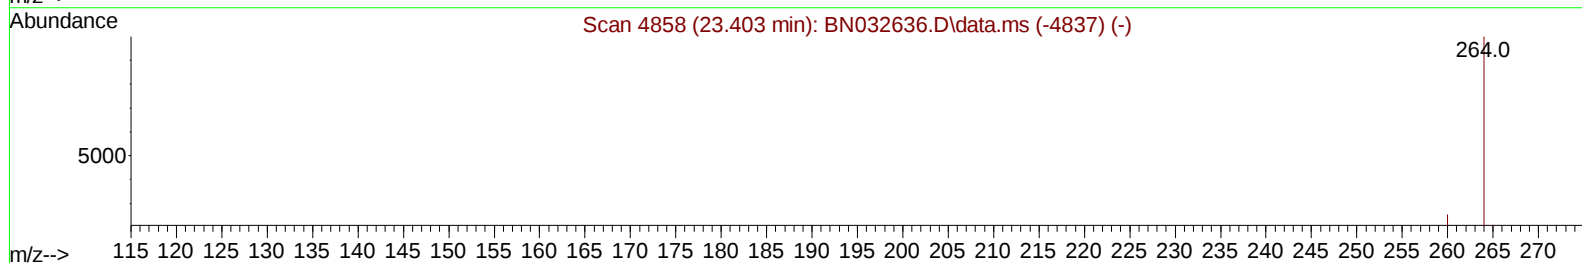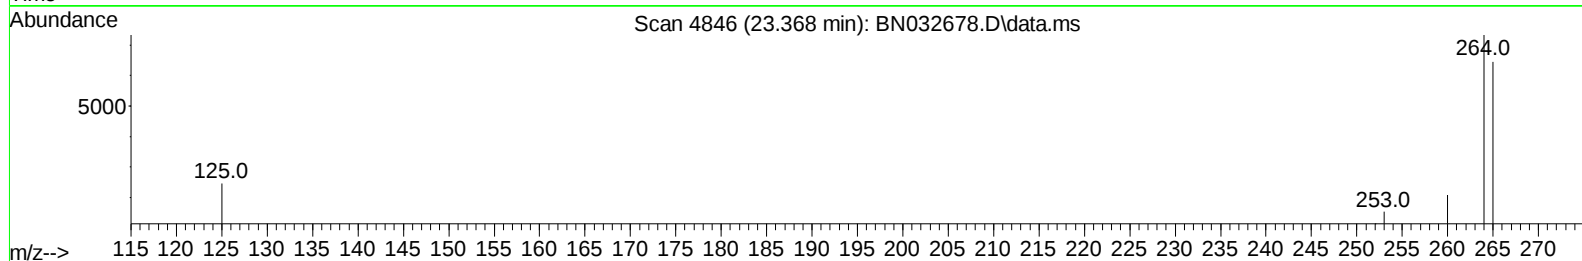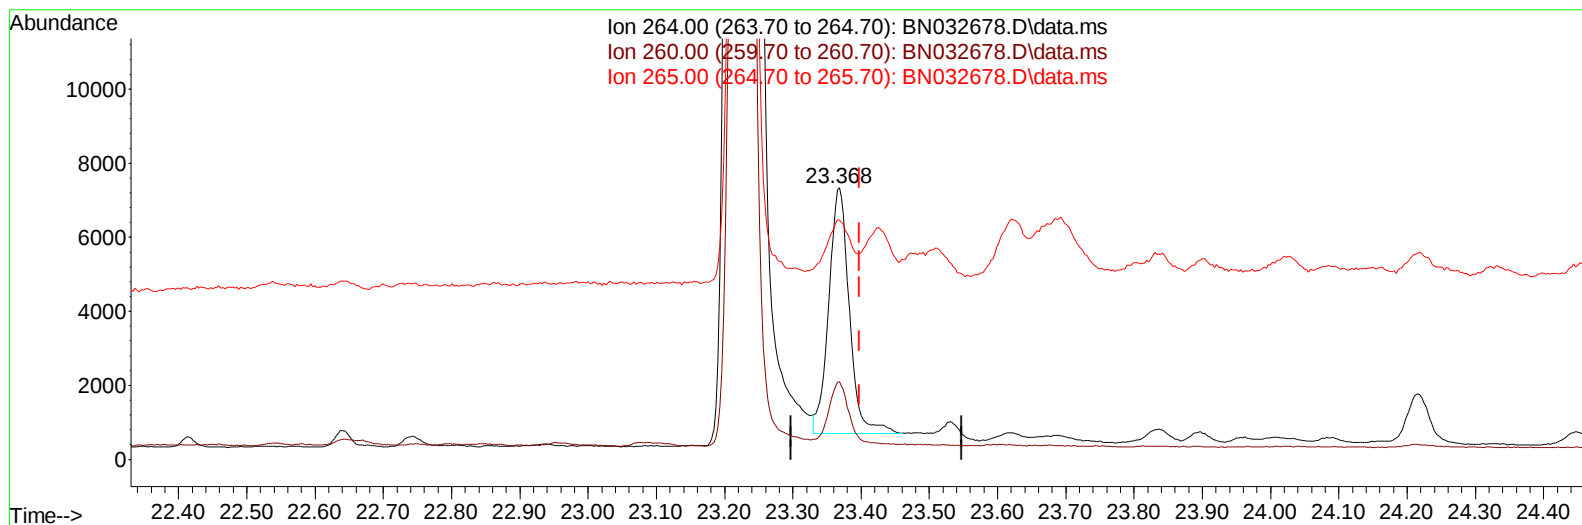

TIC: BN032678.D\data.ms

(23) Perylene-d12 (I)

23.368min (-0.029) 0.40 ng/u1

response 13882

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	28.55
265.00	95.50	88.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

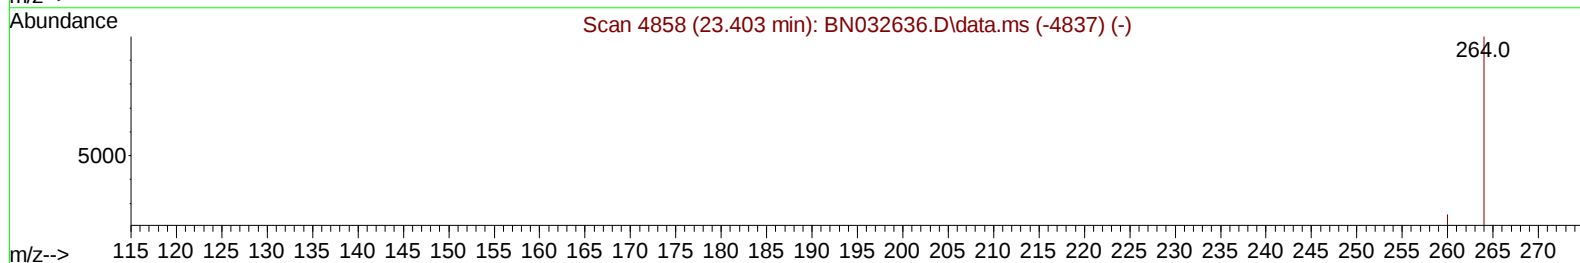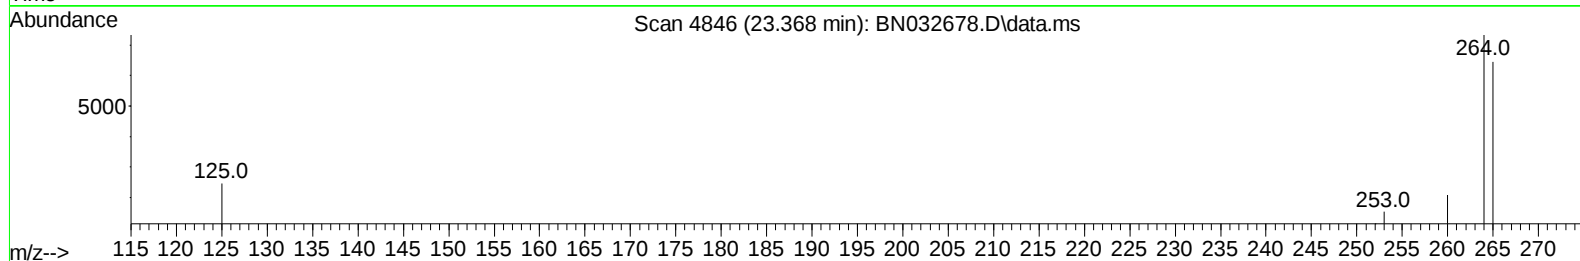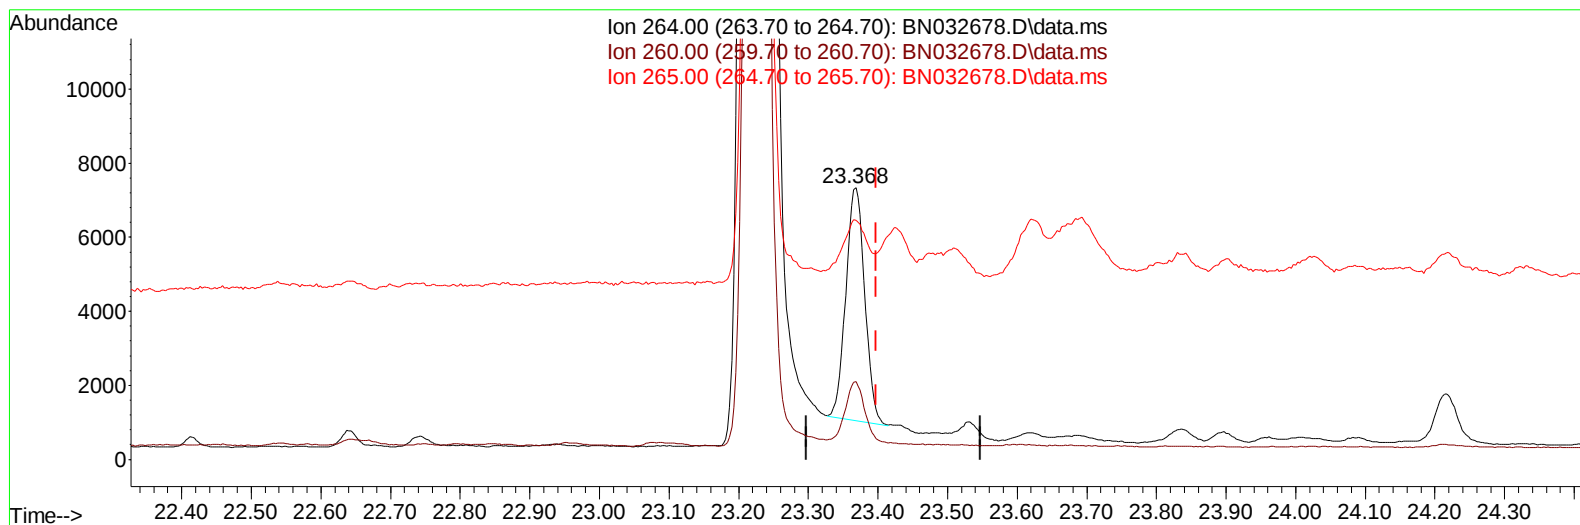

TIC: BN032678.D\data.ms

(23) Perylene-d12 (I)

23.368min (-0.029) 0.40 ng/ul m

response 11809

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.10	28.55
265.00	95.50	88.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

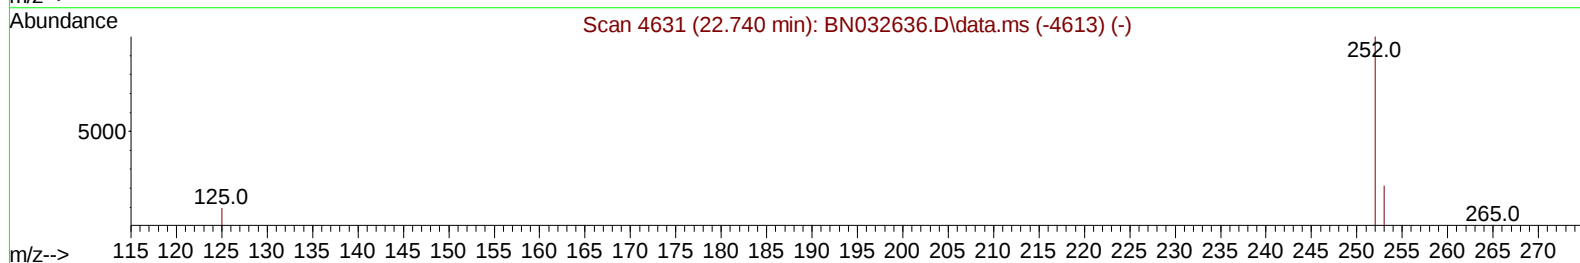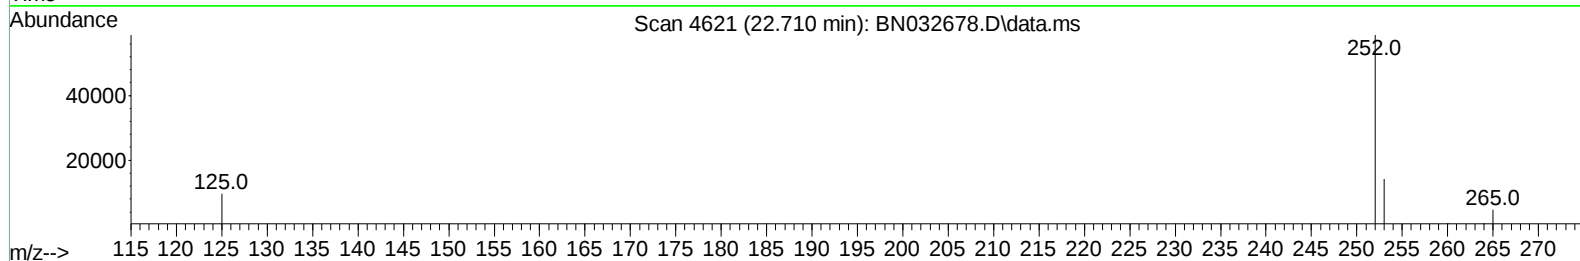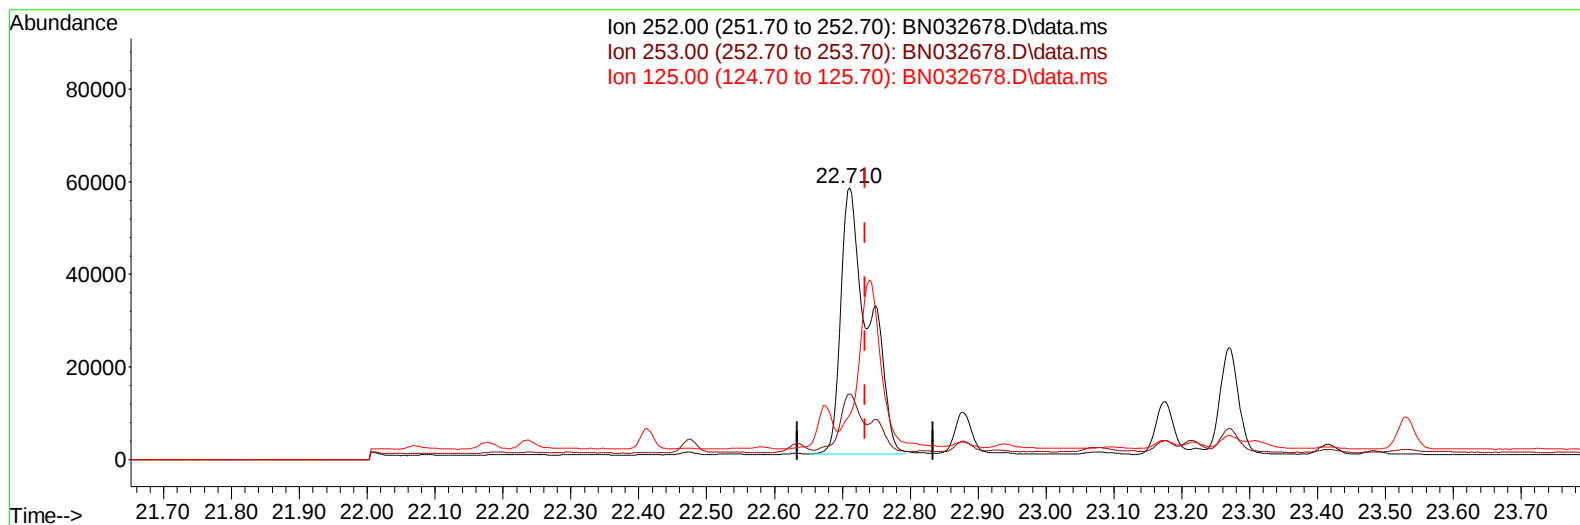

TIC: BN032678.D\data.ms

(24) Benzo(b)fluoranthene

22.710min (-0.023) 3.97 ng/u1

response 165608

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	24.13
125.00	18.00	16.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
 Data File : BN032678.D
 Acq On : 12 Jul 2024 18:36
 Operator : MA/JU
 Sample : P3087-23
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 01:40:24 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
 Supervised By :mohammad ahmed 07/16/2024

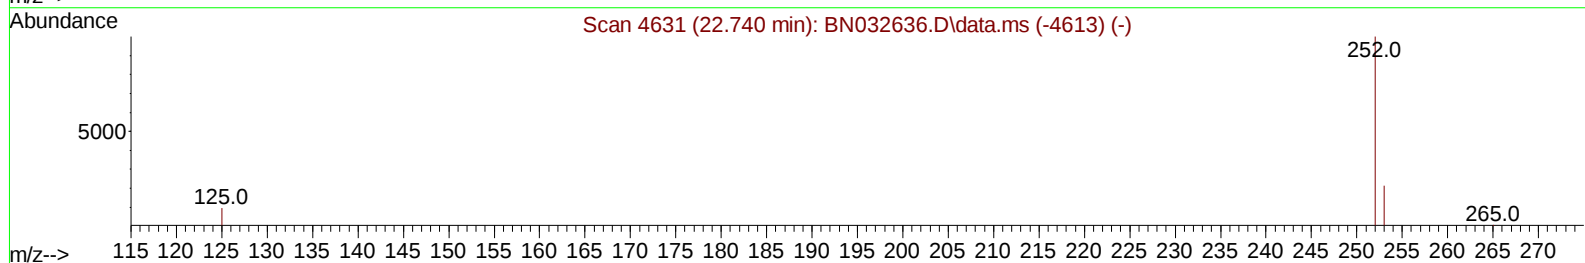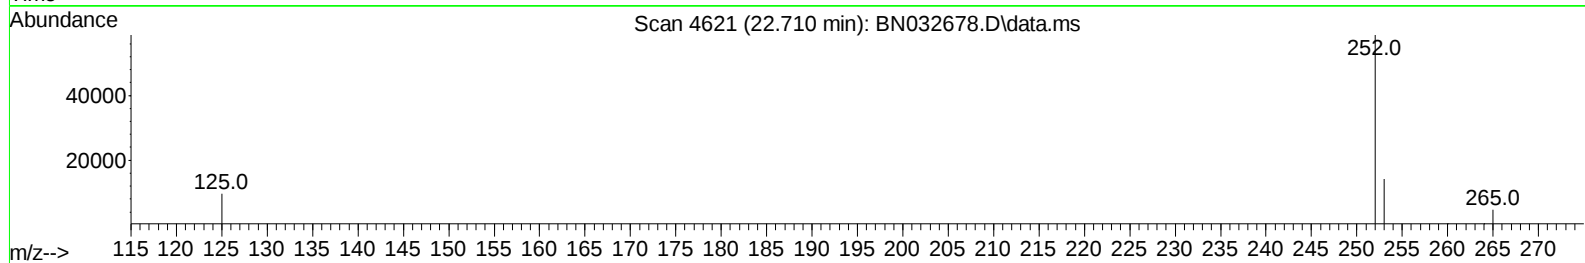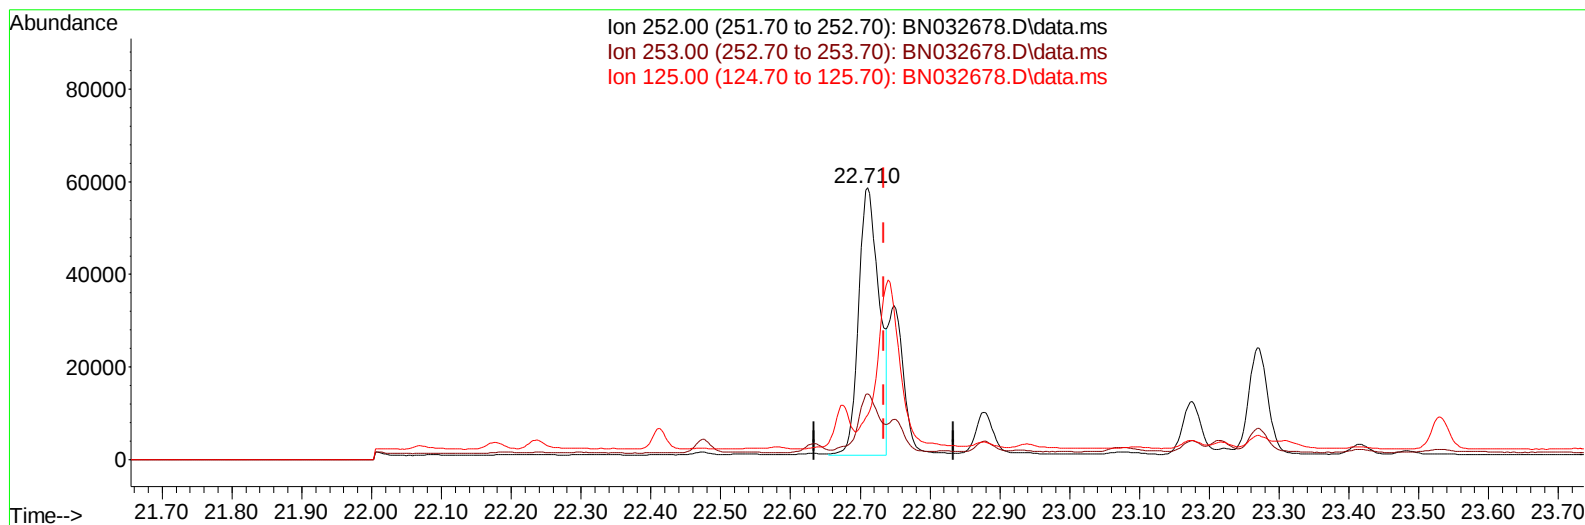

TIC: BN032678.D\data.ms

(24) Benzo(b)fluoranthene

22.710min (-0.023) 2.84 ng/u1 m

response 118453

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	24.13
125.00	18.00	16.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

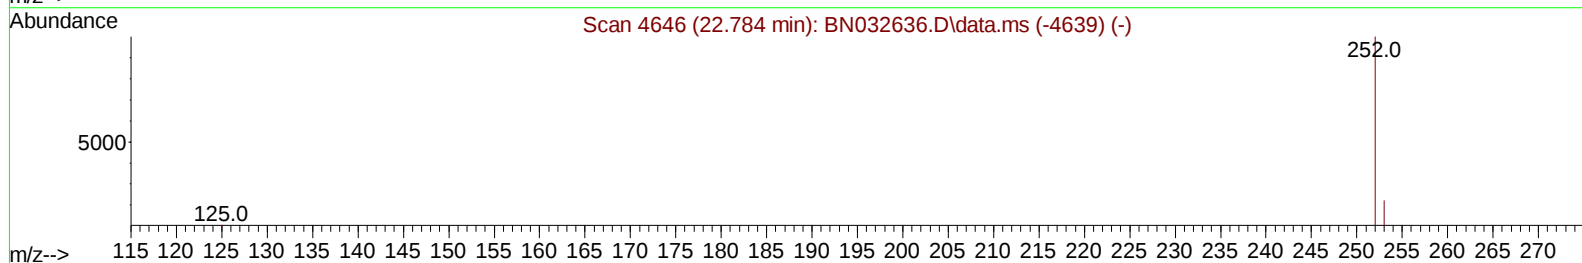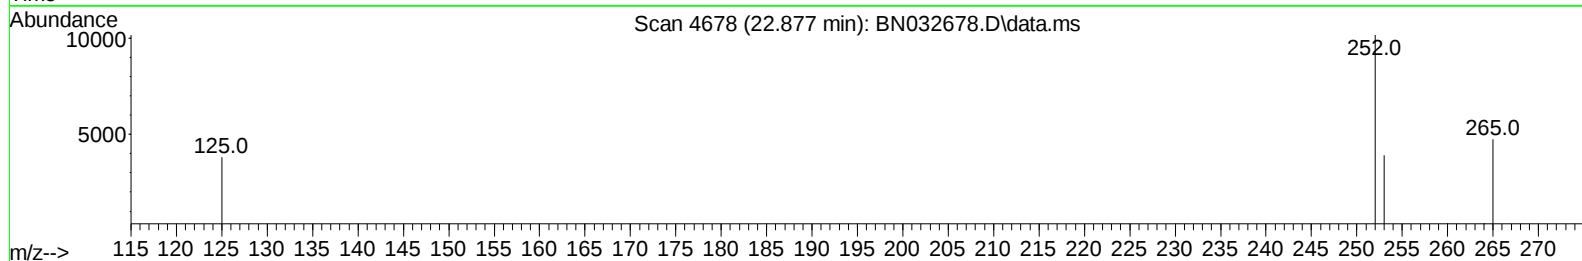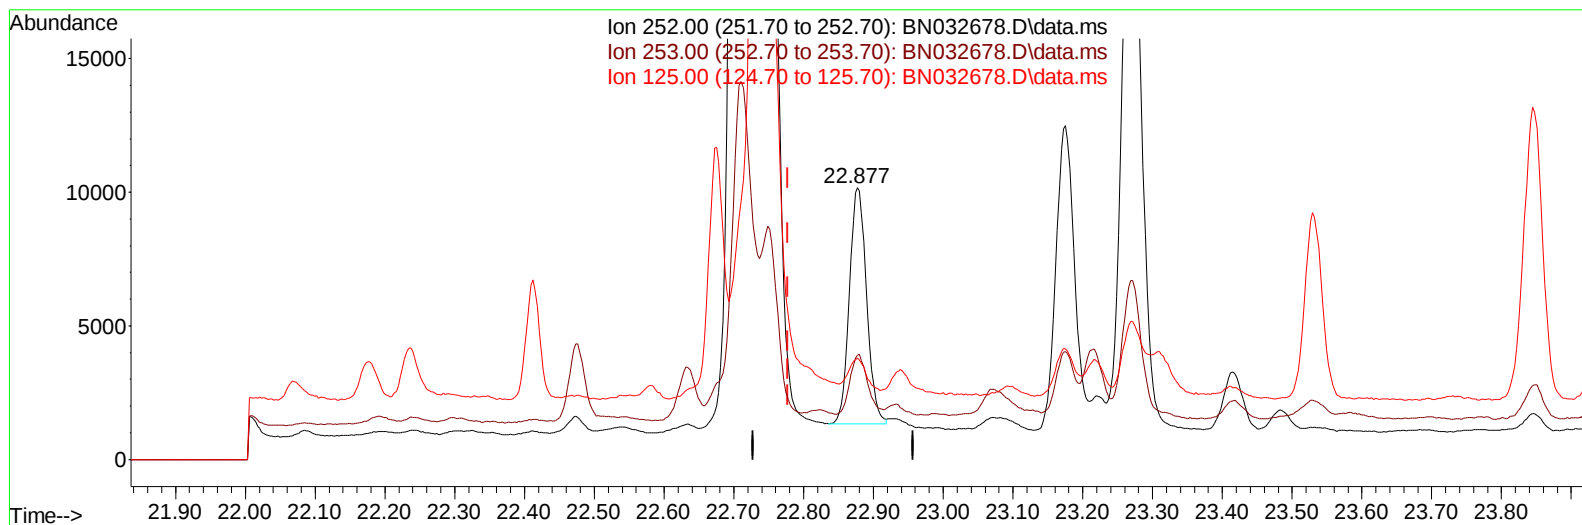

TIC: BN032678.D\data.ms

(25) Benzo(k)fluoranthene

22.877min (+ 0.099) 0.30 ng/u1

response 15109

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	38.41#
125.00	18.50	37.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

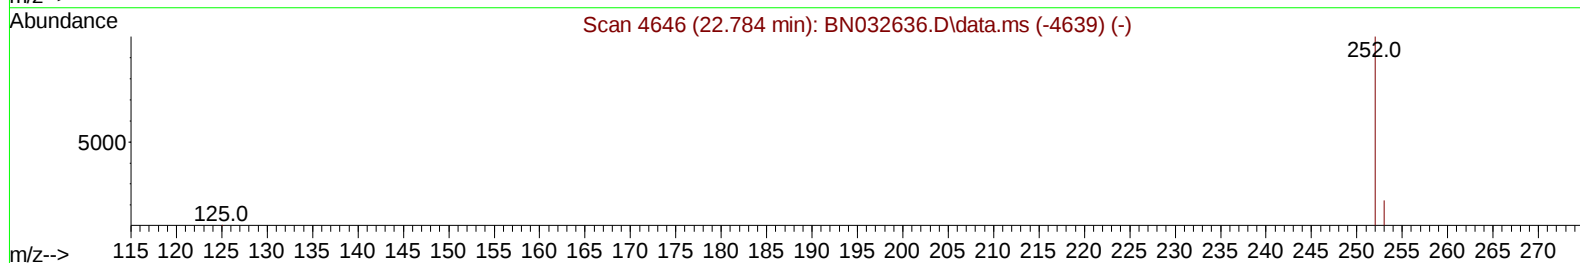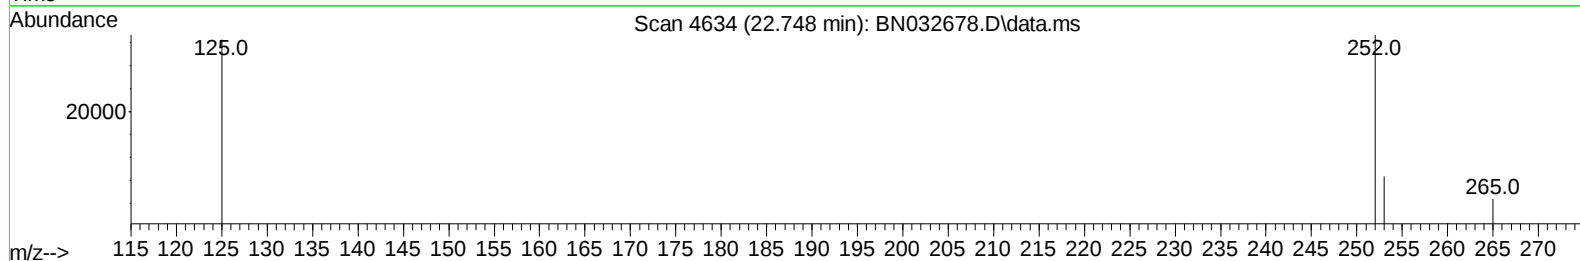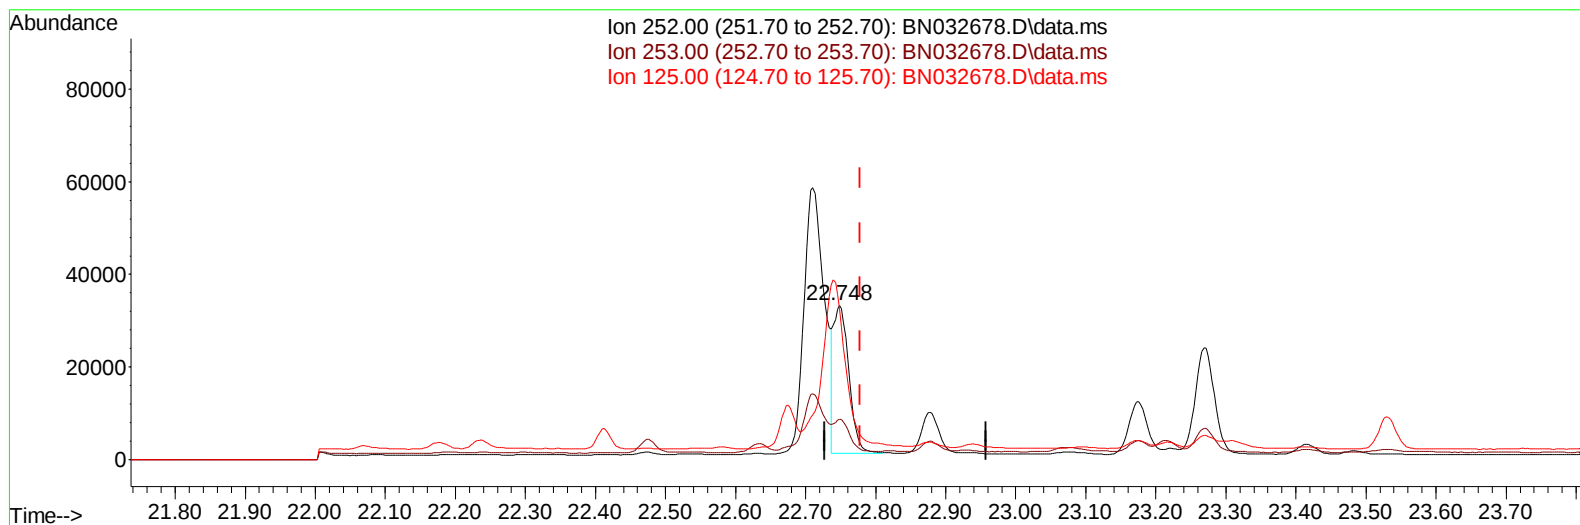

TIC: BN032678.D\data.ms

(25) Benzo(k)fluoranthene

22.748min (-0.029) 0.96 ng/u1 m

response 48591

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	26.19
125.00	18.50	97.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
 Data File : BN032678.D
 Acq On : 12 Jul 2024 18:36
 Operator : MA/JU
 Sample : P3087-23
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4CZ5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/13/2024
 Supervised By :mohammad ahmed 07/16/2024

Quant Time: Jul 13 00:03:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 01:40:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.553	152	4227	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.321	136	12239	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.202	164	6445	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.961	188	12231m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.170	240	10738m	0.400	ng/ul	-0.02
23) Perylene-d12	23.368	264	11809m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	16187	3.189	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.927	152	3960	0.214	ng/ul	-0.04
18) Fluoranthene-d10	18.999	212	7338	0.210	ng/ul	-0.03
Target Compounds						
						Qvalue
5) Naphthalene	10.371	128	5549	0.169	ng/ul	97
7) 2-Methylnaphthalene	12.004	142	2697	0.131	ng/ul	95
8) 1-Methylnaphthalene	12.224	142	1765	0.083	ng/ul	100
10) Acenaphthylene	13.920	152	11645	0.447	ng/ul	99
11) Acenaphthene	14.262	153	1966	0.091	ng/ul	97
12) Fluorene	15.257	166	3179	0.129	ng/ul#	97
14) Pentachlorophenol	16.636	266	202m	0.094	ng/ul	
15) Phenanthrene	16.999	178	57816m	1.736	ng/ul	
16) Anthracene	17.092	178	14344m	0.527	ng/ul	
19) Fluoranthene	19.031	202	130946	2.999	ng/ul	98
20) Pyrene	19.394	202	99506	2.202	ng/ul	99
21) Benzo(a)anthracene	21.156	228	73236m	2.143	ng/ul	
22) Chrysene	21.208	228	83131	1.681	ng/ul	97
24) Benzo(b)fluoranthene	22.710	252	118453m	2.843	ng/ul	
25) Benzo(k)fluoranthene	22.748	252	48591m	0.957	ng/ul	
26) Benzo(a)pyrene	23.269	252	44240	1.227	ng/ul	92
27) Indeno(1,2,3-cd)pyrene	25.576	276	54311	1.112	ng/ul#	96
28) Dibenzo(a,h)anthracene	25.579	278	24666	0.652	ng/ul#	65
29) Benzo(g,h,i)perylene	26.256	276	17075	0.418	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071224\
Data File : BN032678.D
Acq On : 12 Jul 2024 18:36
Operator : MA/JU
Sample : P3087-23
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CZ5

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 01:40:24 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

