




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071323\
Data File : BN026484.D
Acq On : 13 Jul 2023 09:36
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 13 17:03:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 16:59:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :mohammad ahmed 07/14/2023

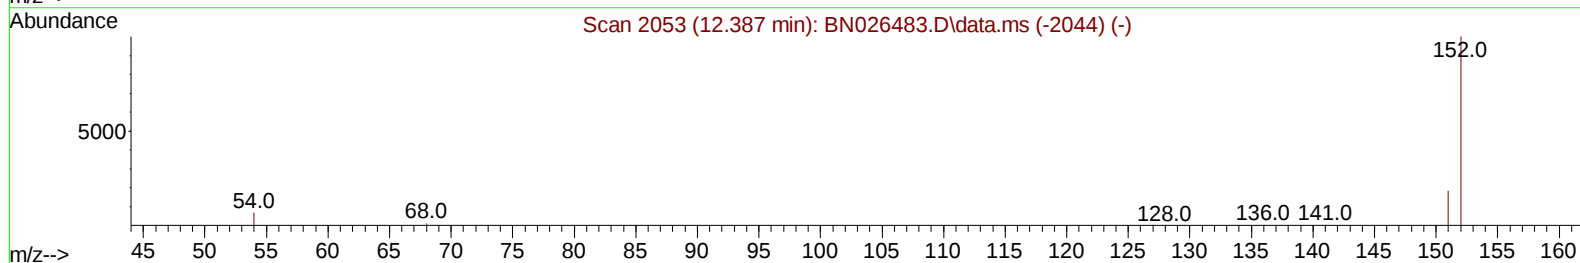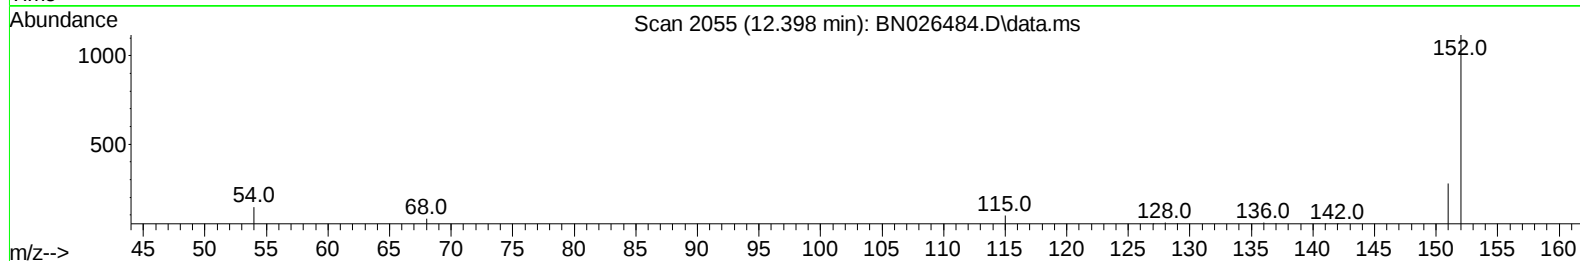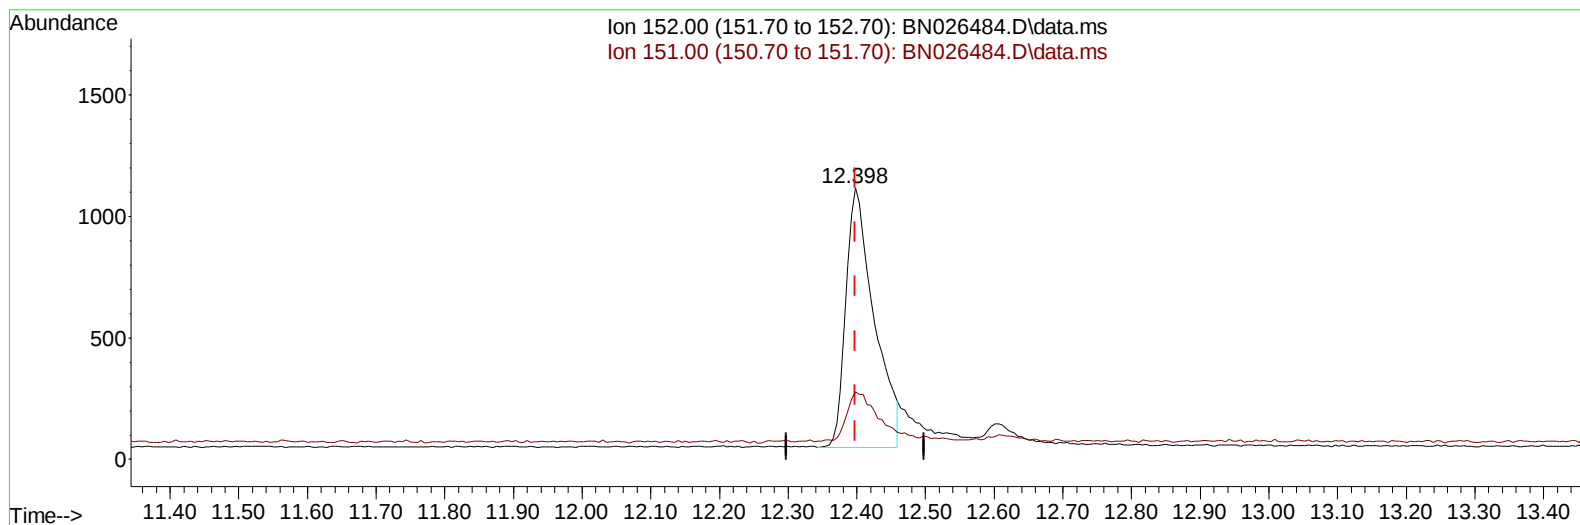

TIC: BN026484.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.398min (+ 0.000) 0.29 ng/u1

response 3037

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	20.51
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071323\
Data File : BN026484.D
Acq On : 13 Jul 2023 09:36
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 13 17:03:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 16:59:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :mohammad ahmed 07/14/2023

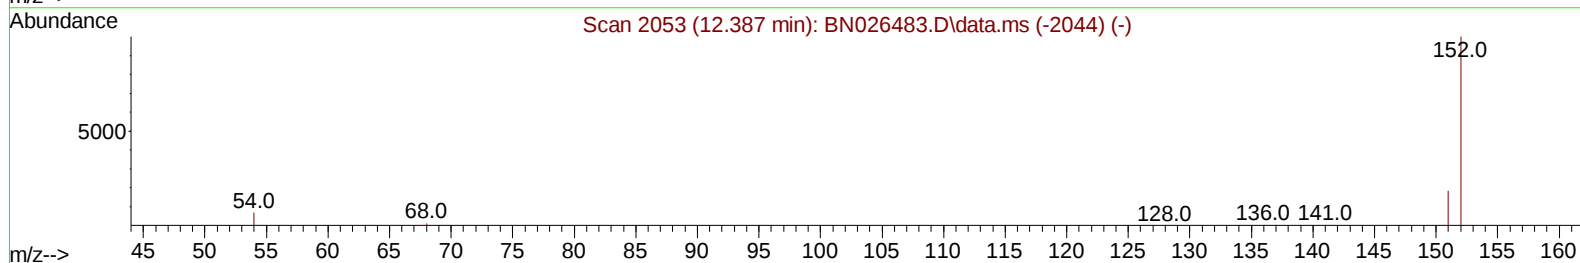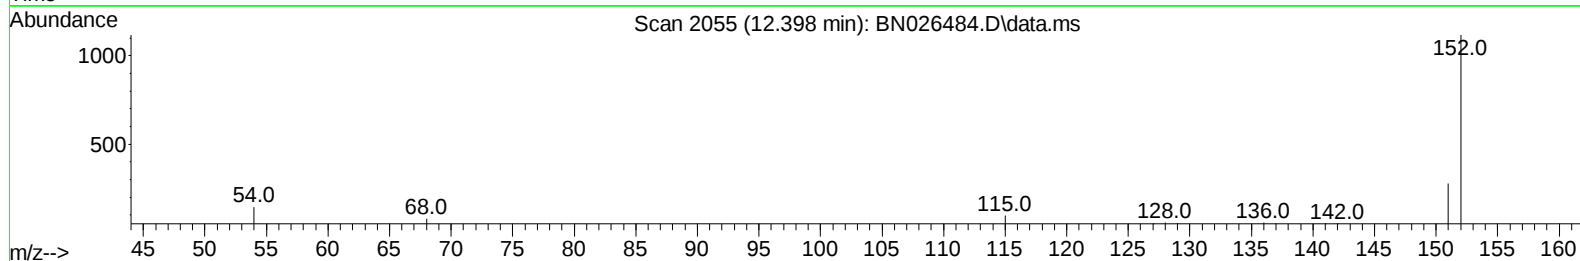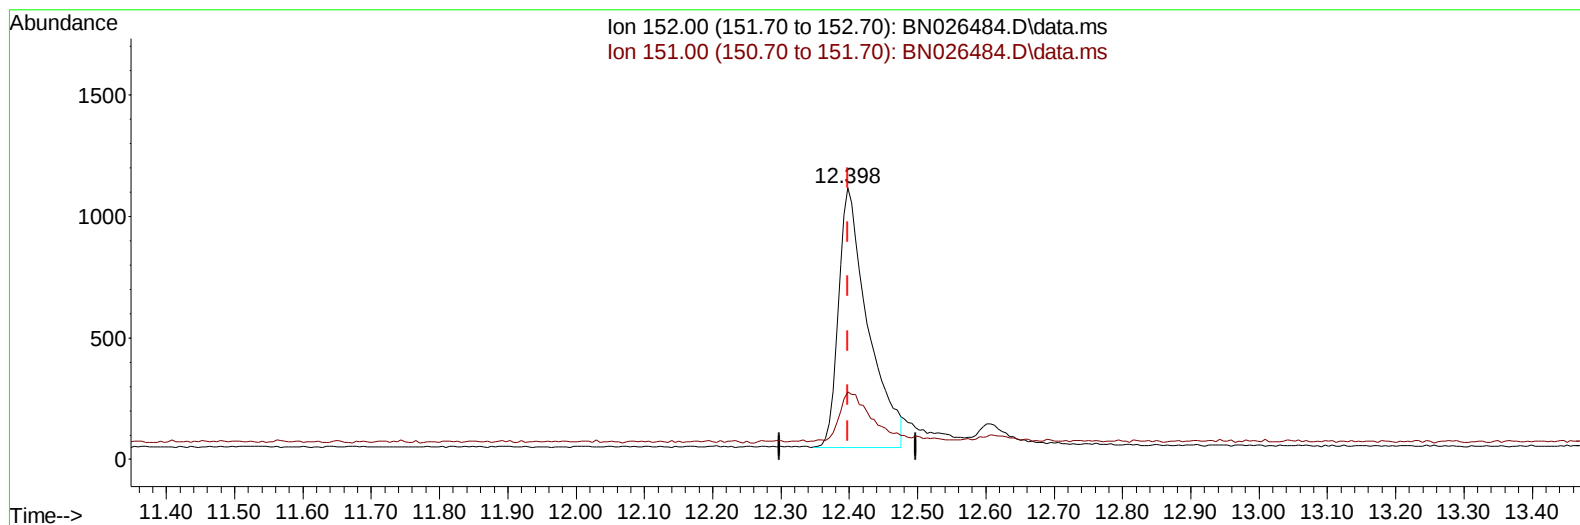

TIC: BN026484.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.398min (+ 0.000) 0.31 ng/ul m

response 3189

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	19.54
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071323\
 Data File : BN026484.D
 Acq On : 13 Jul 2023 09:36
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/14/2023
 Supervised By :mohammad ahmed 07/14/2023

Quant Time: Jul 13 17:03:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 13 16:59:14 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.993	152		2443	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.792	136		7624	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.621	164		4426	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.364	188		7846	0.400	ng/ul	0.00
17) Chrysene-d12	21.564	240		5427	0.400	ng/ul	0.00
23) Perylene-d12	23.990	264		8275	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.339	96		16694	5.189	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.398	152		3189m	0.308	ng/ul	0.00
18) Fluoranthene-d10	19.396	212		5907	0.314	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071323\
Data File : BN026484.D
Acq On : 13 Jul 2023 09:36
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 13 17:03:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 16:59:14 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/14/2023
Supervised By :mohammad ahmed 07/14/2023

