
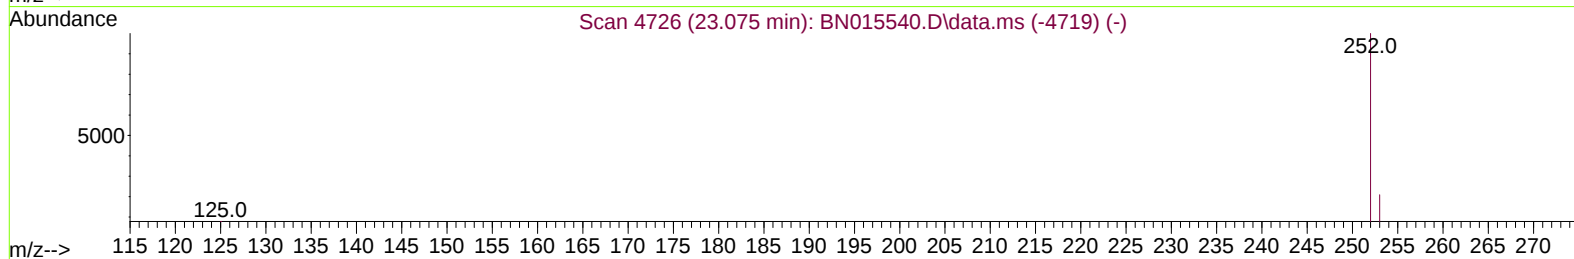
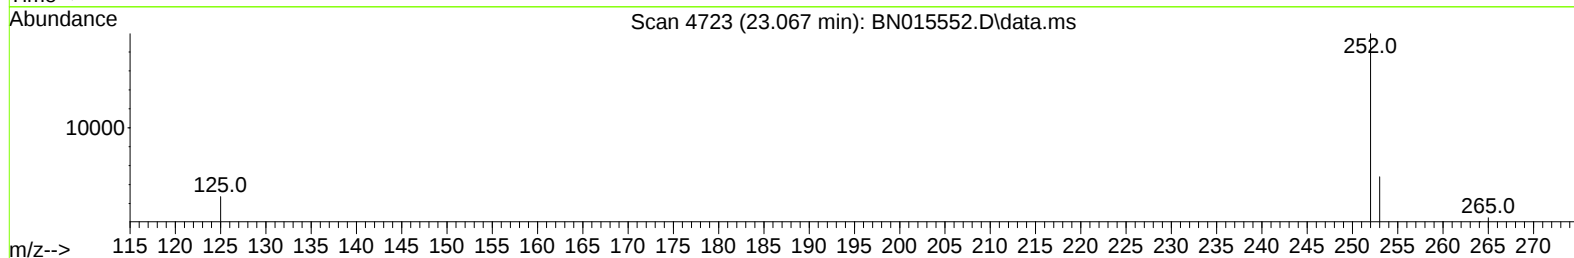


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071221\
Data File : BN015552.D
Acq On : 14 Jul 2021 05:55
Operator : CG/JU
Sample : M2869-11DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Jul 14 07:17:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 14 07:10:56 2021
Response via : Initial Calibration

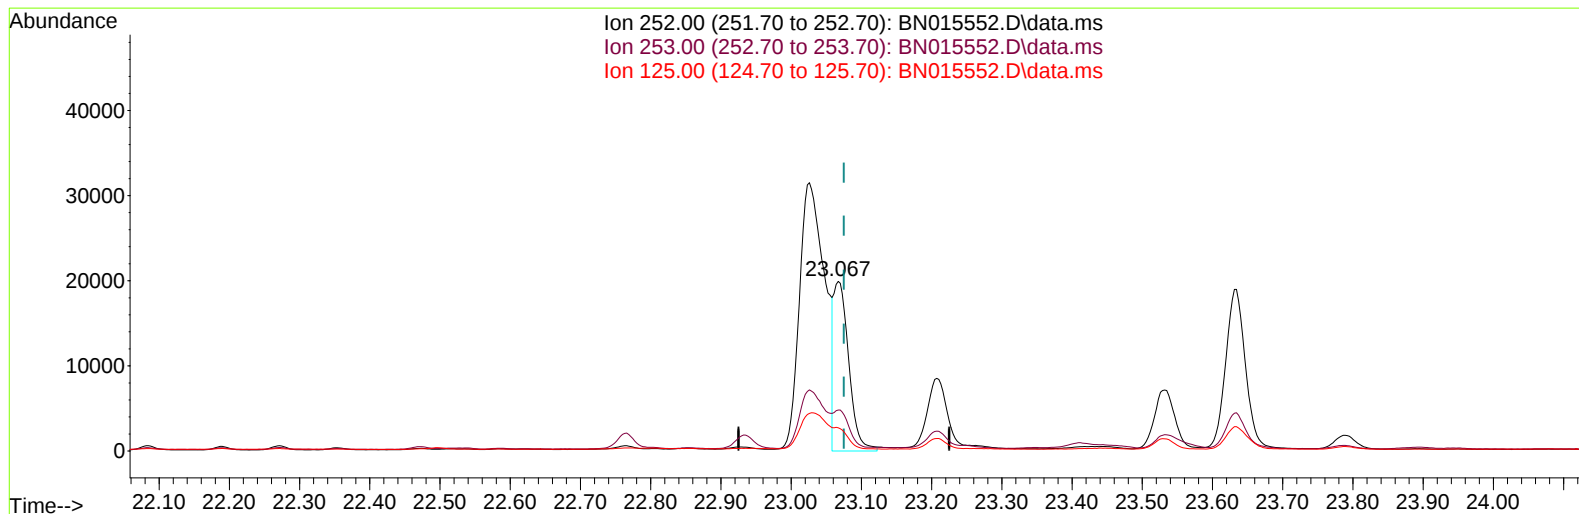

TIC: BN015552.D\data.ms

(25) Benzo(k)fluoranthene

23.067min (-0.008) 0.56 ng/u1 m

response 29371

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.60	24.16
125.00	14.40	13.69
0.00	0.00	0.00