

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071421\
 Data File : BN015571.D
 Acq On : 14 Jul 2021 19:41
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 15 01:05:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 14 11:20:16 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.818	152	15509	0.40	ng	# 0.00
7) Naphthalene-d8	10.597	136	70497	0.40	ng	0.00
13) Acenaphthene-d10	14.446	164	38962	0.40	ng	0.01
19) Phenanthrene-d10	17.188	188	73487	0.40	ng	0.00
29) Chrysene-d12	21.387	240	52724	0.40	ng	# 0.00
35) Perylene-d12	23.745	264	29052	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.420	112	18225	0.46	ng	0.00
5) Phenol-d6	6.988	99	22225	0.45	ng	0.00
8) Nitrobenzene-d5	8.962	82	18127	0.46	ng	0.00
11) 2-Methylnaphthalene-d10	12.190	152	45043	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.931	330	5219	0.53	ng	0.00
15) 2-Fluorobiphenyl	13.063	172	59534	0.38	ng	0.00
27) Fluoranthene-d10	19.227	212	79523	0.37	ng	0.00
31) Terphenyl-d14	19.827	244	58307	0.47	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.382	88	3094	0.43	ng	# 59
3) n-Nitrosodimethylamine	3.724	42	4906	0.36	ng	# 77
6) bis(2-Chloroethyl)ether	7.246	93	19220	0.39	ng	# 85
9) Naphthalene	10.648	128	78102	0.39	ng	97
10) Hexachlorobutadiene	10.939	225	14594	0.38	ng	# 99
12) 2-Methylnaphthalene	12.265	142	52309	0.40	ng	# 89
16) Acenaphthylene	14.155	152	65627	0.38	ng	98
17) Acenaphthene	14.497	154	45918	0.38	ng	99
18) Fluorene	15.487	166	56201	0.38	ng	98
20) 4,6-Dinitro-2-methylph...	15.576	198	384	0.47	ng	# 77
21) 4-Bromophenyl-phenylether	16.385	248	17452	0.37	ng	89
22) Hexachlorobenzene	16.506	284	20069	0.38	ng	# 92
23) Atrazine	16.652	200	11221	0.45	ng	93
24) Pentachlorophenol	16.847	266	3181	0.59	ng	99
25) Phenanthrene	17.237	178	91826	0.39	ng	99
26) Anthracene	17.322	178	75917	0.37	ng	99
28) Fluoranthene	19.257	202	97573	0.38	ng	# 97
30) Pyrene	19.619	202	95788	0.48	ng	99
32) Benzo(a)anthracene	21.376	228	67659	0.37	ng	96
33) Chrysene	21.419	228	74585	0.38	ng	98
34) Bis(2-ethylhexyl)phtha...	21.312	149	30961	0.62	ng	# 87
36) Indeno(1,2,3-cd)pyrene	26.175	276	20896	0.20	ng	# 83
37) Benzo(b)fluoranthene	23.029	252	50434	0.44	ng	# 95
38) Benzo(k)fluoranthene	23.074	252	51584	0.42	ng	# 95
39) Benzo(a)pyrene	23.642	252	35376	0.34	ng	# 90
40) Dibenzo(a,h)anthracene	26.192	278	16258	0.20	ng	# 91
41) Benzo(g,h,i)perylene	26.914	276	16856	0.19	ng	# 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071421\
Data File : BN015571.D
Acq On : 14 Jul 2021 19:41
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 15 01:05:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 14 11:20:16 2021
Response via : Initial Calibration



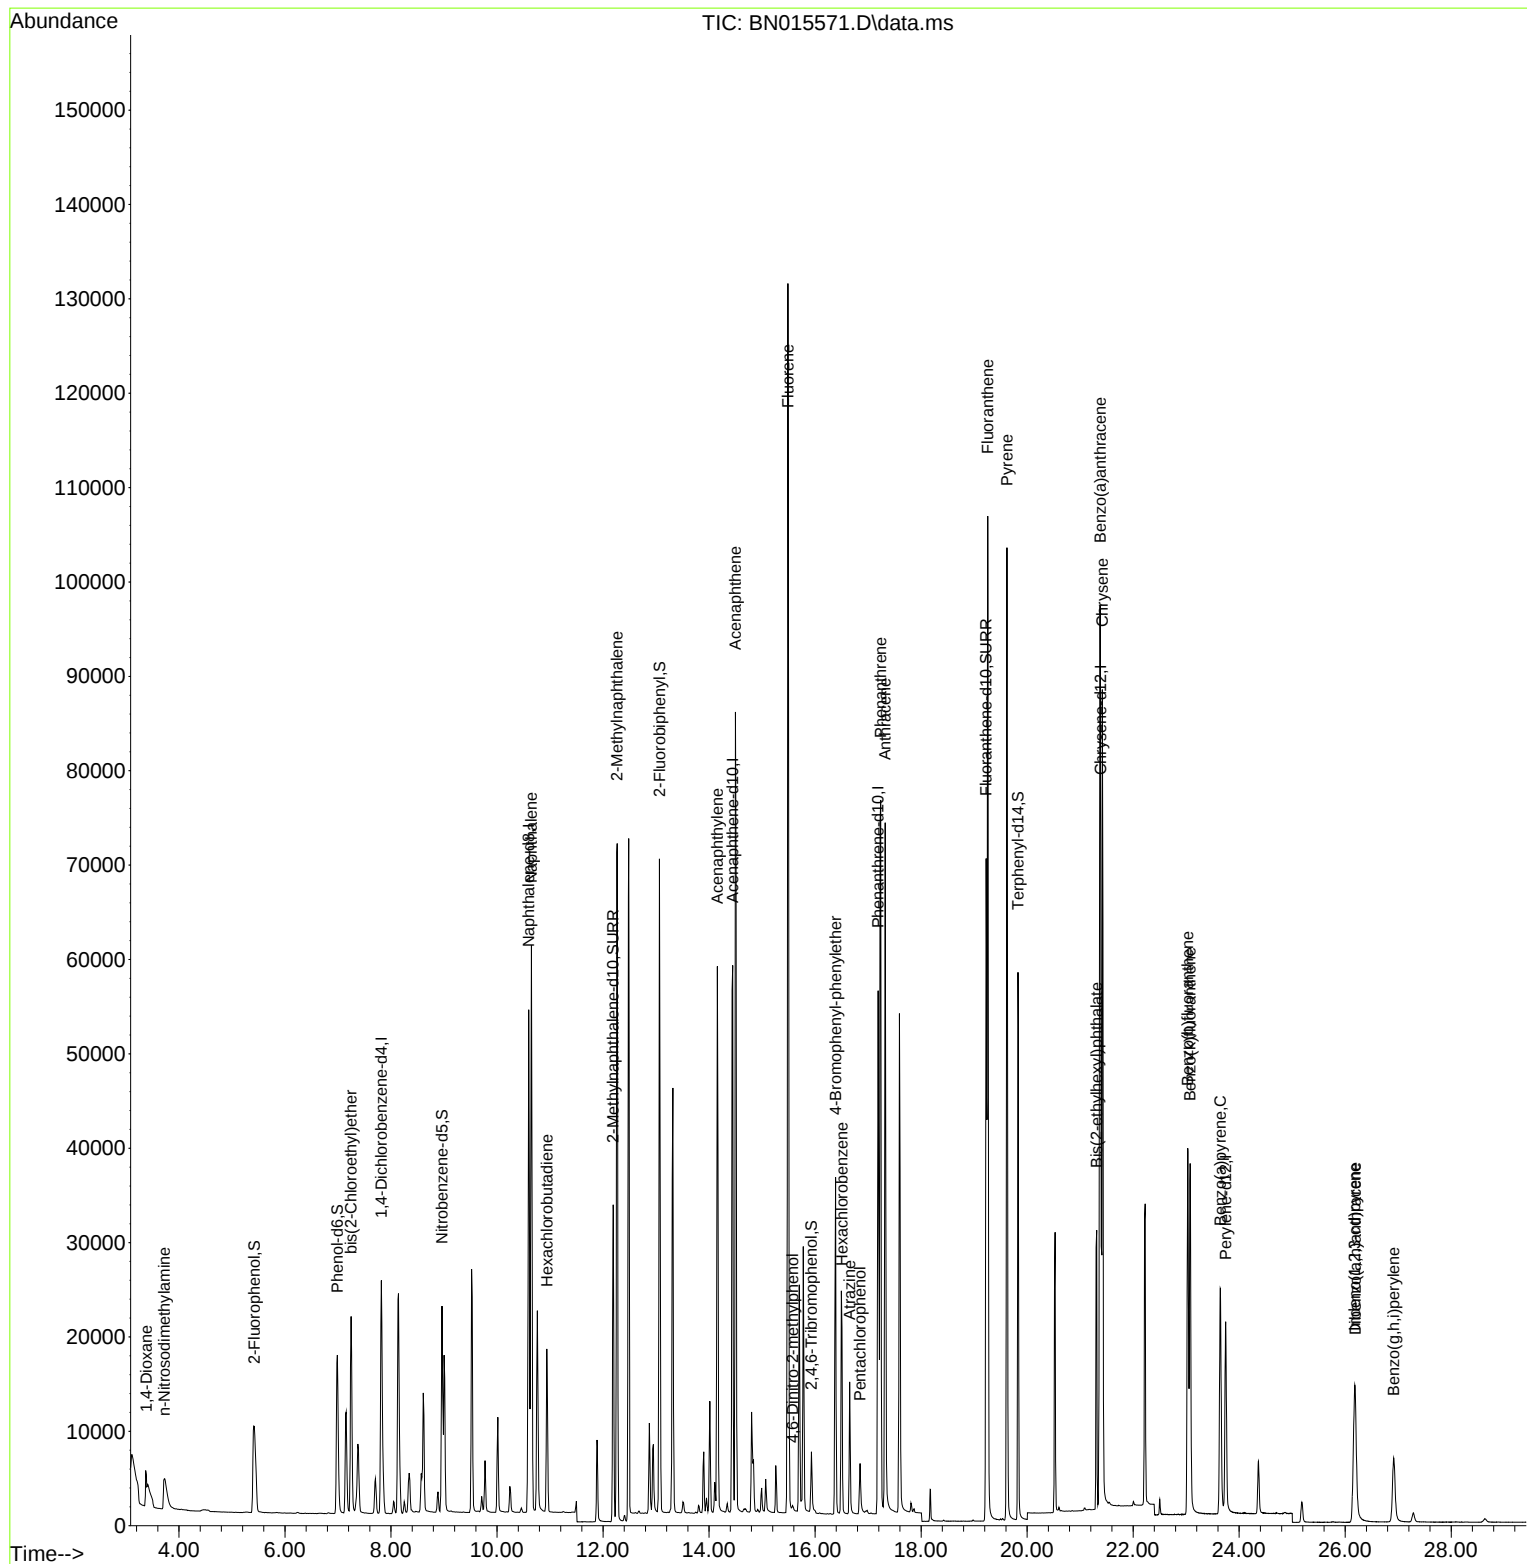




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.818 min Scan# 514
Delta R.T. 0.001 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampled :


Tgt Ion:152 Resp: 15509
Ion Ratio Lower Upper
152 100
150 154.7 119.0 178.6
115 59.6 62.2 93.4#

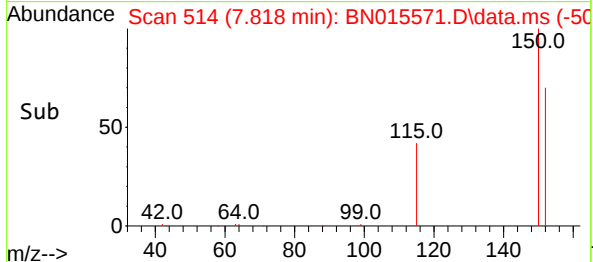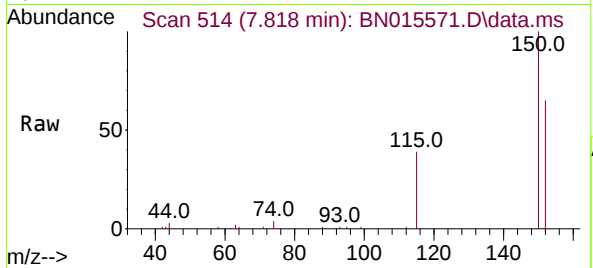

#2
1,4-Dioxane
Concen: 0.43 ng
RT: 3.382 min Scan# 33
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion: 88 Resp: 3094
Ion Ratio Lower Upper
88 100
43 28.3 12.9 19.3#
58 78.0 38.1 57.1#


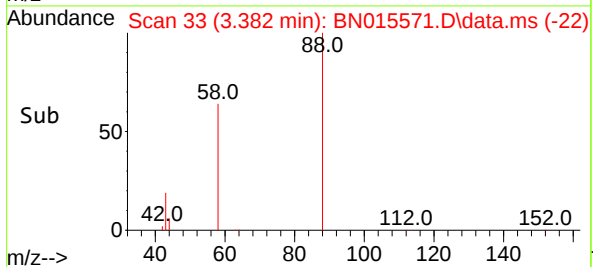

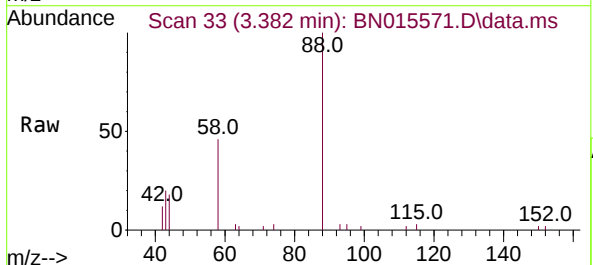


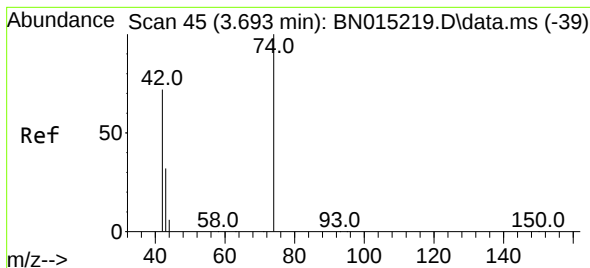

#3
n-Nitrosodimethylamine
Concen: 0.36 ng
RT: 3.724 min Scan# 70
Delta R.T. -0.009 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampled :


Tgt Ion: 42 Resp: 4906
Ion Ratio Lower Upper
42 100
74 152.7 149.5 224.3
44 8.4 4.2 6.2#

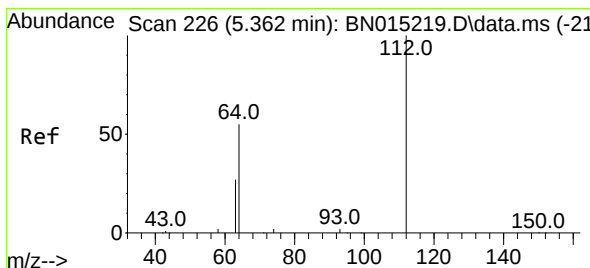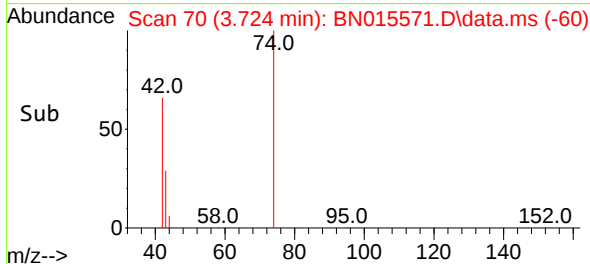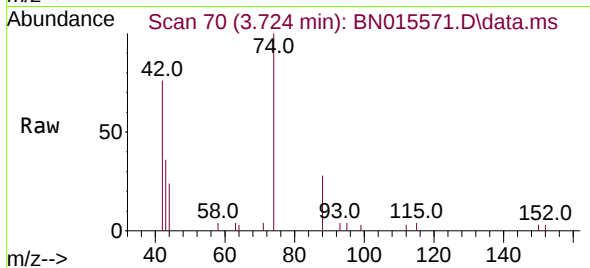

#4
2-Fluorophenol
Concen: 0.46 ng
RT: 5.420 min Scan# 254
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion: 112 Resp: 18225
Ion Ratio Lower Upper
112 100
64 56.0 39.0 58.6
63 27.8 20.6 30.8


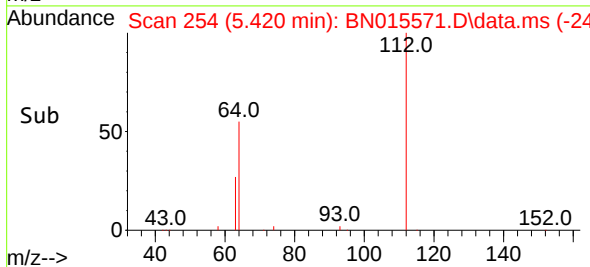

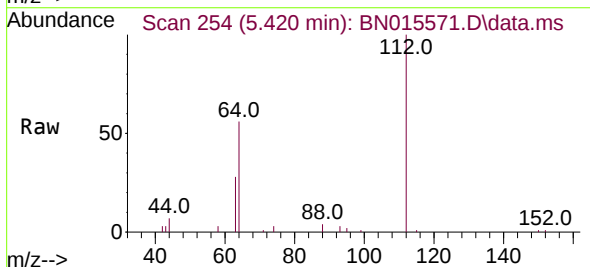


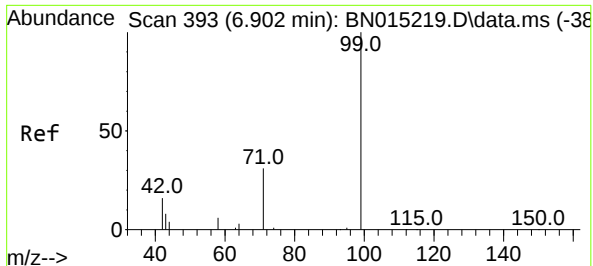

#5
Phenol-d6
Concen: 0.45 ng
RT: 6.988 min Scan# 424
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampled :

Tgt Ion: 99 Resp: 22225
Ion Ratio Lower Upper
99 100
42 16.6 8.9 13.3#
71 30.1 35.6 53.4#

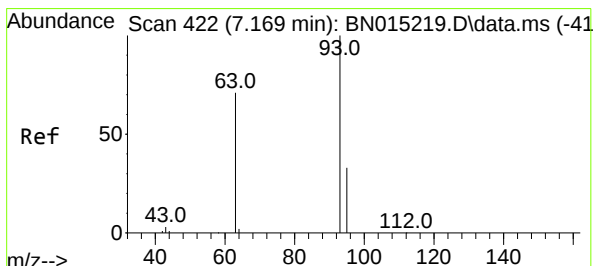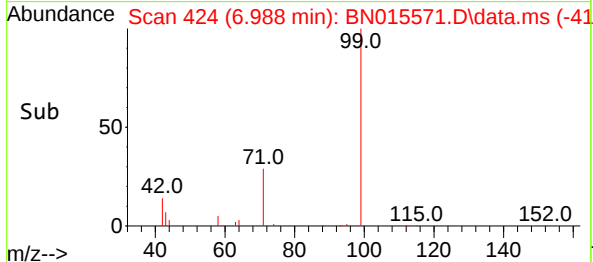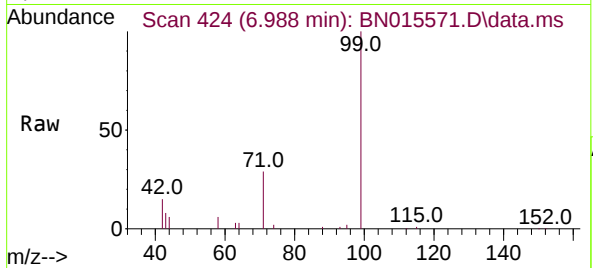

#6
bis(2-Chloroethyl)ether
Concen: 0.39 ng
RT: 7.246 min Scan# 452
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion: 93 Resp: 19220
Ion Ratio Lower Upper
93 100
63 74.7 46.6 70.0#
95 32.9 28.6 42.8


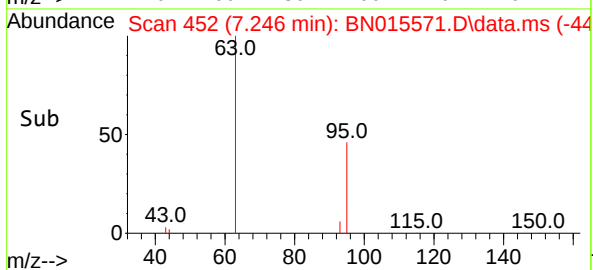

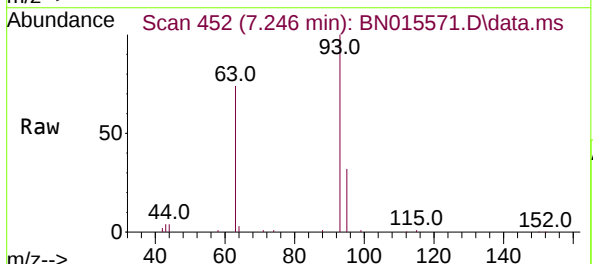




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.597 min Scan# 748
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:136	Resp:	70497
Ion Ratio	Lower	Upper
136	100	
137	11.0	9.8 14.8
54	7.7	5.4 8.2
68	6.4	4.9 7.3

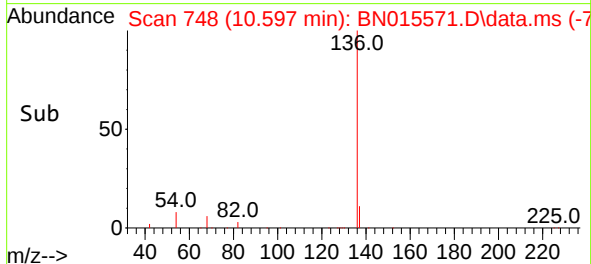

#8
Nitrobenzene-d5
Concen: 0.46 ng
RT: 8.962 min Scan# 619
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion: 82	Resp:	18127
Ion Ratio	Lower	Upper
82	100	
128	38.7	31.6 47.4
54	48.3	29.0 43.4

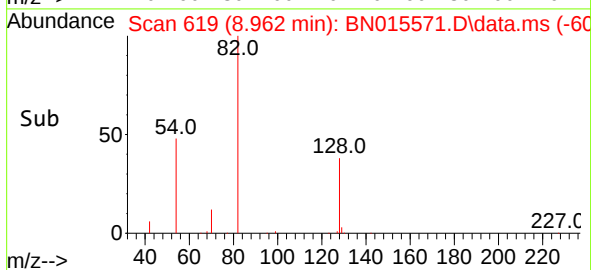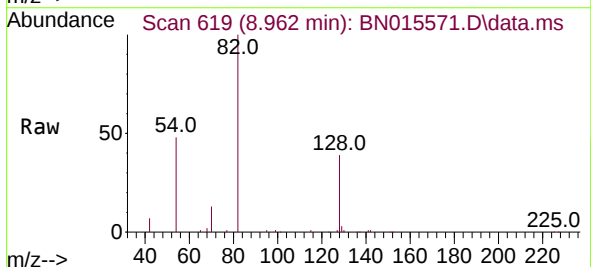

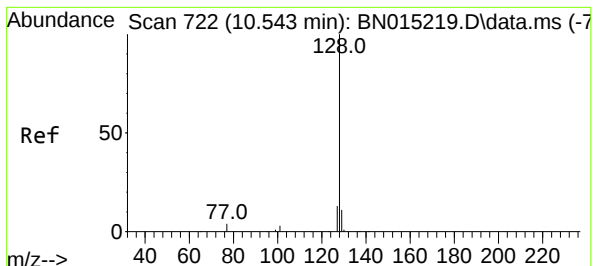

#9

Naphthalene

Concen: 0.39 ng

RT: 10.648 min Scan# 752





Delta R.T. 0.000 min

Lab File: BN015571.D

Acq: 14 Jul 2021 19:41

Tgt Ion:	128	Resp:	78102
Ion Ratio	Lower	Upper	
128	100		
129	10.9	9.1	13.7
127	13.0	11.8	17.6

Instrument :
BNA_N
ClientSampleId :

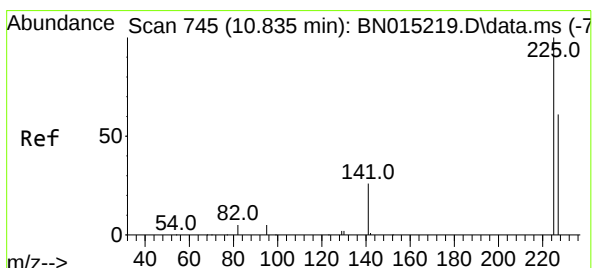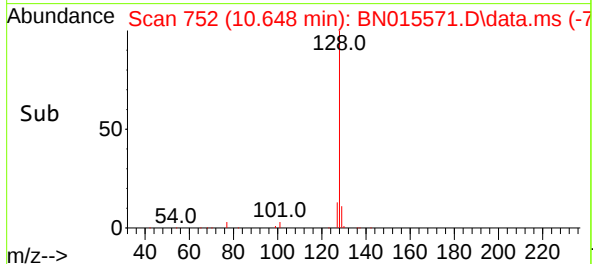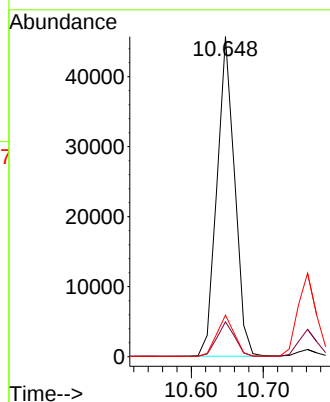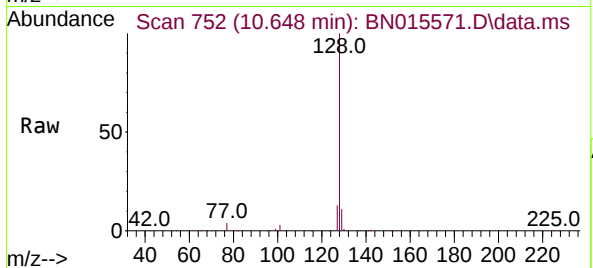

#10

Hexachlorobutadiene

Concen: 0.38 ng




RT: 10.939 min Scan# 775

Delta R.T. 0.000 min

Lab File: BN015571.D

Acq: 14 Jul 2021 19:41

Tgt Ion:	225	Resp:	14594
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.8	50.2	75.2


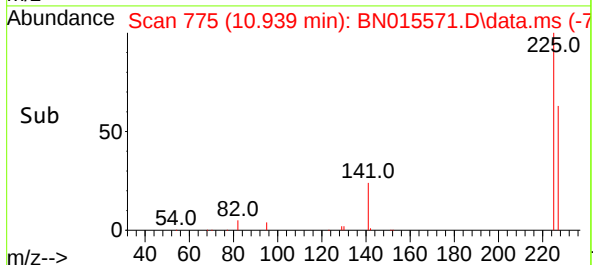
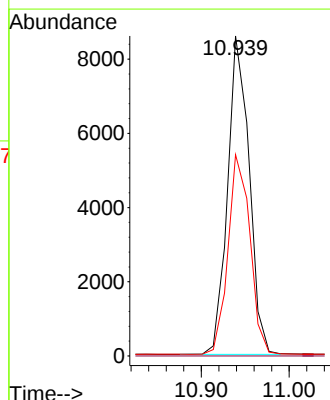
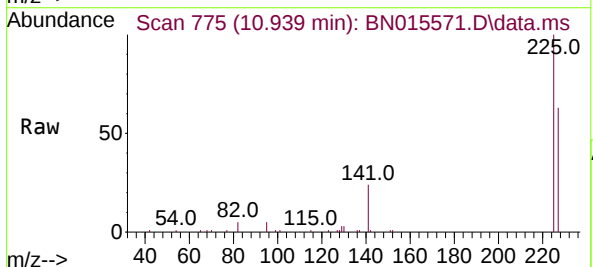




#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.190 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:152 Resp: 45043
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1

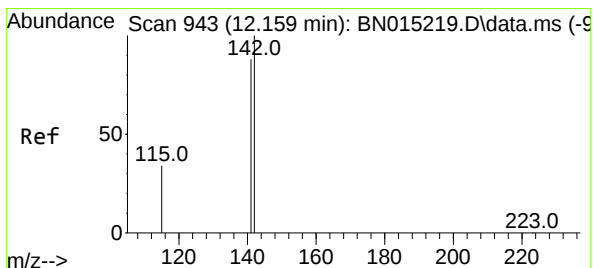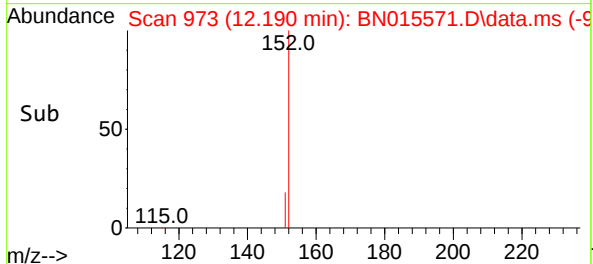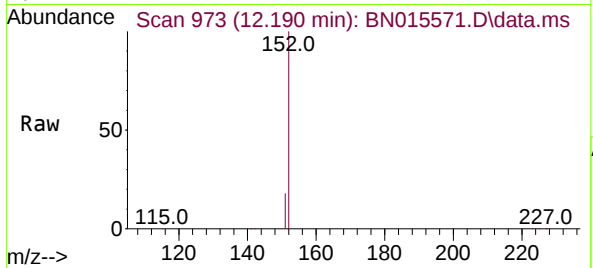

#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.265 min Scan# 990
Delta R.T. 0.005 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:142 Resp: 52309
Ion Ratio Lower Upper
142 100
141 87.9 72.3 108.5
115 32.4 40.7 61.1#


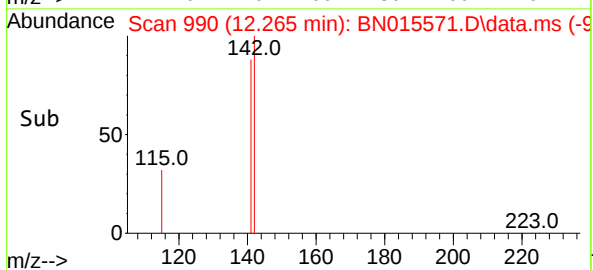

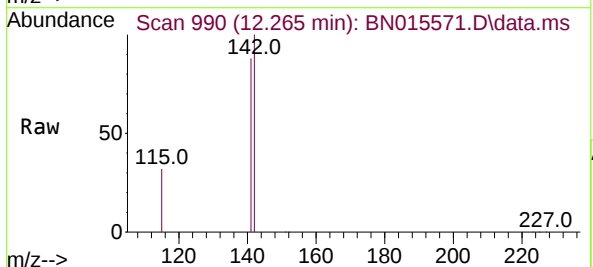




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.446 min Scan# 1197
Delta R.T. 0.013 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:164 Resp: 38962
Ion Ratio Lower Upper
164 100
162 98.7 83.8 125.6
160 43.2 37.4 56.0

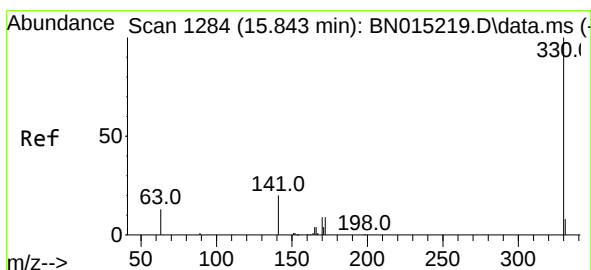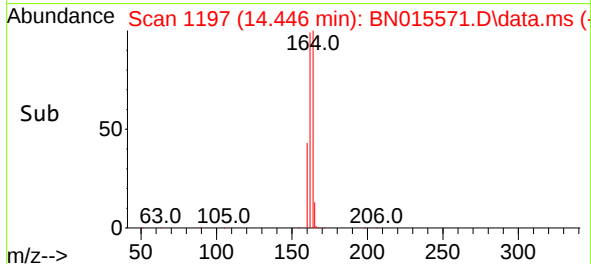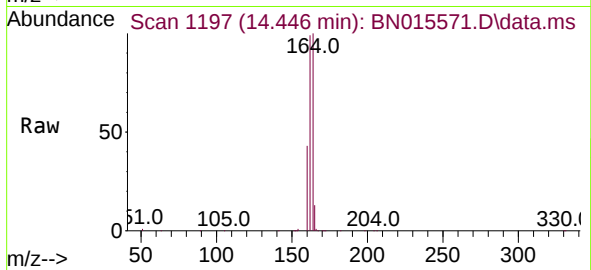

#14
2,4,6-Tribromophenol
Concen: 0.53 ng
RT: 15.931 min Scan# 1314
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:330 Resp: 5219
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.6 22.4 33.6#


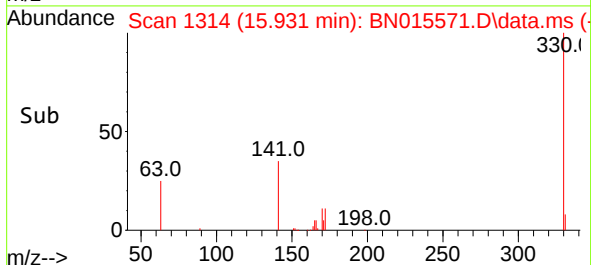

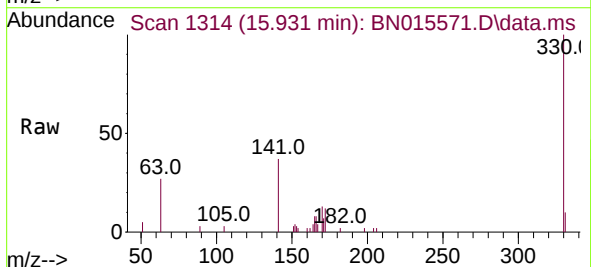




#15
2-Fluorobiphenyl
Concen: 0.38 ng
RT: 13.063 min Scan# 1088
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:172 Resp: 59534
Ion Ratio Lower Upper
172 100
171 35.0 30.6 45.8
170 23.5 20.2 30.4

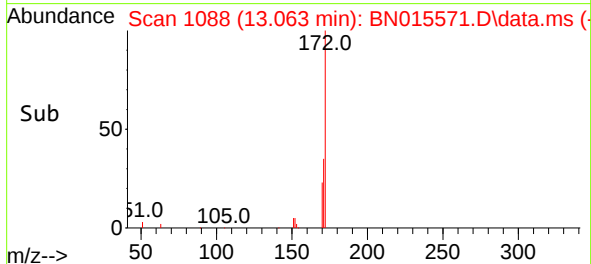

#16
Acenaphthylene
Concen: 0.38 ng
RT: 14.155 min Scan# 1174
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:152 Resp: 65627
Ion Ratio Lower Upper
152 100
151 19.5 16.7 25.1
153 13.0 10.5 15.7


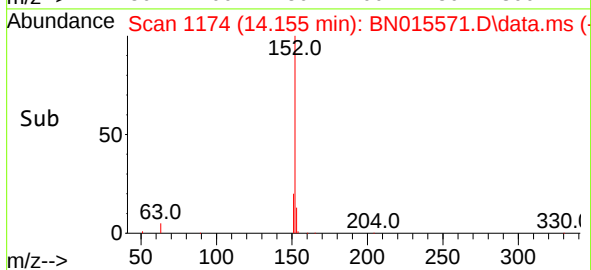

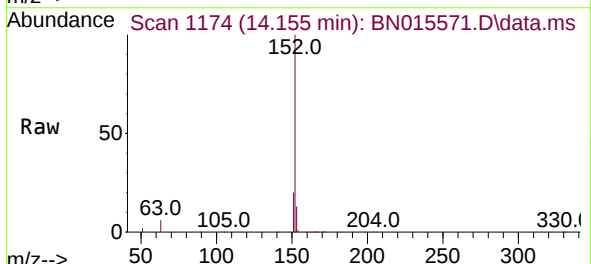




#17
Acenaphthene
Concen: 0.38 ng
RT: 14.497 min Scan# 1201
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:154 Resp: 45918
Ion Ratio Lower Upper
154 100
153 113.4 90.9 136.3
152 55.2 45.8 68.8

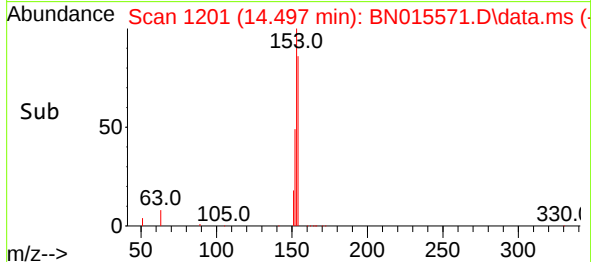

#18
Fluorene
Concen: 0.38 ng
RT: 15.487 min Scan# 1279
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:166 Resp: 56201
Ion Ratio Lower Upper
166 100
165 97.3 79.2 118.8
167 13.5 10.7 16.1


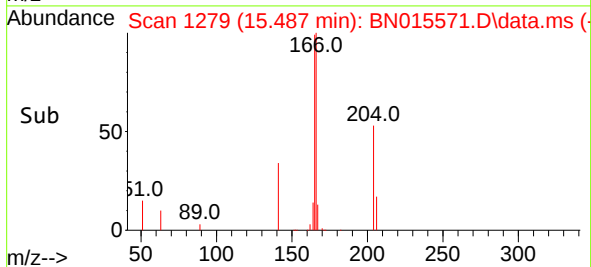

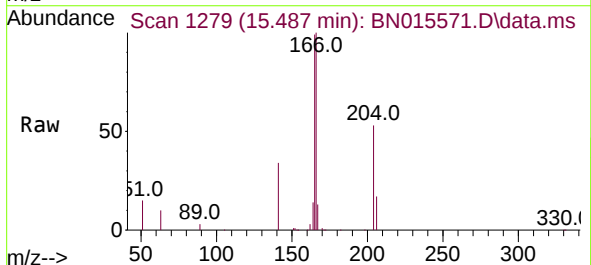




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.188 min Scan# 1417
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampled :


Tgt Ion:188 Resp: 73487
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.9 9.0 13.4

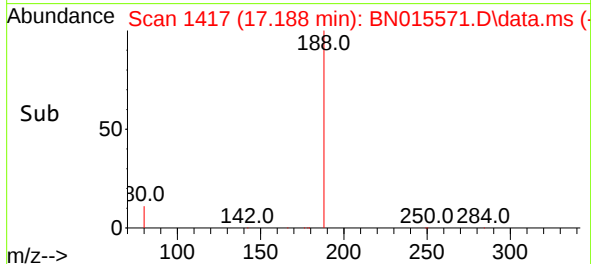

#20
4,6-Dinitro-2-methylphenol
Concen: 0.47 ng
RT: 15.576 min Scan# 1286
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:198 Resp: 384
Ion Ratio Lower Upper
198 100
182 28.1 34.5 51.7#
77 0.0 0.0 0.0


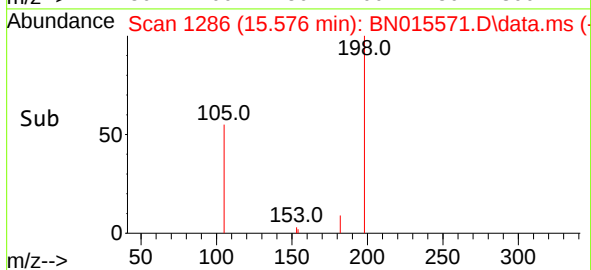

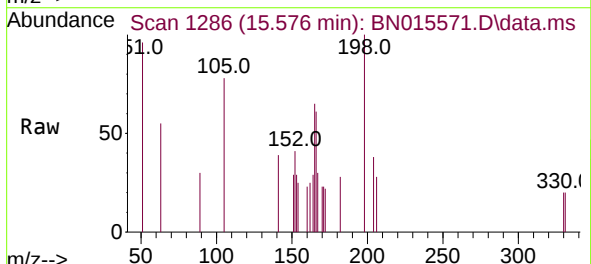


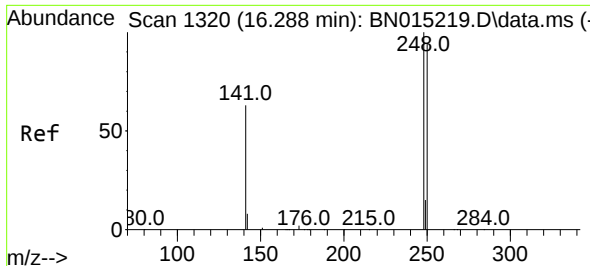

#21
4-Bromophenyl-phenylether
Concen: 0.37 ng
RT: 16.385 min Scan# 1351
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampled :


Tgt Ion:248 Resp: 17452
Ion Ratio Lower Upper
248 100
250 96.6 86.2 129.4
141 51.8 36.2 54.2

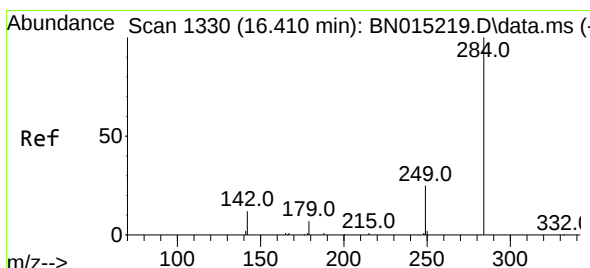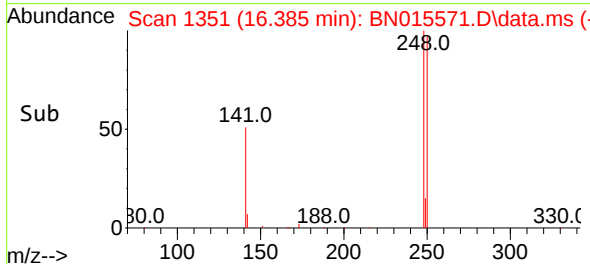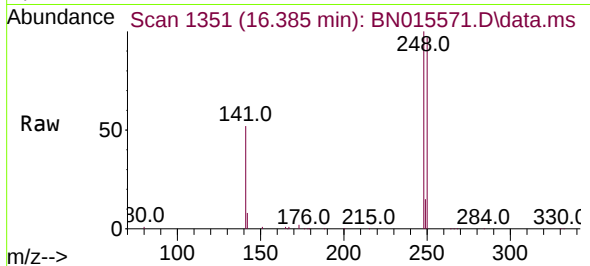

#22
Hexachlorobenzene
Concen: 0.38 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.012 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:284 Resp: 20069
Ion Ratio Lower Upper
284 100
142 34.5 22.2 33.2#
249 31.0 26.6 39.8


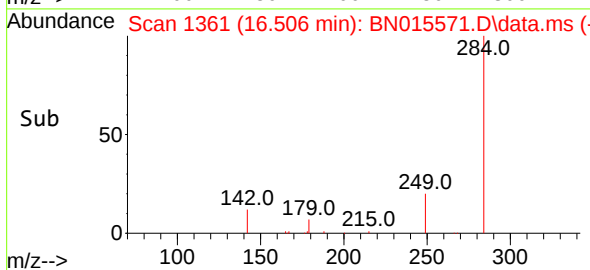

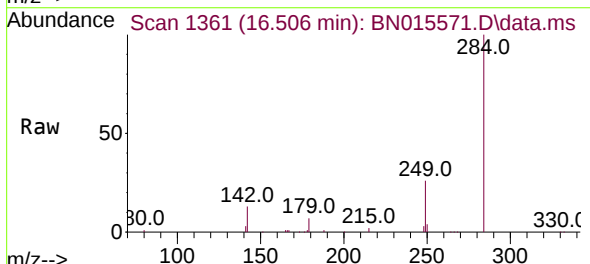


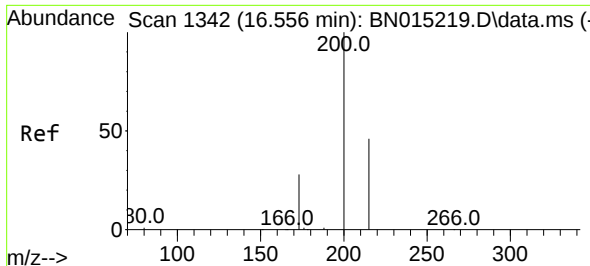

#23
Atrazine
Concen: 0.45 ng
RT: 16.652 min Scan# 1373
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampled :

Tgt Ion:200 Resp: 11221
Ion Ratio Lower Upper
200 100
173 27.7 21.7 32.5
215 46.9 43.1 64.7

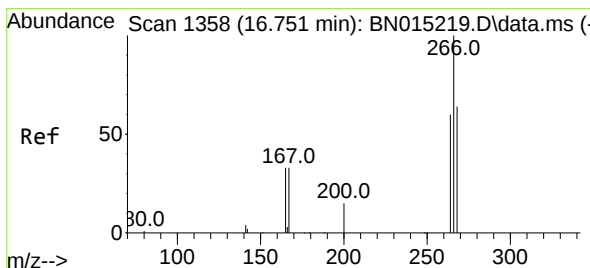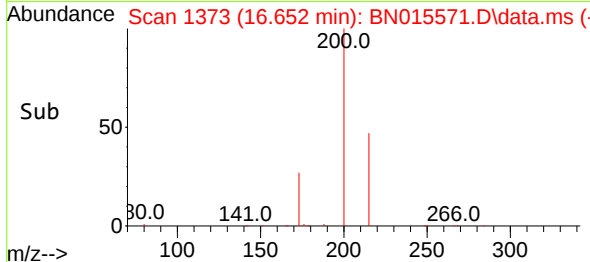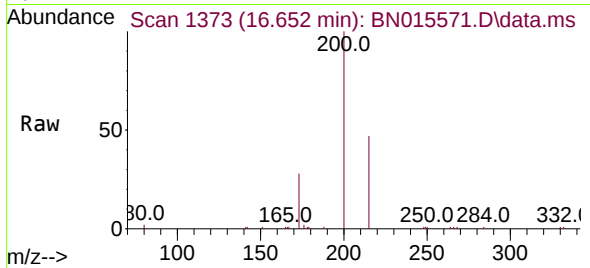

#24
Pentachlorophenol
Concen: 0.59 ng
RT: 16.847 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:266 Resp: 3181
Ion Ratio Lower Upper
266 100
264 63.4 51.0 76.4
268 64.7 50.6 76.0


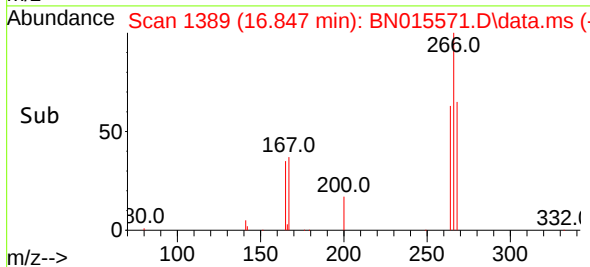

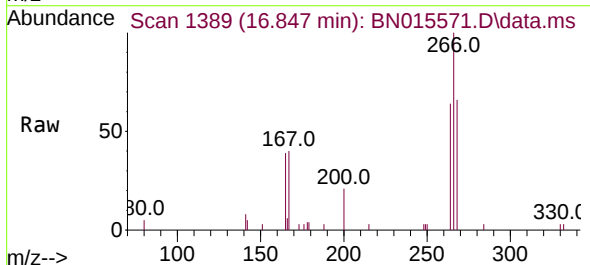




#25
Phenanthrene
Concen: 0.39 ng
RT: 17.237 min Scan# 1421
Delta R.T. 0.012 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:178 Resp: 91826
Ion Ratio Lower Upper
178 100
176 18.7 15.6 23.4
179 15.5 12.1 18.1

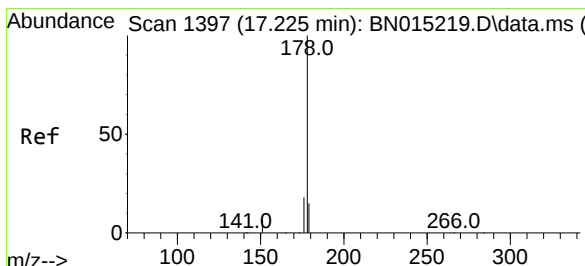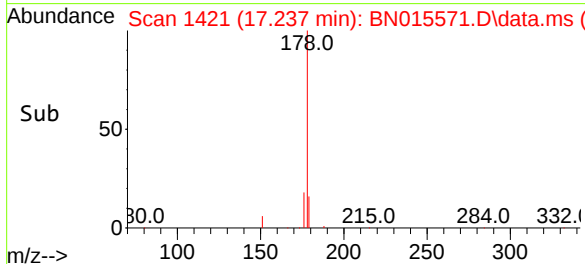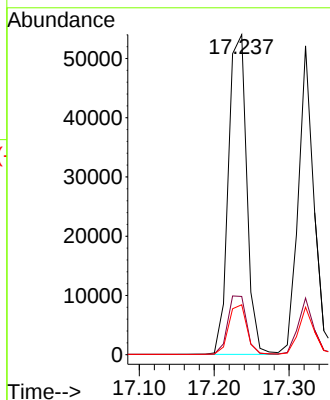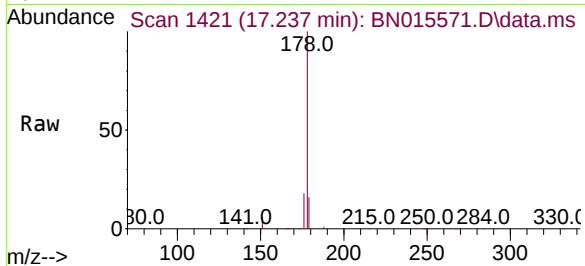

#26
Anthracene
Concen: 0.37 ng
RT: 17.322 min Scan# 1428
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:178 Resp: 75917
Ion Ratio Lower Upper
178 100
176 18.2 15.1 22.7
179 15.3 12.2 18.2


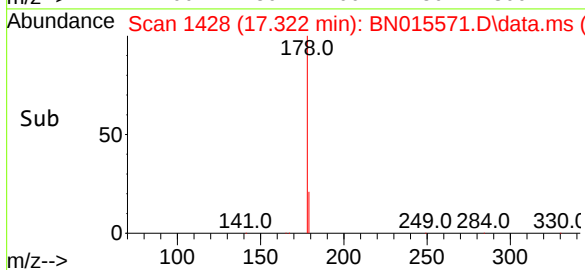
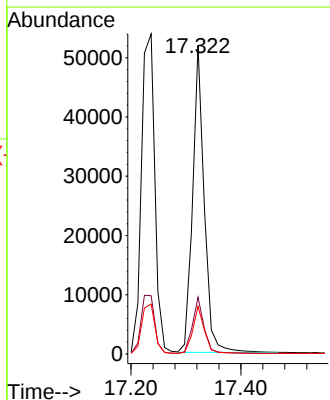
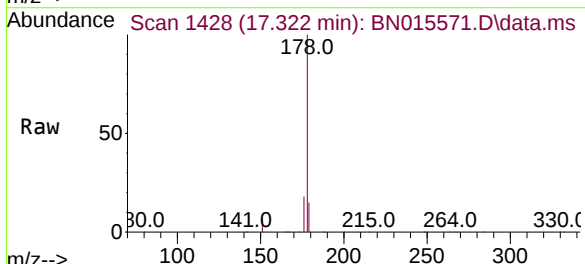


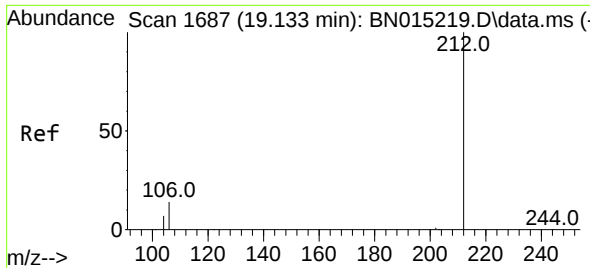

#27
Fluoranthene-d10
Concen: 0.37 ng
RT: 19.227 min Scan# 1729
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:212 Resp: 79523
Ion Ratio Lower Upper
212 100
106 14.2 7.0 10.6#
104 7.8 4.1 6.1#

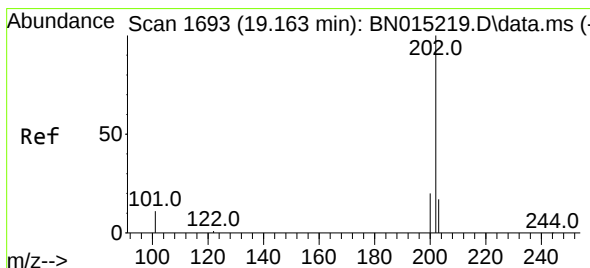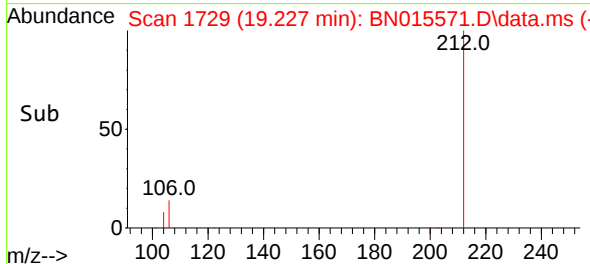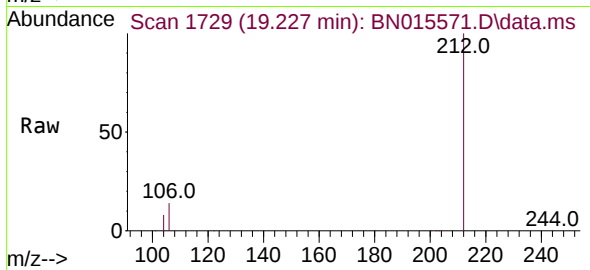

#28
Fluoranthene
Concen: 0.38 ng
RT: 19.257 min Scan# 1735
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:202 Resp: 97573
Ion Ratio Lower Upper
202 100
101 11.8 6.6 10.0#
203 17.3 13.9 20.9

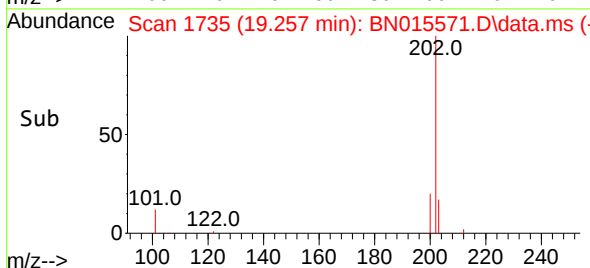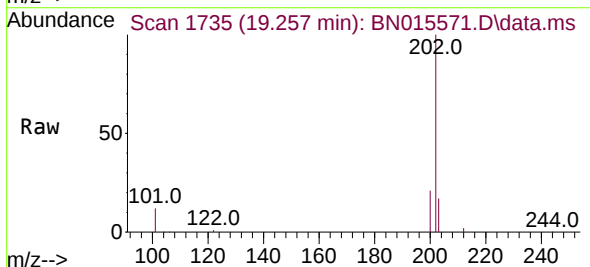



#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.387 min Scan# 2016

Delta R.T. 0.000 min

Lab File: BN015571.D

Acq: 14 Jul 2021 19:41





Tgt Ion:240 Resp: 52724

Ion Ratio Lower Upper

240 100

120 9.3 4.2 6.4#

236 26.4 21.4 32.2

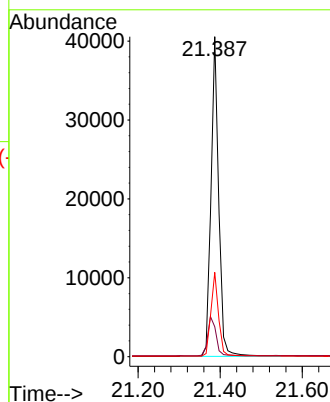

#30

Pyrene

Concen: 0.48 ng

RT: 19.619 min Scan# 1808

Delta R.T. 0.000 min

Lab File: BN015571.D

Acq: 14 Jul 2021 19:41




Tgt Ion:202 Resp: 95788


Ion Ratio Lower Upper

202 100

200 20.6 16.9 25.3

203 17.4 13.9 20.9


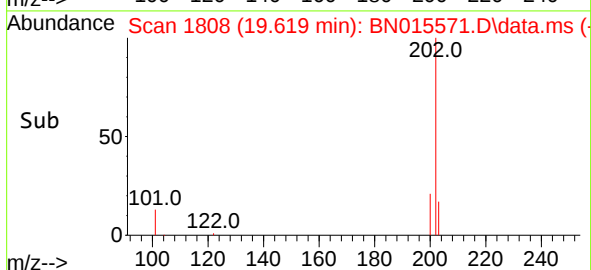
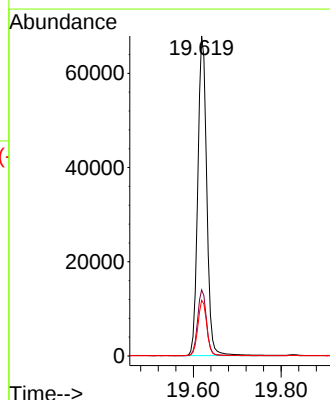





#31
Terphenyl-d14
Concen: 0.47 ng
RT: 19.827 min Scan# 1850
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:244 Resp: 58307
Ion Ratio Lower Upper
244 100
212 7.7 6.3 9.5
122 13.8 6.2 9.2#

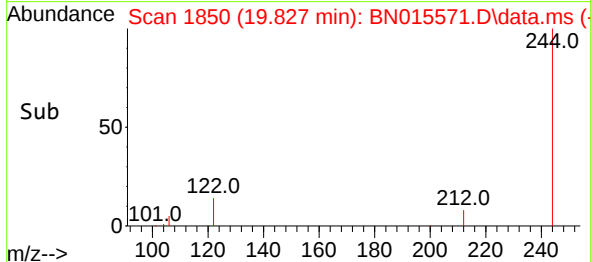

#32
Benzo(a)anthracene
Concen: 0.37 ng
RT: 21.376 min Scan# 2015
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:228 Resp: 67659
Ion Ratio Lower Upper
228 100
226 25.6 23.0 34.6
229 20.3 15.7 23.5


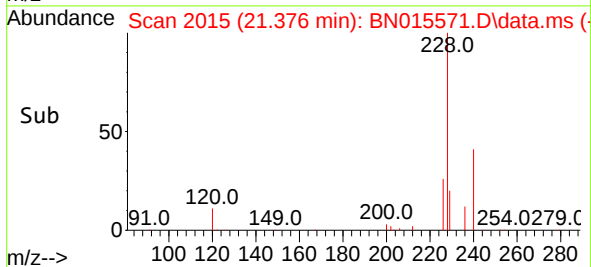

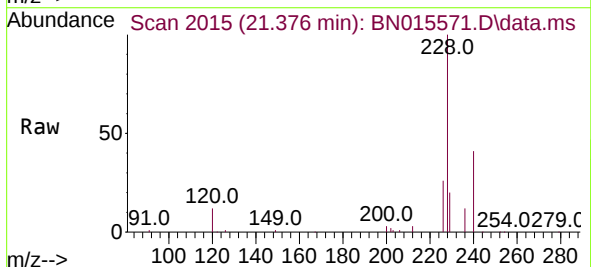




#33
Chrysene
Concen: 0.38 ng
RT: 21.419 min Scan# 2019
Delta R.T. -0.010 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:	228	Resp:	74585
Ion Ratio	Lower	Upper	
228	100		
226	30.0	25.0	37.6
229	19.1	15.9	23.9

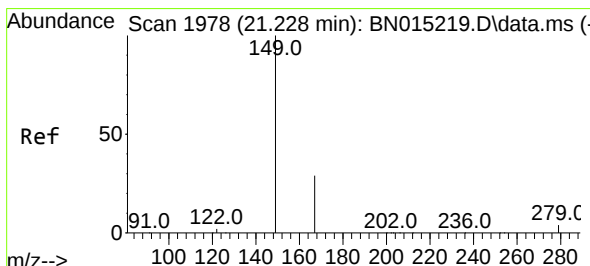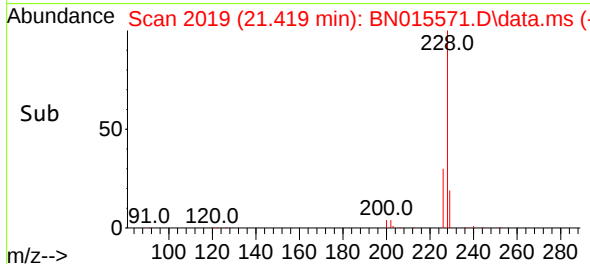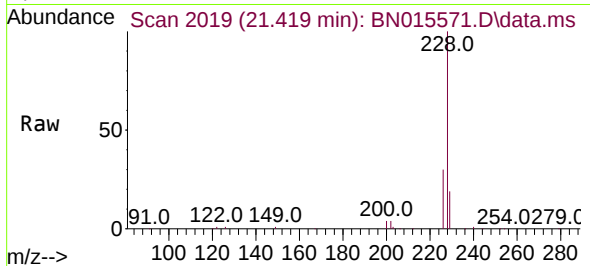

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.62 ng
RT: 21.312 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41


Tgt Ion:	149	Resp:	30961
Ion Ratio	Lower	Upper	
149	100		
167	27.9	28.9	43.3#
279	3.6	4.9	7.3#

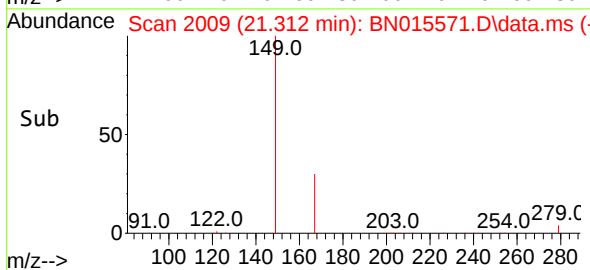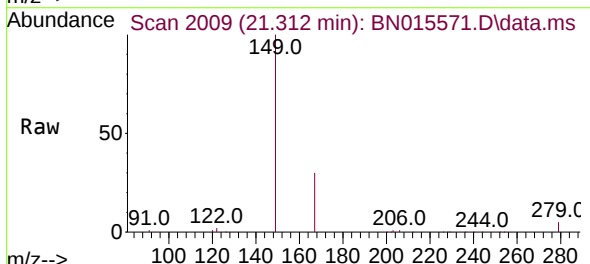






#35
Perylene-d12
Concen: 0.40 ng
RT: 23.745 min Scan# 2503
Delta R.T. -0.003 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Instrument :
BNA_N
ClientSampled :



Tgt Ion:264 Resp: 29052




Ion	Ratio	Lower	Upper
264	100		
260	24.9	20.6	31.0
265	25.5	21.4	32.2

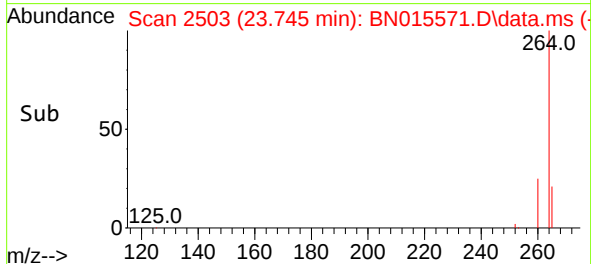

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.20 ng
RT: 26.175 min Scan# 3213
Delta R.T. -0.003 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:276 Resp: 20896


Ion	Ratio	Lower	Upper
276	100		
138	32.0	10.0	15.0#
277	25.0	20.4	30.6

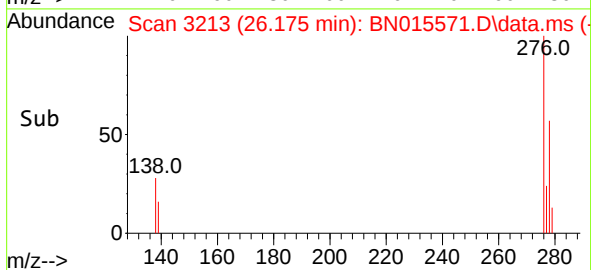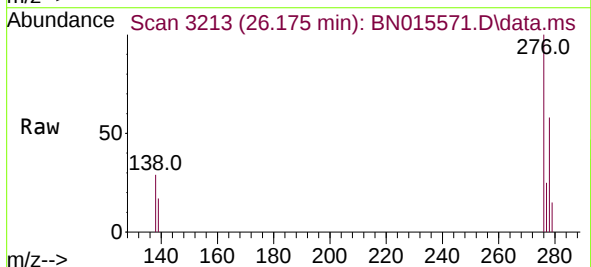






#37
Benzo(b)fluoranthene
Concen: 0.44 ng
RT: 23.029 min Scan# 2294
Delta R.T. -0.003 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Instrument :
BNA_N
ClientSampleId :






Tgt Ion:252 Resp: 50434
Ion Ratio Lower Upper
252 100
253 22.6 18.5 27.7
125 13.8 5.8 8.6#



#38
Benzo(k)fluoranthene
Concen: 0.42 ng
RT: 23.074 min Scan# 2307
Delta R.T. -0.007 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Tgt Ion:252 Resp: 51584
Ion Ratio Lower Upper
252 100
253 22.4 19.1 28.7
125 11.4 5.4 8.0#

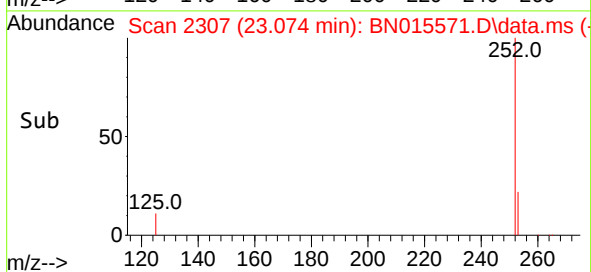



#39

Benzo(a)pyrene

Concen: 0.34 ng

RT: 23.642 min Scan# 2473





Delta R.T. -0.003 min

Lab File: BN015571.D

Acq: 14 Jul 2021 19:41

Tgt Ion:252	Resp:	35376
Ion Ratio	Lower	Upper
252	100	
253	23.5	19.4 29.2
125	21.3	7.4 11.2#

Instrument :
BNA_N
ClientSampleId :

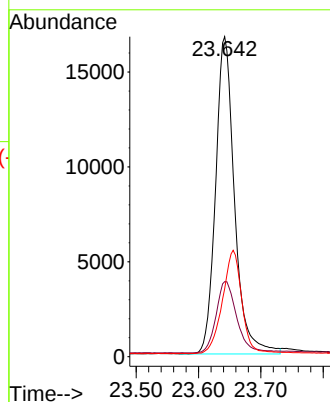

#40

Dibenzo(a,h)anthracene

Concen: 0.20 ng




RT: 26.192 min Scan# 3218


Delta R.T. -0.003 min

Lab File: BN015571.D

Acq: 14 Jul 2021 19:41

Tgt Ion:278	Resp:	16258
Ion Ratio	Lower	Upper
278	100	
139	20.9	9.0 13.4#
279	25.4	21.0 31.4

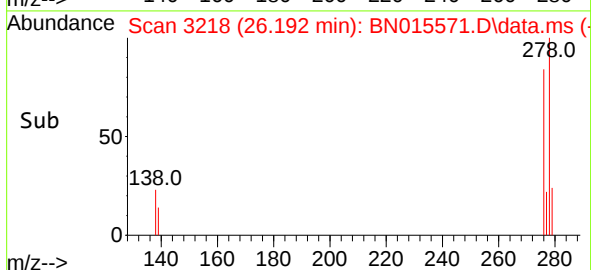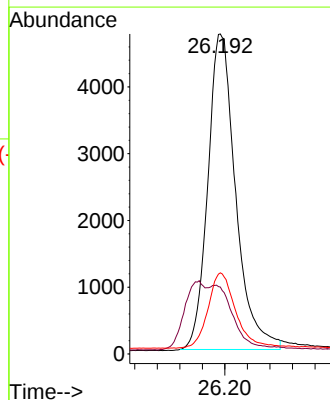

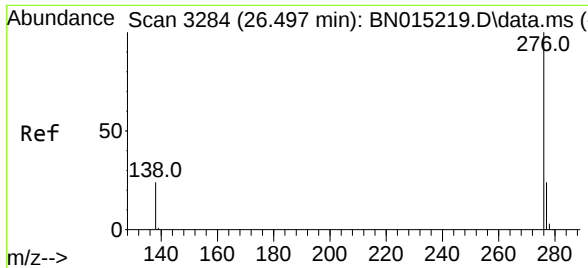

#41
Benzo(g,h,i)perylene
Concen: 0.19 ng
RT: 26.914 min Scan# 3429
Delta R.T. -0.003 min
Lab File: BN015571.D
Acq: 14 Jul 2021 19:41

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:276 Resp: 16856
Ion Ratio Lower Upper
276 100
277 24.8 19.7 29.5
138 24.0 9.8 14.6#

