
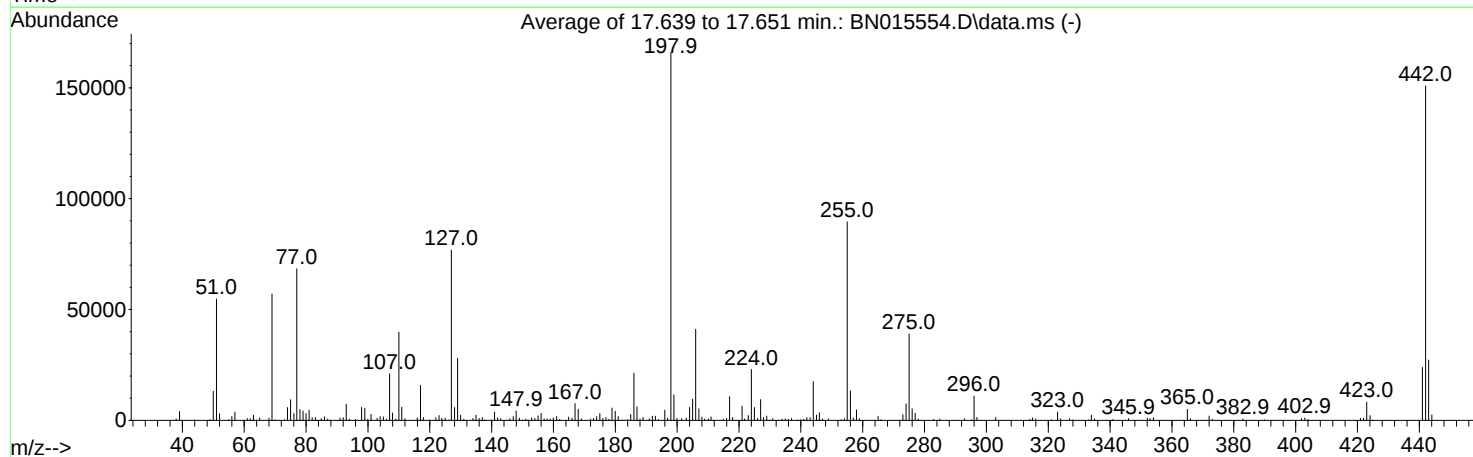


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071421\
 Data File : BN015554.D
 Acq On : 14 Jul 2021 08:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 14 11:20:16 2021

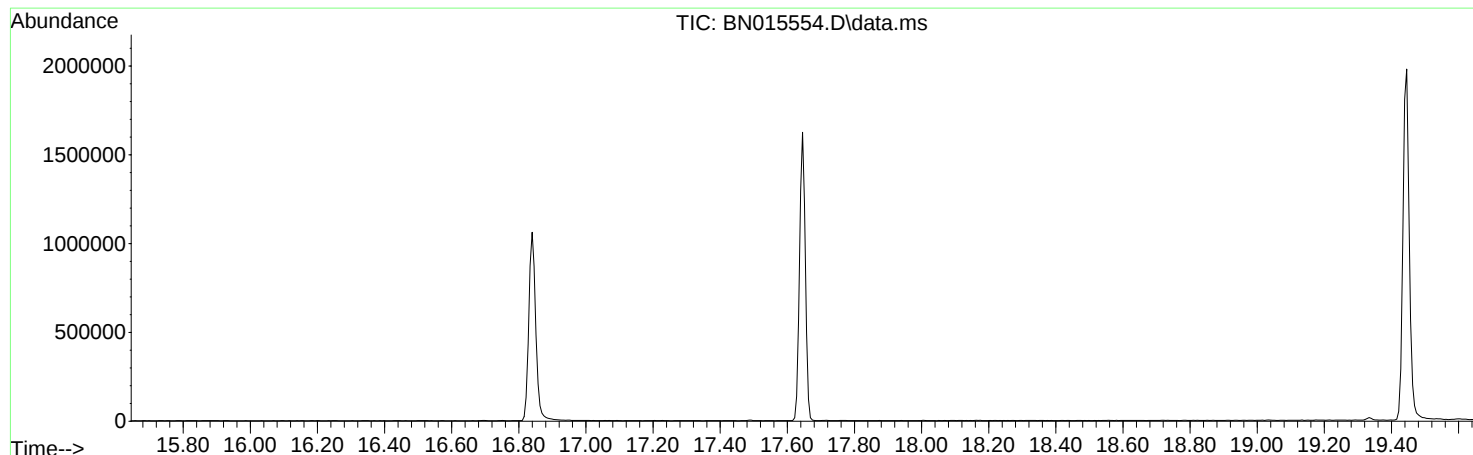




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	54739	PASS
68	69	0.00	2	1.6	918	PASS
69	198	0.00	100	34.3	56989	PASS
70	69	0.00	2	0.4	224	PASS
127	198	10	80	46.3	76779	PASS
197	198	0.00	2	0.6	1021	PASS
198	198	100	100	100.0	165931	PASS
199	198	5	9	6.9	11472	PASS
275	198	10	60	23.5	38973	PASS
365	198	1	100	3.0	5018	PASS
441	198	0.01	100	14.4	23921	PASS
442	442	50	100	100.0	150859	PASS
443	442	15	24	18.1	27243	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071421\
Data File : BN015554.D
Acq On : 14 Jul 2021 08:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 05:41:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

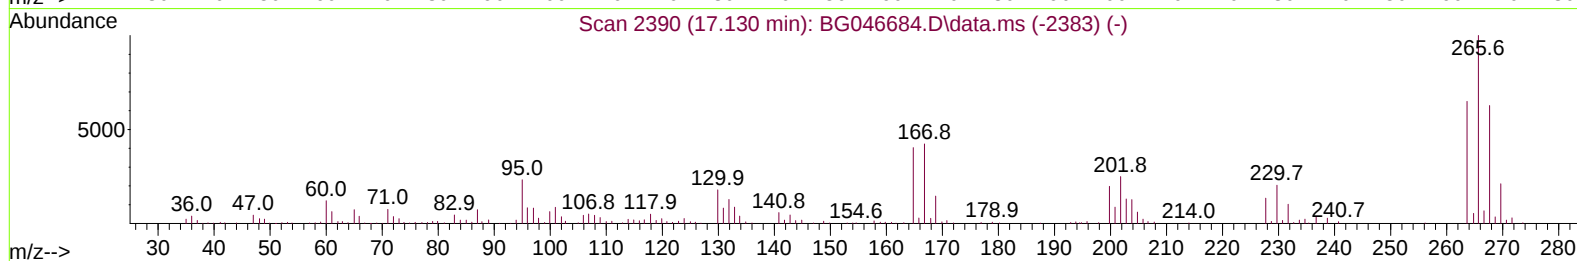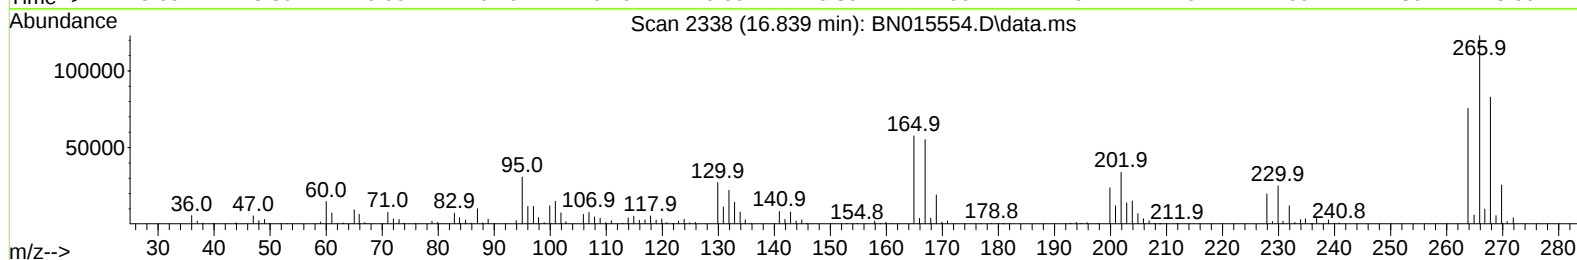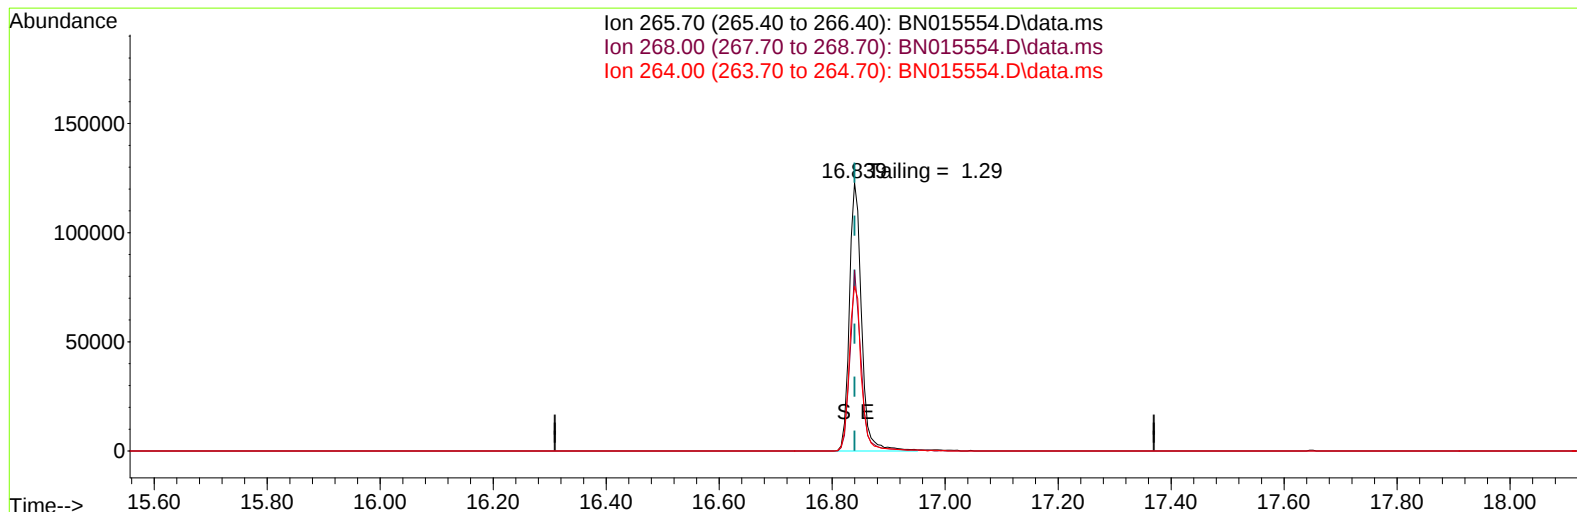

TIC: BN015554.D\data.ms

(70) Pentachlorophenol (C)

16.839min (0.000) 32943.67 ng




response 184593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.41
264.00	61.60	61.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071421\
Data File : BN015554.D
Acq On : 14 Jul 2021 08:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 15 05:41:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

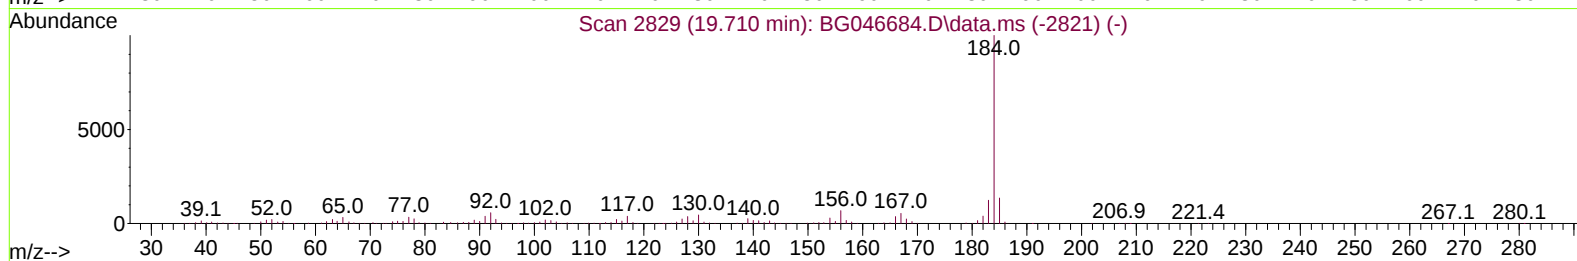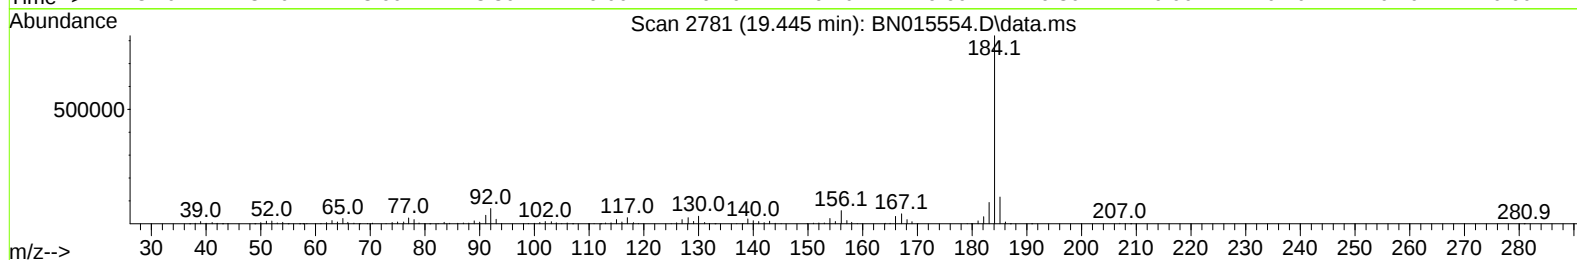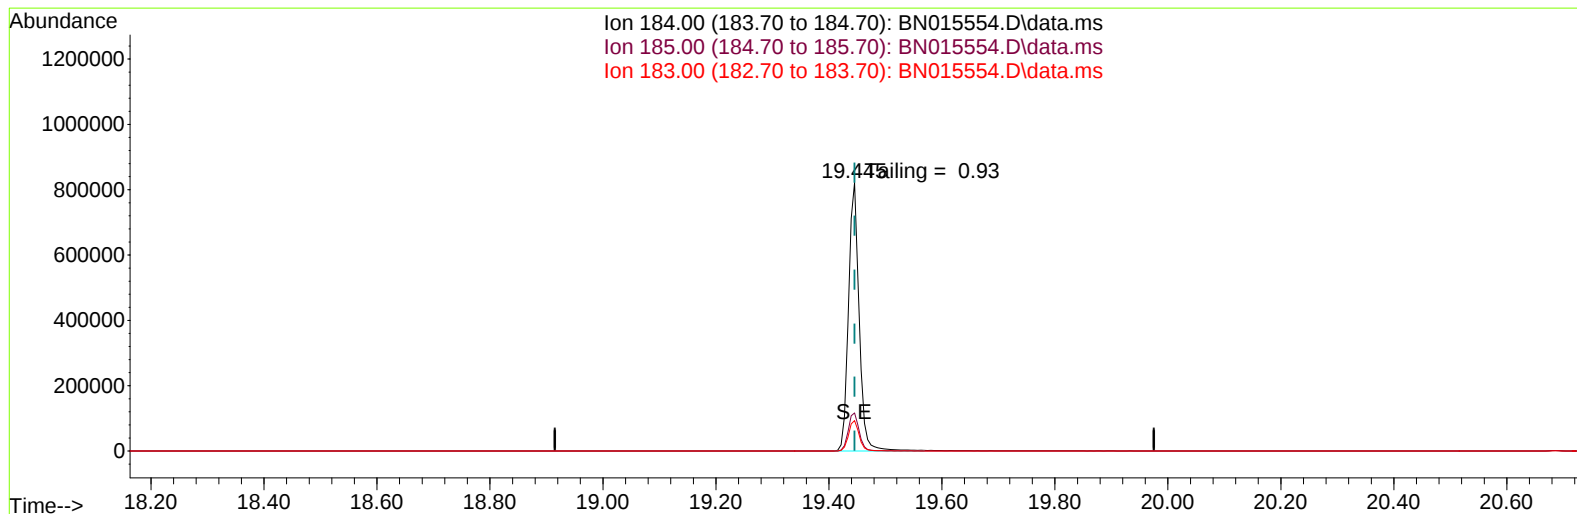

TIC: BN015554.D\data.ms

(77) Benzidine

19.445min (0.000) 0.00 ng

response 1079305

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.22
183.00	13.20	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2021	BNA_N	<u>BN015554.D</u>
Compound Name	Response	Retention Time
DDT	478314	20.68
DDD	40278	20.24
DDE	5521	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45799	524113	8.74