

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071423\
 Data File : BN026503.D
 Acq On : 14 Jul 2023 16:57
 Operator : MA/JU
 Sample : PB153998BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 15 01:54:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 01:53:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	2047	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	6275	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.584	164	4334	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	9904	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.529	240	8556	0.400	ng/ul	# 0.00
23) Perylene-d12	23.938	264	11433	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	8875	3.292	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.365	152	3126	0.366	ng/ul	0.01
18) Fluoranthene-d10	19.363	212	14778	0.498	ng/ul	0.00
Target Compounds						
					Qvalue	
14) Pentachlorophenol	17.013	266	57	0.023	ng/ul#	76
20) Pyrene	19.721	202	2637	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.780	252	5803	0.146	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071423\
Data File : BN026503.D
Acq On : 14 Jul 2023 16:57
Operator : MA/JU
Sample : PB153998BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 15 01:54:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 01:53:23 2023
Response via : Initial Calibration

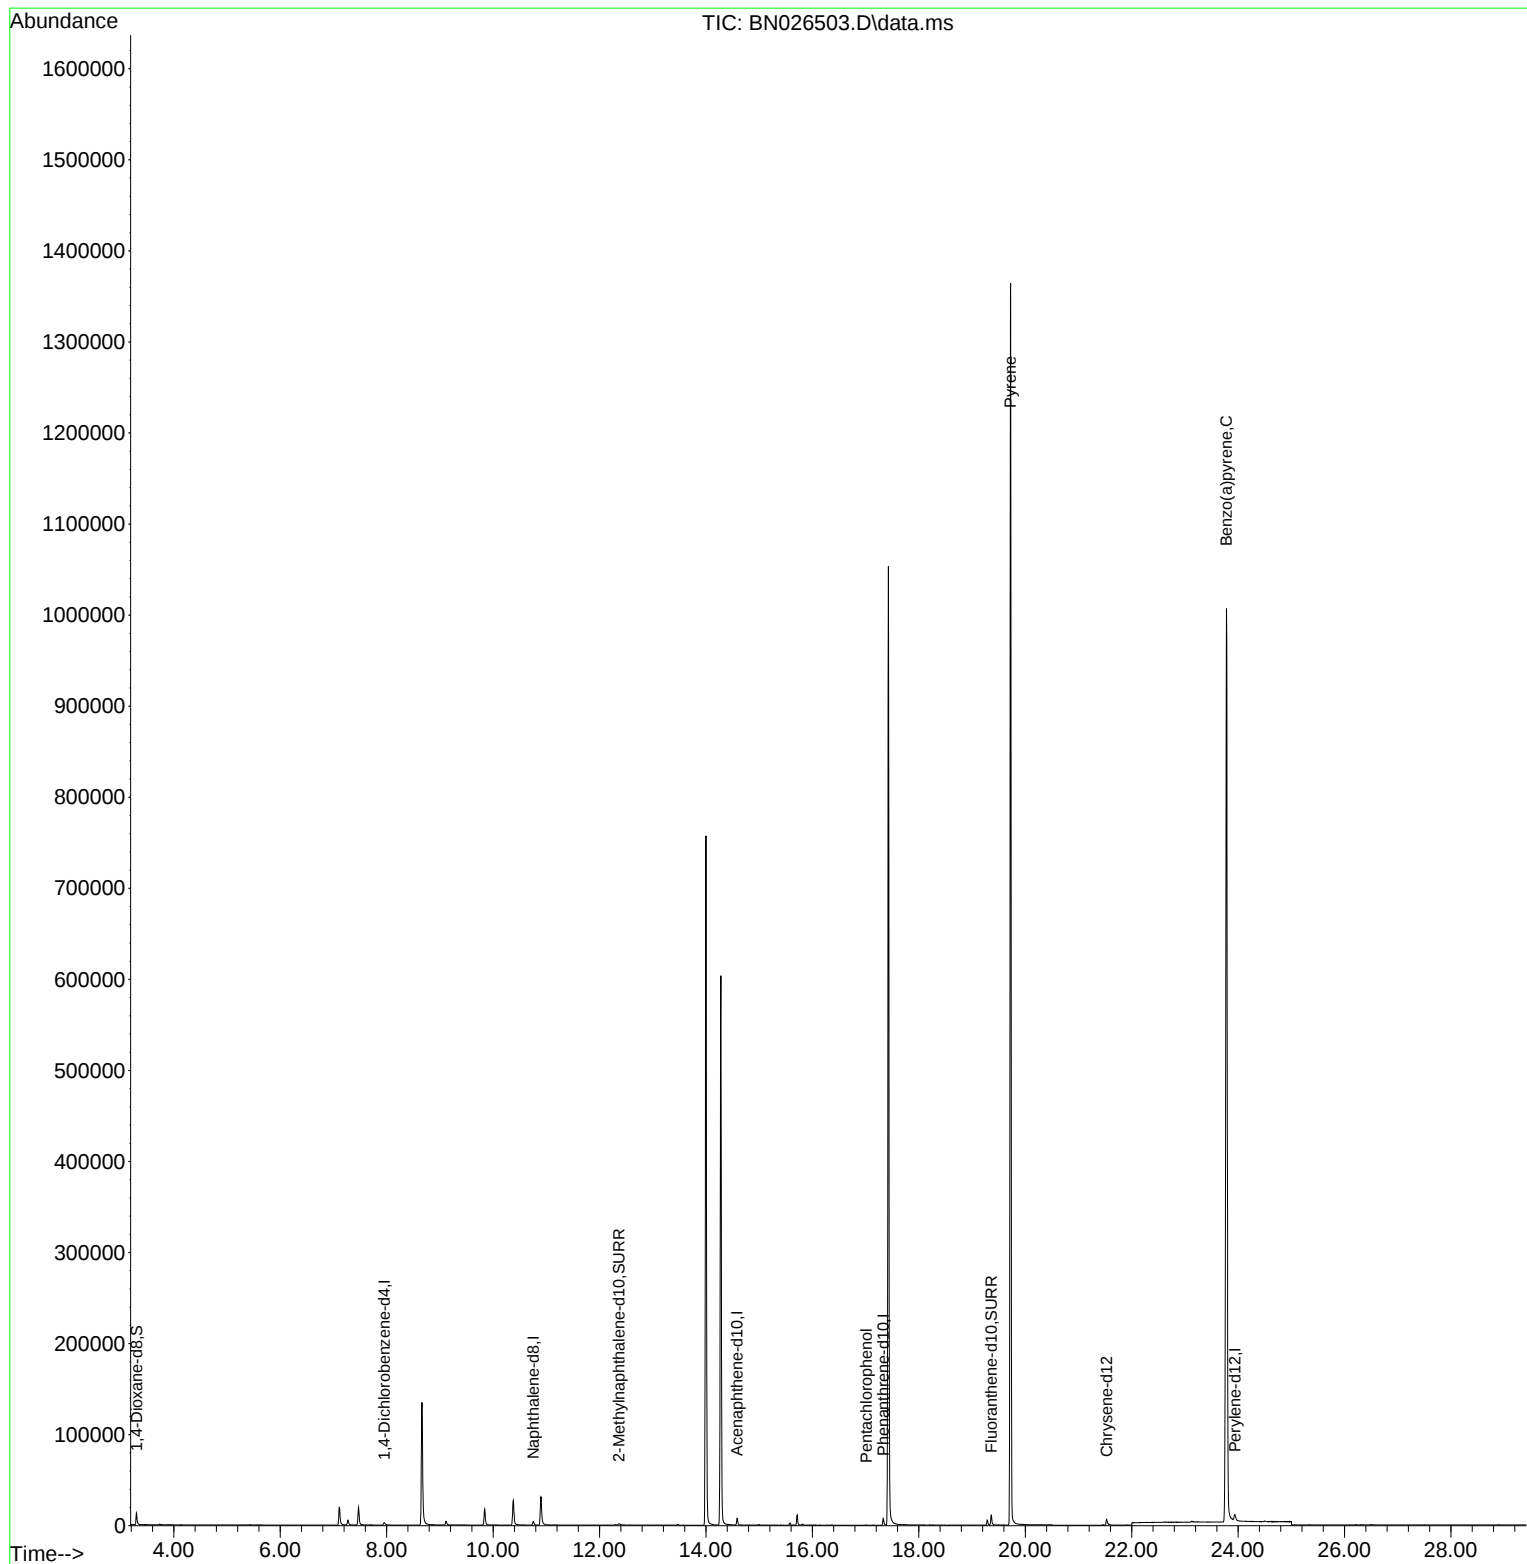



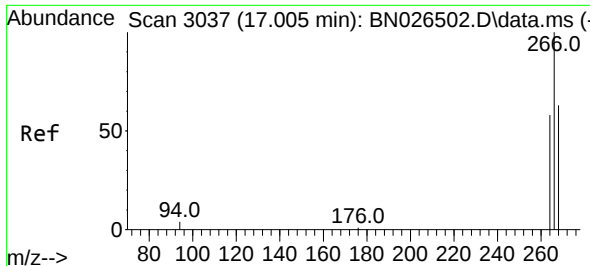


#14
 Pentachlorophenol
 Concen: 0.023 ng/ul
 RT: 17.013 min Scan# 3037
 Delta R.T. 0.008 min
 Lab File: BN026503.D
 Acq: 14 Jul 2023 16:57

Instrument :
 BNA_N
 ClientSampleId :



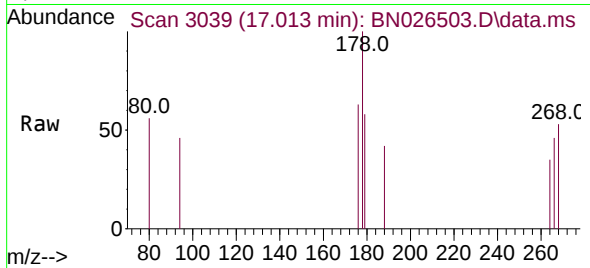



Tgt Ion:266 Resp: 57
 Ion Ratio Lower Upper
 266 100
 264 42.1 52.0 78.0#
 268 50.9 53.0 79.6#

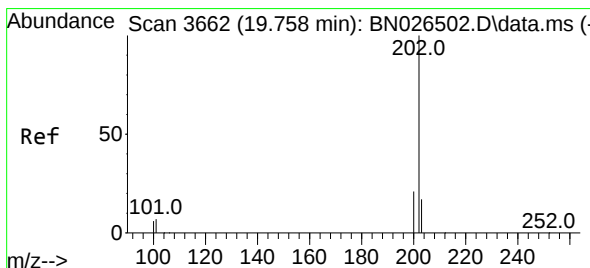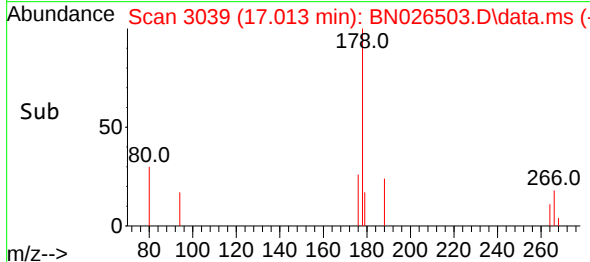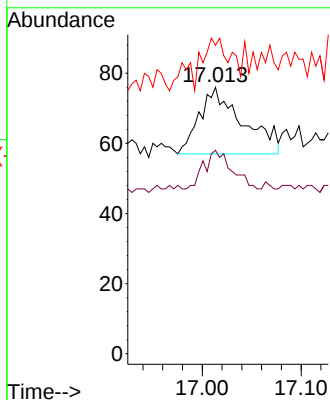

#20
 Pyrene
 Concen: 0.061 ng/ul
 RT: 19.721 min Scan# 3654
 Delta R.T. -0.037 min
 Lab File: BN026503.D
 Acq: 14 Jul 2023 16:57

Tgt Ion:202 Resp: 2637
 Ion Ratio Lower Upper
 202 100
 101 208.6 8.0 12.0#
 100 1775.9 6.2 9.2#

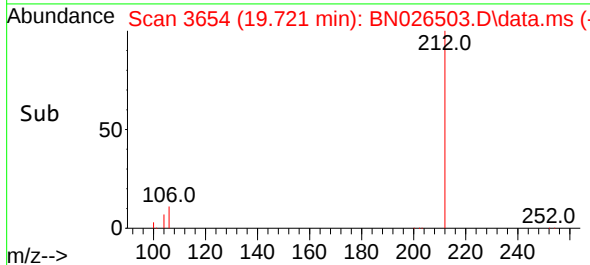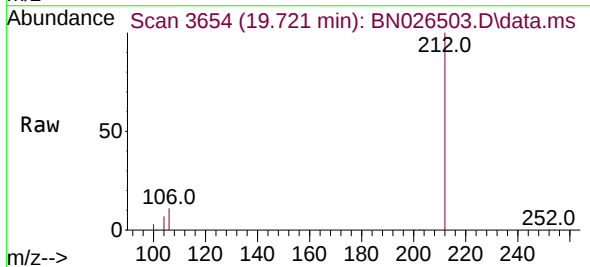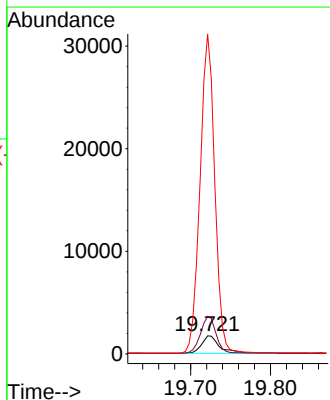

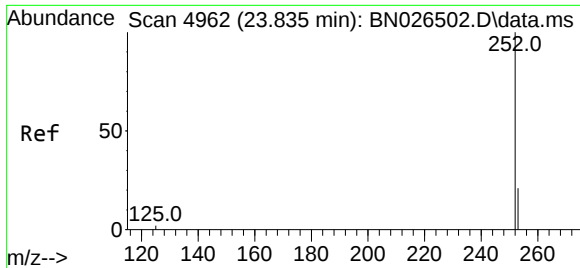

#26

Benzo(a)pyrene

Concen: 0.146 ng/ul

RT: 23.780 min Scan# 49

Delta R.T. -0.056 min


Lab File: BN026503.D

Acq: 14 Jul 2023 16:57

Instrument :

BNA_N

ClientSampleId :

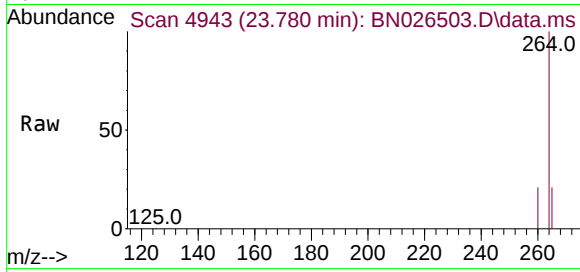

Tgt Ion:252 Resp: 5803

Ion Ratio Lower Upper

252 100

253 50.0 32.6 49.0#

125 49.1 19.3 28.9#

