

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071425\
 Data File : BN037484.D
 Acq On : 14 Jul 2025 09:49
 Operator : RC/JU
 Sample : PB168696BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB168696BL

Quant Time: Jul 14 10:56:25 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 11 15:38:34 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.731	152	2133	0.400	ng	0.00
7) Naphthalene-d8	10.509	136	4972	0.400	ng	0.00
13) Acenaphthene-d10	14.355	164	2255	0.400	ng	-0.01
19) Phenanthrene-d10	17.099	188	3944	0.400	ng	0.00
29) Chrysene-d12	21.286	240	2959	0.400	ng	0.00
35) Perylene-d12	23.525	264	2878	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.319	112	1749	0.352	ng	0.00
5) Phenol-d6	6.886	99	2094	0.335	ng	0.00
8) Nitrobenzene-d5	8.864	82	1333	0.369	ng	0.00
11) 2-Methylnaphthalene-d10	12.101	152	2408	0.356	ng	0.00
14) 2,4,6-Tribromophenol	15.845	330	109	0.143	ng	0.00
15) 2-Fluorobiphenyl	12.988	172	4883	0.379	ng	0.00
27) Fluoranthene-d10	19.132	212	3492	0.351	ng	0.00
31) Terphenyl-d14	19.736	244	2573	0.417	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.214	149	71	0.021	ng	Qvalue # 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071425\
Data File : BN037484.D
Acq On : 14 Jul 2025 09:49
Operator : RC/JU
Sample : PB168696BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB168696BL


Quant Time: Jul 14 10:56:25 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 11 15:38:34 2025
Response via : Initial Calibration

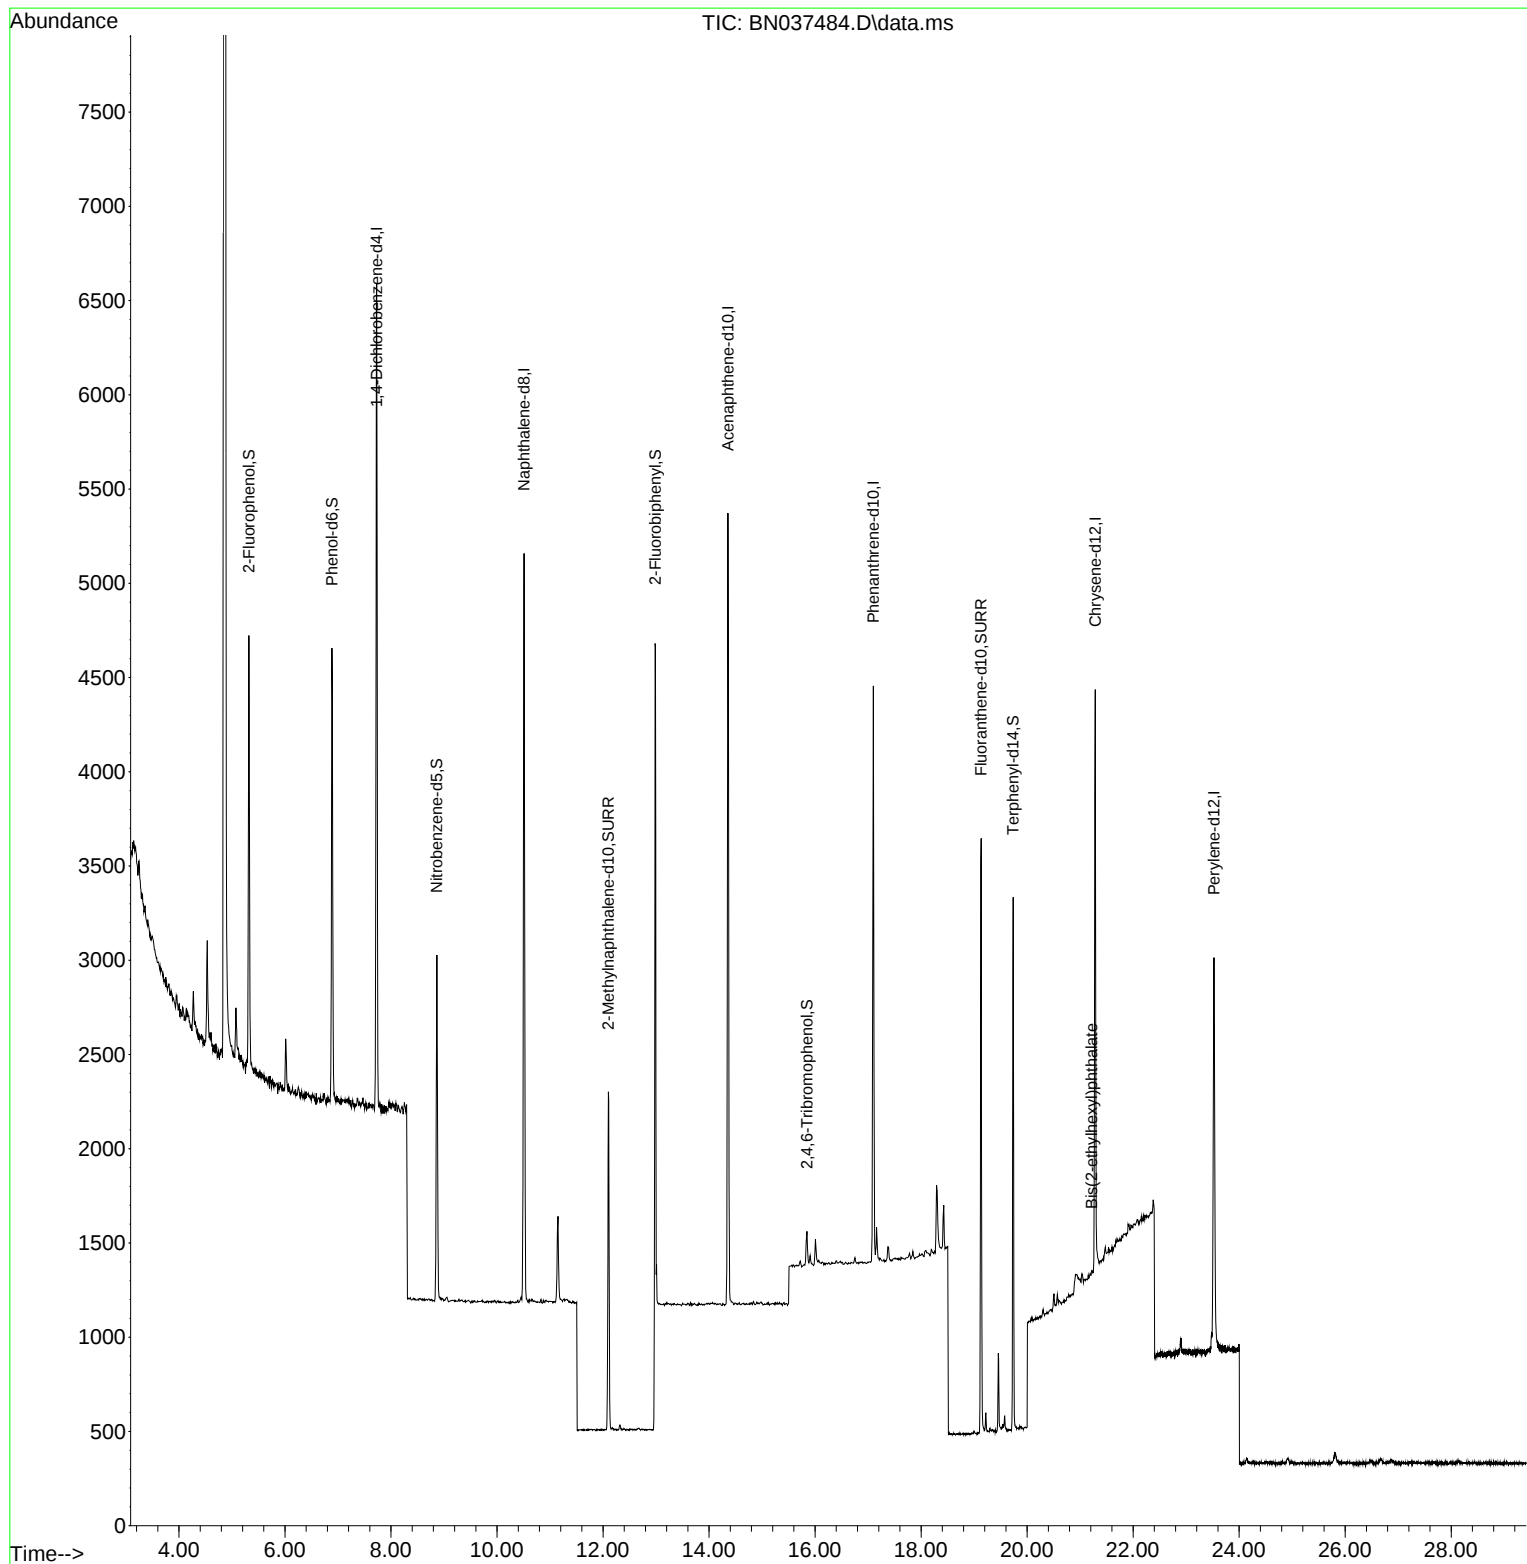

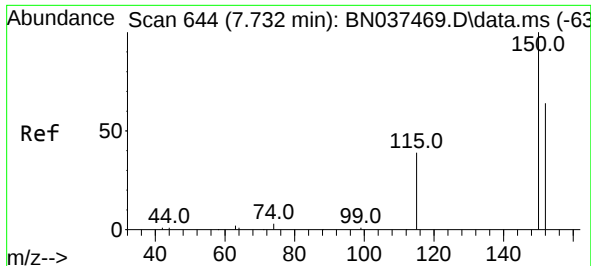




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.731 min Scan# 64
 Delta R.T. -0.001 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49

Instrument :
 BNA_N
 ClientSampleId :
 PB168696BL

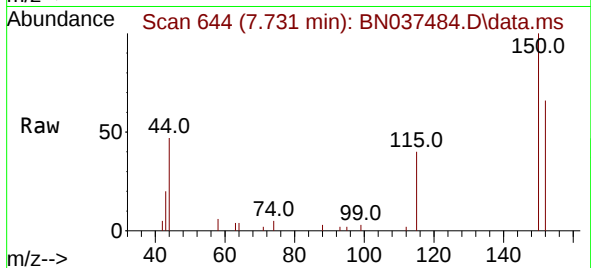

Tgt Ion:152 Resp: 2133




Ion	Ratio	Lower	Upper
152	100		
150	150.6	122.5	183.7
115	59.7	49.9	74.9

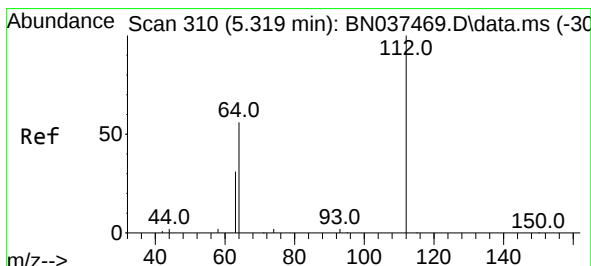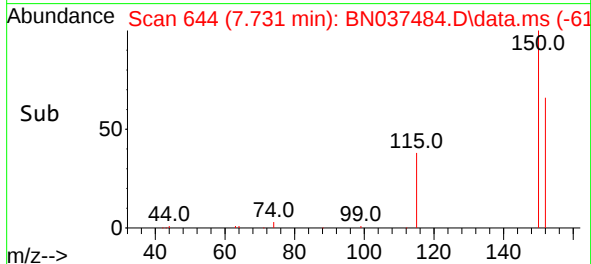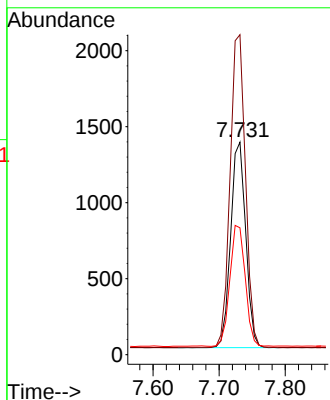


#4
 2-Fluorophenol
 Concen: 0.352 ng
 RT: 5.319 min Scan# 310
 Delta R.T. -0.000 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49

Tgt Ion:112 Resp: 1749

Ion	Ratio	Lower	Upper
112	100		
64	57.4	45.4	68.0
63	31.6	24.7	37.1


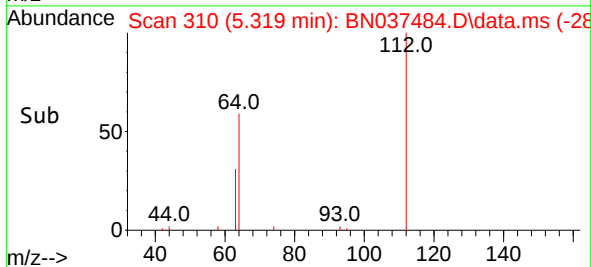
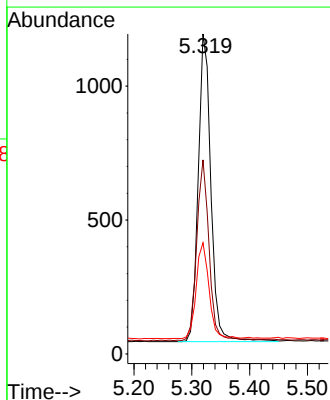
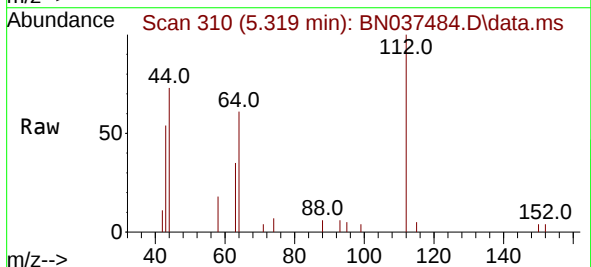


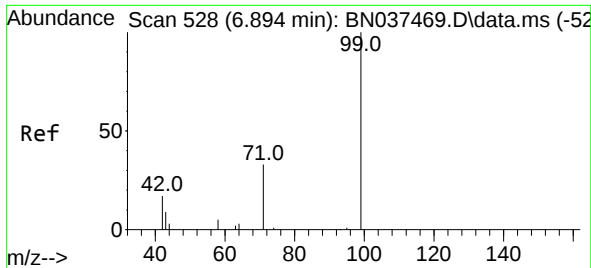

#5
Phenol-d6
Concen: 0.335 ng
RT: 6.886 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN037484.D
Acq: 14 Jul 2025 09:49




Instrument :
BNA_N
ClientSampleId :
PB168696BL


Tgt Ion:	99	Resp:	2094
Ion	Ratio	Lower	Upper
99	100		
42	23.6	19.5	29.3
71	38.2	29.4	44.2

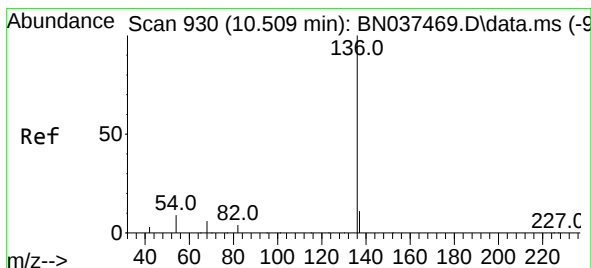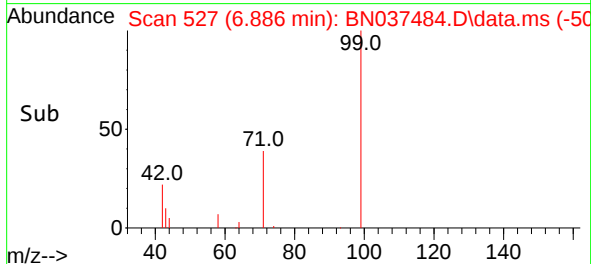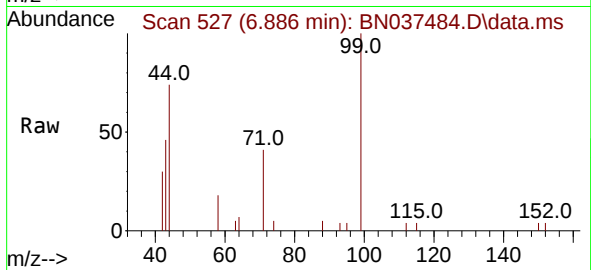

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.509 min Scan# 930
Delta R.T. -0.000 min
Lab File: BN037484.D
Acq: 14 Jul 2025 09:49

Tgt Ion:	136	Resp:	4972
Ion	Ratio	Lower	Upper
136	100		
137	12.4	10.0	15.0
54	9.2	9.0	13.6
68	6.1	6.1	9.1


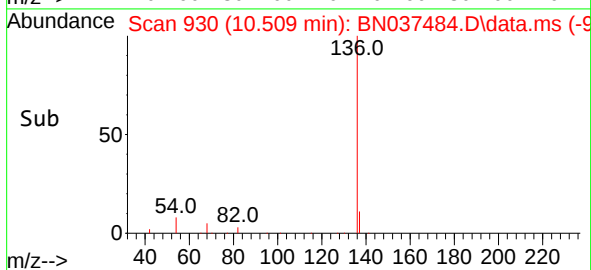

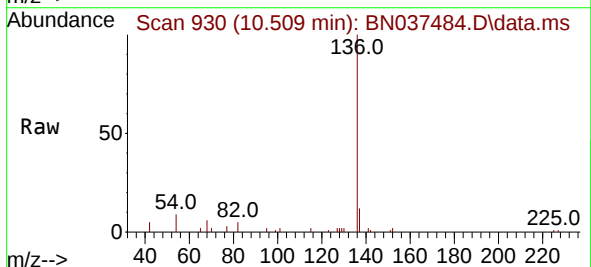


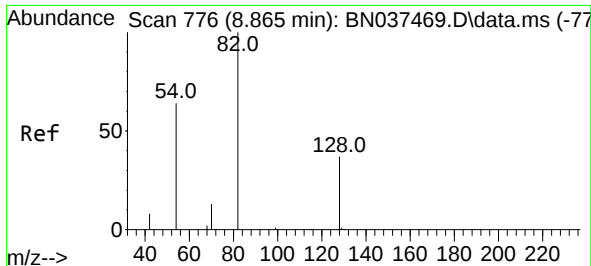

#8
 Nitrobenzene-d5
 Concen: 0.369 ng
 RT: 8.864 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49




Instrument :
 BNA_N
 ClientSampleId :
 PB168696BL


Tgt Ion: 82 Resp: 1333
 Ion Ratio Lower Upper
 82 100
 128 41.3 33.1 49.7
 54 61.9 53.0 79.4

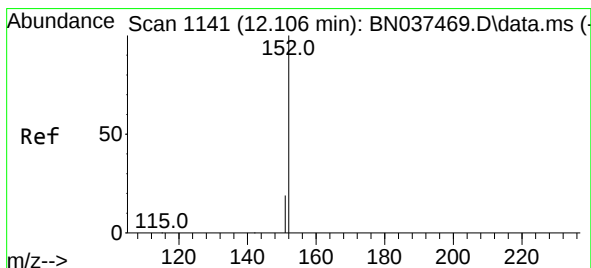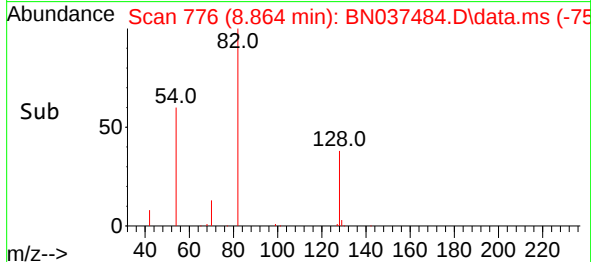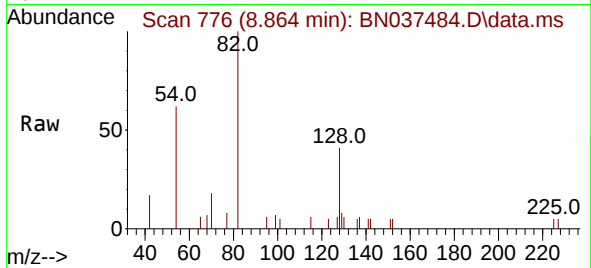

#11
 2-Methylnaphthalene-d10
 Concen: 0.356 ng
 RT: 12.101 min Scan# 1140
 Delta R.T. -0.005 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49

Tgt Ion: 152 Resp: 2408
 Ion Ratio Lower Upper
 152 100
 151 21.3 17.0 25.6


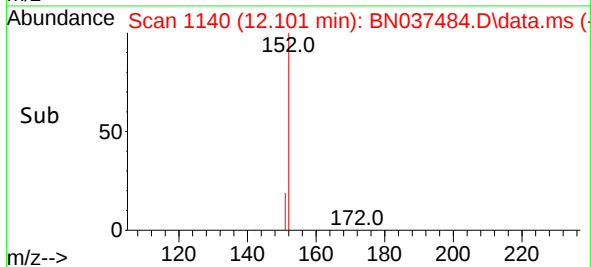

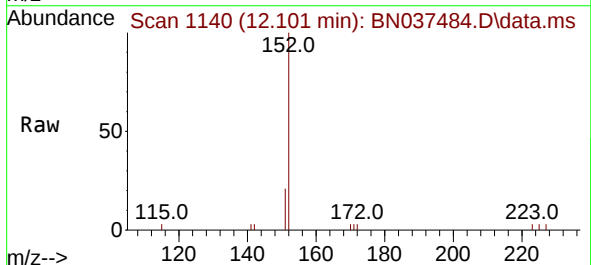


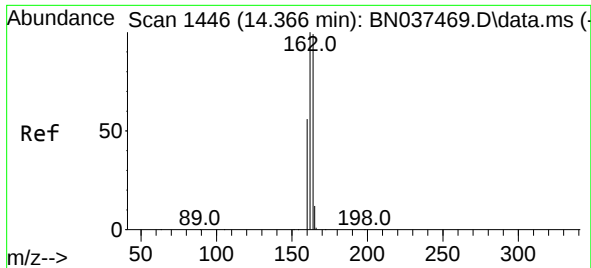

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.355 min Scan# 1445
 Delta R.T. -0.011 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49




Instrument :
 BNA_N
 ClientSampleId :
 PB168696BL


Tgt Ion:164 Resp: 2255
 Ion Ratio Lower Upper
 164 100
 162 104.3 81.1 121.7
 160 59.8 46.5 69.7

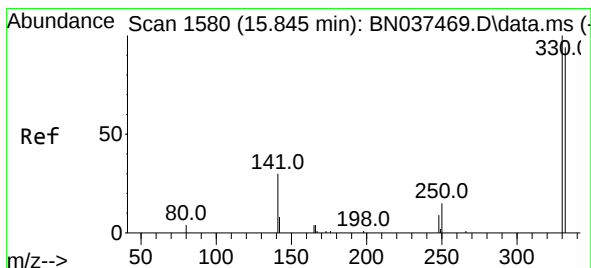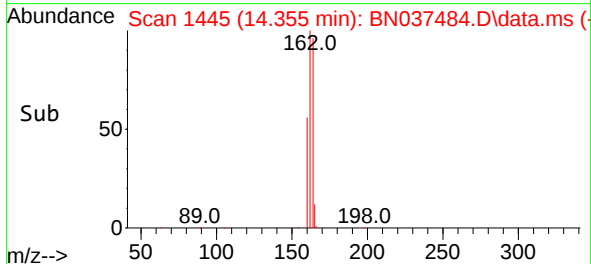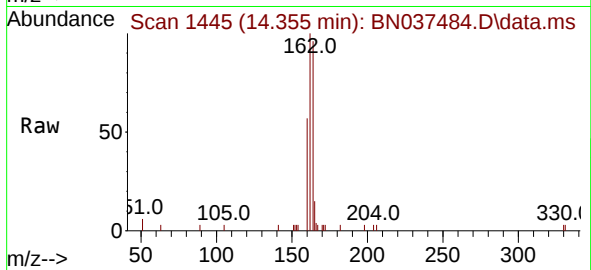

#14
 2,4,6-Tribromophenol
 Concen: 0.143 ng
 RT: 15.845 min Scan# 1580
 Delta R.T. -0.000 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49

Tgt Ion:330 Resp: 109
 Ion Ratio Lower Upper
 330 100
 332 99.1 82.0 123.0
 141 49.5 36.2 54.2


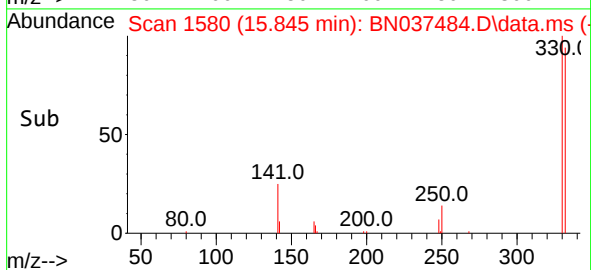

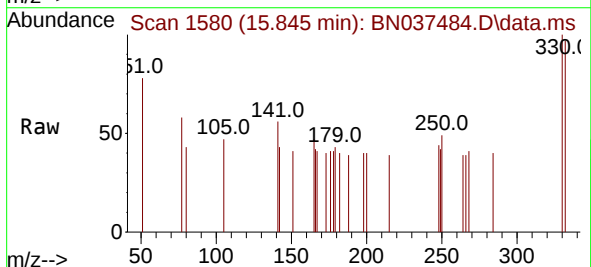


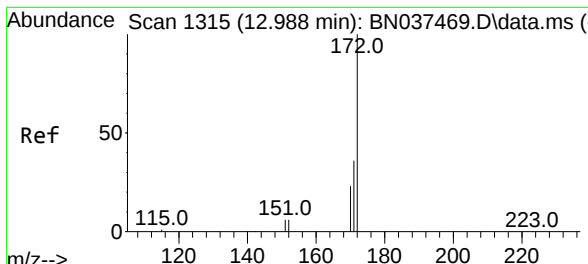

#15
2-Fluorobiphenyl
Concen: 0.379 ng
RT: 12.988 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN037484.D
Acq: 14 Jul 2025 09:49




Instrument :
BNA_N
ClientSampleId :
PB168696BL


Tgt Ion:172	Resp:	4883
Ion Ratio	Lower	Upper
172	100	
171	36.4	29.8 44.8
170	23.9	20.0 30.0

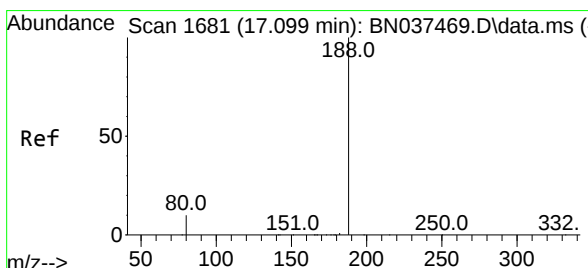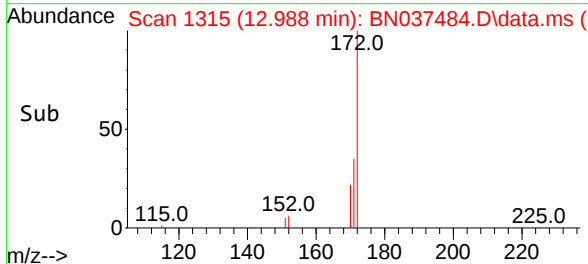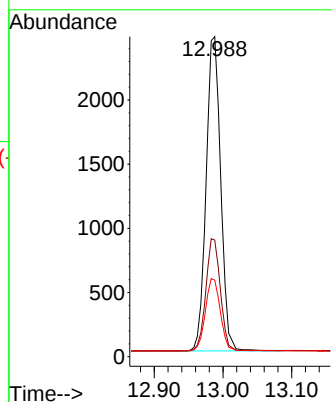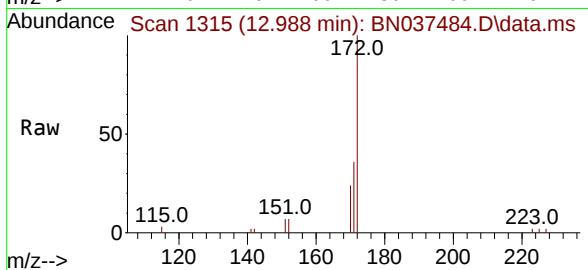

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.099 min Scan# 1681
Delta R.T. -0.000 min
Lab File: BN037484.D
Acq: 14 Jul 2025 09:49

Tgt Ion:188	Resp:	3944
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	9.6	9.3 13.9


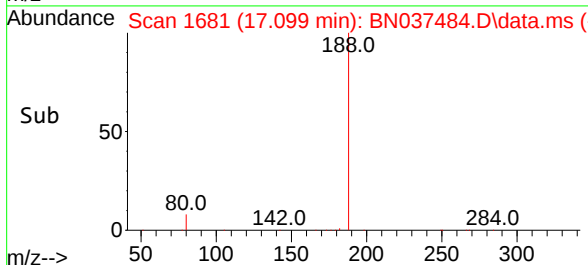

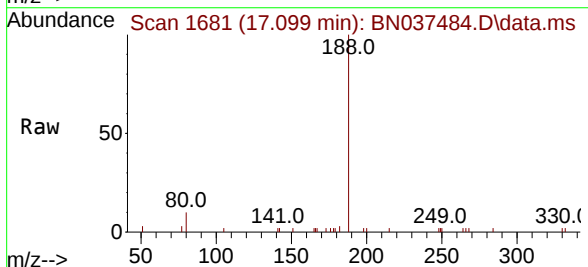


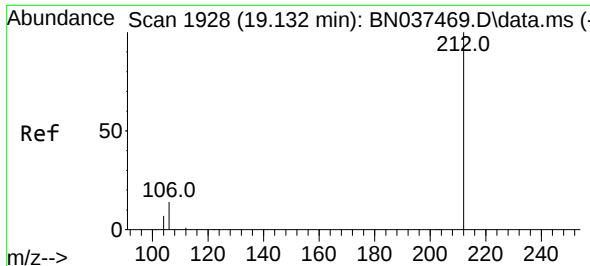

#27
Fluoranthene-d10
Concen: 0.351 ng
RT: 19.132 min Scan# 1928
Delta R.T. -0.000 min
Lab File: BN037484.D
Acq: 14 Jul 2025 09:49




Instrument :
BNA_N
ClientSampleId :
PB168696BL


Tgt Ion:212 Resp: 3492
Ion Ratio Lower Upper
212 100
106 13.8 11.7 17.5
104 8.2 6.6 10.0

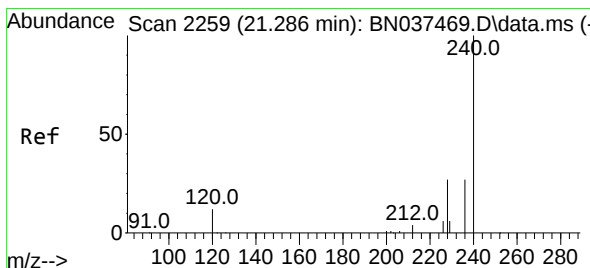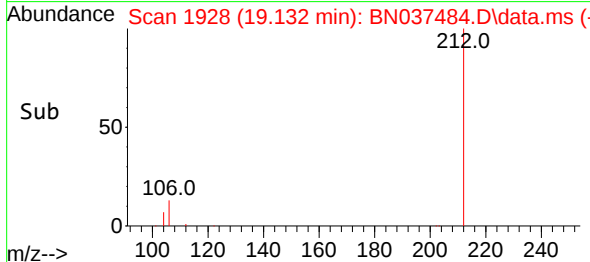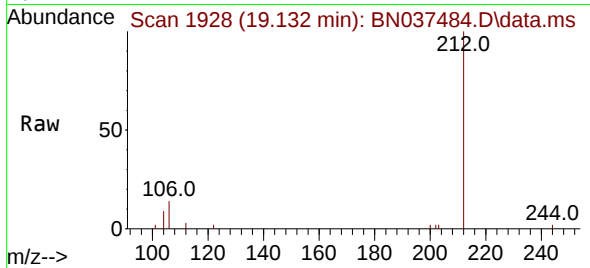

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.286 min Scan# 2259
Delta R.T. -0.000 min
Lab File: BN037484.D
Acq: 14 Jul 2025 09:49

Tgt Ion:240 Resp: 2959
Ion Ratio Lower Upper
240 100
120 13.0 12.4 18.6
236 28.3 22.9 34.3


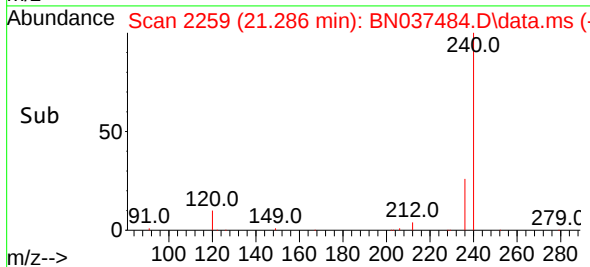

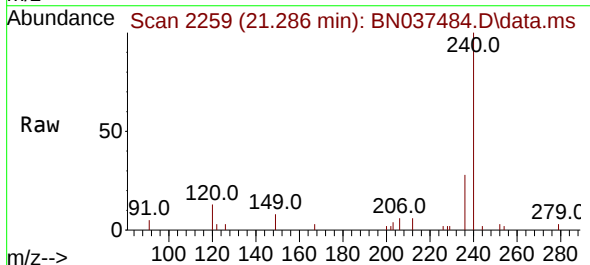


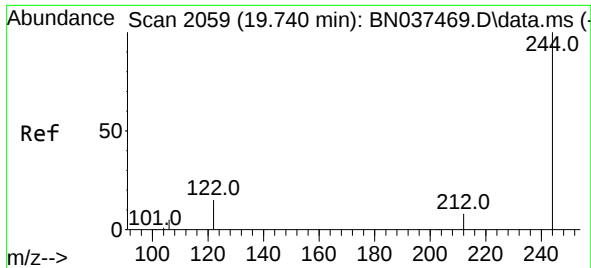

#31
 Terphenyl-d14
 Concen: 0.417 ng
 RT: 19.736 min Scan# 2058
 Delta R.T. -0.005 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49




Instrument :
 BNA_N
 ClientSampleId :
 PB168696BL


Tgt Ion:244 Resp: 2573
 Ion Ratio Lower Upper
 244 100
 212 10.6 8.7 13.1
 122 17.9 14.1 21.1

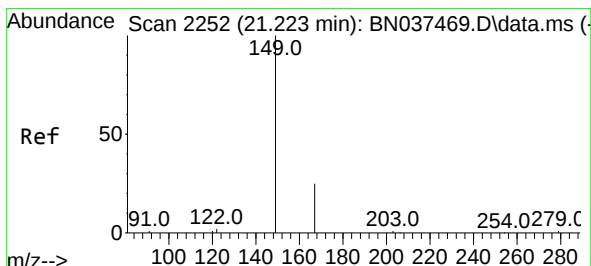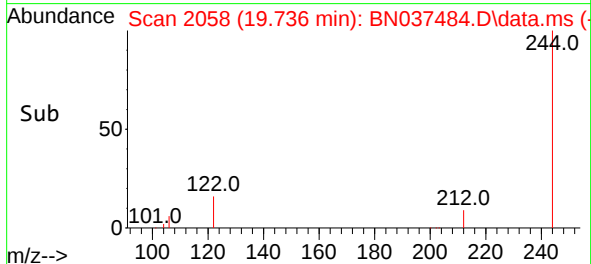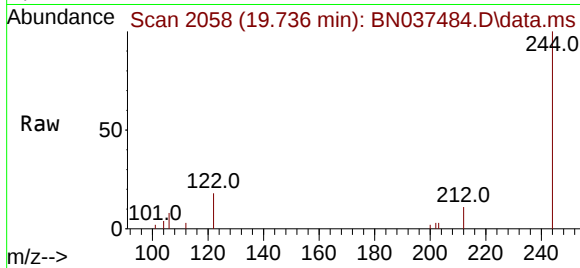

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.021 ng
 RT: 21.214 min Scan# 2251
 Delta R.T. -0.009 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49

Tgt Ion:149 Resp: 71
 Ion Ratio Lower Upper
 149 100
 167 16.9 19.4 29.2#
 279 12.7 2.5 3.7#

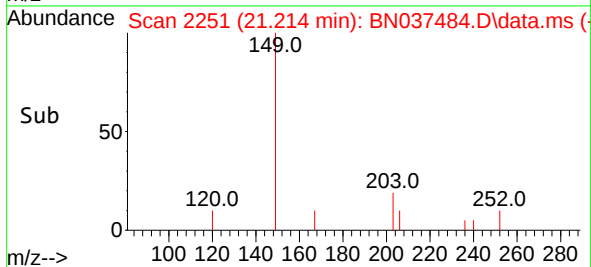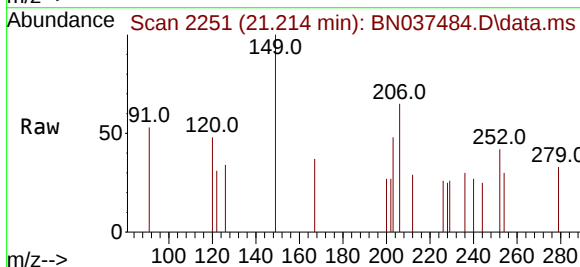

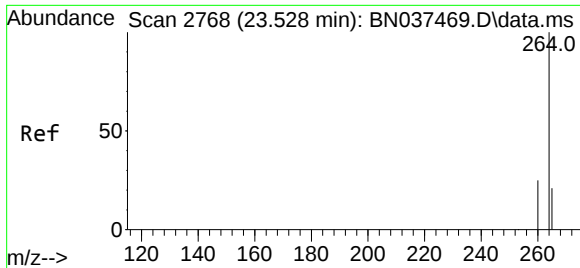

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.525 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: BN037484.D
 Acq: 14 Jul 2025 09:49

Instrument :
 BNA_N
 ClientSampleId :
 PB168696BL

Tgt Ion:	264	Resp:	2878
Ion Ratio	Lower	Upper	
264	100		
260	27.5	21.7	32.5
265	54.0	41.6	62.4

