

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071519\
 Data File : BN006846.D
 Acq On : 15 Jul 2019 13:10
 Operator : HP/JU
 Sample : K3762-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF487

Manual Integrations
 APPROVED

mohammad
 7/16/2019 8:37:52 AM

Quant Time: Jul 15 14:58:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3014	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10917	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5631	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	12356m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	10143m	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	9193m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	4040	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	11443m	0.32	ng/ul	0.00
Target Compounds						
13) Anthracene	17.13	178	1958m	0.057	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071519\
Data File : BN006846.D
Acq On : 15 Jul 2019 13:10
Operator : HP/JU
Sample : K3762-05
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BF487

Manual Integrations
APPROVED

mohammad
7/16/2019 8:37:52 AM

Quant Time: Jul 15 14:58:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

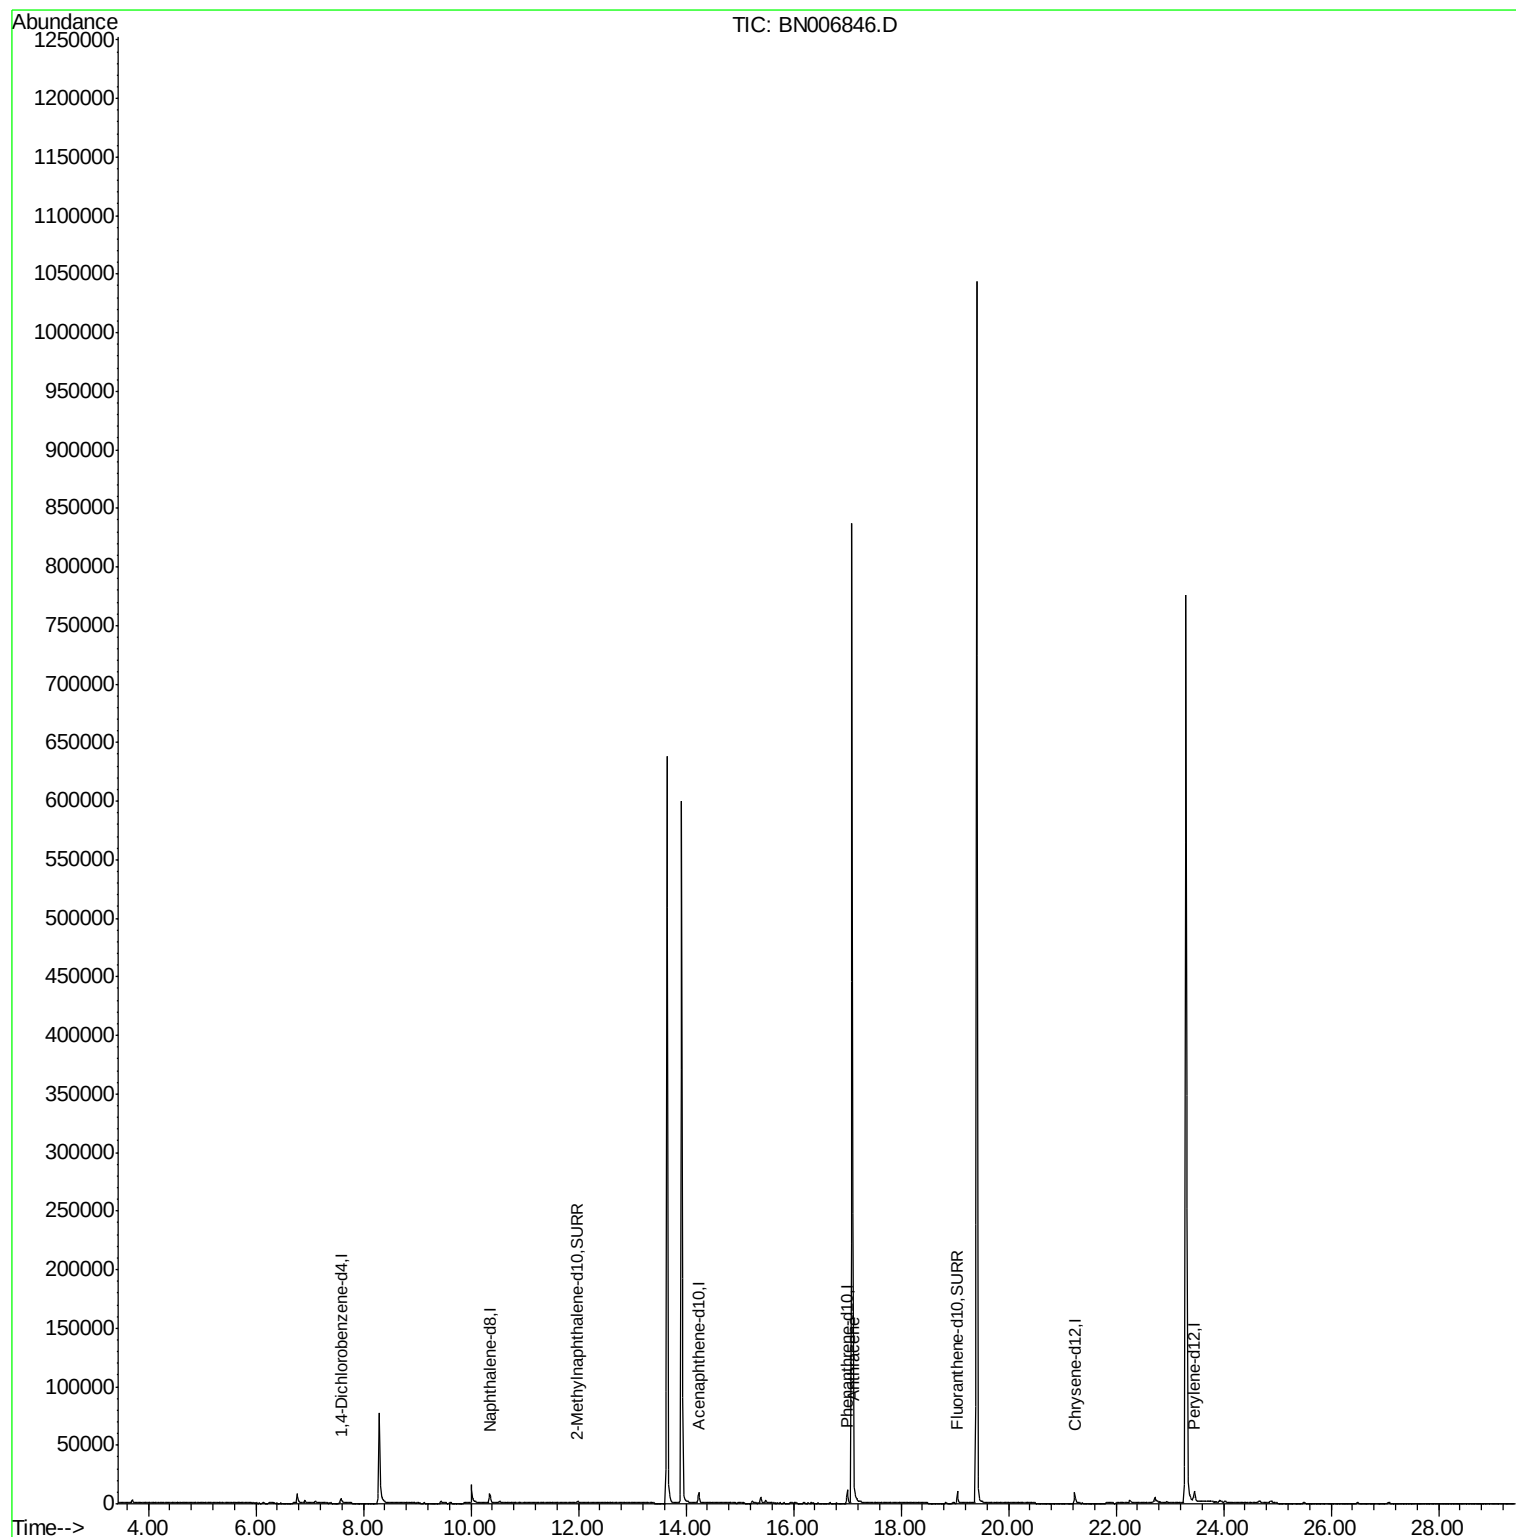

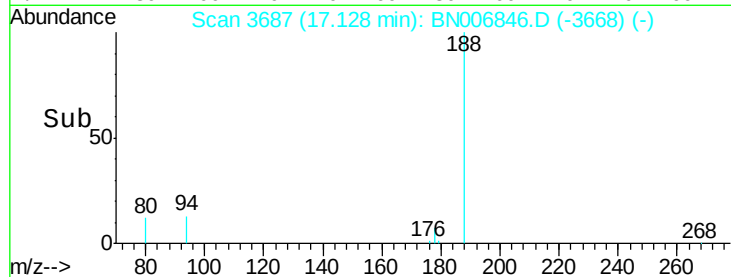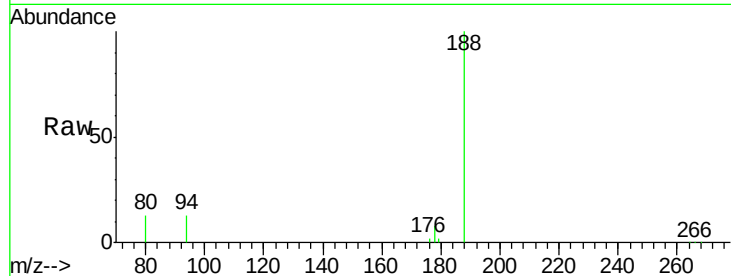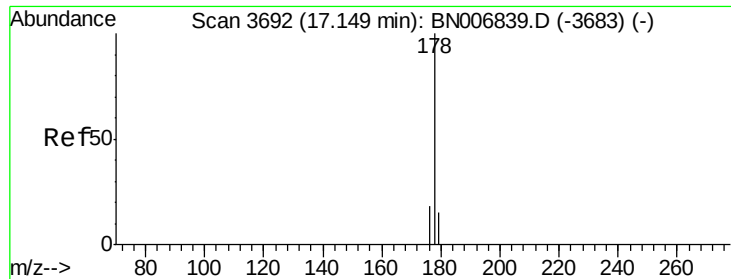

#13

Anthracene

Concen: 0.057 ng/ul m

RT: 17.13 min Scan# 3687

Delta R.T. -0.02 min

Lab File: BN006846.D

Acq: 15 Jul 2019 13:10

Instrument :

BNA_N

ClientSampleId :

BF487

Tgt Ion	Ratio	Lower	Upper
178	100		
179	22.8	12.7	19.1#
176	24.4	15.8	23.6#

Manual Integrations
APPROVED

mohammad
7/16/2019 8:37:52 AM

