

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071519\
 Data File : BN006847.D
 Acq On : 15 Jul 2019 13:45
 Operator : HP/JU
 Sample : K3762-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF488

Manual Integrations
 APPROVED

mohammad
 7/16/2019 8:37:56 AM

Quant Time: Jul 15 14:40:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2840	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10133	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5319	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	11487m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	8682m	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	8190m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	4314	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	11011m	0.33	ng/ul	0.00
Target Compounds						
13) Anthracene	17.13	178	2708m	0.085	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071519\
Data File : BN006847.D
Acq On : 15 Jul 2019 13:45
Operator : HP/JU
Sample : K3762-06
Misc :
ALS Vial : 10 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BF488

Manual Integrations
APPROVED

mohammad
7/16/2019 8:37:56 AM

Quant Time: Jul 15 14:40:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

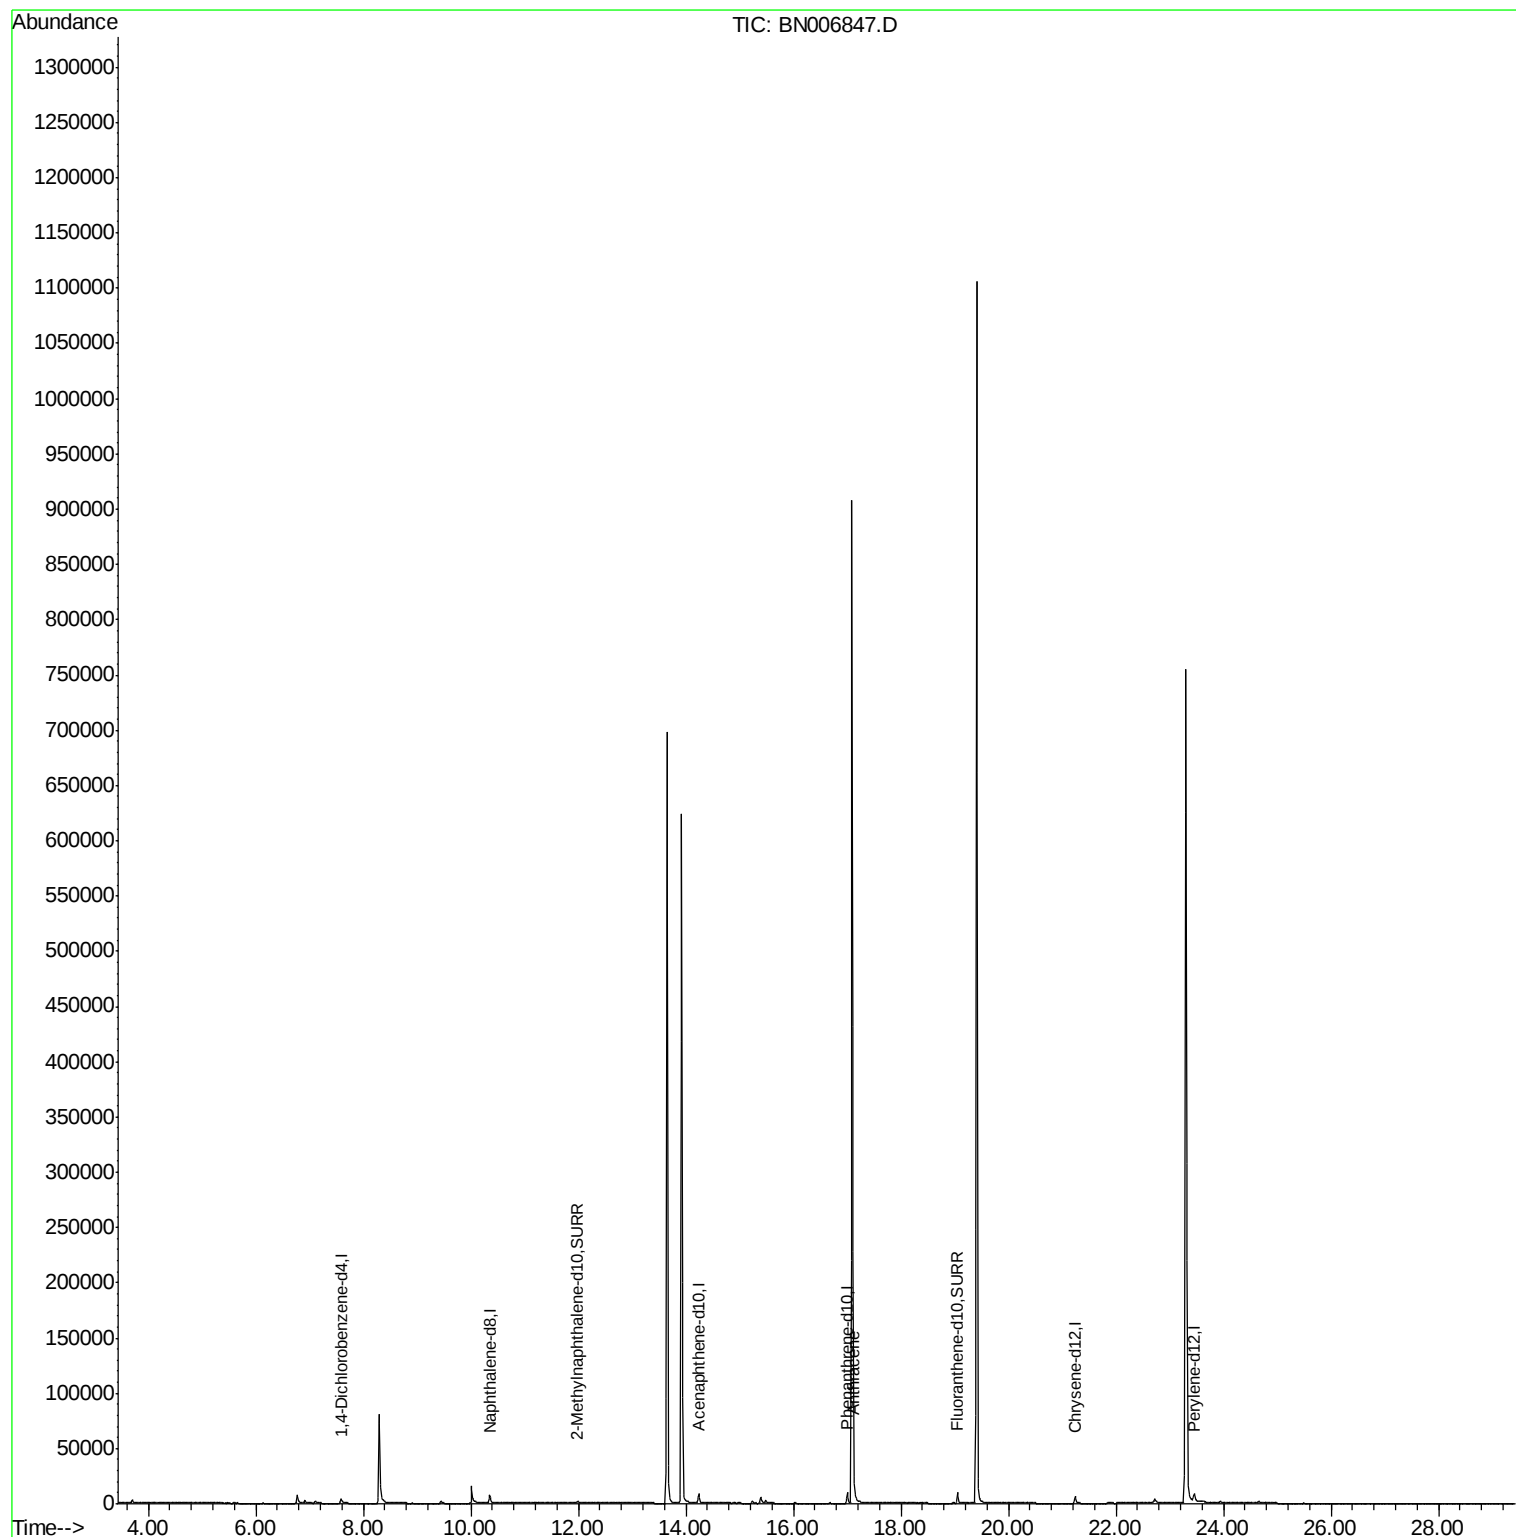

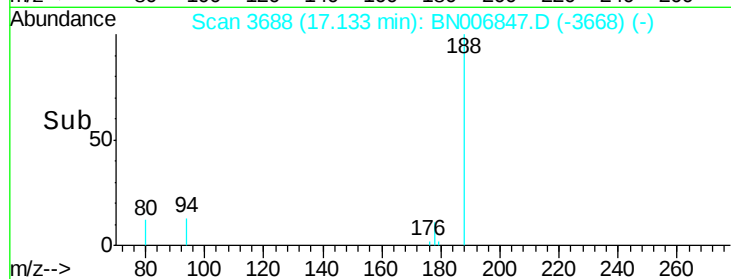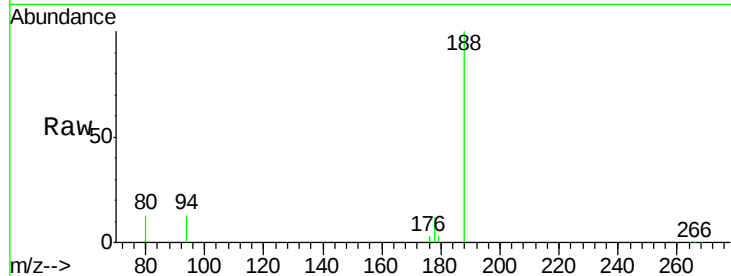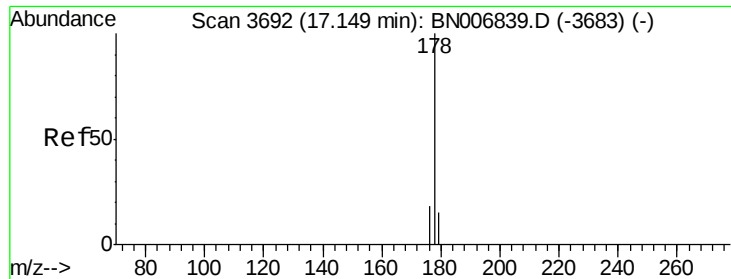

#13

Anthracene

Concen: 0.085 ng/ul m

RT: 17.13 min Scan# 3688

Delta R.T. -0.02 min

Lab File: BN006847.D

Acq: 15 Jul 2019 13:45

Instrument :

BNA_N

ClientSampleId :

BF488

Tgt Ion:178 Resp: 2708

Ion Ratio Lower Upper

178 100

179 21.1 12.7 19.1#

176 22.7 15.8 23.6

Manual Integrations

APPROVED

mohammad

7/16/2019 8:37:56 AM

