
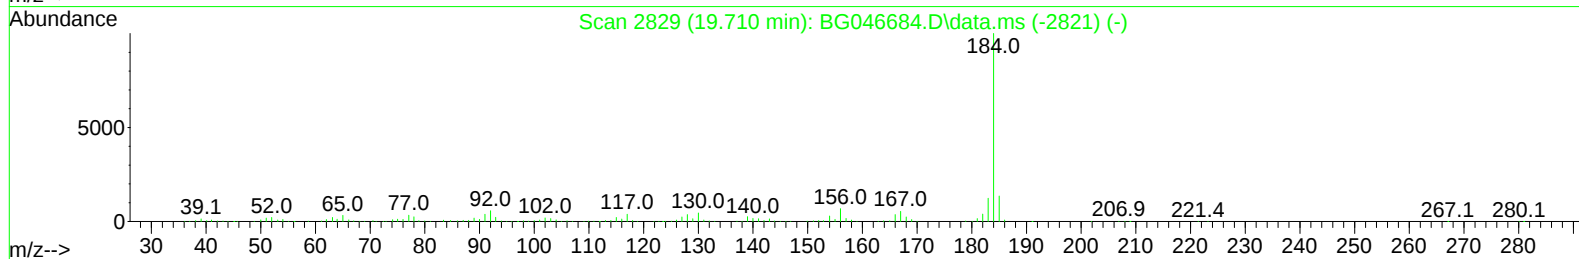
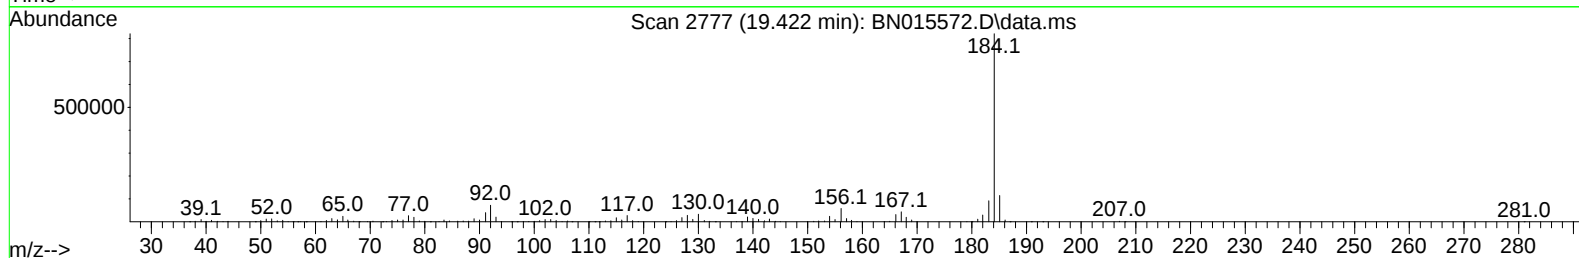


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071521\
Data File : BN015572.D
Acq On : 15 Jul 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 11:00:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

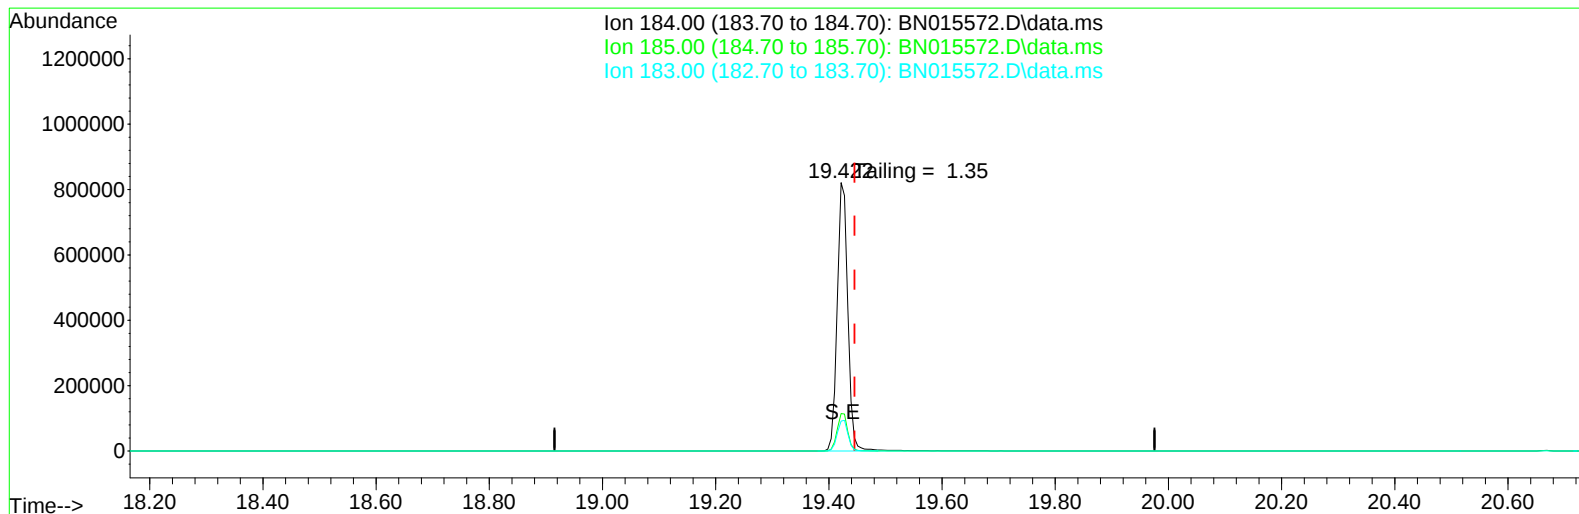

TIC: BN015572.D\data.ms

(77) Benzidine




19.422min (-0.024) 0.00 ng

response 1073956

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	11.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071521\
Data File : BN015572.D
Acq On : 15 Jul 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 11:00:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

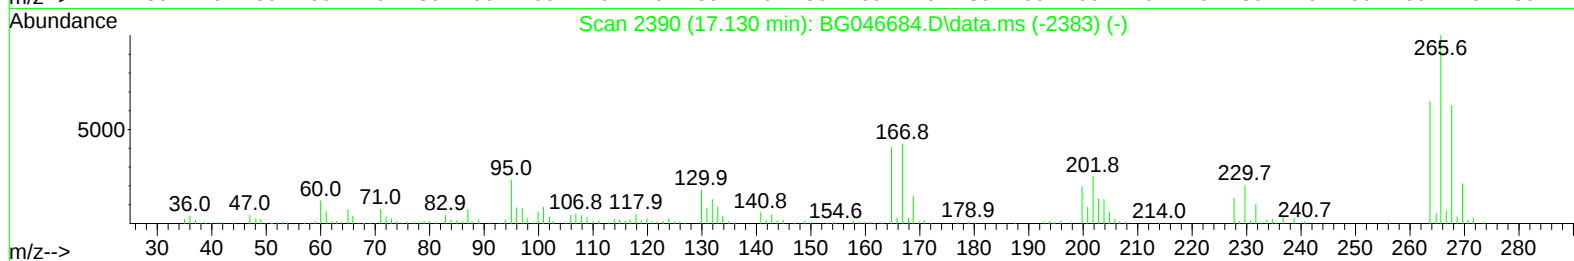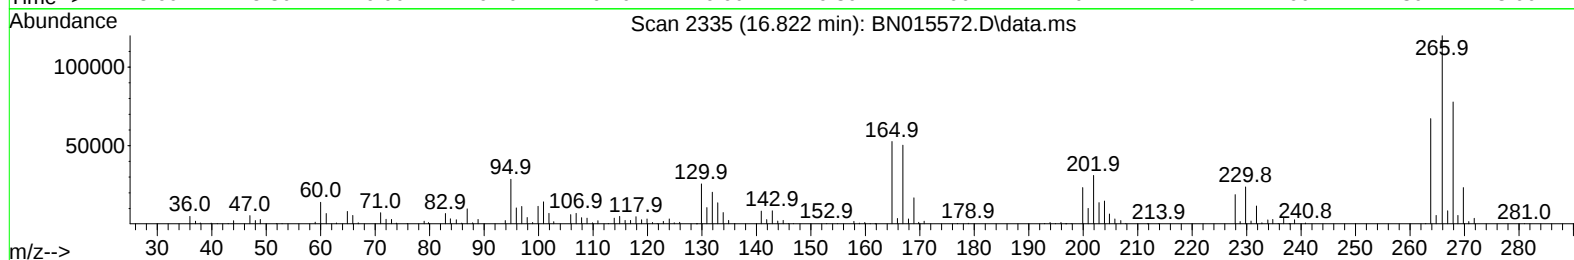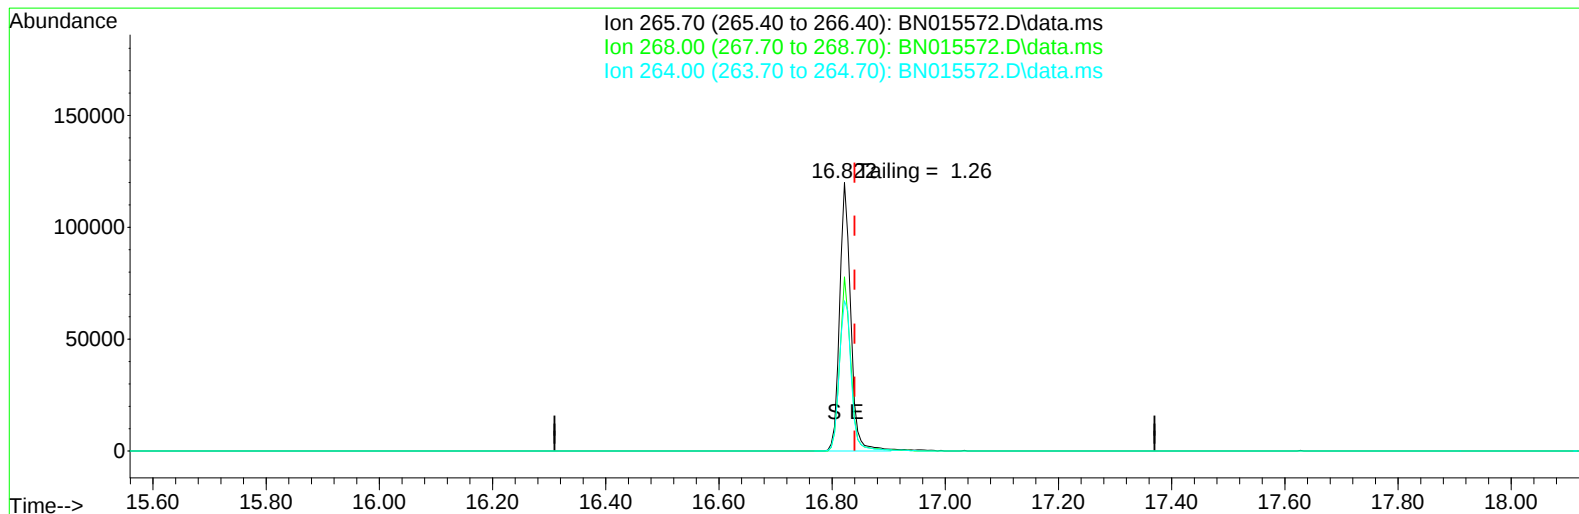

TIC: BN015572.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.018) 23370.58 ng

response 164699

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.89
264.00	61.60	56.01
0.00	0.00	0.00