
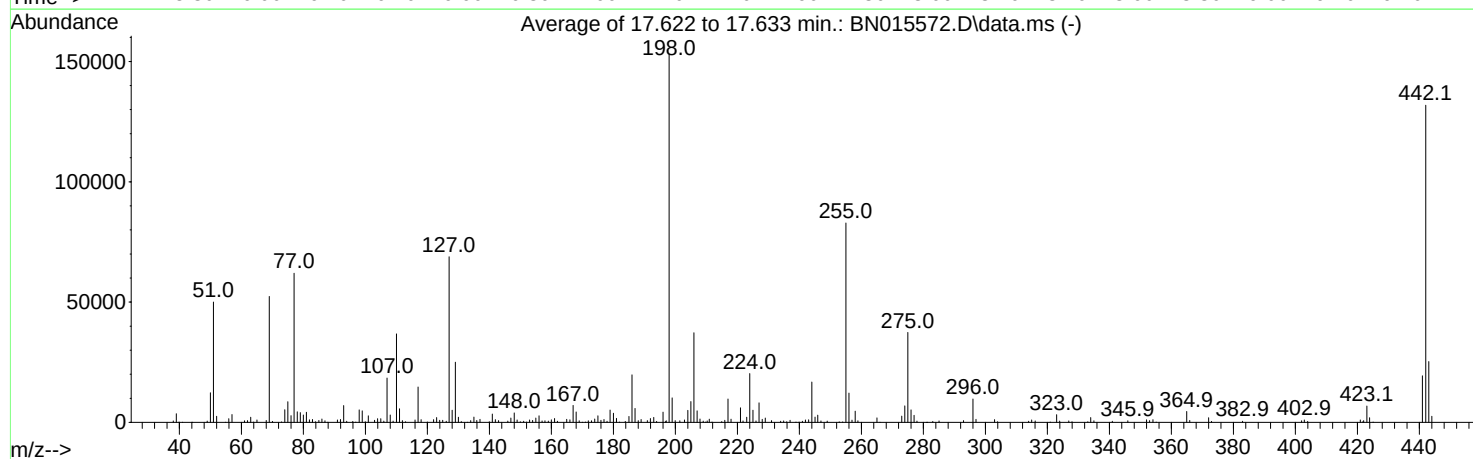


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN071521\  
 Data File : BN015572.D  
 Acq On : 15 Jul 2021 09:47  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN071521.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jul 15 15:46:51 2021

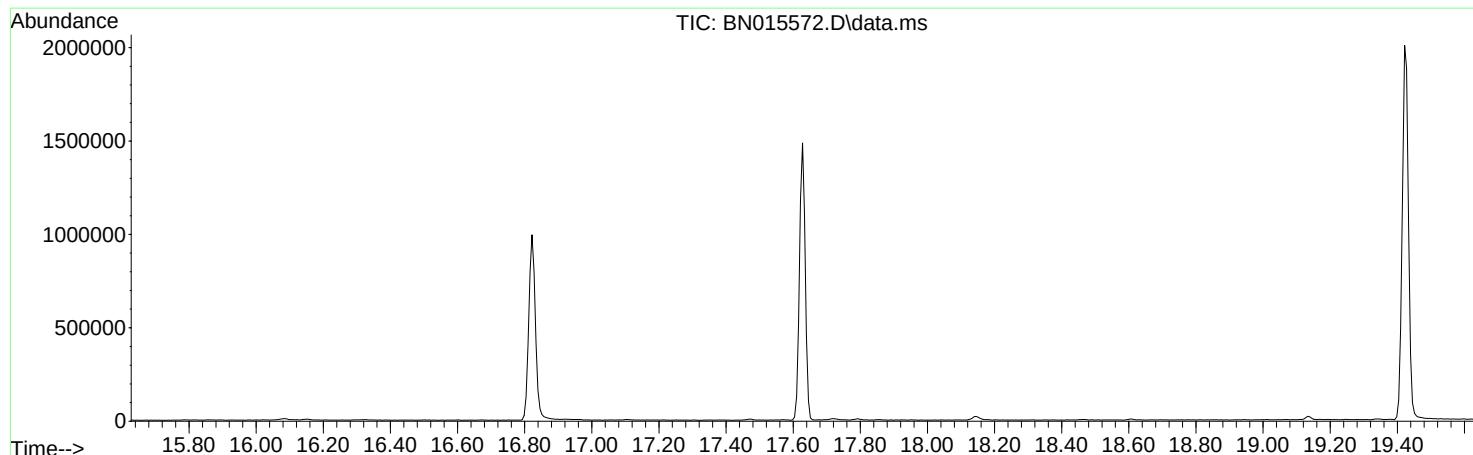




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.7         | 50011      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 831        | PASS                |
| 69             | 198             | 0.00            | 100             | 34.2         | 52344      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.8          | 397        | PASS                |
| 127            | 198             | 10              | 80              | 45.0         | 68829      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 696        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 152917     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 10167      | PASS                |
| 275            | 198             | 10              | 60              | 24.4         | 37376      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 4551       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.7         | 19360      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 131813     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 25251      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN071521\  
Data File : BN015572.D  
Acq On : 15 Jul 2021 09:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jul 15 11:00:58 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 15 05:41:44 2021  
Response via : Initial Calibration

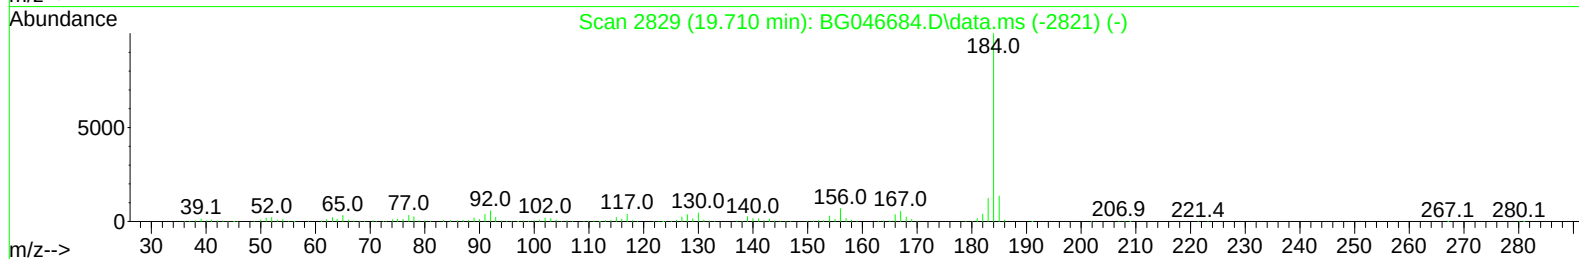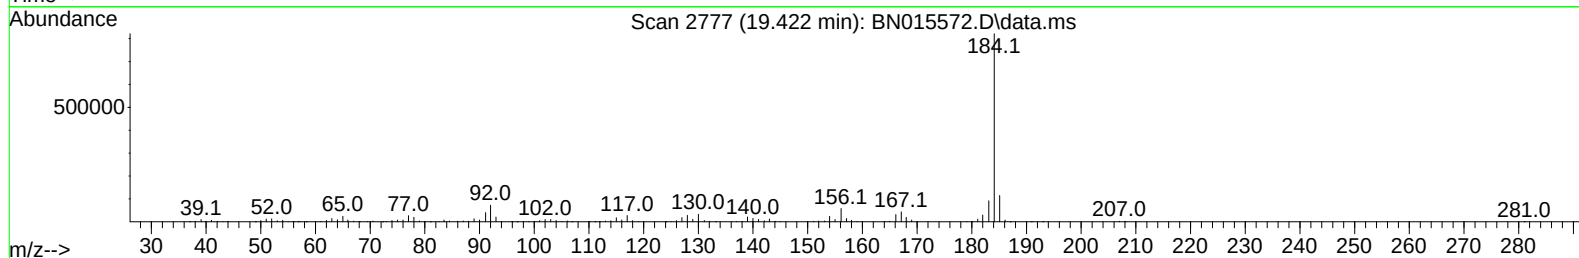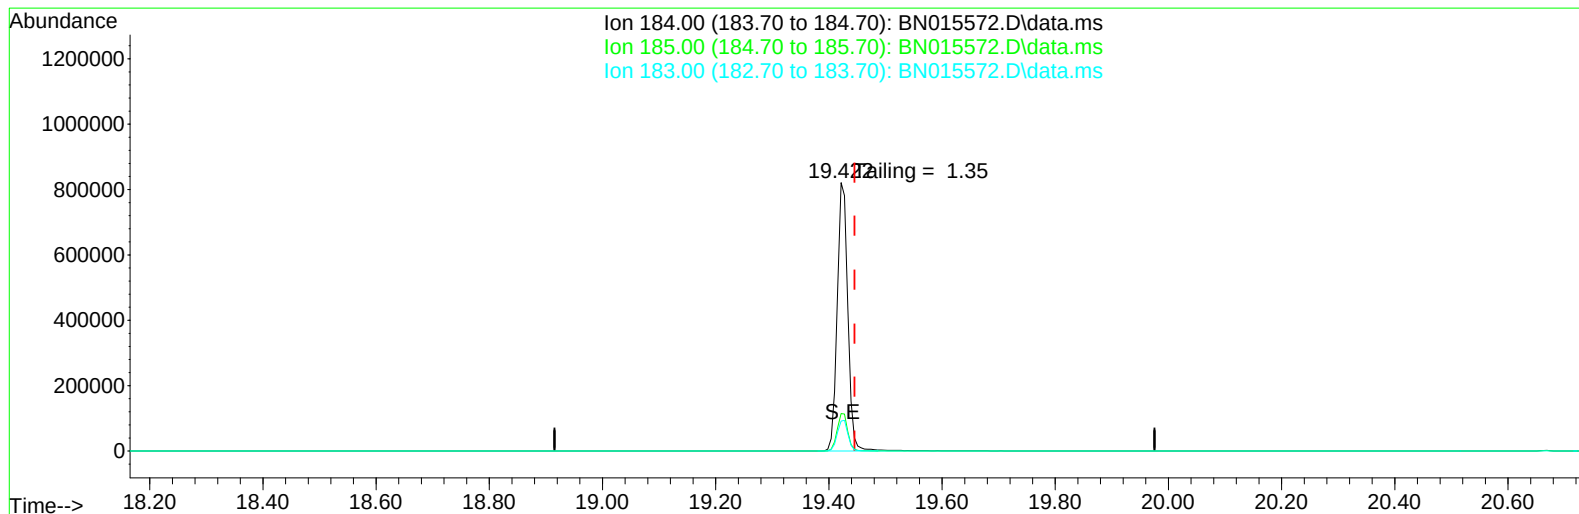

TIC: BN015572.D\data.ms

**(77) Benzidine**

19.422min (-0.024) 0.00 ng




response 1073956

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.96  |
| 183.00 | 13.20  | 11.16  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN071521\  
 Data File : BN015572.D  
 Acq On : 15 Jul 2021 09:47  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Jul 15 11:00:58 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jul 15 05:41:44 2021  
 Response via : Initial Calibration

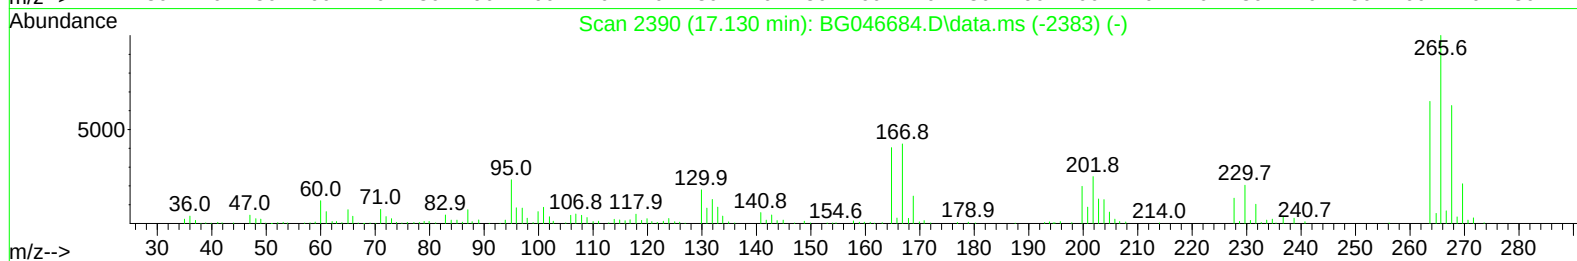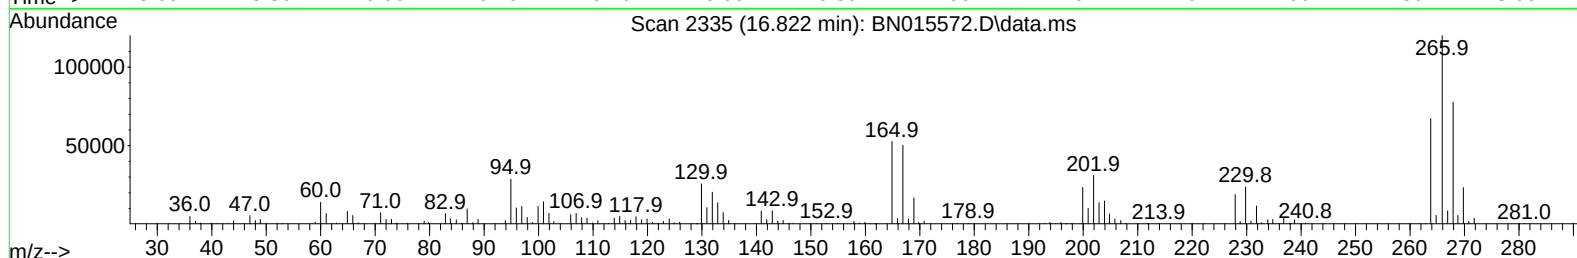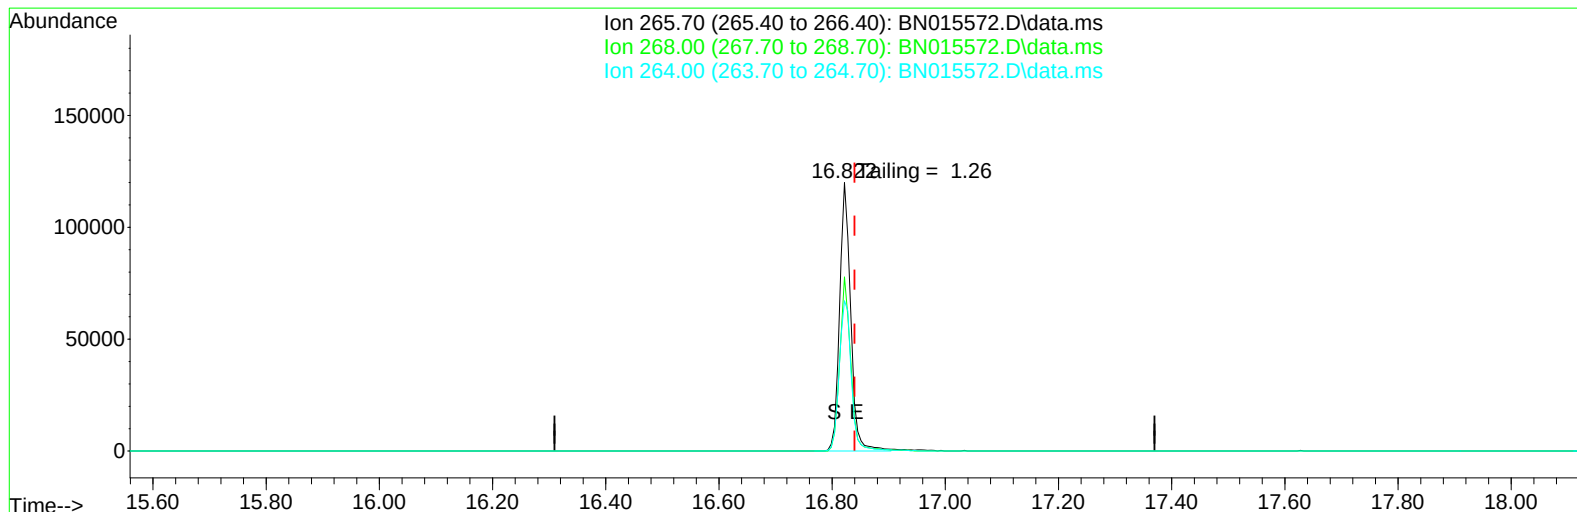

TIC: BN015572.D\data.ms

**(70) Pentachlorophenol (C)**

16.822min (-0.018) 23370.58 ng

response 164699

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.89  |
| 264.00 | 61.60  | 56.01  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/15/2021     | BNA_N            | <u>BN015572.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 465081           | 20.66              |
| DDD           | 911              | 20.22              |
| DDE           | 670              | 19.71              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 1581          | 466662           | 0.34               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP