

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071523\
 Data File : BN026516.D
 Acq On : 15 Jul 2023 17:30
 Operator : MA/JU
 Sample : PB154014BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK014

Quant Time: Jul 16 00:55:11 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 01:53:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.947	152	2832	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.754	136	8859	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.584	164	5890	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	13477	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.523	240	10825	0.400	ng/ul	# 0.00
23) Perylene-d12	23.932	264	12337	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	26080	6.992	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	4769	0.396	ng/ul	0.00
18) Fluoranthene-d10	19.359	212	15775	0.420	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.721	202	2565	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.774	252	4952	0.116	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071523\
Data File : BN026516.D
Acq On : 15 Jul 2023 17:30
Operator : MA/JU
Sample : PB154014BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK014

Quant Time: Jul 16 00:55:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 01:53:23 2023
Response via : Initial Calibration




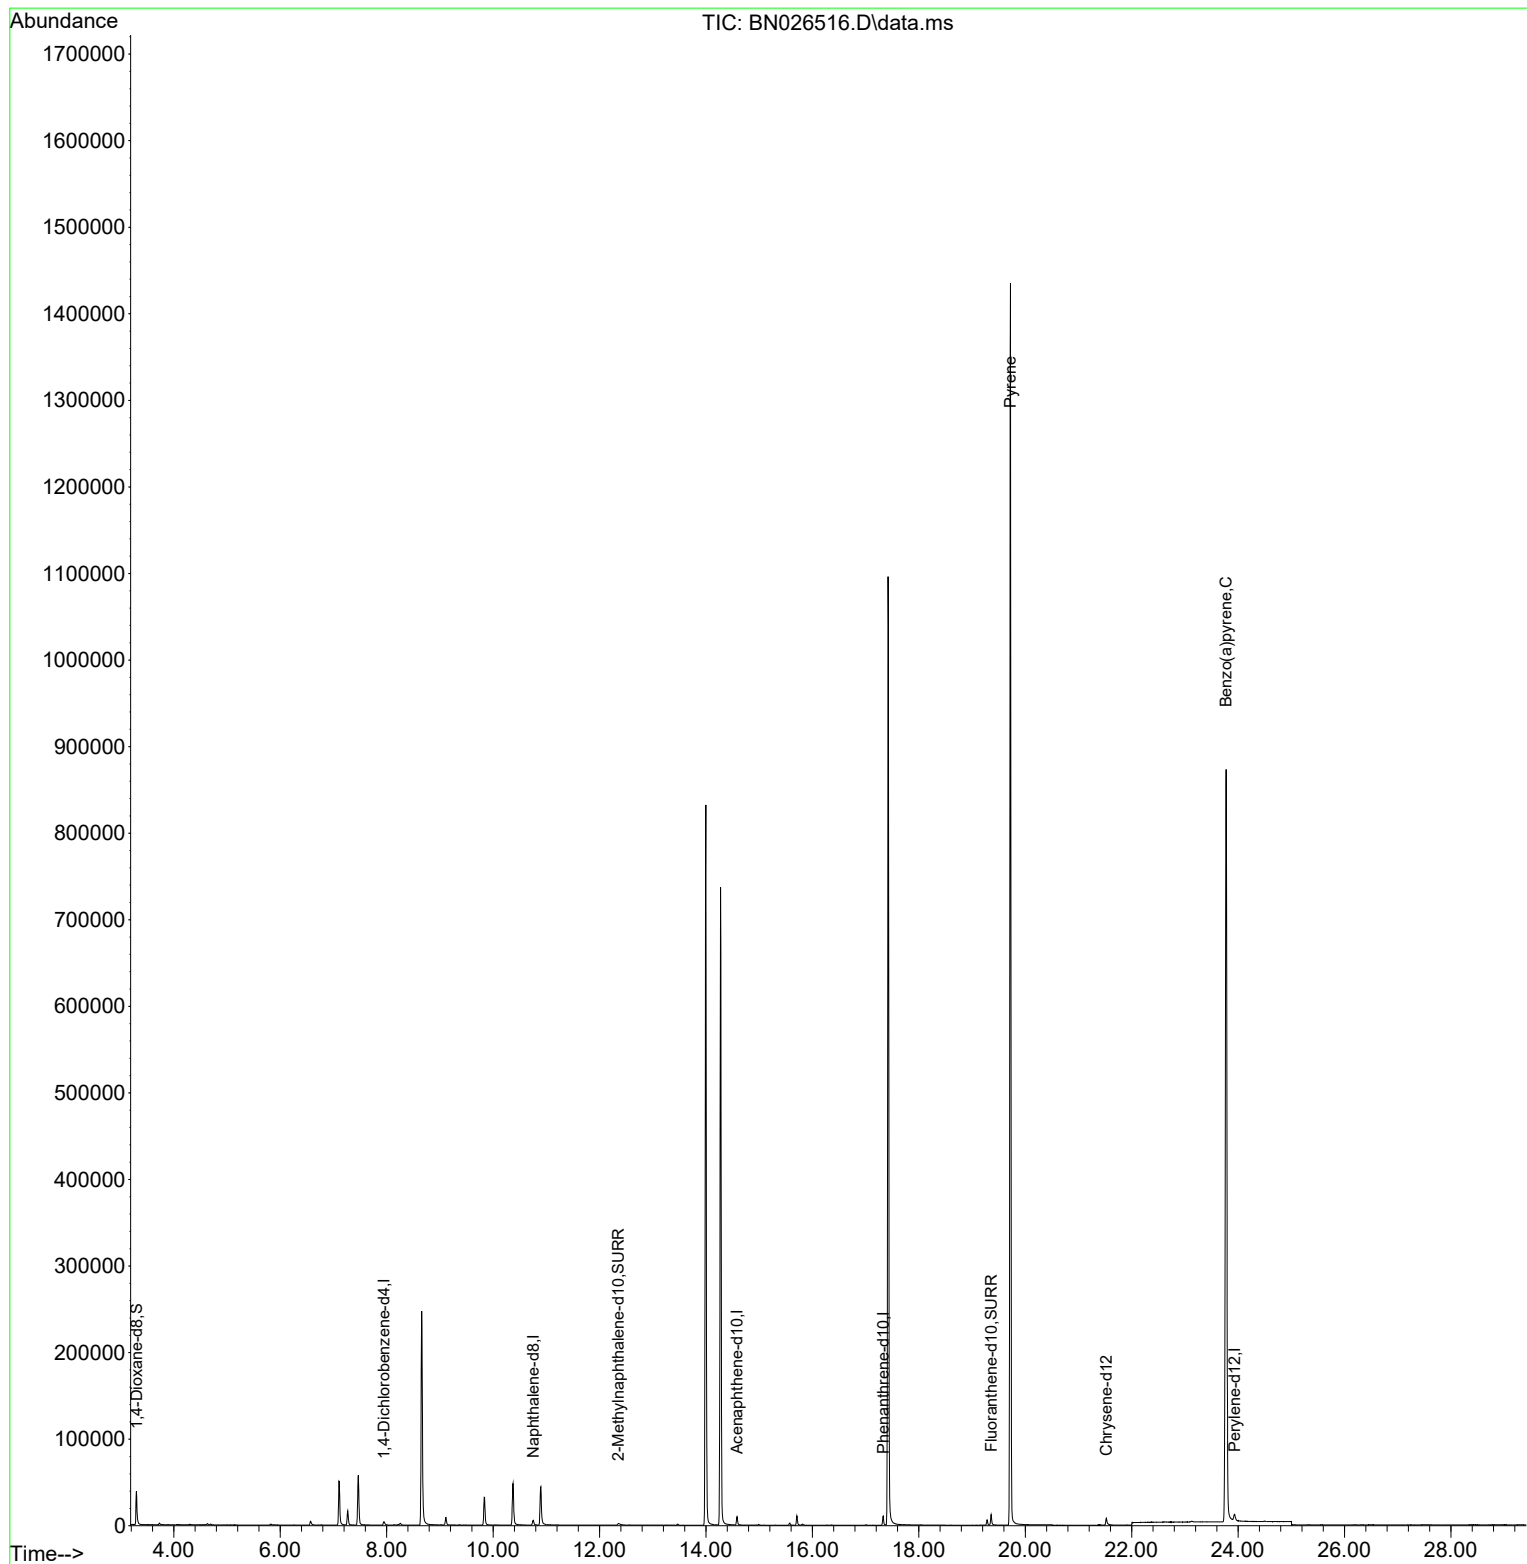


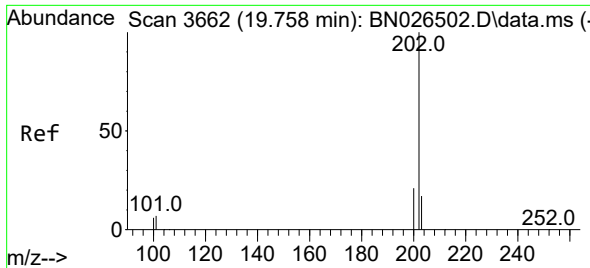

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.721 min Scan# 30
Delta R.T. -0.037 min
Lab File: BN026516.D
Acq: 15 Jul 2023 17:30

Instrument :
BNA_N
ClientSampleId :
SBLK014

Tgt Ion:202 Resp: 2565
Ion Ratio Lower Upper
202 100
101 194.7 8.0 12.0#
100 1565.5 6.2 9.2#

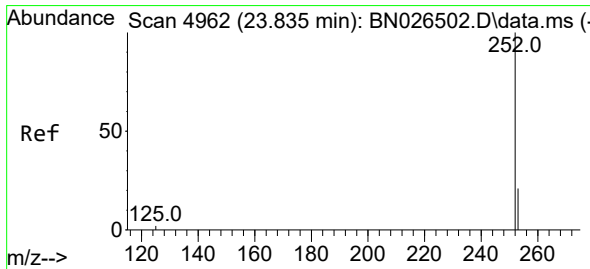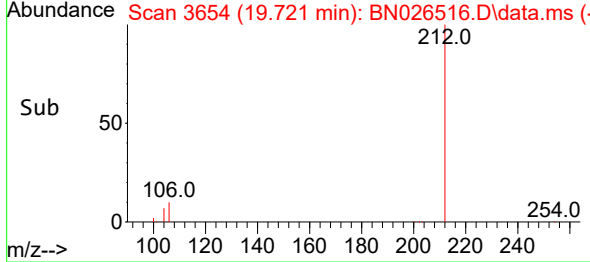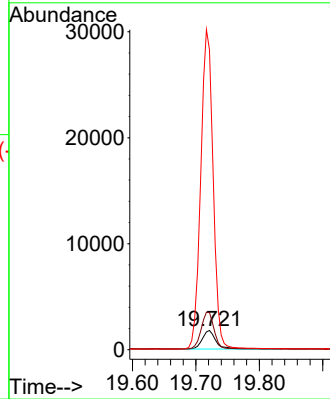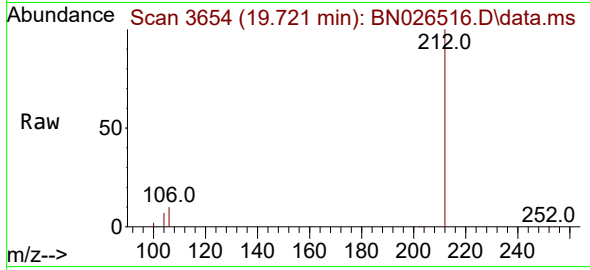

#26
Benzo(a)pyrene
Concen: 0.116 ng/ul
RT: 23.774 min Scan# 4941
Delta R.T. -0.061 min
Lab File: BN026516.D
Acq: 15 Jul 2023 17:30

Tgt Ion:252 Resp: 4952
Ion Ratio Lower Upper
252 100
253 53.3 32.6 49.0#
125 51.3 19.3 28.9#

