

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071523\
 Data File : BN026520.D
 Acq On : 15 Jul 2023 20:10
 Operator : MA/JU
 Sample : 03414-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4633

Quant Time: Jul 16 00:55:43 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 01:53:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	2624	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.748	136	8097	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.579	164	5470	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	12164	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	8915	0.400	ng/ul	# 0.00
23) Perylene-d12	23.928	264	8671	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	8699	2.517	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	1856	0.169	ng/ul	-0.01
18) Fluoranthene-d10	19.358	212	5042	0.163	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.797	128	6979	0.314	ng/ul	99
7) 2-Methylnaphthalene	12.414	142	324	0.026	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071523\
Data File : BN026520.D
Acq On : 15 Jul 2023 20:10
Operator : MA/JU
Sample : 03414-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4633

Quant Time: Jul 16 00:55:43 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 01:53:23 2023
Response via : Initial Calibration

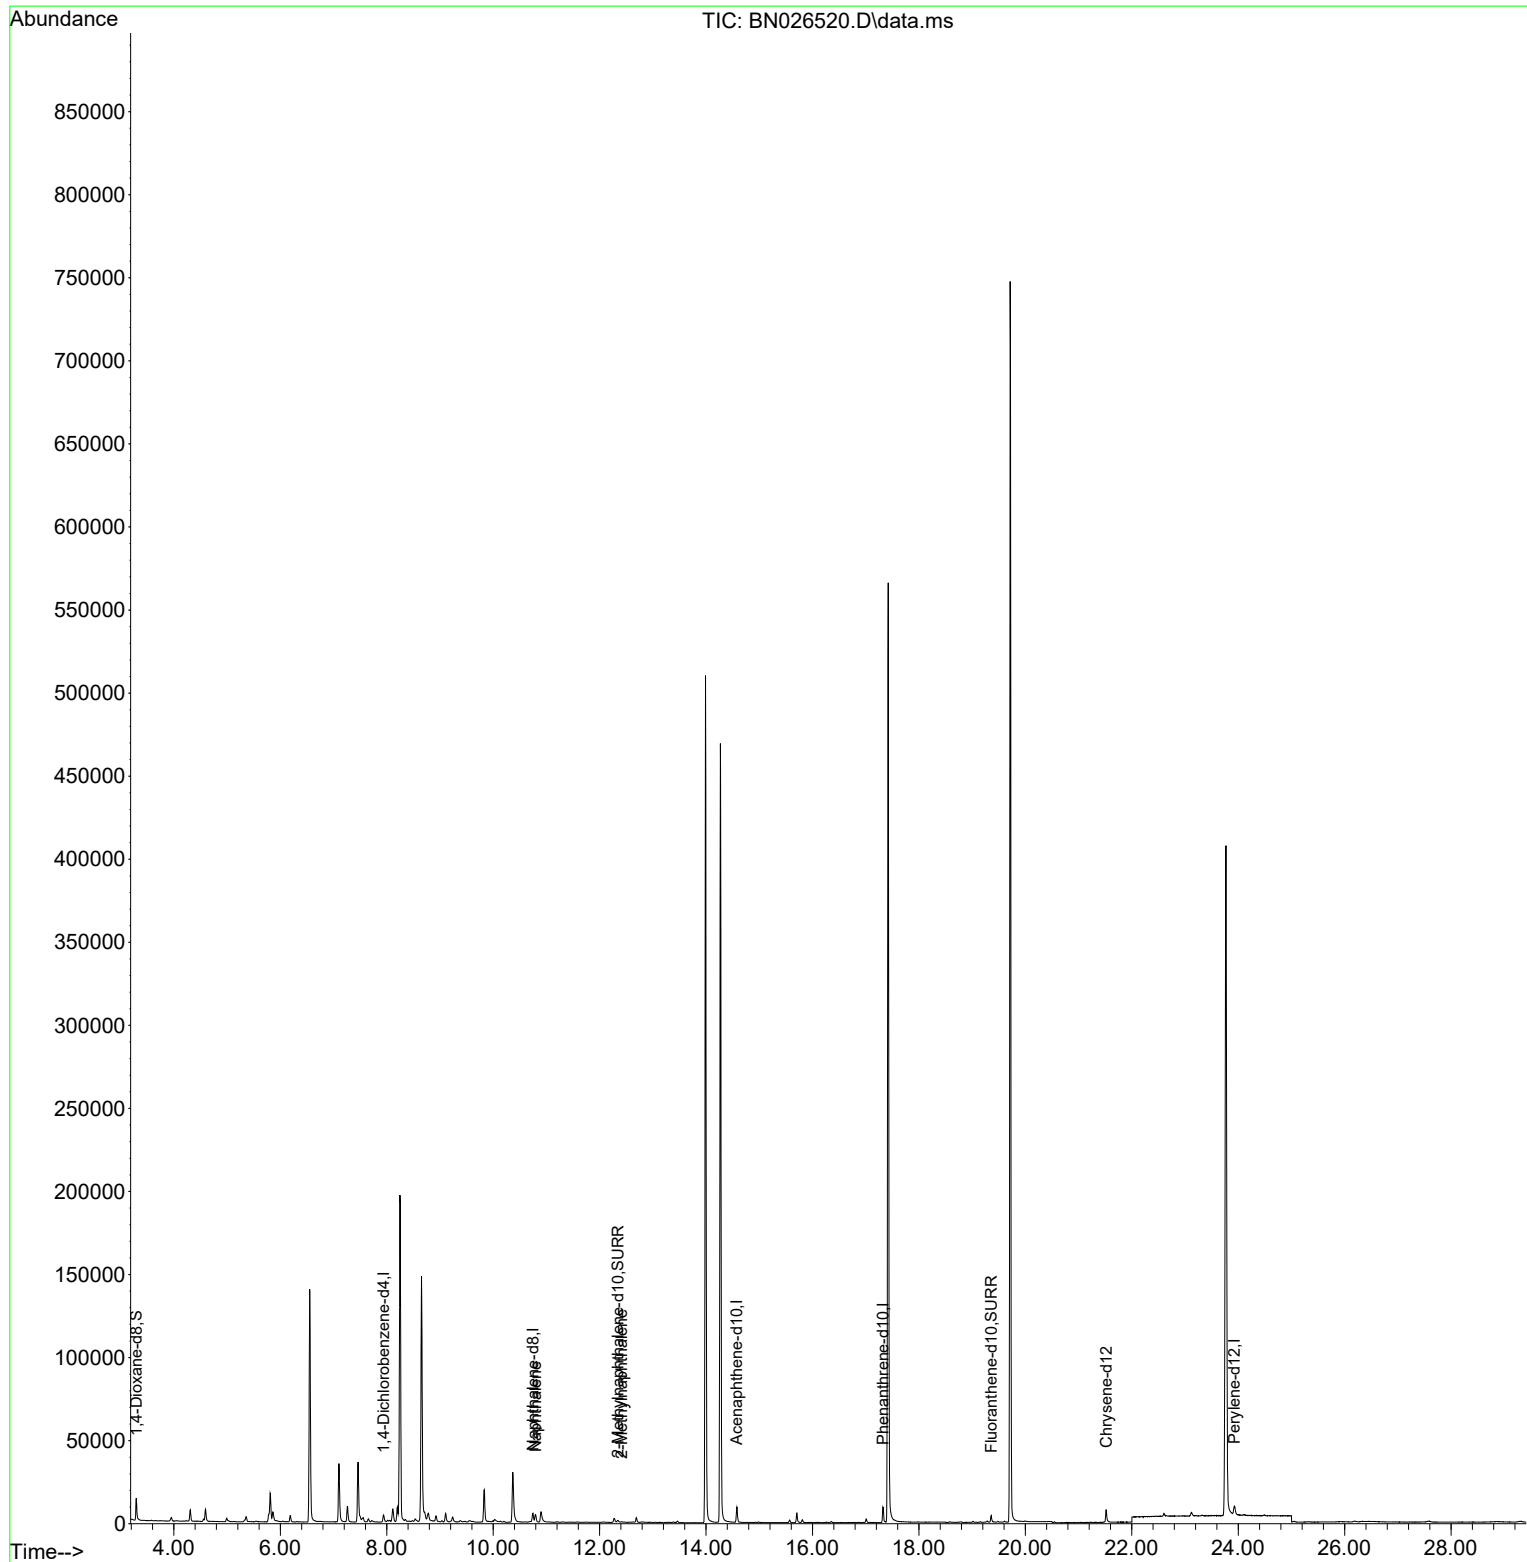

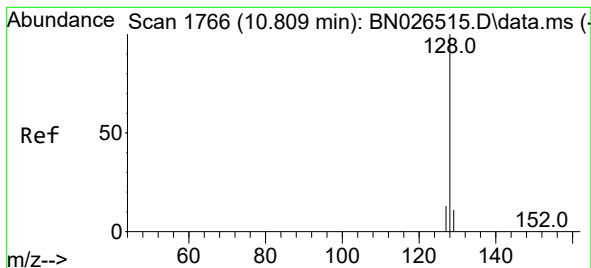

#5

Naphthalene

Concen: 0.314 ng/ul

RT: 10.797 min Scan# 11

Delta R.T. -0.017 min

Lab File: BN026520.D

Acq: 15 Jul 2023 20:10

Instrument :

BNA_N

ClientSampleId :

A4633





Tgt Ion:128 Resp: 6979

Ion Ratio Lower Upper

128 100

129 13.1 10.2 15.2

127 14.6 11.4 17.0

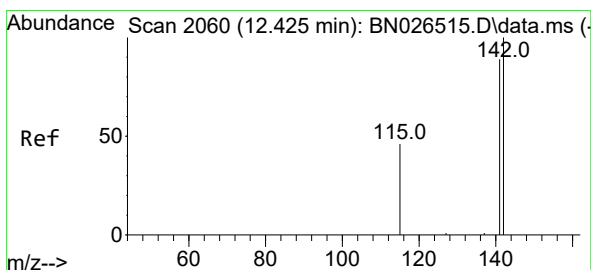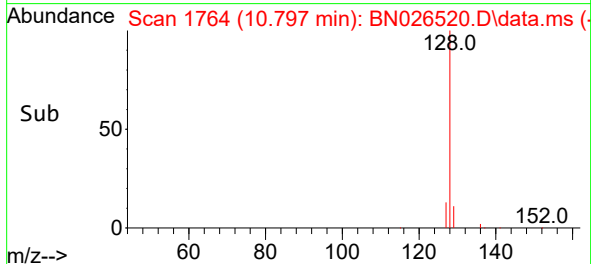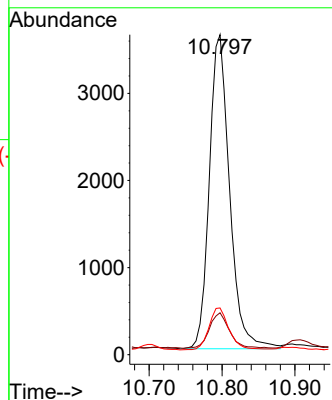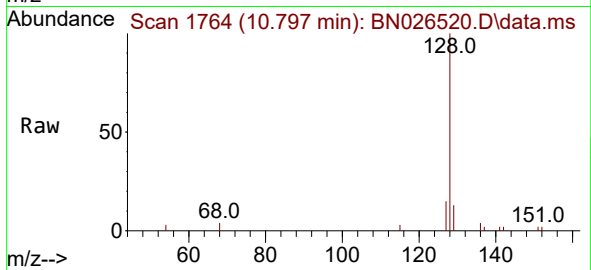

#7

2-Methylnaphthalene

Concen: 0.026 ng/ul

RT: 12.414 min Scan# 2058

Delta R.T. -0.011 min

Lab File: BN026520.D

Acq: 15 Jul 2023 20:10

Tgt Ion:142 Resp: 324

Ion Ratio Lower Upper

142 100

141 92.6 72.3 108.5

