


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
 Data File : BN006861.D
 Acq On : 16 Jul 2019 11:54
 Operator : HP/JU
 Sample : K3772-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A52N2

Manual Integrations
 APPROVED

mohammad
 7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:19:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

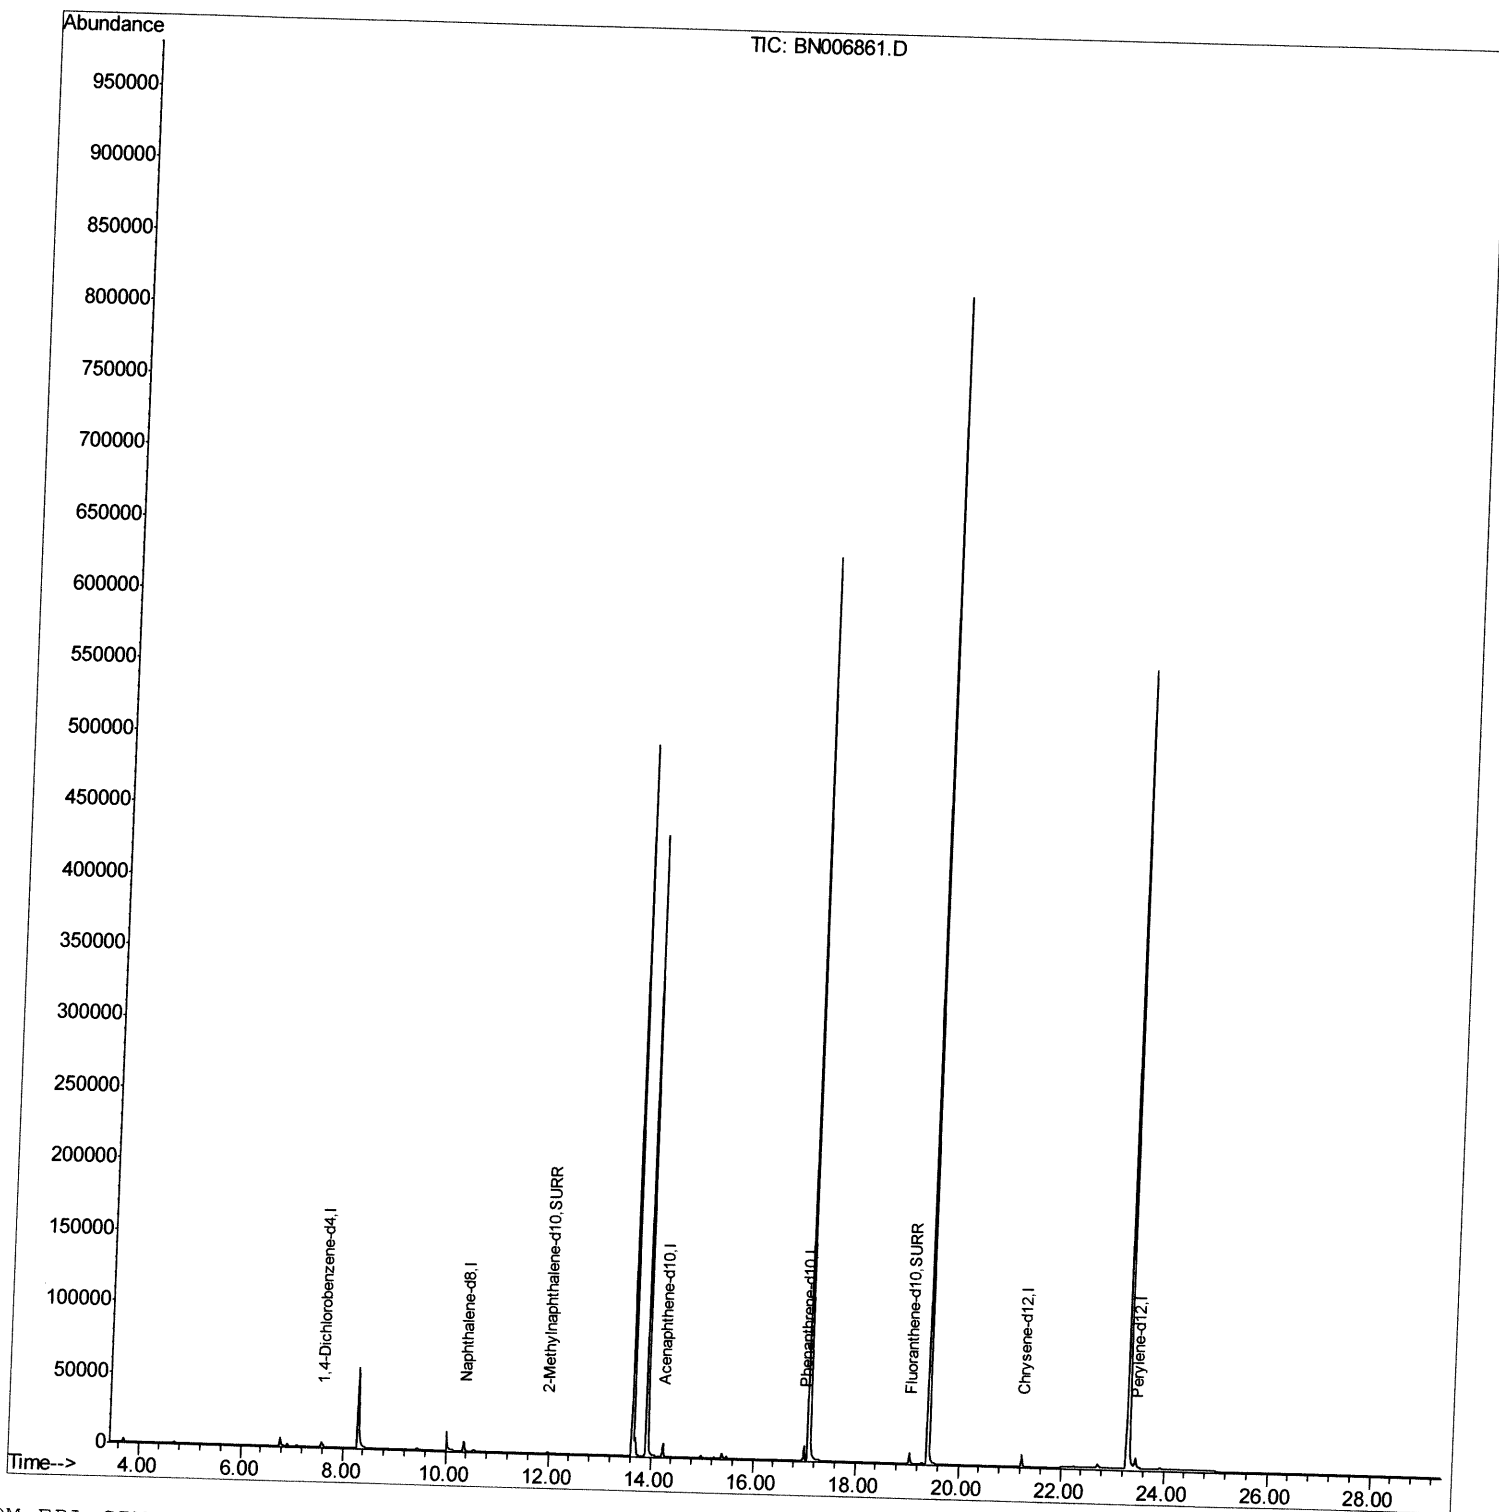

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
 Data File : BN006861.D
 Acq On : 16 Jul 2019 11:54
 Operator : HP/JU
 Sample : K3772-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A52N2

Manual Integrations
 APPROVED

mohammad
 7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:17:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

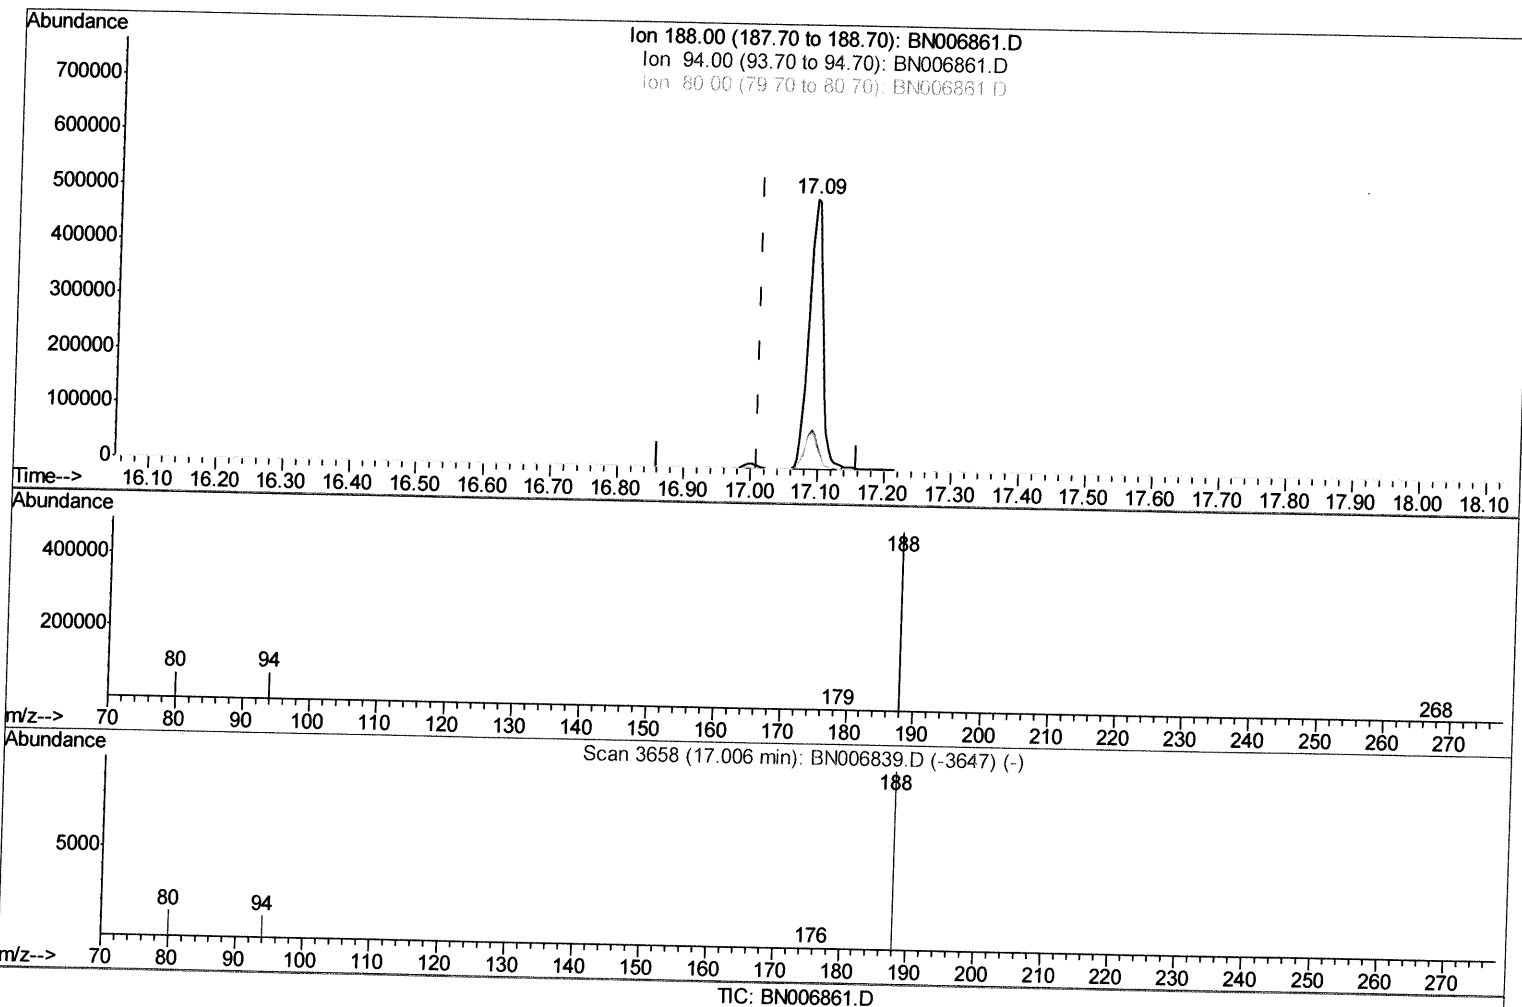

(10) Phenanthrene-d10 (I)

17.090min (+0.080) 0.40ng/ul

response 715220

Ion	Exp%	Act%
188.00	100	100
94.00	13.70	14.50
80.00	14.80	13.82
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006861.D
Acq On : 16 Jul 2019 11:54
Operator : HP/JU
Sample : K3772-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52N2

Manual Integrations
APPROVED

mohammad
7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:17:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

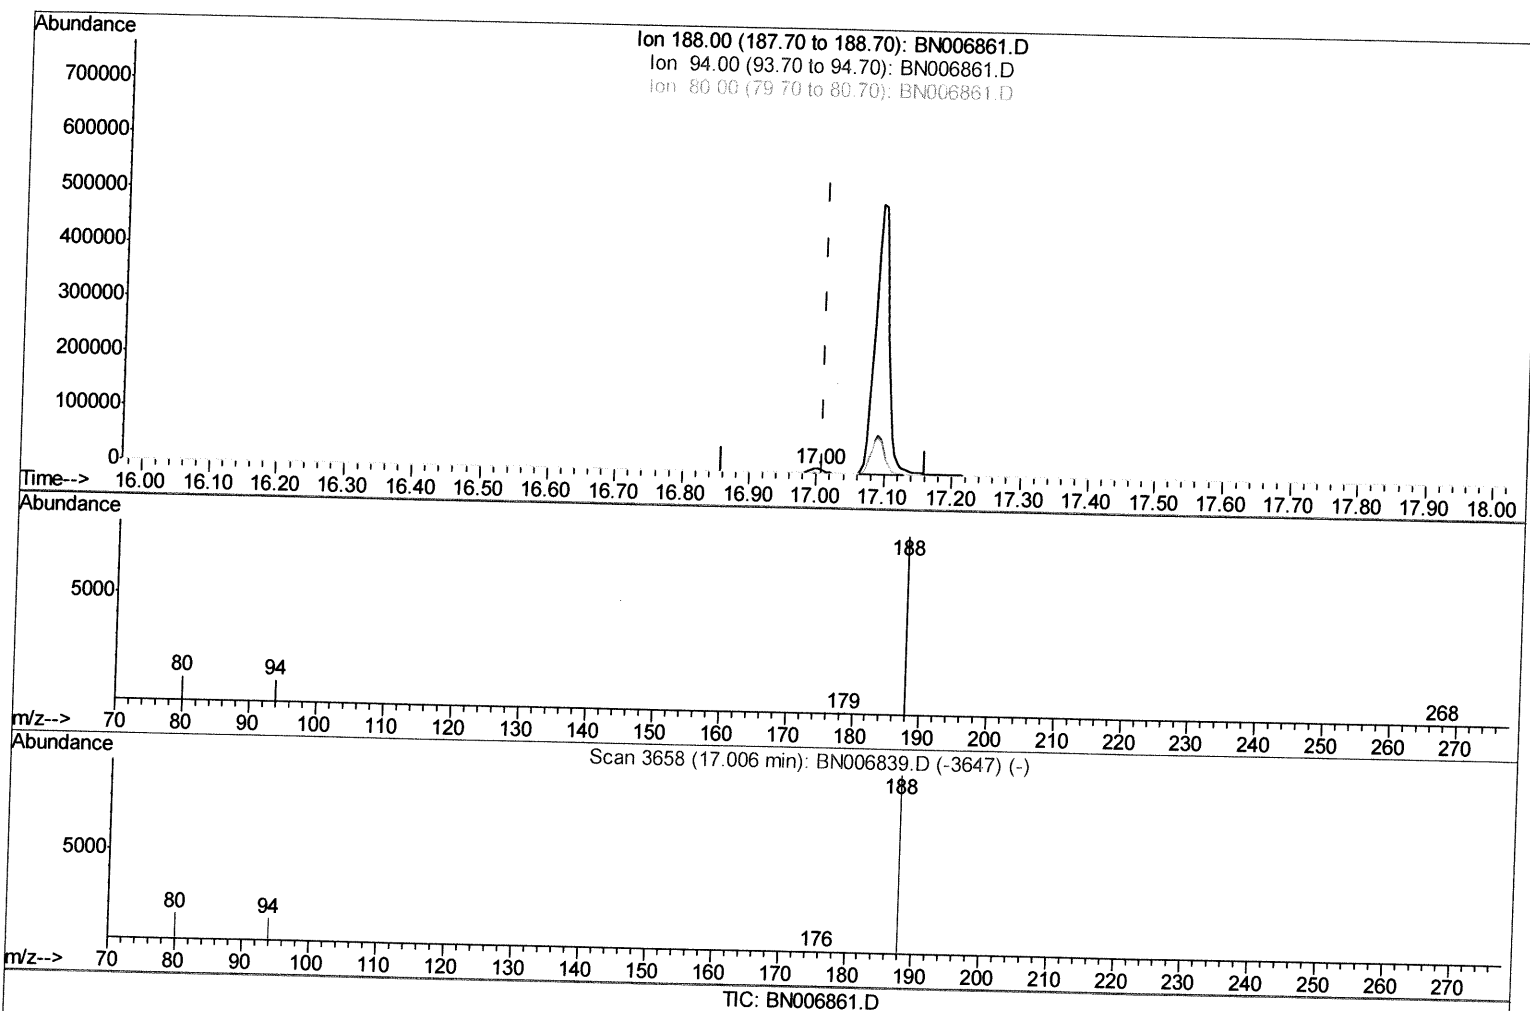

(10) Phenanthrene-d10 (I)

17.002min (-0.008) 0.40ng/ul m JU 07/17/19

response 11695

Ion	Exp%	Act%
188.00	100	100
94.00	13.70	12.32
80.00	14.80	13.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006861.D
Acq On : 16 Jul 2019 11:54
Operator : HP/JU
Sample : K3772-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52N2

Manual Integrations
APPROVED

mohammad
7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:17:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

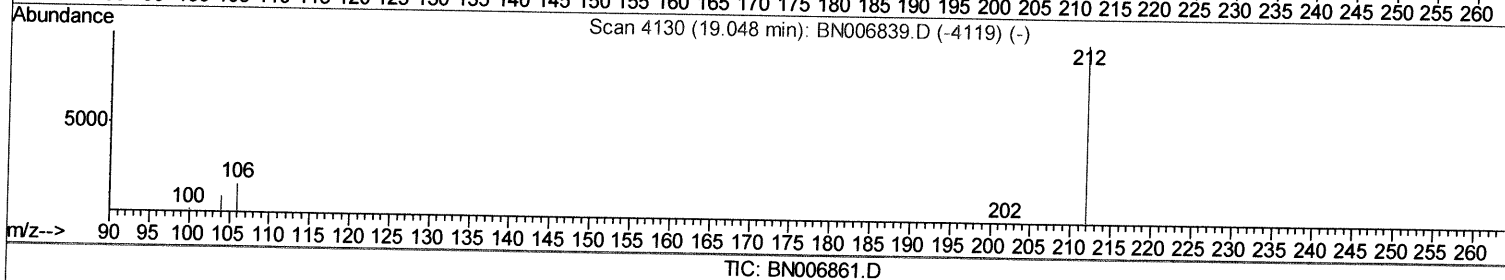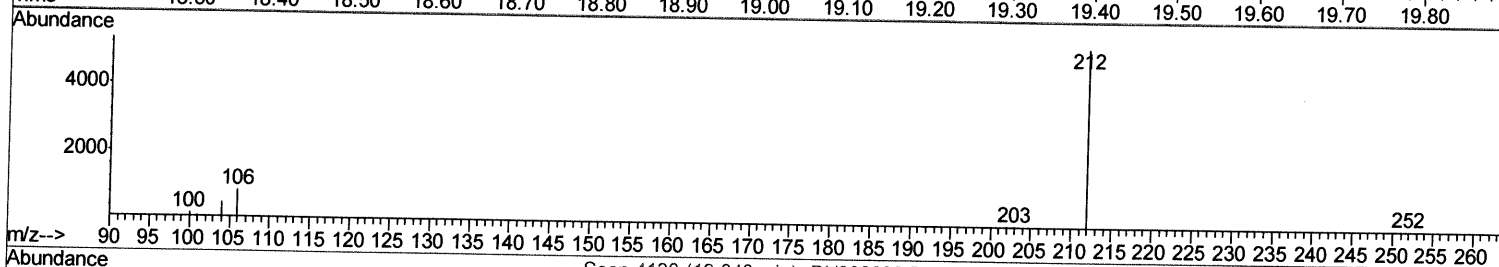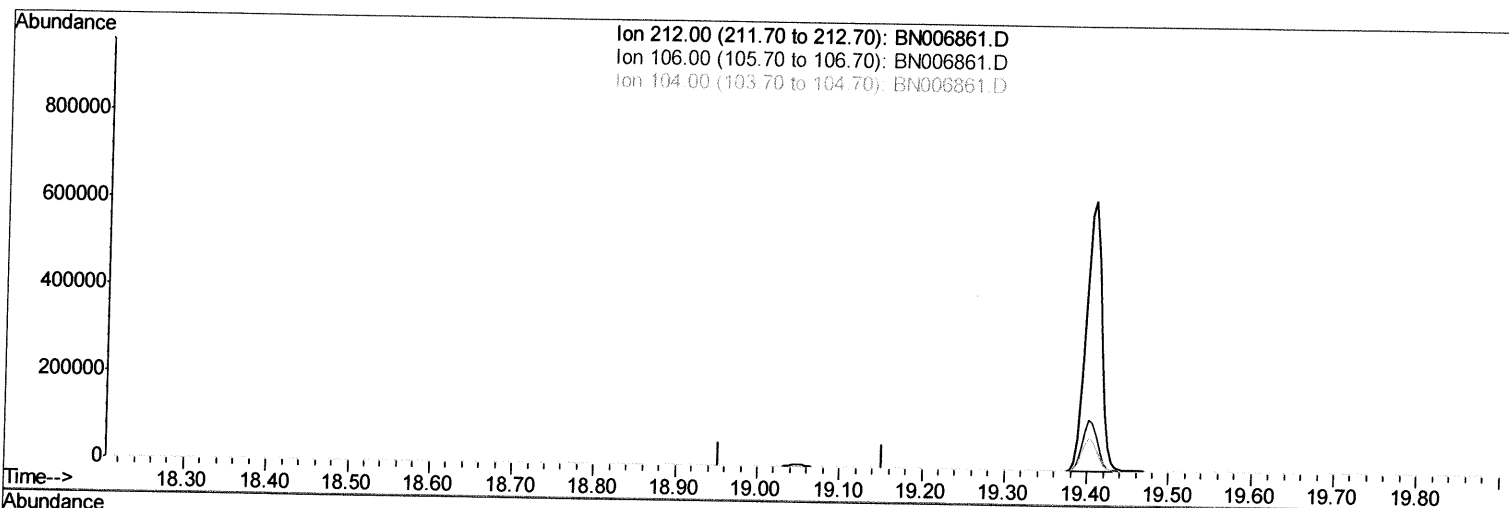

(14) Fluoranthene-d10 (SURR)

19.053min (-19.053) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	17.80	0.00#
104.00	9.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006861.D
Acq On : 16 Jul 2019 11:54
Operator : HP/JU
Sample : K3772-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52N2

Manual Integrations
APPROVED

mohammad
7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:17:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

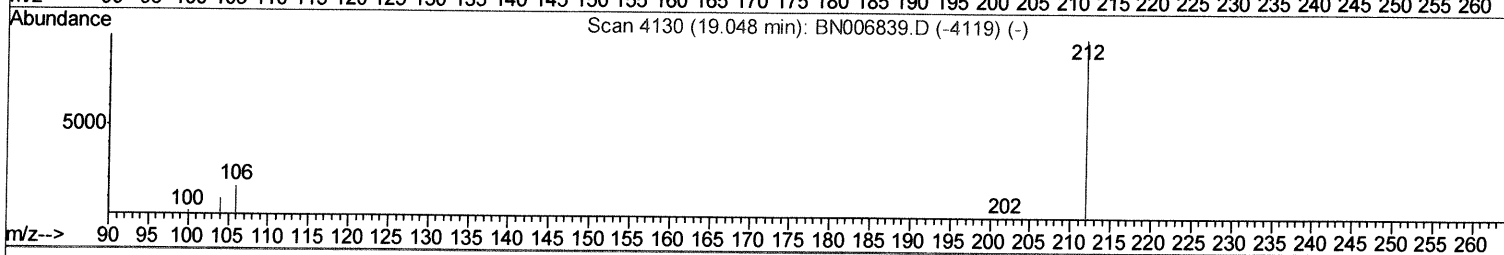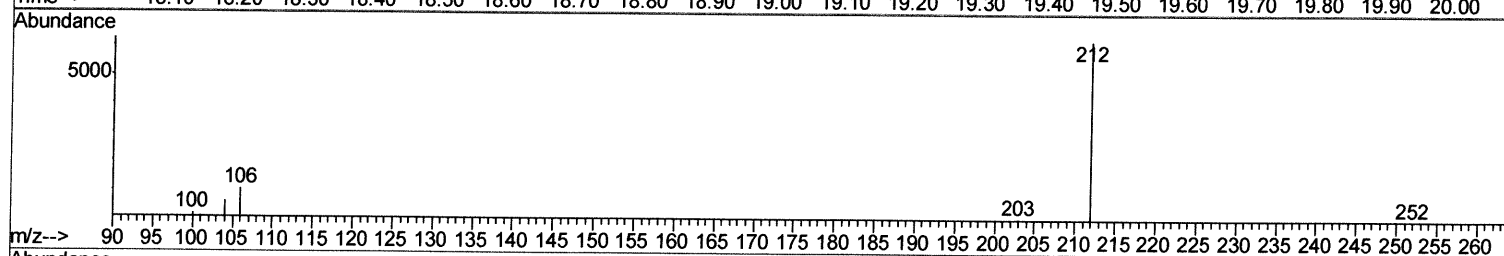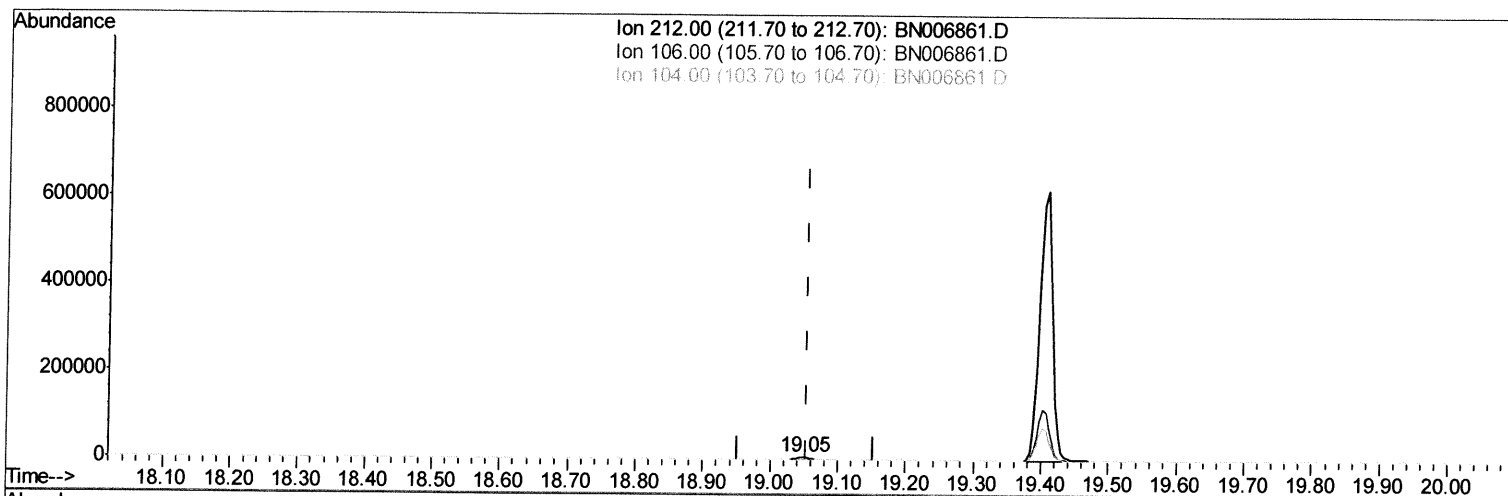

TIC: BN006861.D

(14) Fluoranthene-d10 (SURR)

19.048min (-0.005) 0.26ng/ul m

JU
07/17/19

response 8998

Ion	Exp%	Act%
212.00	100	100
106.00	17.80	0.00#
104.00	9.70	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006861.D
Acq On : 16 Jul 2019 11:54
Operator : HP/JU
Sample : K3772-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52N2

Manual Integrations
APPROVED

mohammad
7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:17:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

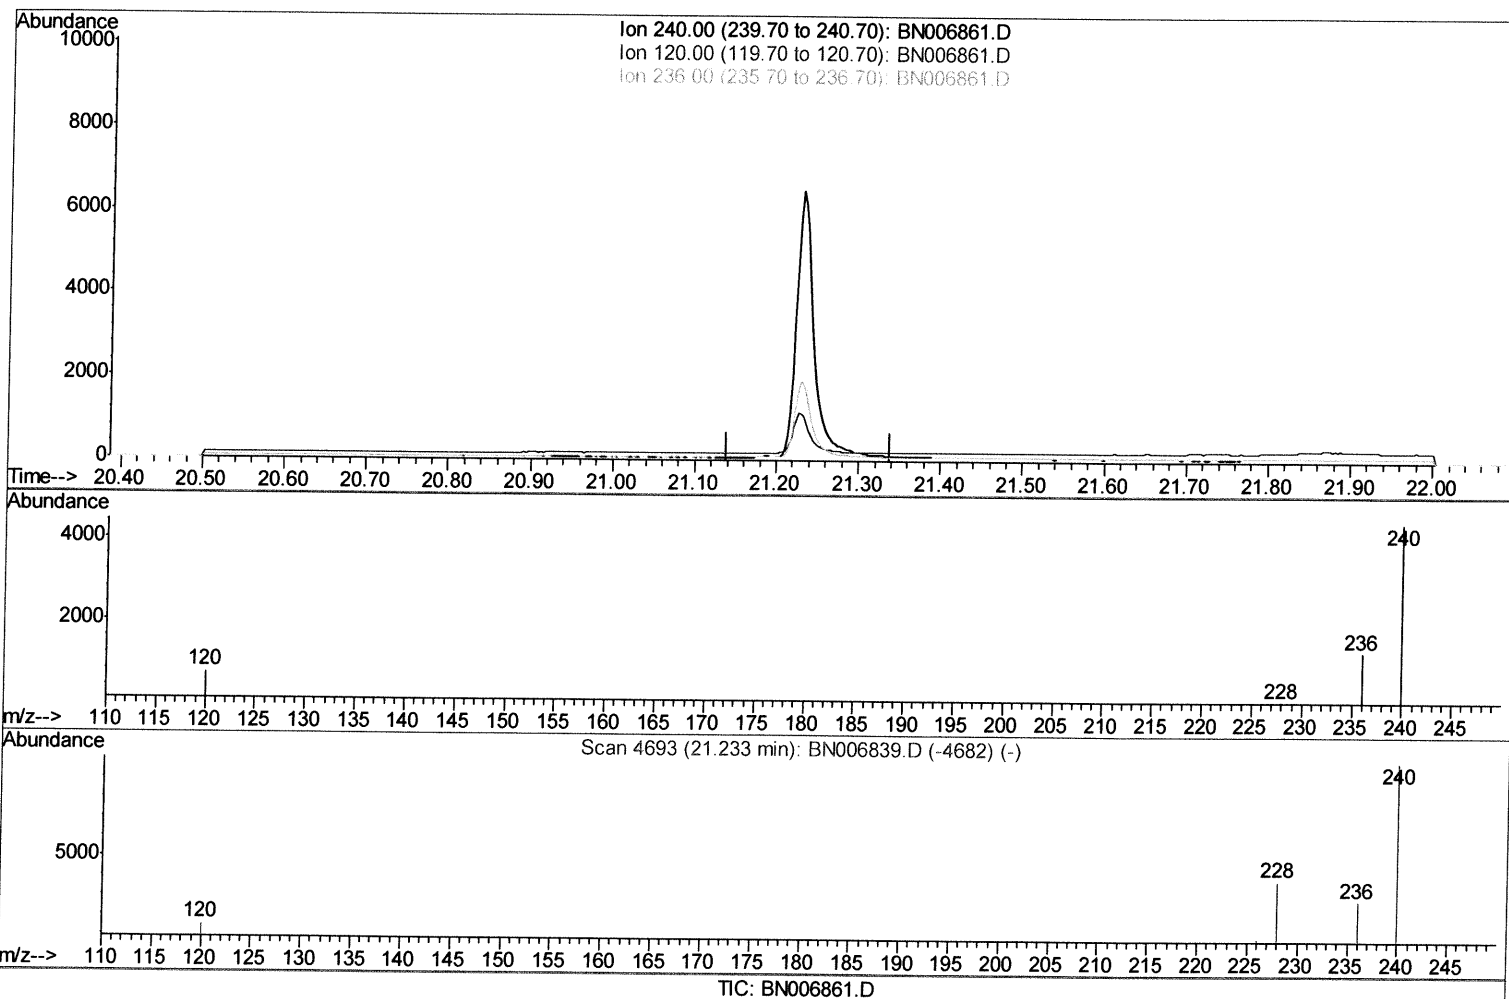

(16) Chrysene-d12 (I)

21.239min (-21.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.20	0.00#
236.00	30.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
 Data File : BN006861.D
 Acq On : 16 Jul 2019 11:54
 Operator : HP/JU
 Sample : K3772-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A52N2

Manual Integrations
 APPROVED

mohammad
 7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:17:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

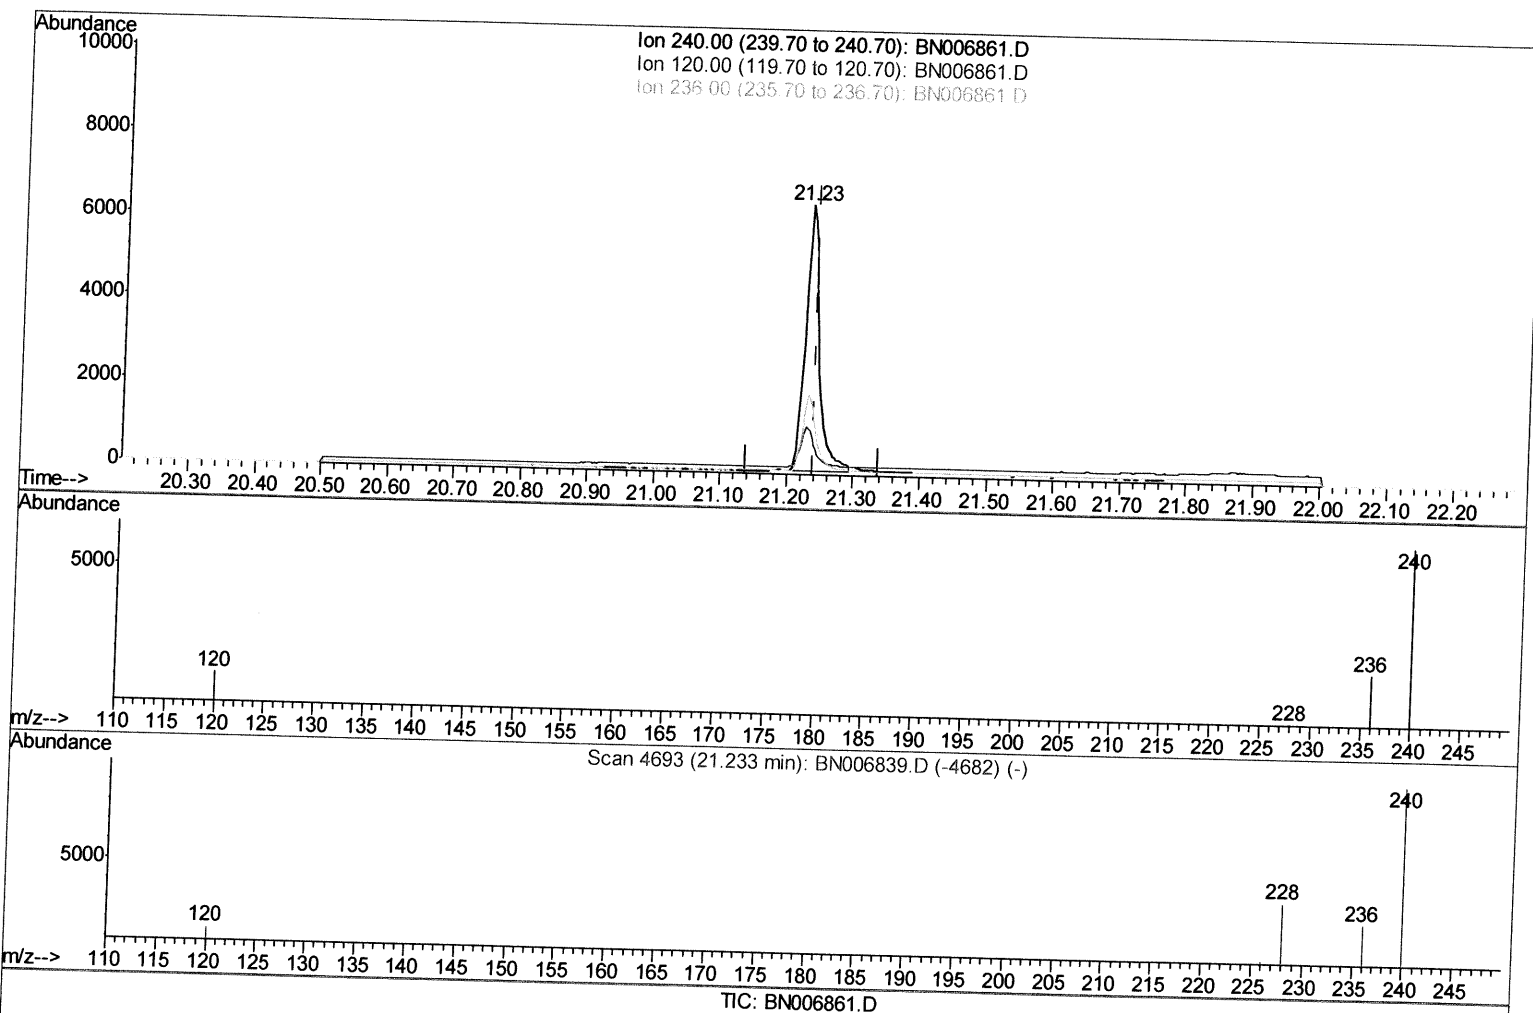

(16) Chrysene-d12 (I)

21.230min (-0.009) 0.40ng/ul m ^{JU} 07/17/19

response 9506

Ion	Exp%	Act%
240.00	100	100
120.00	20.20	17.47
236.00	30.00	29.61
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006861.D
Acq On : 16 Jul 2019 11:54
Operator : HP/JU
Sample : K3772-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52N2

Manual Integrations
APPROVED

mohammad
7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:18:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

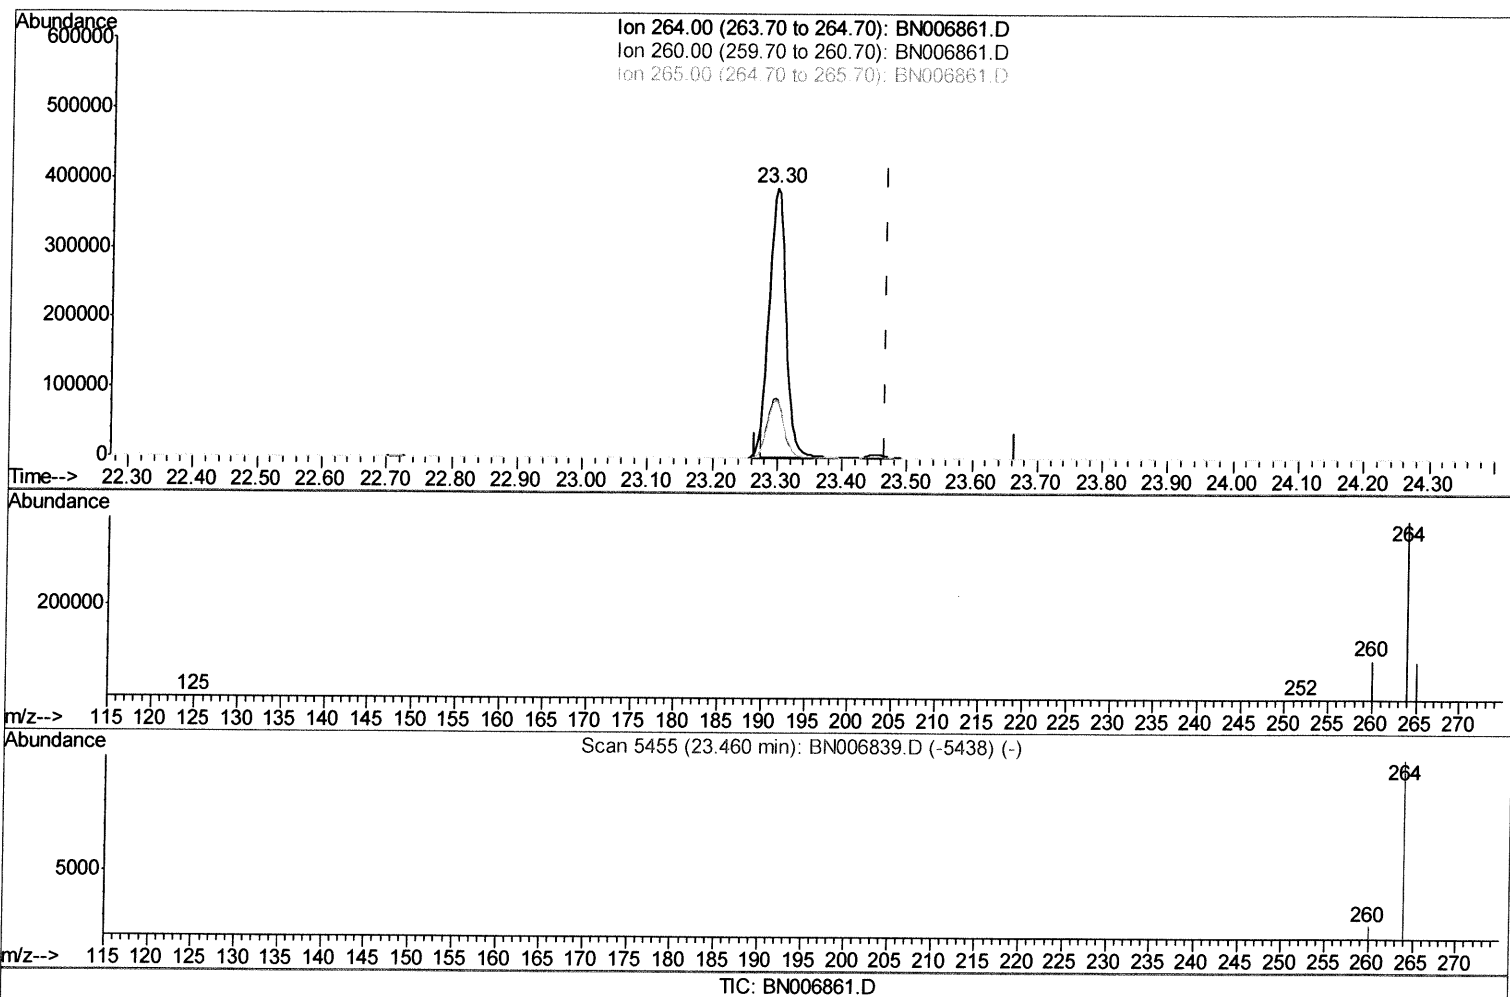

(20) Perylene-d12 (I)

23.297min (-0.170) 0.40ng/ul

response 693561

Ion	Exp%	Act%
-----	------	------

264.00	100	100
--------	-----	-----

260.00	27.80	22.32
--------	-------	-------

265.00	36.10	21.35#
--------	-------	--------

0.00	0.00	0.00
------	------	------

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
 Data File : BN006861.D
 Acq On : 16 Jul 2019 11:54
 Operator : HP/JU
 Sample : K3772-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A52N2

Manual Integrations
 APPROVED

mohammad
 7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:18:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

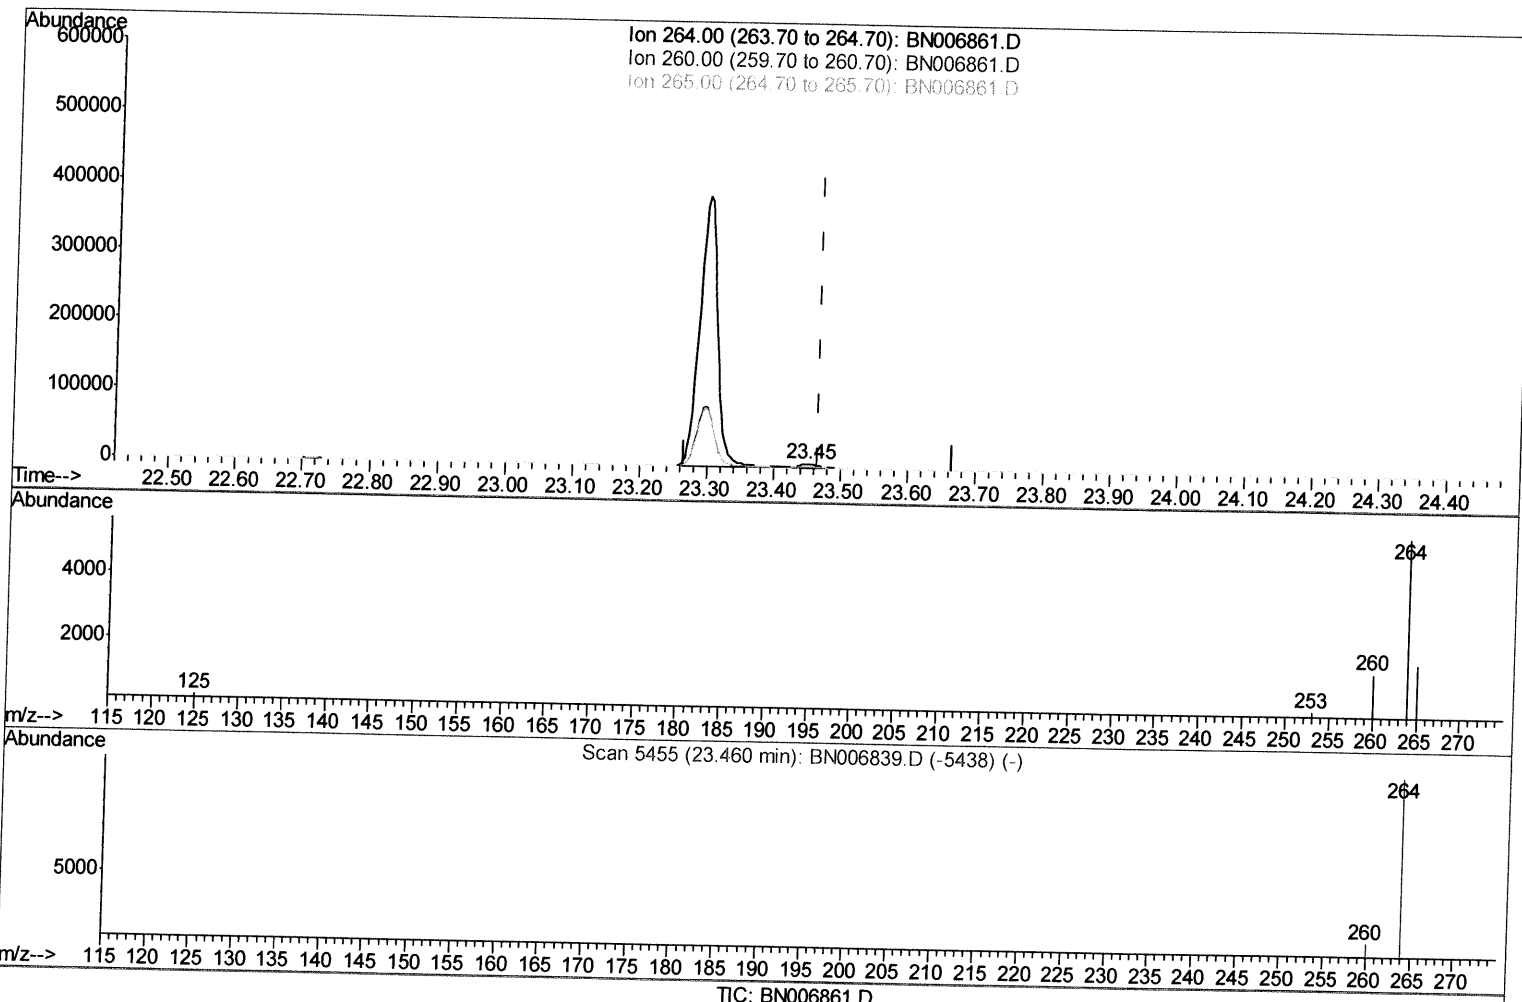

(20) Perylene-d12 (I)

23.452min (-0.015) 0.40ng/ul m *JU 07/17/19*

response 8464

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	26.64
265.00	36.10	31.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006861.D
Acq On : 16 Jul 2019 11:54
Operator : HP/JU
Sample : K3772-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52N2

Manual Integrations
APPROVED

mohammad
7/17/2019 7:41:39 AM

Quant Time: Jul 16 14:19:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2847	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10287	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5278	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	11695m	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	9506m	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	8464m	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.98	152	3059	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	8998m	0.26	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

JS 07/17/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed