


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006862.D
Acq On : 16 Jul 2019 12:29
Operator : HP/JU
Sample : K3772-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52P0

Manual Integrations
APPROVED

mohammad
7/17/2019 7:42:28 AM

Quant Time: Jul 16 14:20:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

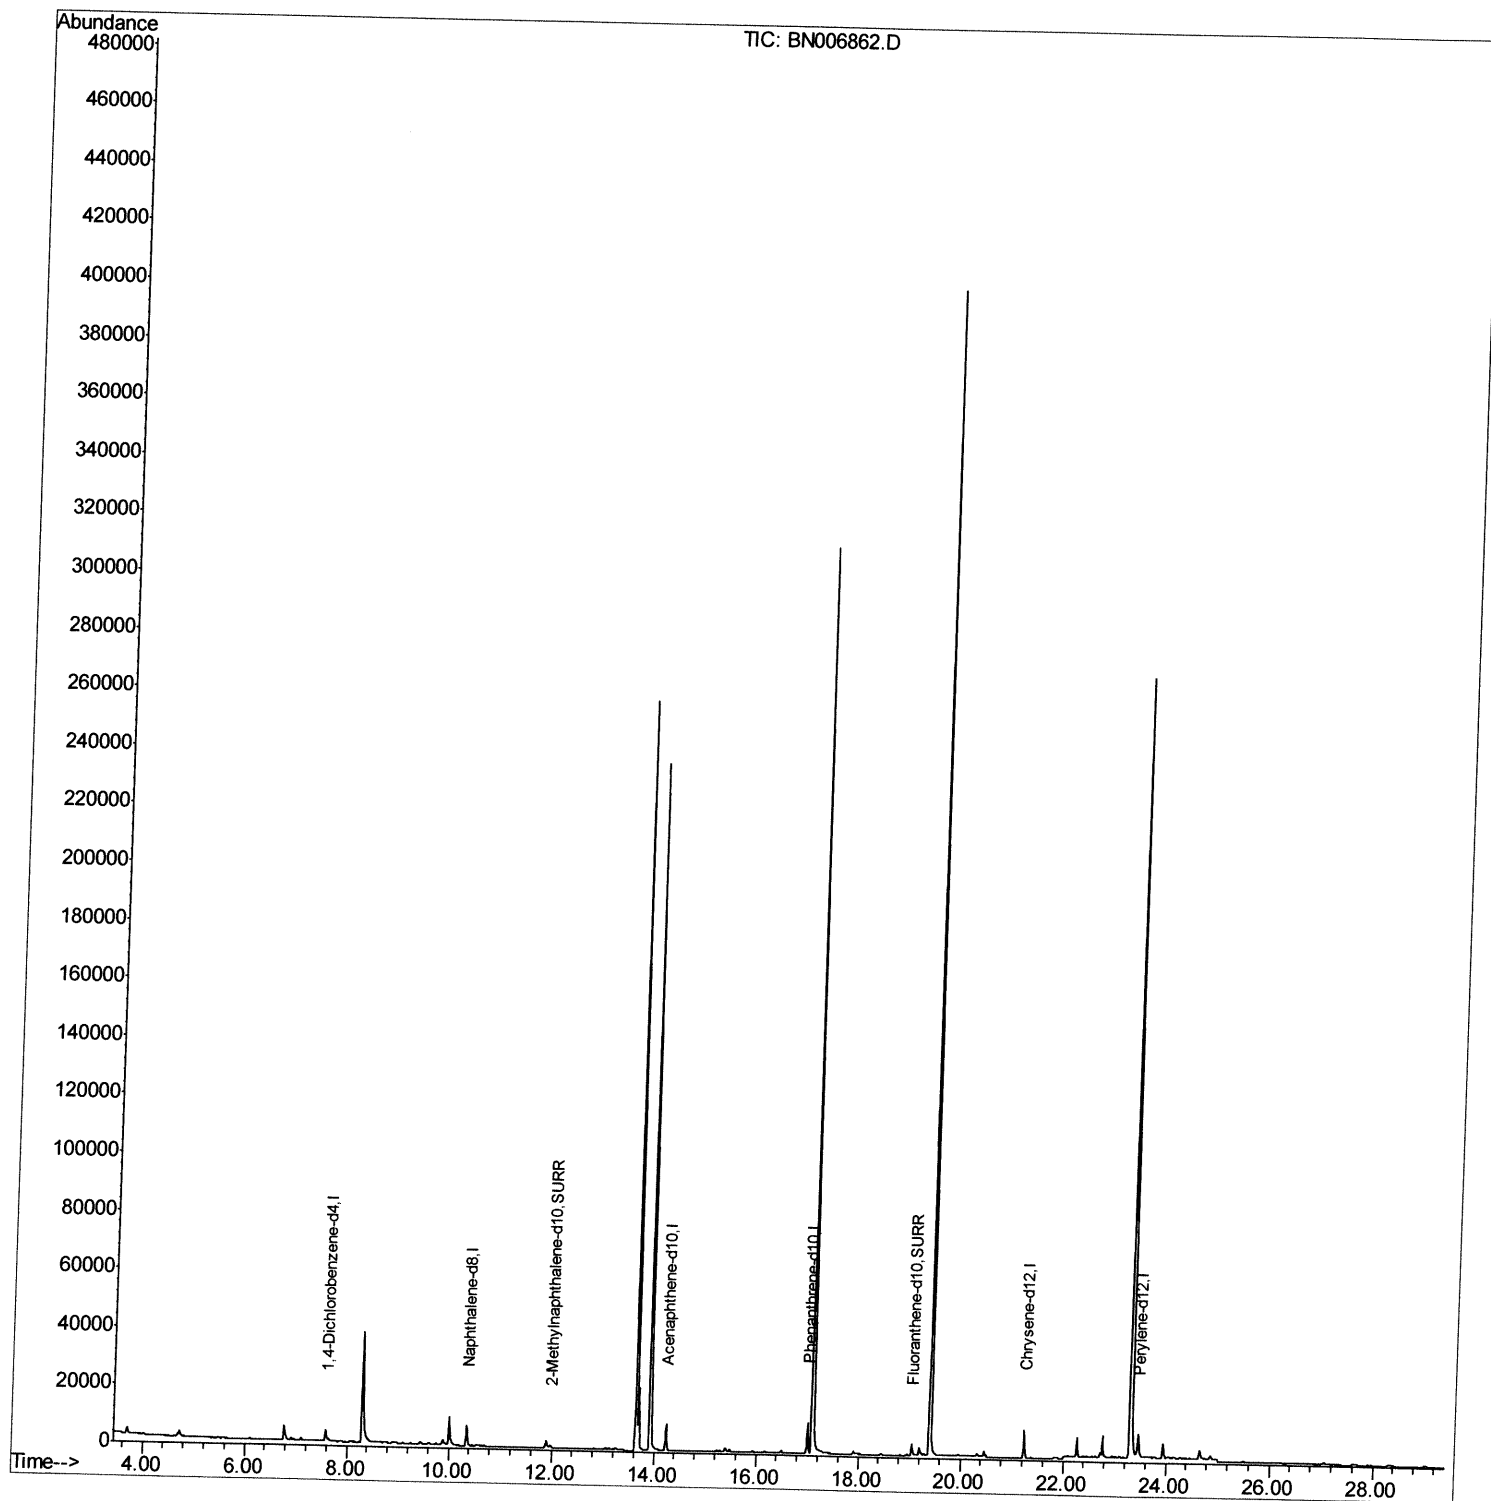

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
 Data File : BN006862.D
 Acq On : 16 Jul 2019 12:29
 Operator : HP/JU
 Sample : K3772-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 A52P0

Manual Integrations
 APPROVED

mohammad
 7/17/2019 7:42:28 AM

Quant Time: Jul 16 14:19:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

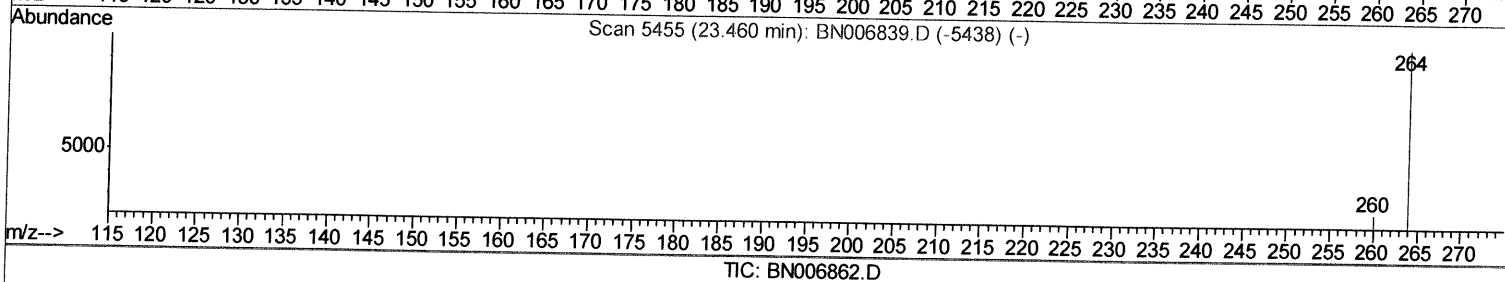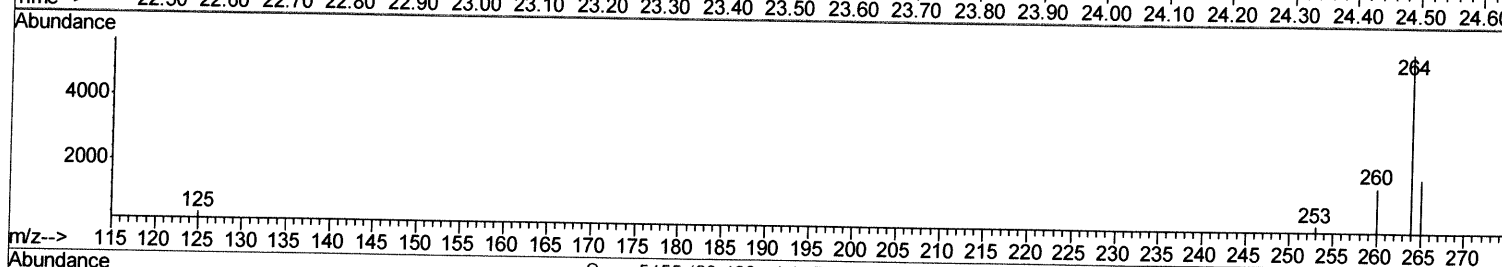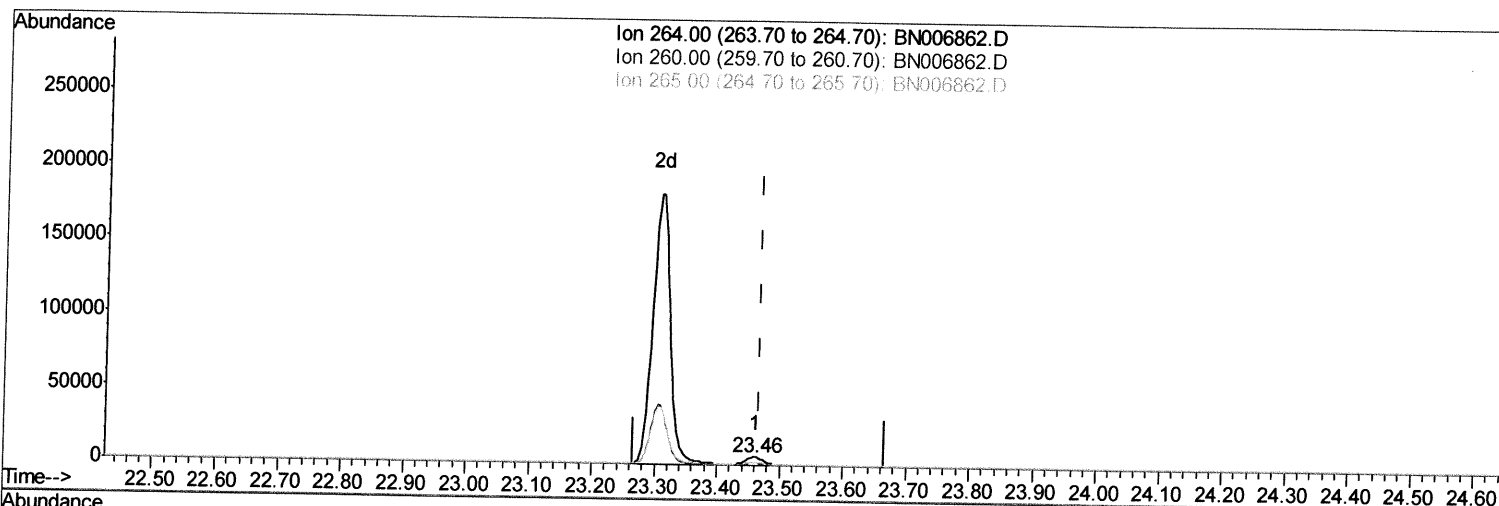

(20) Perylene-d12 (I)

23.460min (-0.006) 0.40ng/ul

response 12627

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	27.35
265.00	36.10	32.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006862.D
Acq On : 16 Jul 2019 12:29
Operator : HP/JU
Sample : K3772-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A52P0

Manual Integrations
APPROVED

mohammad
7/17/2019 7:42:28 AM

Quant Time: Jul 16 14:19:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

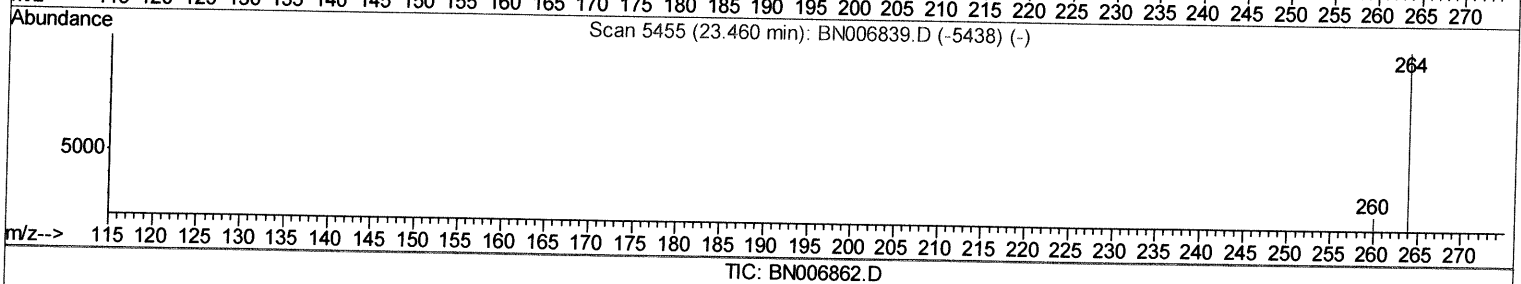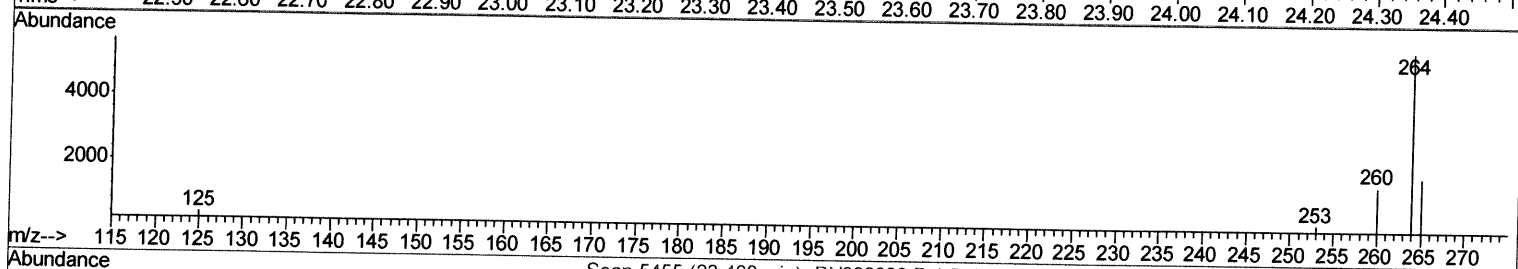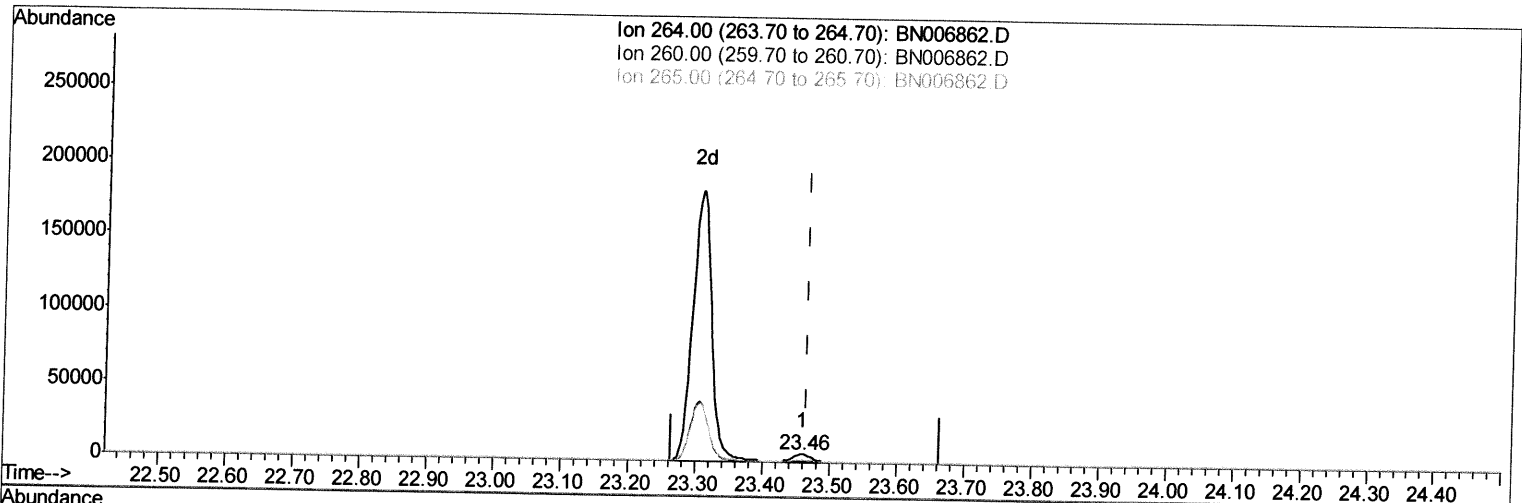

(20) Perylene-d12 (I)

23.460min (-0.006) 0.40ng/ul m

JU
07/17/19

response 9184

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	27.35
265.00	36.10	32.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071619\
Data File : BN006862.D
Acq On : 16 Jul 2019 12:29
Operator : HP/JU
Sample : K3772-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A52P0

Manual Integrations
APPROVED

mohammad
7/17/2019 7:42:28 AM

Quant Time: Jul 16 14:20:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2870	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10312	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5388	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	12004	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	10018	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	9184m>	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.97	152	1736	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	4572	0.13	ng/ul	0.00

Target Compounds

Qvalue

Ju 07/17/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed