
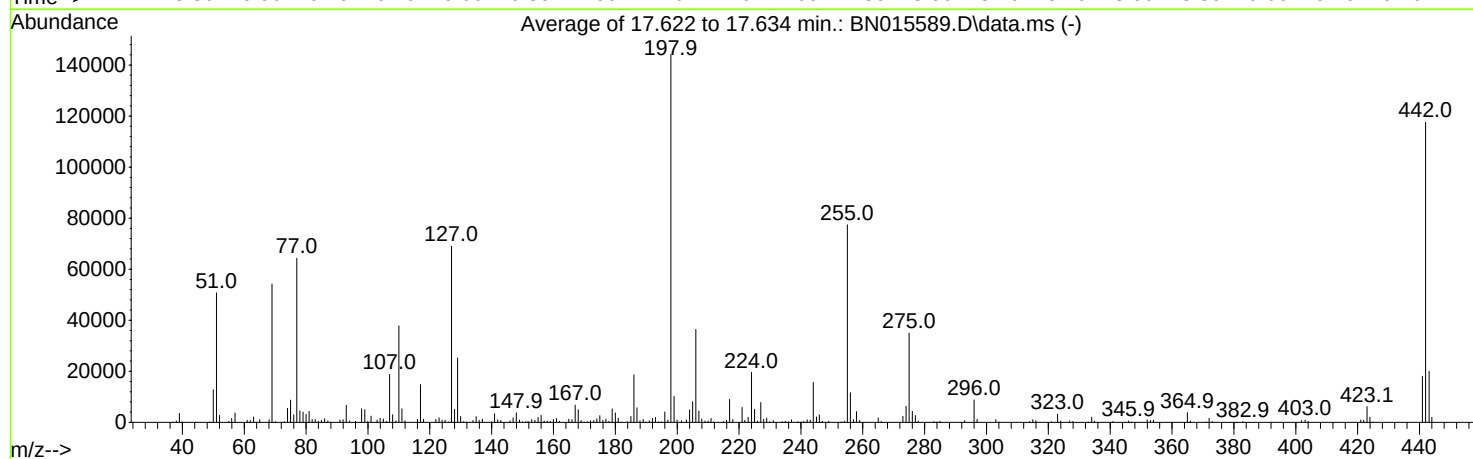


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071621\
 Data File : BN015589.D
 Acq On : 16 Jul 2021 09:29
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN071521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 15 15:46:51 2021

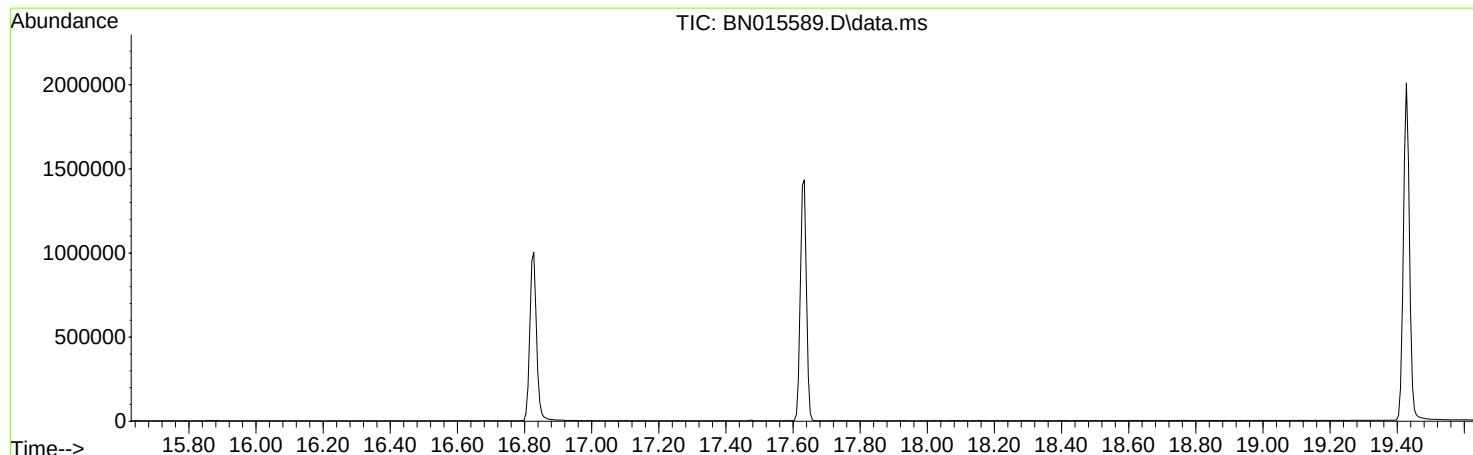

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	50704	PASS
68	69	0.00	2	1.8	992	PASS
69	198	0.00	100	37.6	54211	PASS
70	69	0.00	2	0.4	235	PASS
127	198	10	80	47.9	69008	PASS
197	198	0.00	2	0.6	919	PASS
198	198	100	100	100.0	144120	PASS
199	198	5	9	7.0	10141	PASS
275	198	10	60	24.3	34957	PASS
365	198	1	100	2.6	3815	PASS
441	198	0.01	100	12.5	18077	PASS
442	442	50	100	100.0	117568	PASS
443	442	15	24	17.0	19973	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/16/2021	BNA_N	BN015589.D
Compound Name	Response	Retention Time
DDT	515699	20.66
DDD	1903	20.23
DDE	609	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2512	518211	0.48

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071621\
Data File : BN015589.D
Acq On : 16 Jul 2021 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 16 11:40:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

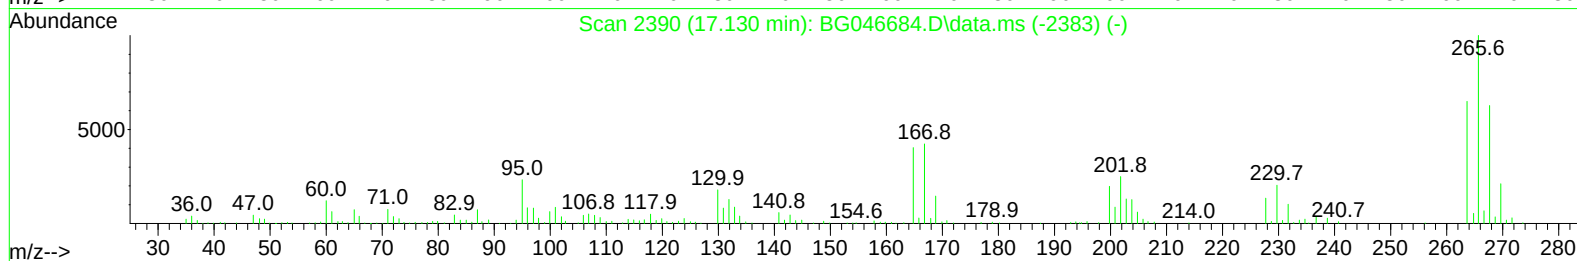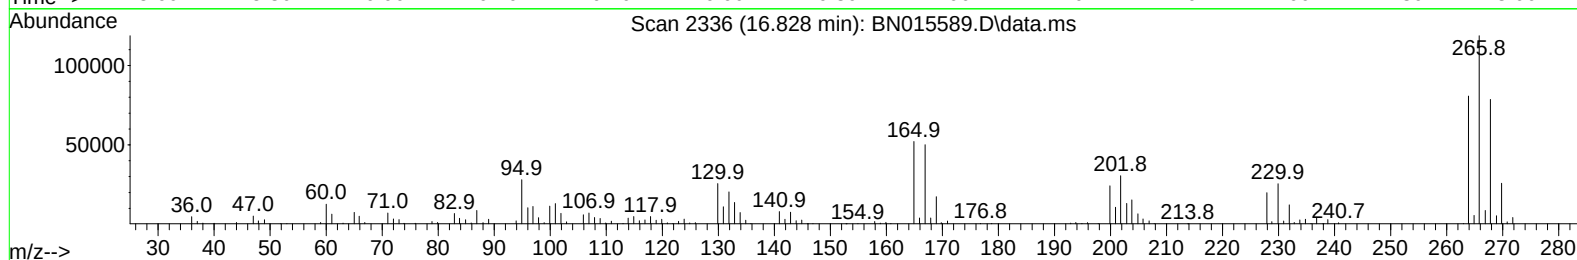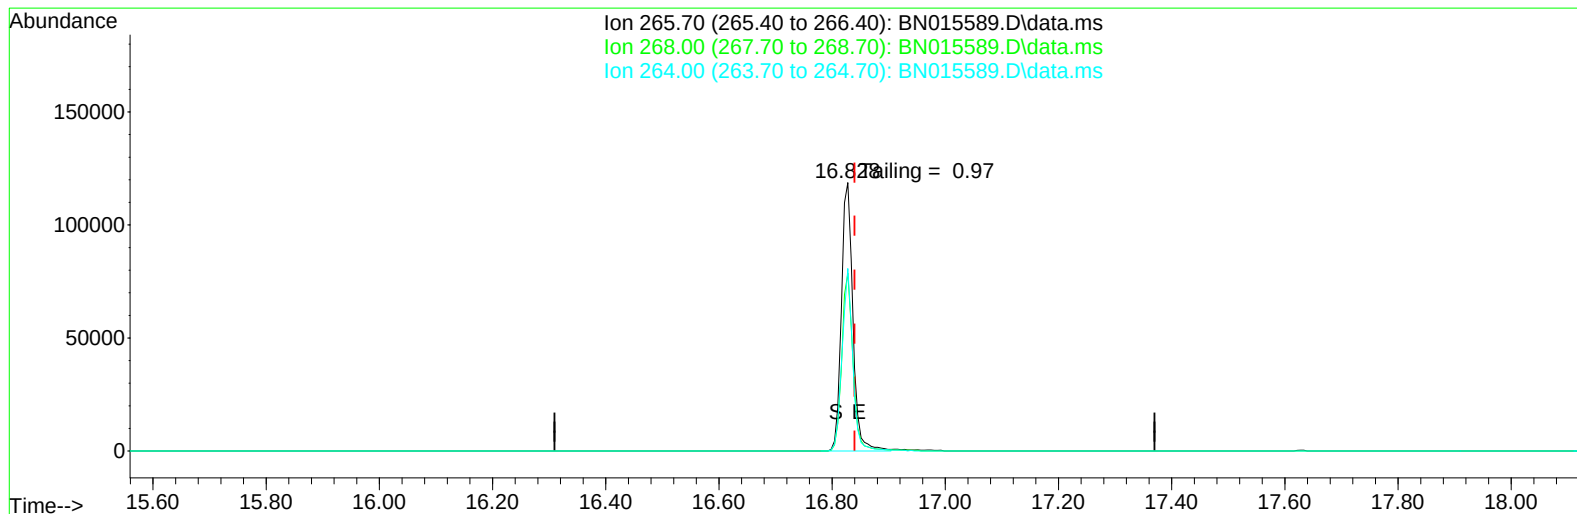

TIC: BN015589.D\data.ms

(70) Pentachlorophenol (C)

16.828min (-0.012) 26241.00 ng




response 168453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.24
264.00	61.60	67.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071621\
Data File : BN015589.D
Acq On : 16 Jul 2021 09:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 16 11:40:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

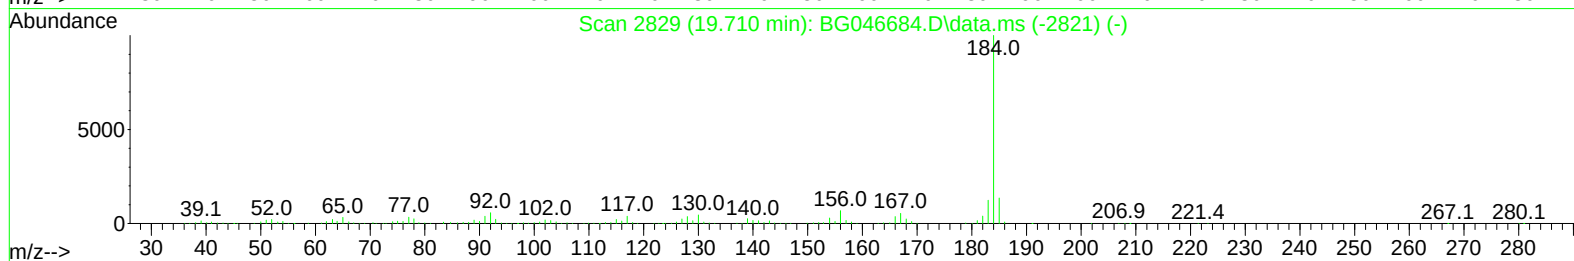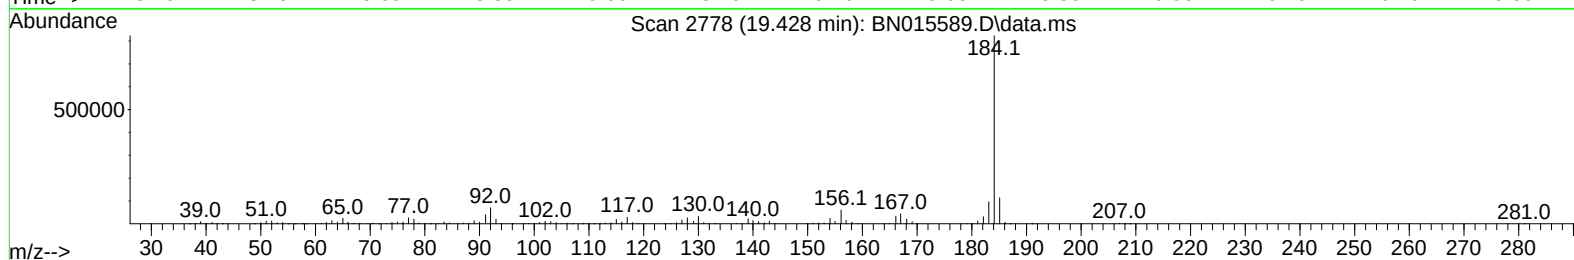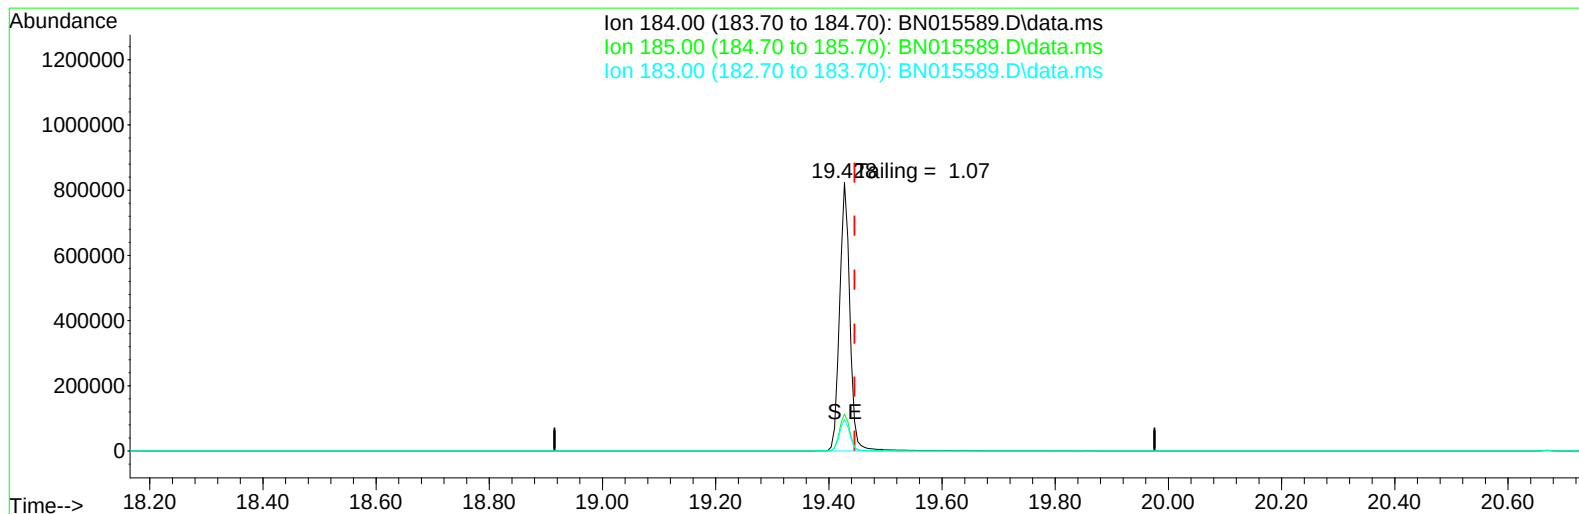

TIC: BN015589.D\data.ms

(77) Benzidine

19.428min (-0.018) 0.00 ng

response 1040955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.84
183.00	13.20	11.73
0.00	0.00	0.00