

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071719\
 Data File : BN006875.D
 Acq On : 17 Jul 2019 16:36
 Operator : HP/JU
 Sample : PB121410BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 18 01:08:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	3207	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	11784	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5891	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	885986	0.40	ng/ul	0.08
16) Chrysene-d12	21.26	240	7621	0.40	ng/ul	0.02
20) Perylene-d12	23.33	264	853364	0.40	ng/ul	-0.13
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	3969	0.22	ng/ul	0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
9) Fluorene	15.24	166	1585	0.062	ng/ul#	14
17) Pyrene	19.41	202	1571	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071719\
Data File : BN006875.D
Acq On : 17 Jul 2019 16:36
Operator : HP/JU
Sample : PB121410BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 18 01:08:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration




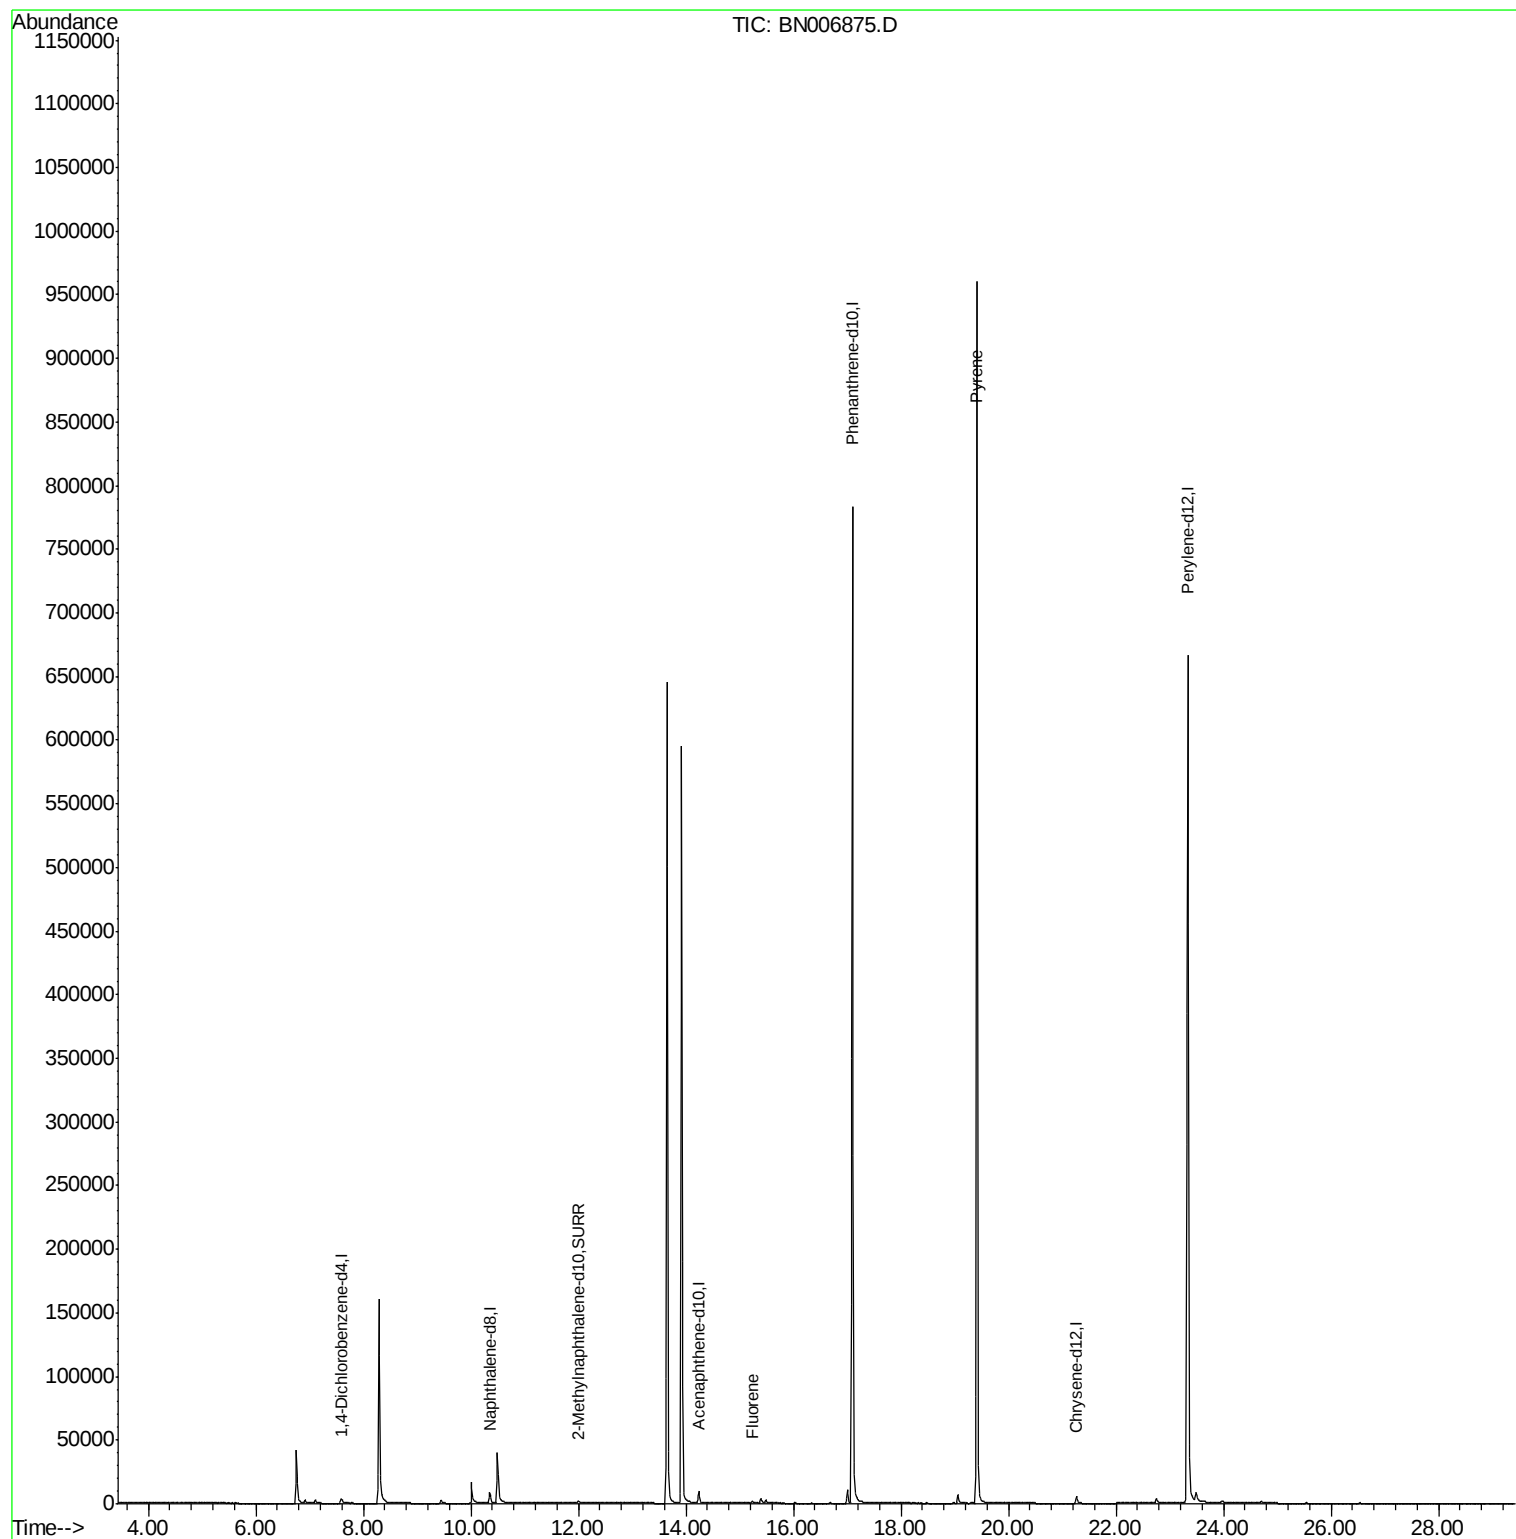


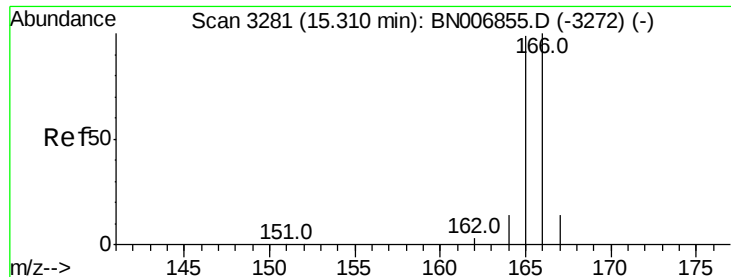

#9
Fluorene
 Concen: 0.062 ng/ul
 RT: 15.24 min Scan# 3265
 Delta R.T. -0.07 min
 Lab File: BN006875.D
 Acq: 17 Jul 2019 16:36

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 1585
 Ion Ratio Lower Upper
 166 100
 165 8.6 78.2 117.4#
 167 35.9 11.3 16.9#

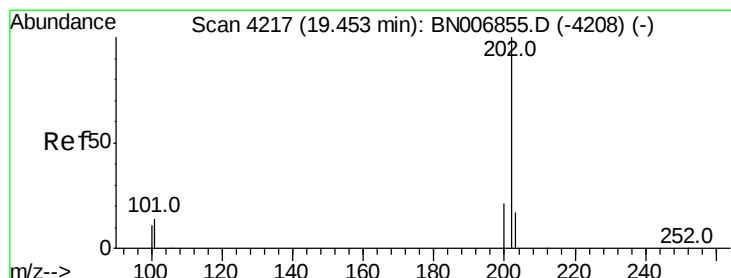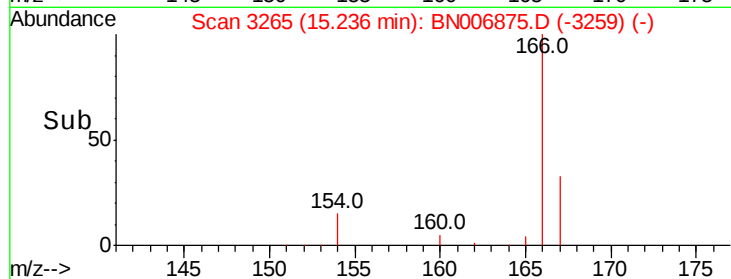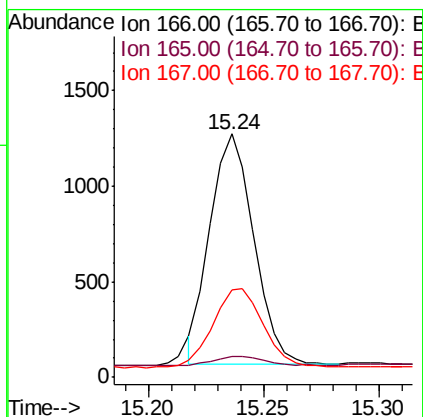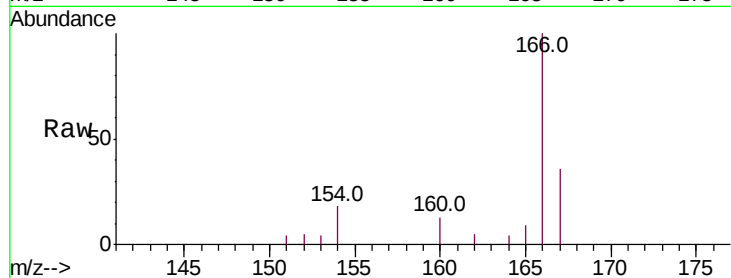

#17
Pyrene
 Concen: 0.045 ng/ul
 RT: 19.41 min Scan# 4208
 Delta R.T. -0.04 min
 Lab File: BN006875.D
 Acq: 17 Jul 2019 16:36

Tgt Ion:202 Resp: 1571
 Ion Ratio Lower Upper
 202 100
 101 182.1 12.2 18.2#
 100 1254.0 9.8 14.8#

