

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071719\
 Data File : BN006882.D
 Acq On : 17 Jul 2019 20:41
 Operator : HP/JU
 Sample : K3772-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 18 01:08:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3424	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	12322	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	6252	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	787227	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	753205	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	3452	0.18	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.30	166	792	0.029	ng/ul#	Ovalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071719\
Data File : BN006882.D
Acq On : 17 Jul 2019 20:41
Operator : HP/JU
Sample : K3772-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 18 01:08:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

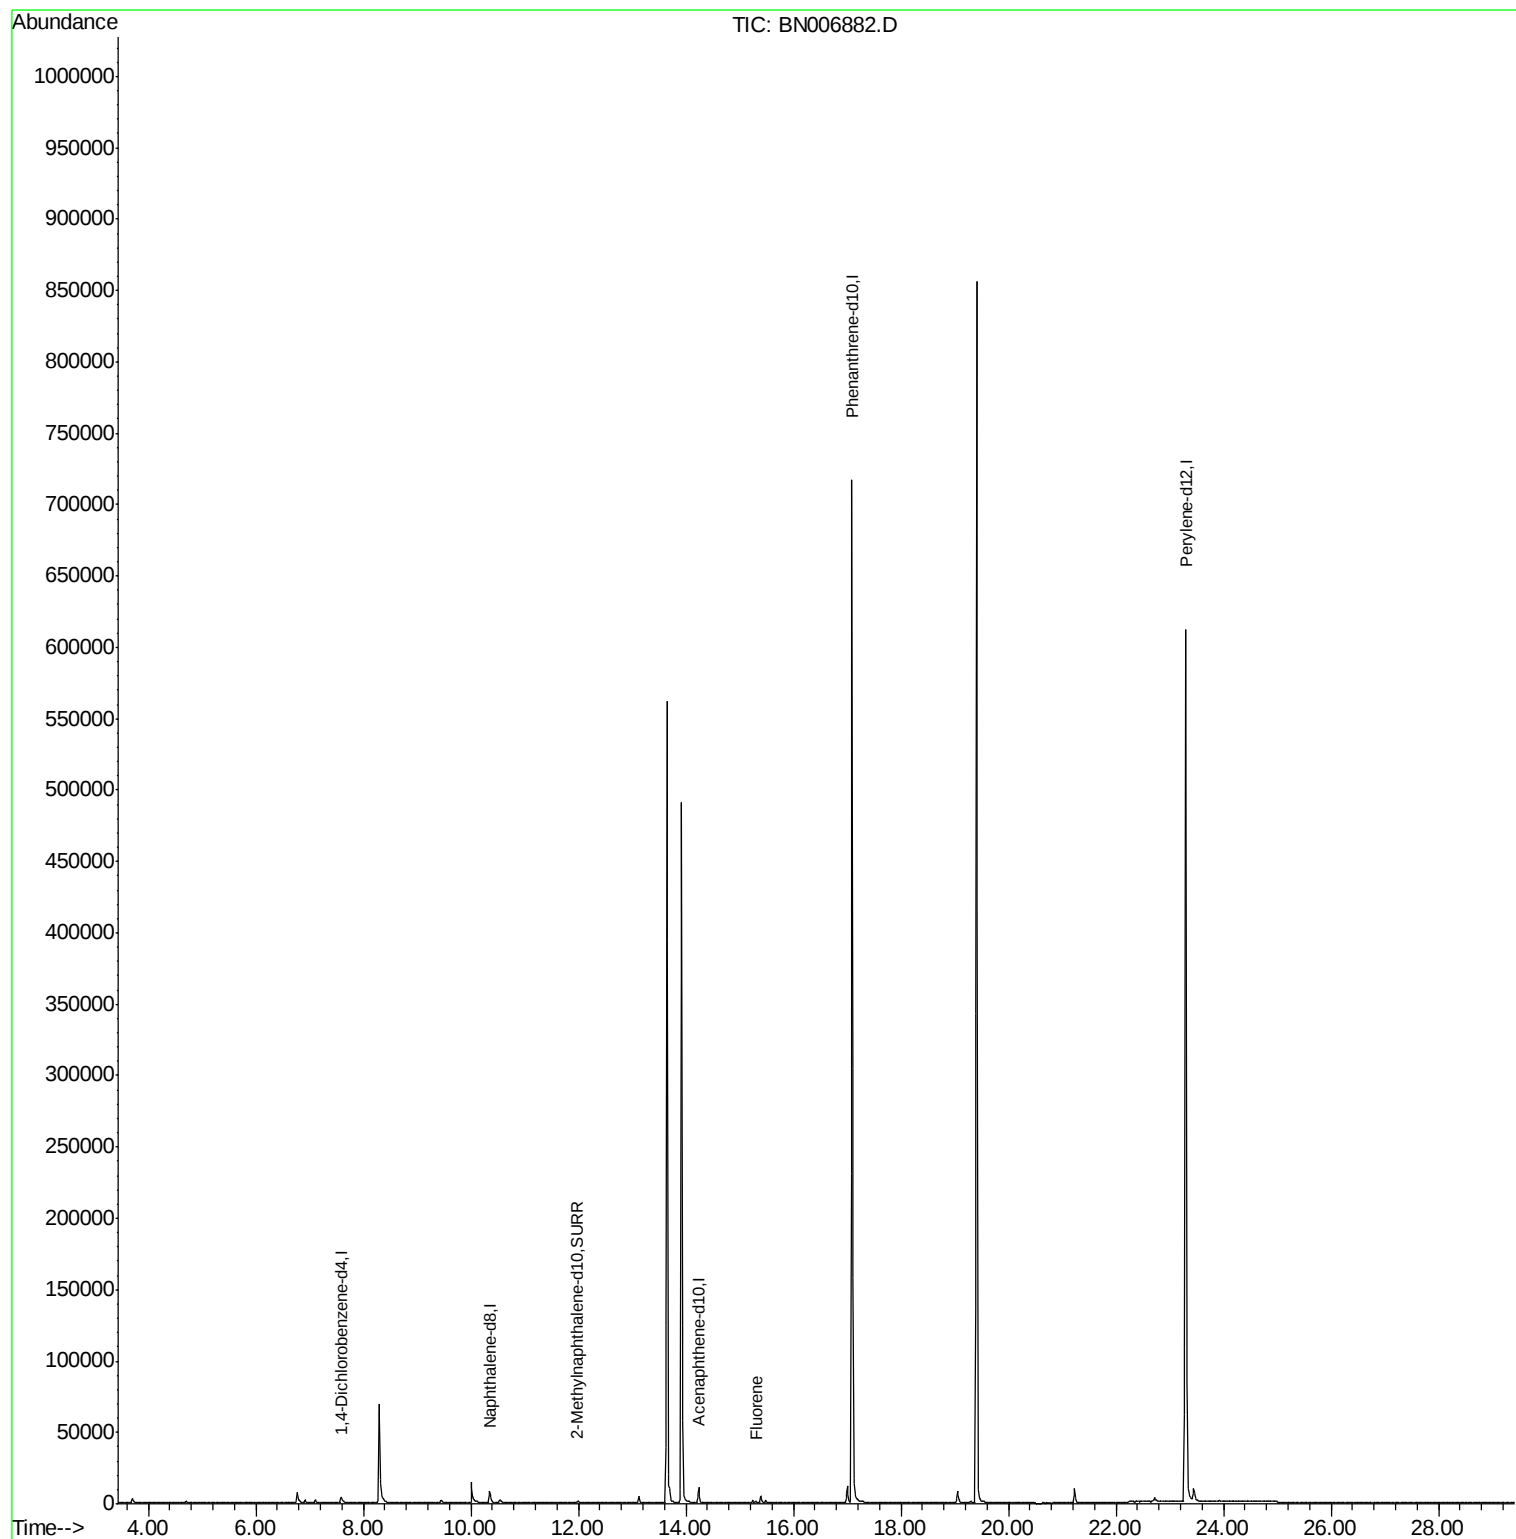

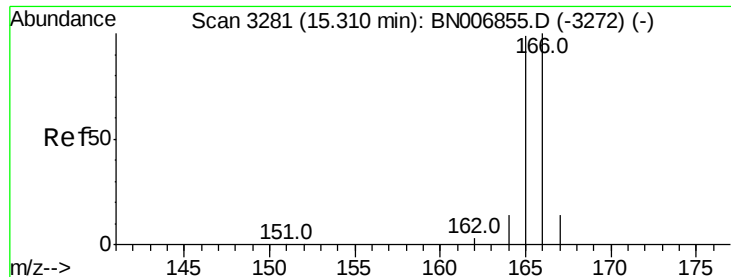

#9

Fluorene

Concen: 0.029 ng/ul

RT: 15.30 min Scan# 3278

Delta R.T. -0.01 min

Lab File: BN006882.D

Acq: 17 Jul 2019 20:41

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 792

Ion Ratio Lower Upper

166 100

165 95.7 78.2 117.4

167 24.2 11.3 16.9#

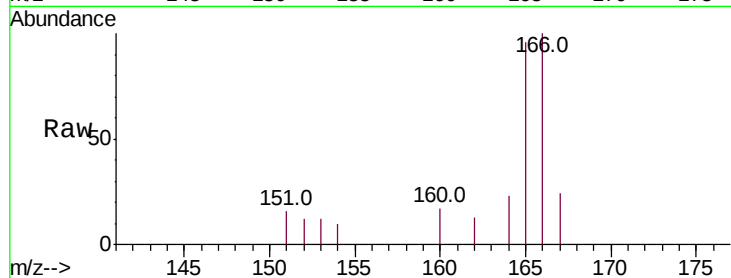

Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

