

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026529.D
 Acq On : 17 Jul 2023 10:20
 Operator : MA/JU
 Sample : 03457-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C49

Quant Time: Jul 18 03:03:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	2573	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	7250	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	4793	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	10854	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.523	240	8284	0.400	ng/ul	# 0.00
23) Perylene-d12	23.932	264	8486	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	13695	4.041	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.359	152	2358	0.239	ng/ul	0.01
18) Fluoranthene-d10	19.354	212	9110	0.317	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.717	202	1500	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.771	252	2447	0.083	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026529.D
Acq On : 17 Jul 2023 10:20
Operator : MA/JU
Sample : 03457-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C49

Quant Time: Jul 18 03:03:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration




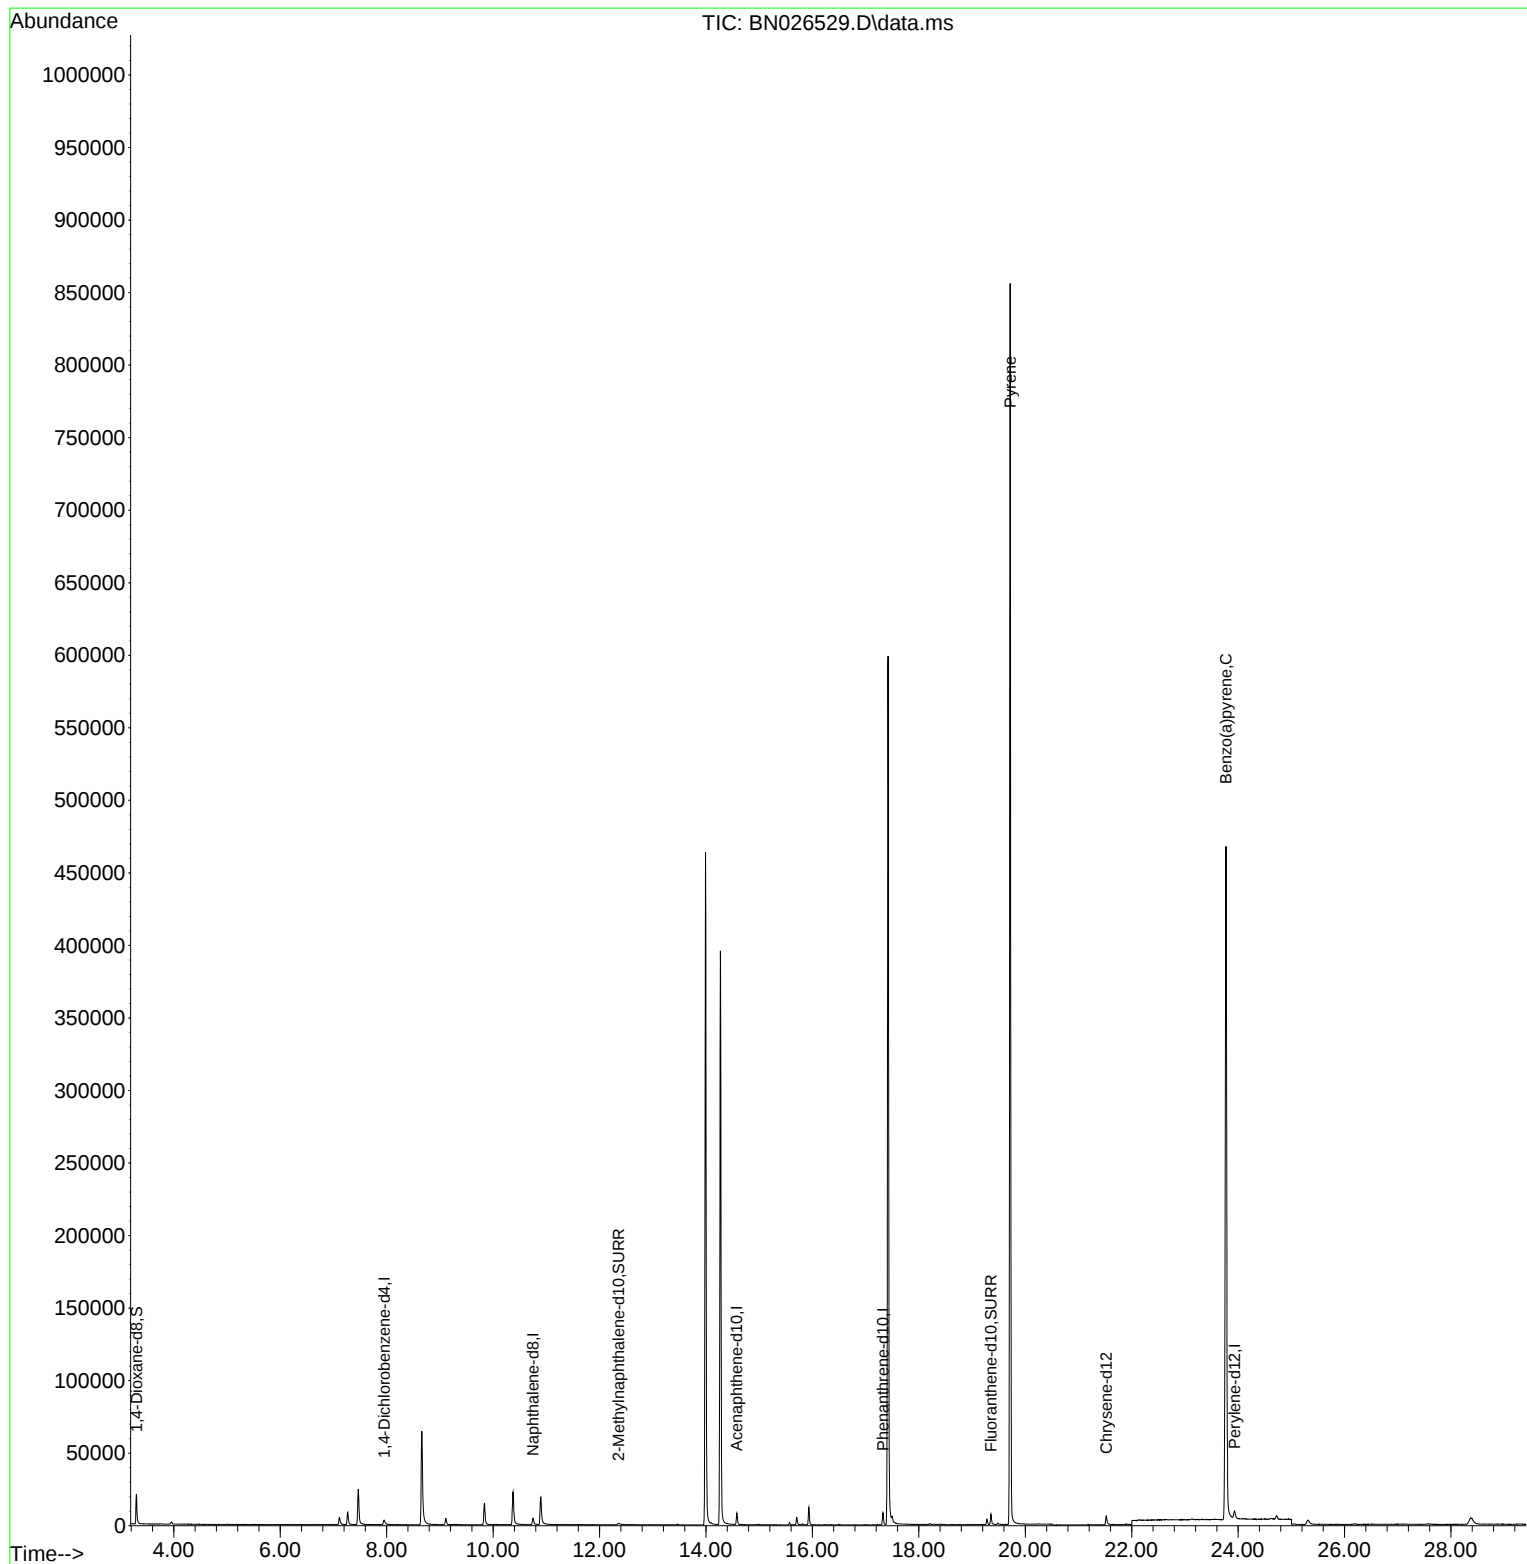


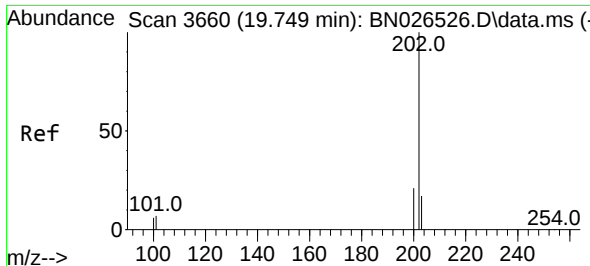

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.717 min Scan# 30
Delta R.T. -0.033 min
Lab File: BN026529.D
Acq: 17 Jul 2023 10:20

Instrument :
BNA_N
ClientSampleId :
C0C49

Tgt Ion:202 Resp: 1500
Ion Ratio Lower Upper
202 100
101 193.6 8.0 12.0#
100 1554.4 6.2 9.2#

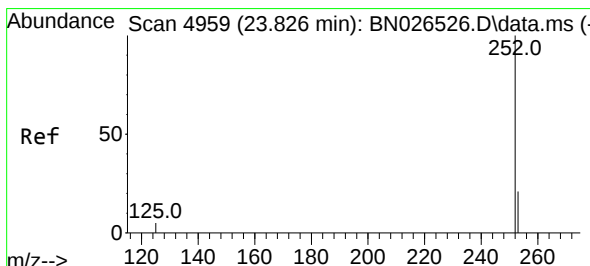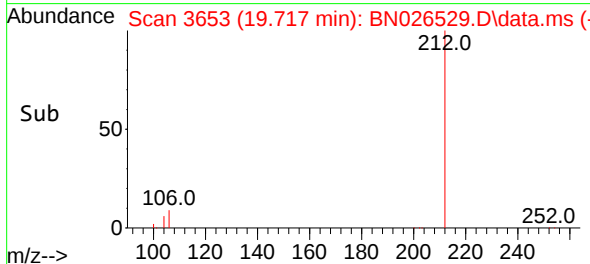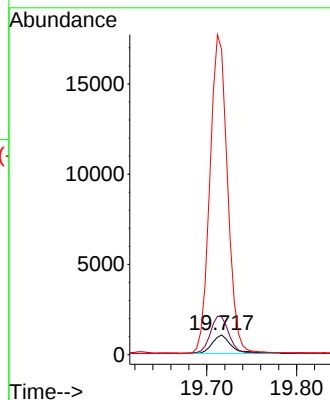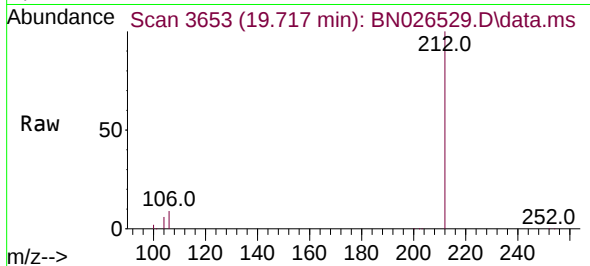

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.771 min Scan# 4940
Delta R.T. -0.056 min
Lab File: BN026529.D
Acq: 17 Jul 2023 10:20

Tgt Ion:252 Resp: 2447
Ion Ratio Lower Upper
252 100
253 66.1 32.6 49.0#
125 62.0 19.3 28.9#

