

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026530.D
 Acq On : 17 Jul 2023 10:57
 Operator : MA/JU
 Sample : 03457-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C52

Quant Time: Jul 18 03:03:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	2463	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	7194	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	4616	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	10107	0.400	ng/ul	0.00
17) Chrysene-d12	21.520	240	7758	0.400	ng/ul	# 0.00
23) Perylene-d12	23.929	264	8633	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	13166	4.059	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	2660	0.272	ng/ul	0.00
18) Fluoranthene-d10	19.354	212	7979	0.297	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.717	202	1382	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.768	252	2393	0.080	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026530.D
Acq On : 17 Jul 2023 10:57
Operator : MA/JU
Sample : 03457-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C52

Quant Time: Jul 18 03:03:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

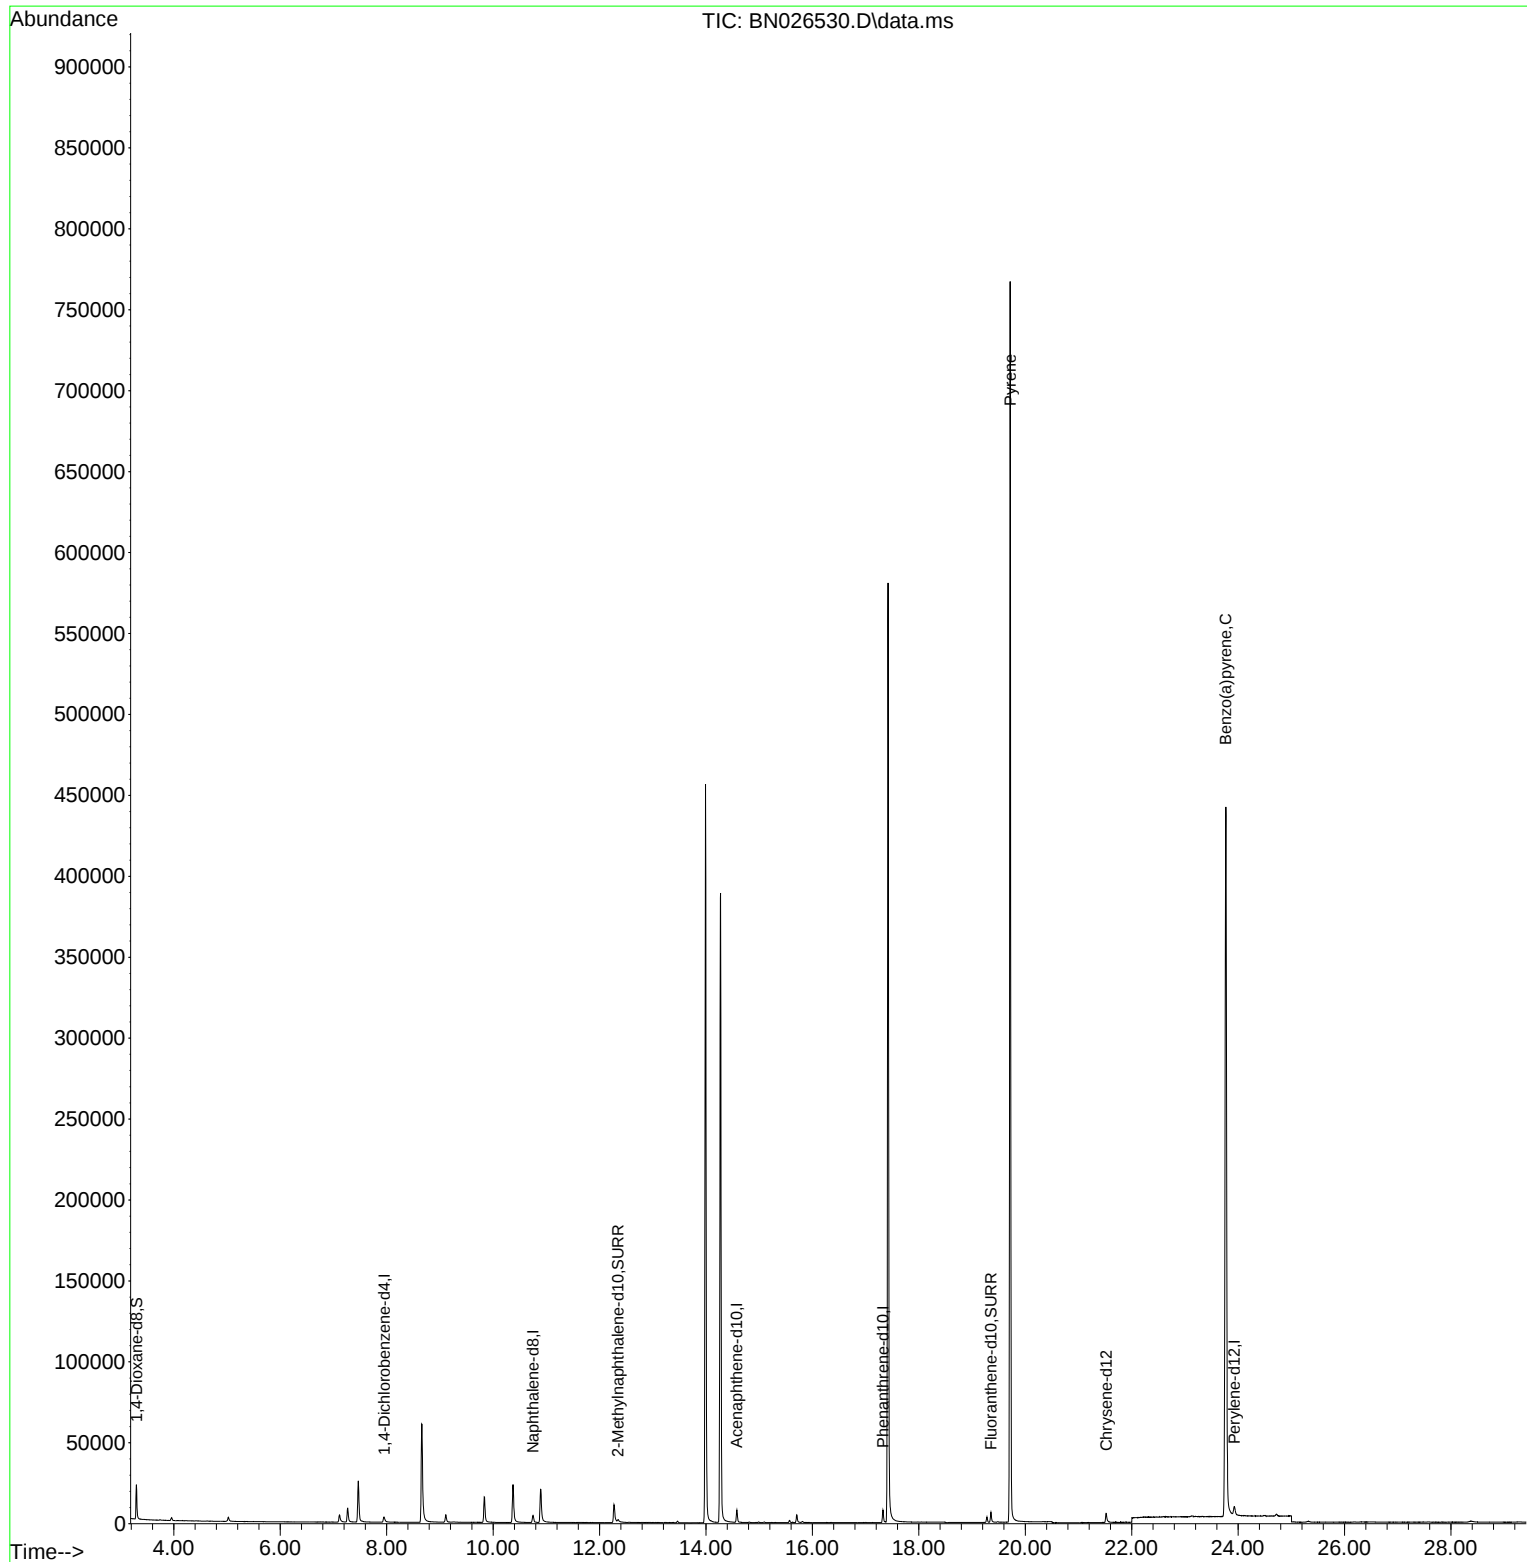

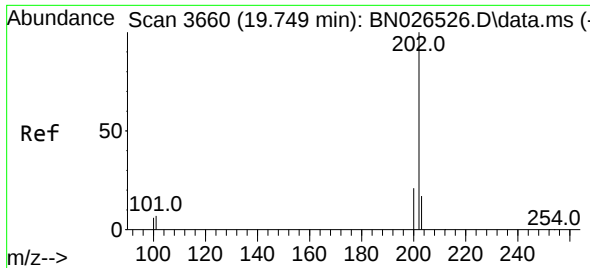

#20

Pyrene

Concen: 0.035 ng/ul

RT: 19.717 min Scan# 3

Delta R.T. -0.033 min

Lab File: BN026530.D

Acq: 17 Jul 2023 10:57

Instrument :

BNA_N

ClientSampleId :

C0C52





Tgt Ion:202 Resp: 1382

Ion Ratio Lower Upper

202 100

101 195.1 8.0 12.0#

100 1518.5 6.2 9.2#

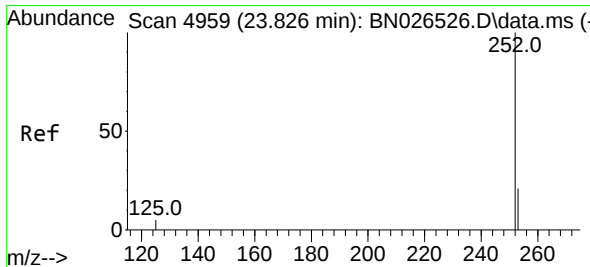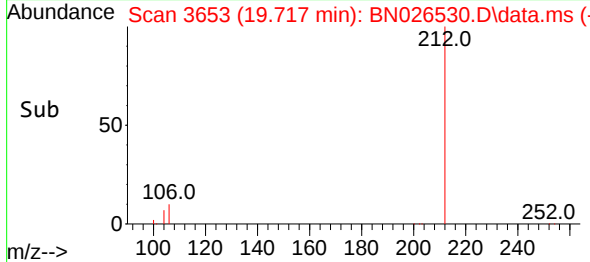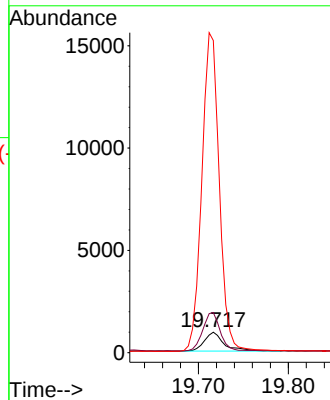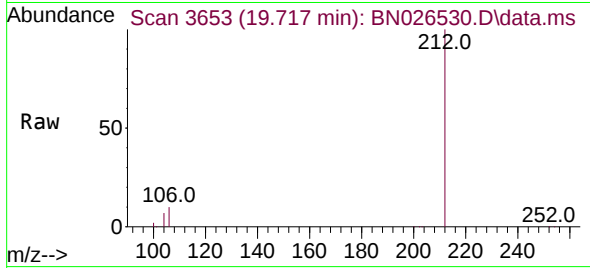

#26

Benzo(a)pyrene

Concen: 0.080 ng/ul

RT: 23.768 min Scan# 4939

Delta R.T. -0.059 min

Lab File: BN026530.D

Acq: 17 Jul 2023 10:57

Tgt Ion:252 Resp: 2393

Ion Ratio Lower Upper

252 100

253 71.9 32.6 49.0#

125 64.8 19.3 28.9#

