

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026534.D
 Acq On : 17 Jul 2023 13:24
 Operator : MA/JU
 Sample : 03457-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C50

Quant Time: Jul 18 03:04:15 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	2196	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	6576	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.584	164	4217	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	9082	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.523	240	8326	0.400	ng/ul	# 0.00
23) Perylene-d12	23.932	264	8889	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	8609	2.977	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.365	152	2188	0.245	ng/ul	0.02
18) Fluoranthene-d10	19.359	212	7503	0.260	ng/ul	0.00
Target Compounds						
					Qvalue	
26) Benzo(a)pyrene	23.774	252	952	0.031	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026534.D
Acq On : 17 Jul 2023 13:24
Operator : MA/JU
Sample : 03457-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C50


Quant Time: Jul 18 03:04:15 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

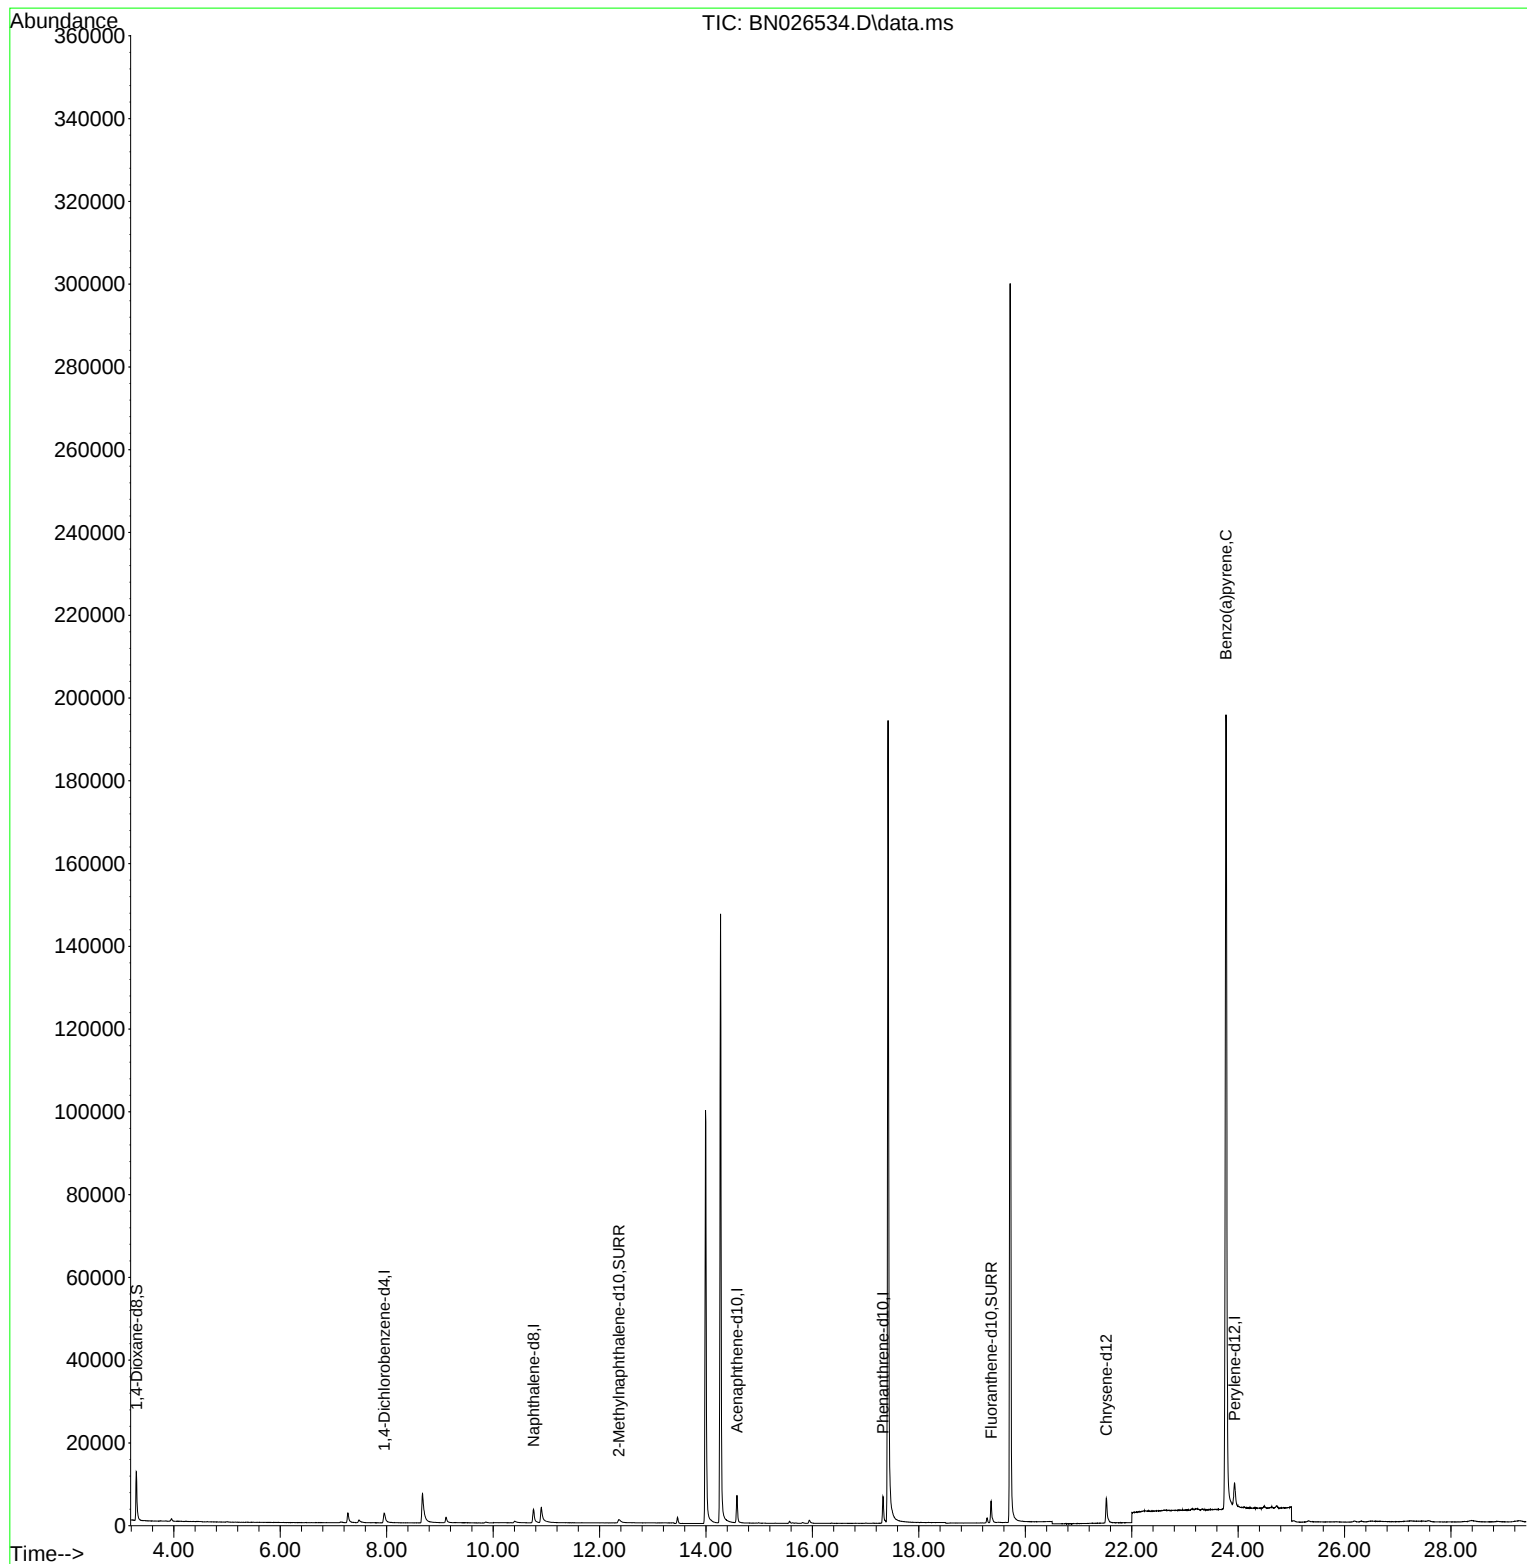

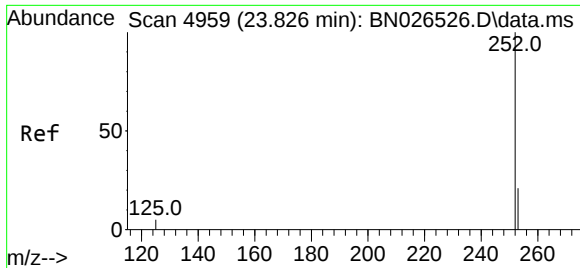

#26
 Benzo(a)pyrene
 Concen: 0.031 ng/ul
 RT: 23.774 min Scan# 4959
 Delta R.T. -0.053 min
 Lab File: BN026534.D
 Acq: 17 Jul 2023 13:24

Instrument :
 BNA_N
 ClientSampleId :
 C0C50

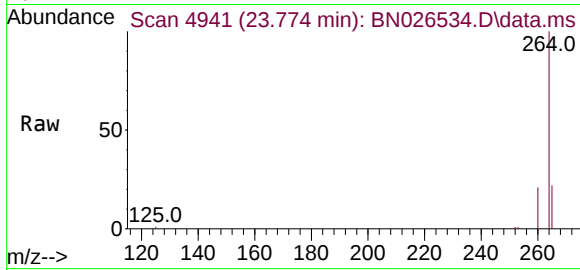

Tgt Ion:252 Resp: 952

Ion	Ratio	Lower	Upper
252	100		
253	96.4	32.6	49.0#
125	82.6	19.3	28.9#

