

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026536.D
 Acq On : 17 Jul 2023 14:39
 Operator : MA/JU
 Sample : 03457-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C47

Quant Time: Jul 18 03:04:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	2204	0.400	ng/ul	0.00
4) Naphthalene-d8	10.747	136	6106	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	4049	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	9085	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.528	240	7307	0.400	ng/ul	# 0.00
23) Perylene-d12	23.937	264	7951	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	12846	4.426	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.358	152	2842	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.358	212	9042	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.716	202	1687	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.776	252	2832	0.103	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026536.D
Acq On : 17 Jul 2023 14:39
Operator : MA/JU
Sample : 03457-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C47

Quant Time: Jul 18 03:04:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration




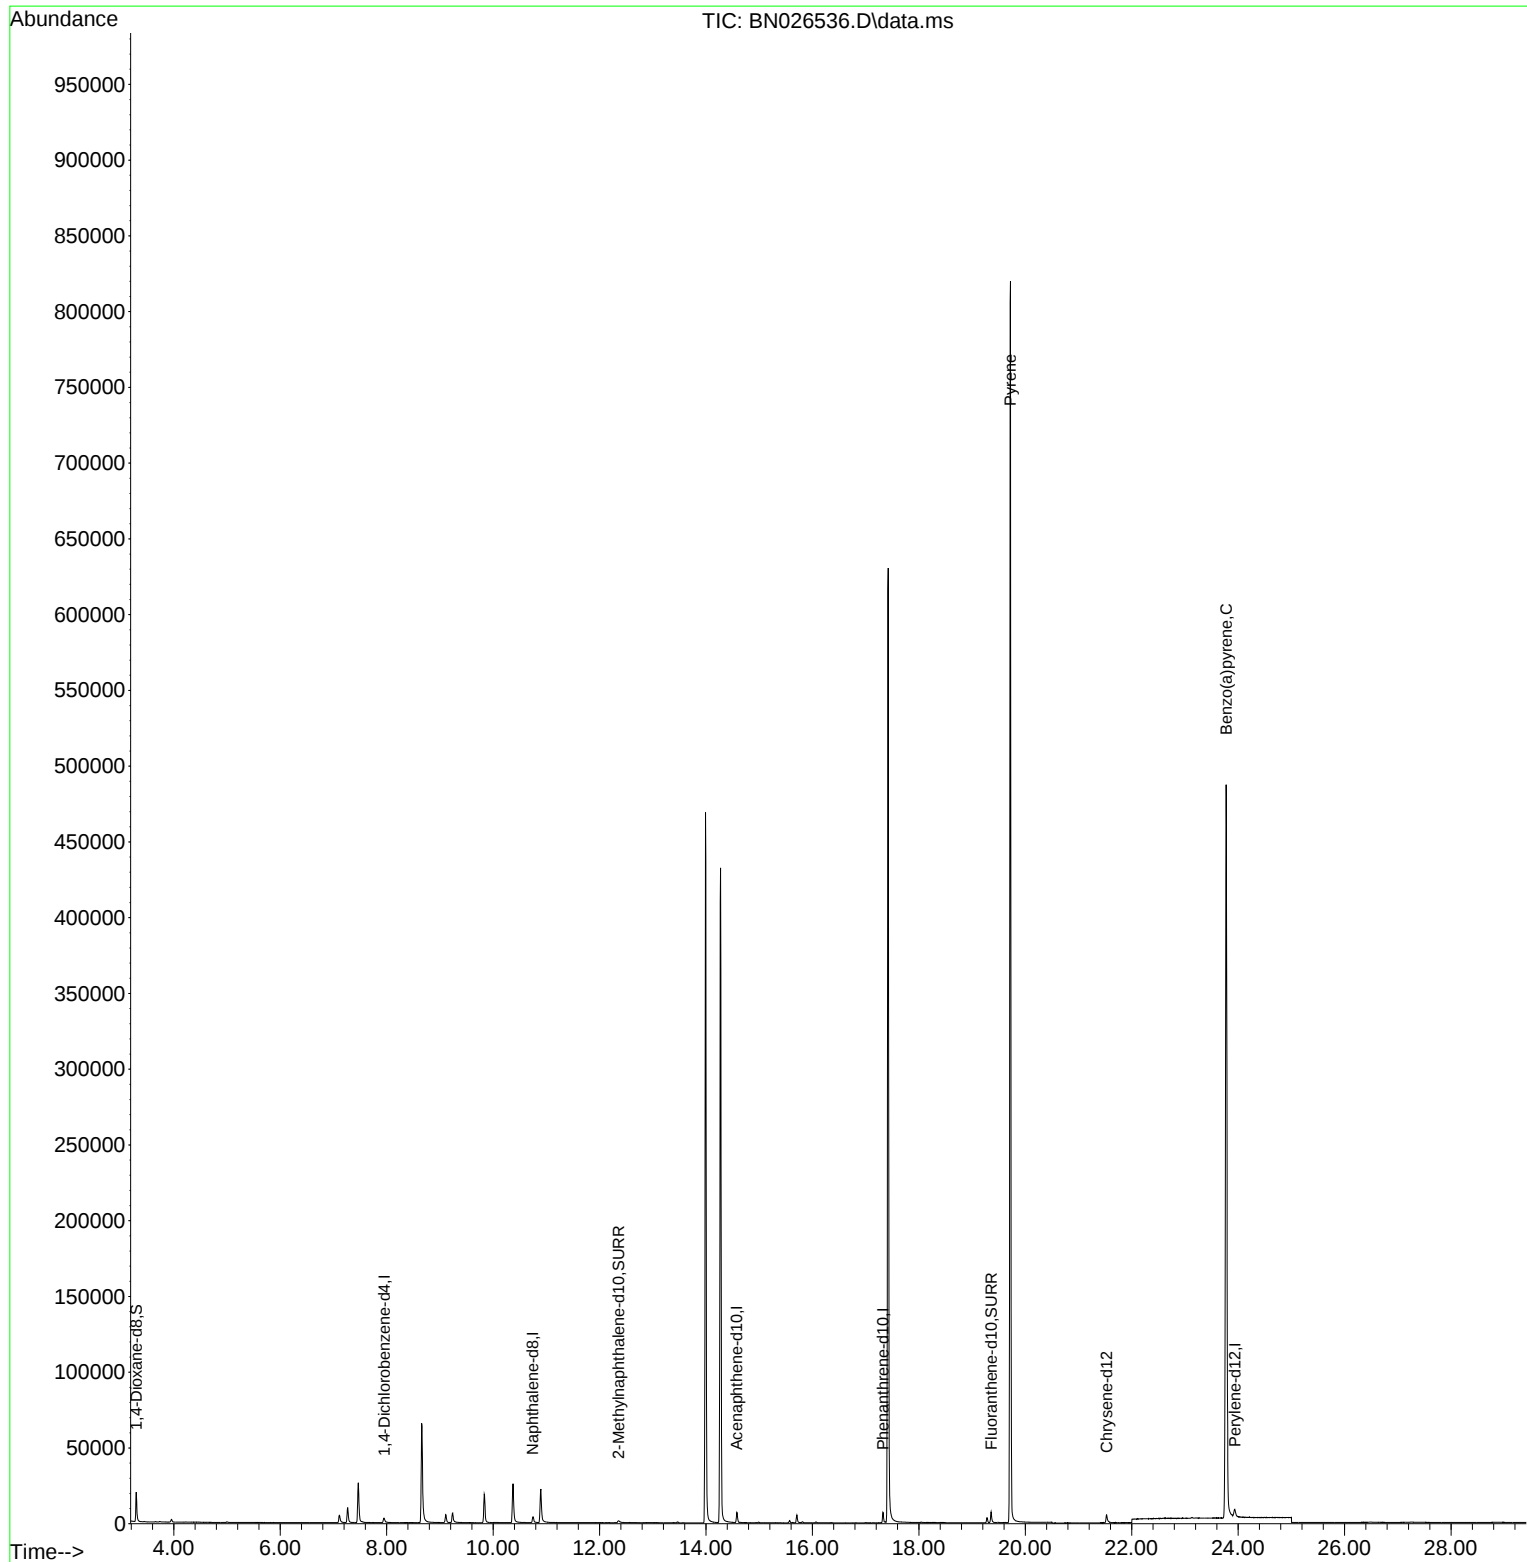


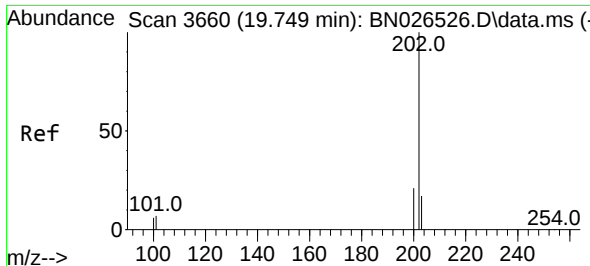

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.716 min Scan# 3653
Delta R.T. -0.033 min
Lab File: BN026536.D
Acq: 17 Jul 2023 14:39

Instrument :
BNA_N
ClientSampleId :
C0C47

Tgt Ion:202 Resp: 1687
Ion Ratio Lower Upper
202 100
101 214.4 8.0 12.0#
100 1808.4 6.2 9.2#

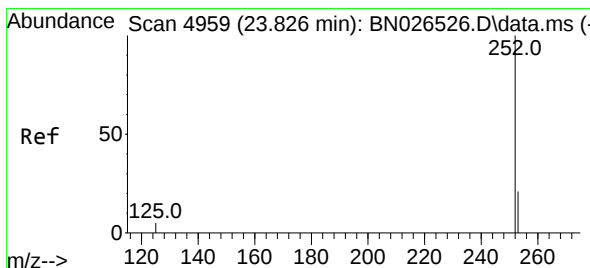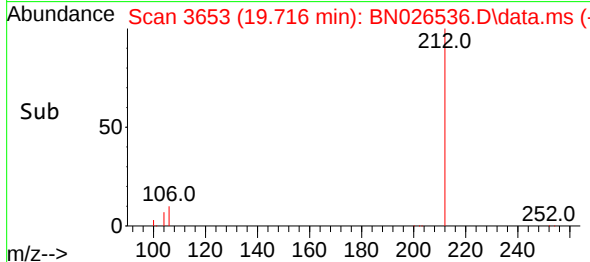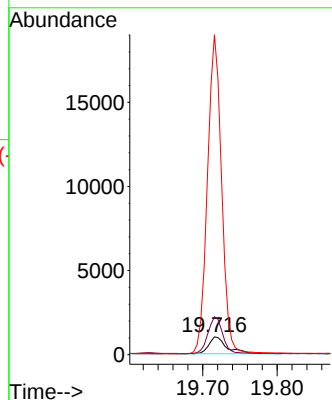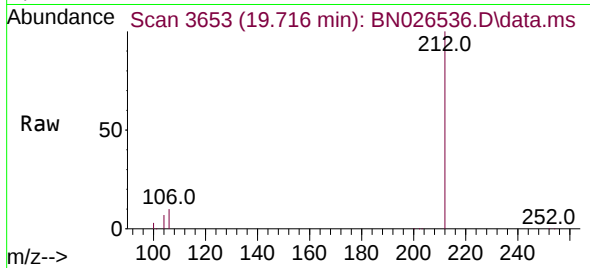

#26
Benzo(a)pyrene
Concen: 0.103 ng/ul
RT: 23.776 min Scan# 4942
Delta R.T. -0.051 min
Lab File: BN026536.D
Acq: 17 Jul 2023 14:39

Tgt Ion:252 Resp: 2832
Ion Ratio Lower Upper
252 100
253 63.6 32.6 49.0#
125 44.3 19.3 28.9#

