

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026540.D
 Acq On : 17 Jul 2023 17:08
 Operator : MA/JU
 Sample : PB153904BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK904

Quant Time: Jul 18 03:05:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	2343	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	6118	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	4222	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	9529	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.526	240	7139	0.400	ng/ul	# 0.00
23) Perylene-d12	23.932	264	8121	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	15367	4.980	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.365	152	2127	0.256	ng/ul	0.02
18) Fluoranthene-d10	19.359	212	7468	0.302	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.716	202	1339	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.768	252	2377	0.084	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026540.D
Acq On : 17 Jul 2023 17:08
Operator : MA/JU
Sample : PB153904BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK904

Quant Time: Jul 18 03:05:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

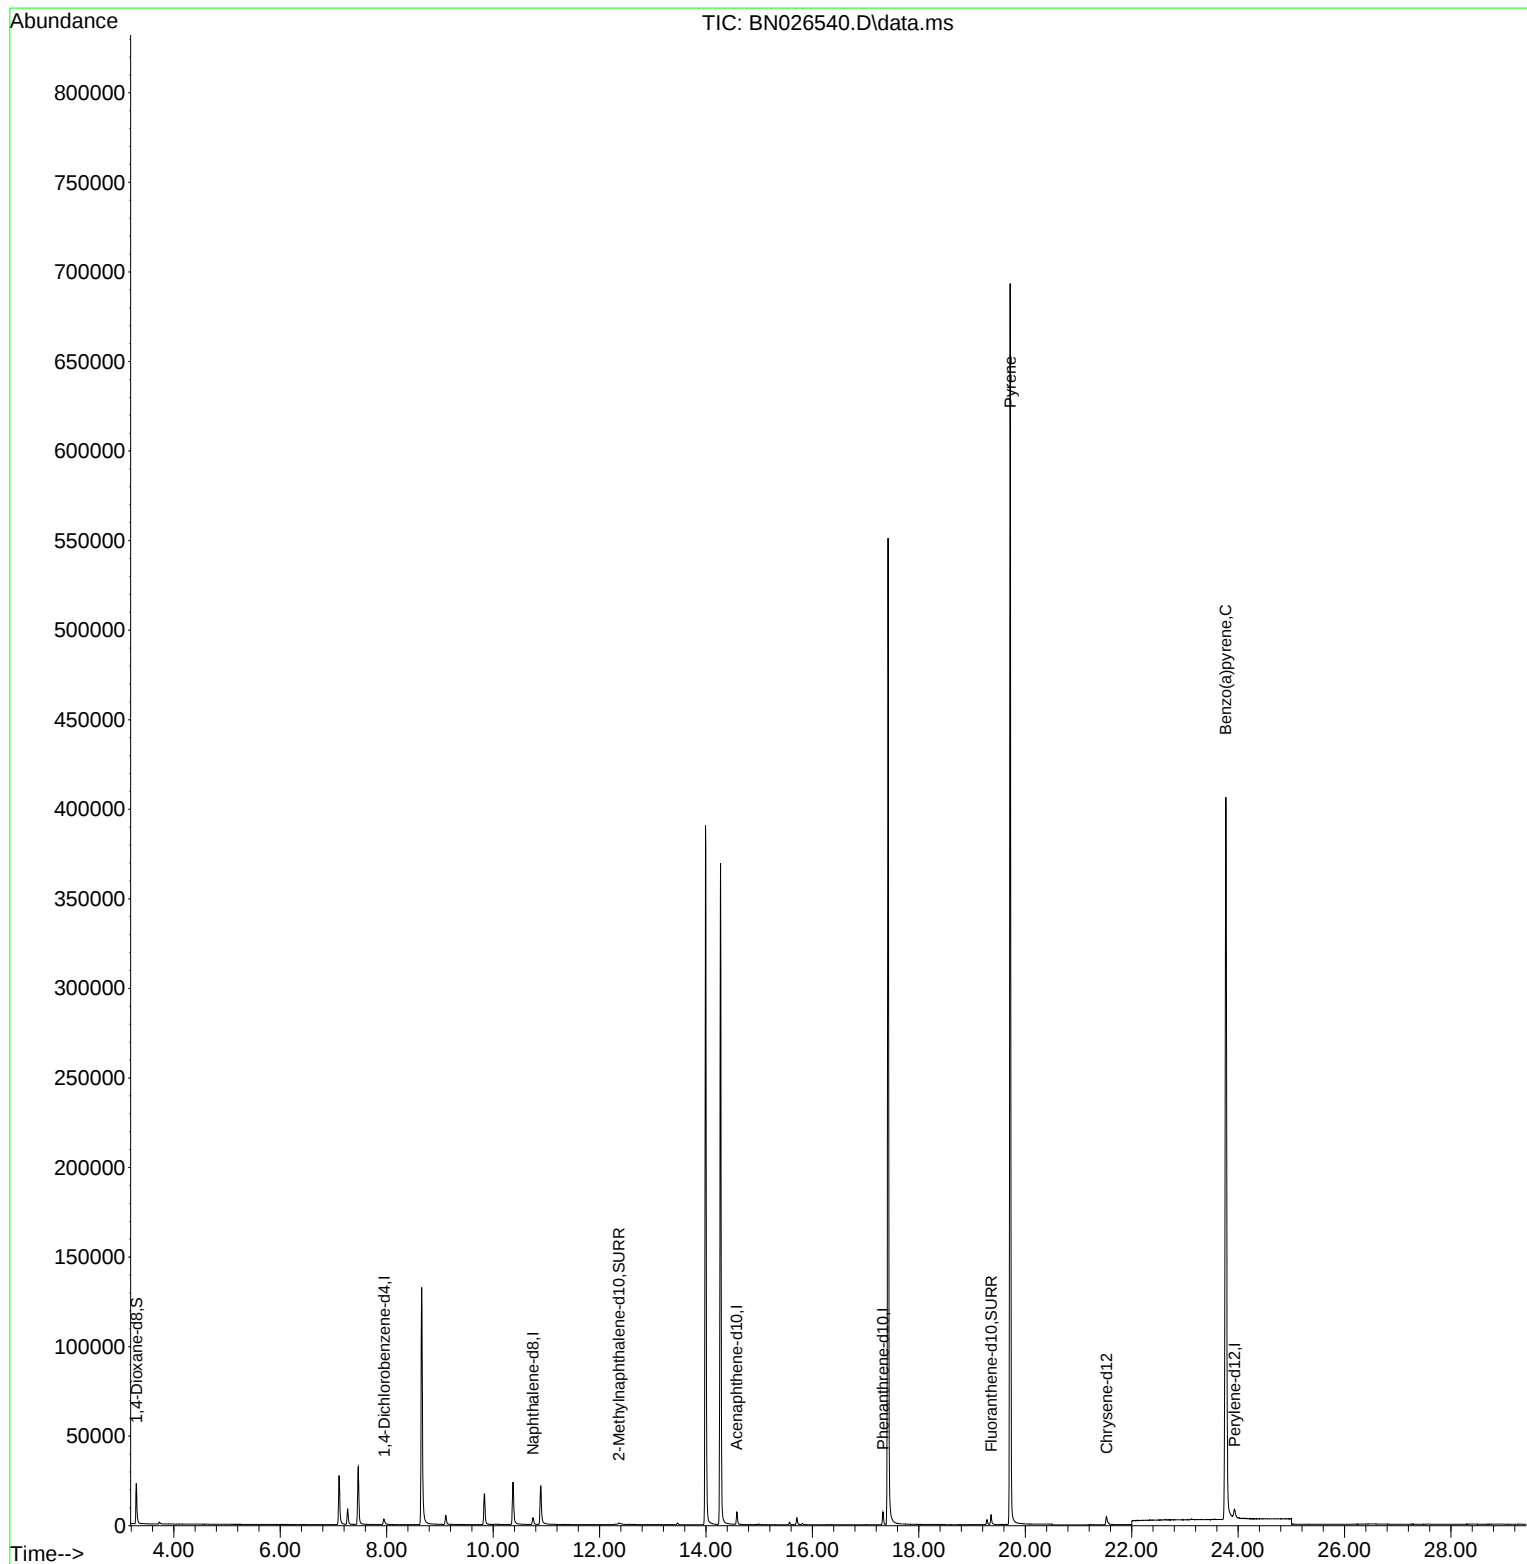

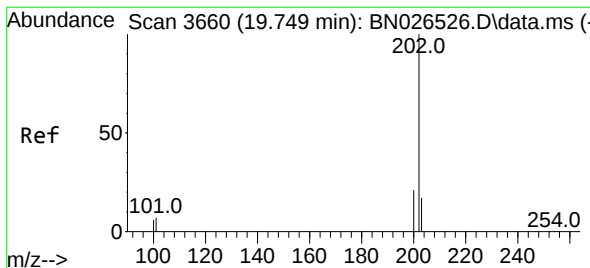

#20

Pyrene

Concen: 0.037 ng/ul

RT: 19.716 min Scan# 3

Delta R.T. -0.033 min

Lab File: BN026540.D

Acq: 17 Jul 2023 17:08

Instrument :





BNA_N

ClientSampleId :

SBLK904

Tgt Ion:202 Resp: 1339

Ion	Ratio	Lower	Upper
202	100		
101	207.8	8.0	12.0#
100	1710.8	6.2	9.2#

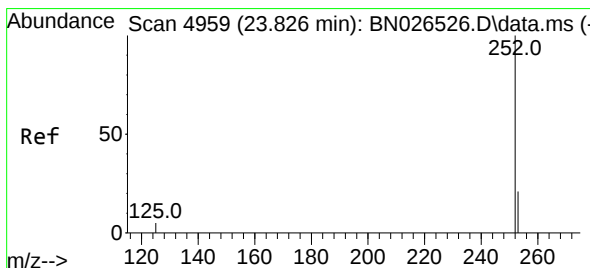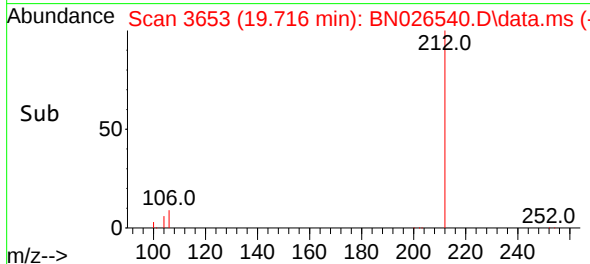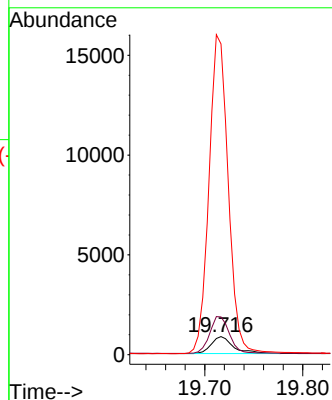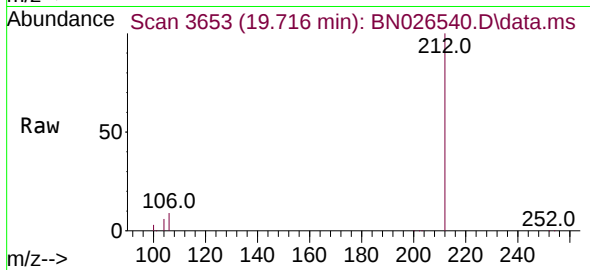

#26

Benzo(a)pyrene

Concen: 0.084 ng/ul

RT: 23.768 min Scan# 4939

Delta R.T. -0.059 min

Lab File: BN026540.D

Acq: 17 Jul 2023 17:08

Tgt Ion:252 Resp: 2377

Ion	Ratio	Lower	Upper
252	100		
253	65.7	32.6	49.0#
125	47.2	19.3	28.9#

