

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026546.D
 Acq On : 17 Jul 2023 20:53
 Operator : MA/JU
 Sample : 03458-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A46L8

Quant Time: Jul 18 04:22:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	3100	0.400	ng/ul	0.00
4) Naphthalene-d8	10.747	136	9719	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	6305	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	14150	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.516	240	11743	0.400	ng/ul	# 0.00
23) Perylene-d12	23.928	264	11479	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	19529	4.783	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.353	152	2971	0.225	ng/ul	0.00
18) Fluoranthene-d10	19.353	212	9341	0.229	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.764	252	2909	0.073	ng/ul#	Qvalue 50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026546.D
Acq On : 17 Jul 2023 20:53
Operator : MA/JU
Sample : 03458-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A46L8

Quant Time: Jul 18 04:22:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

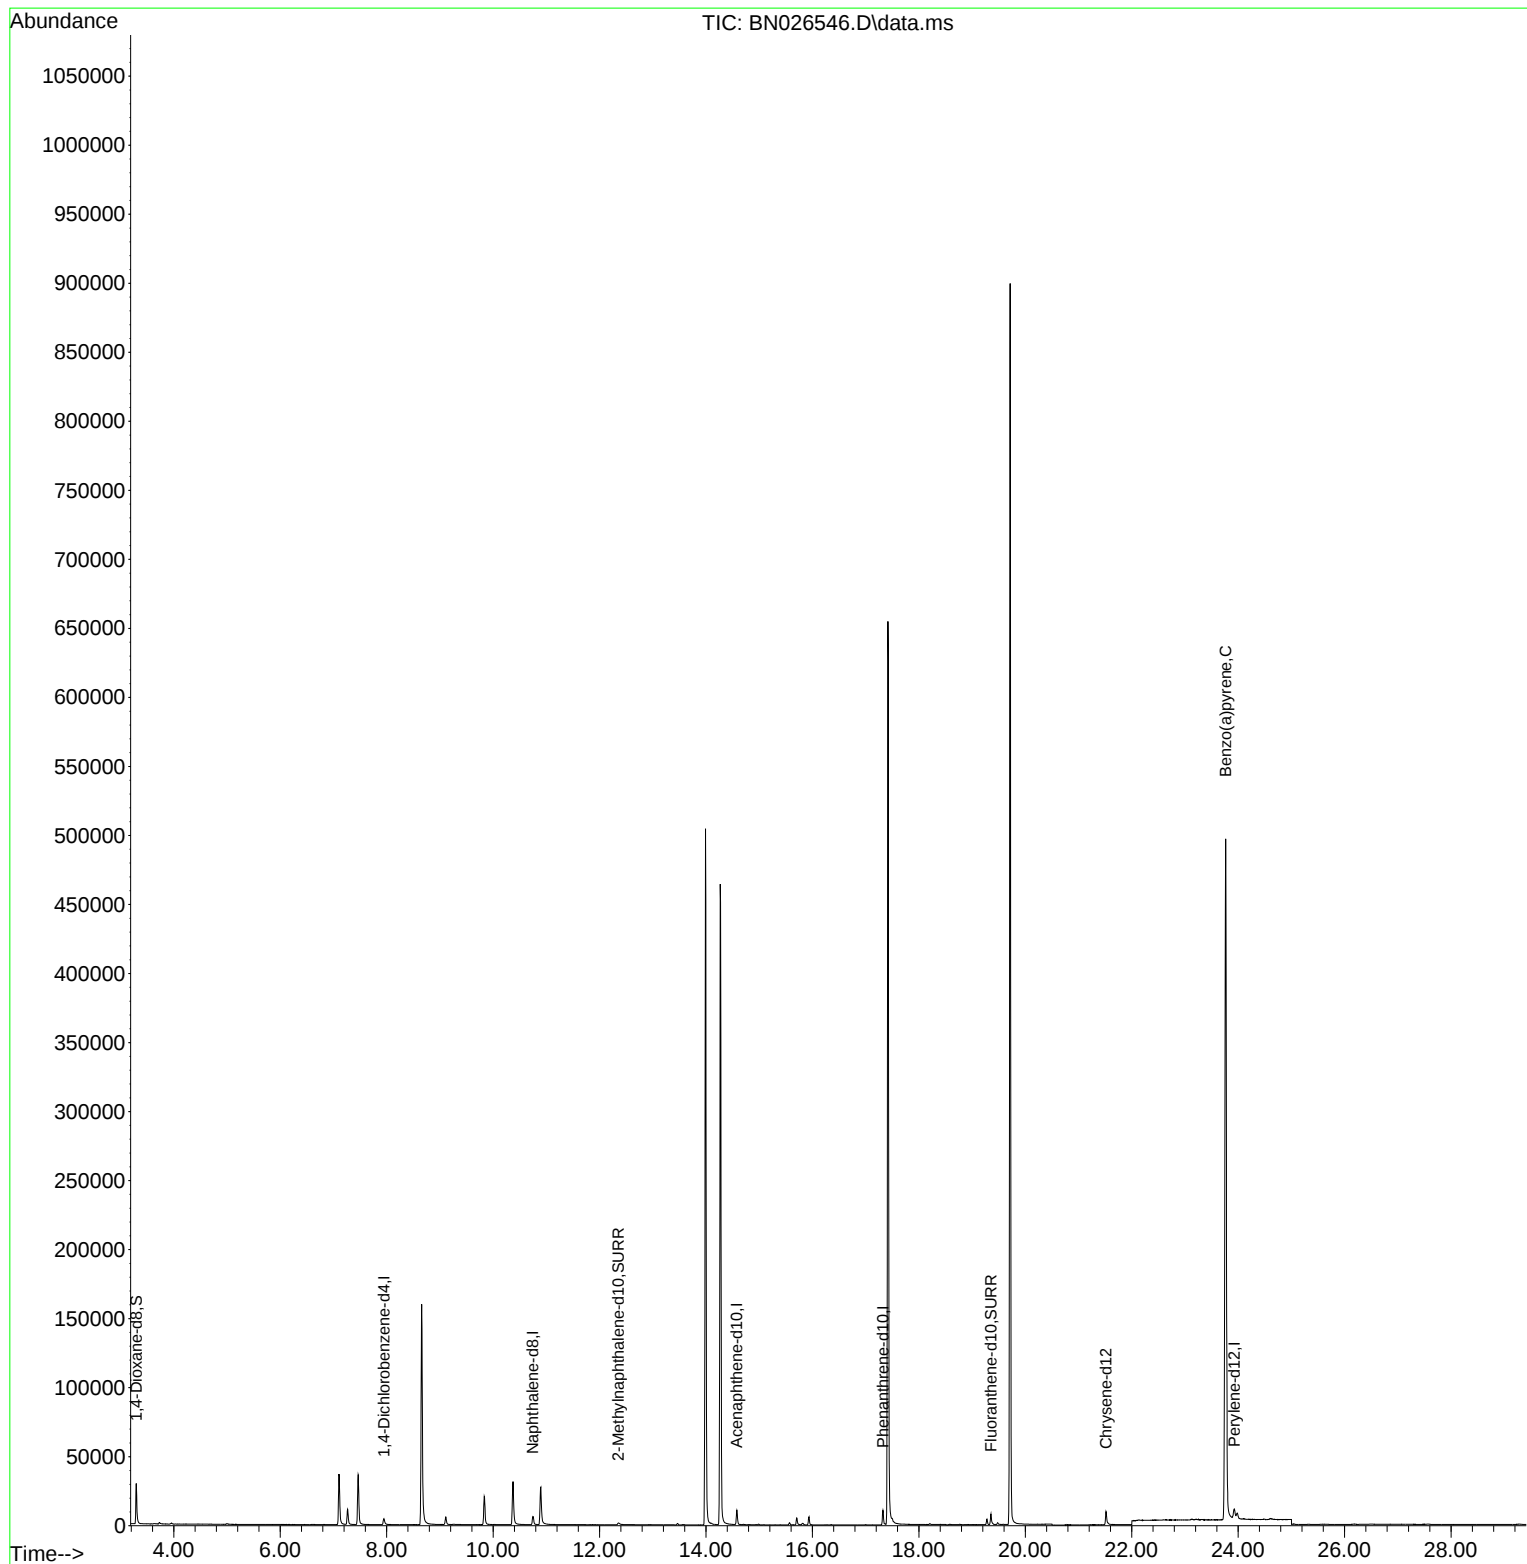

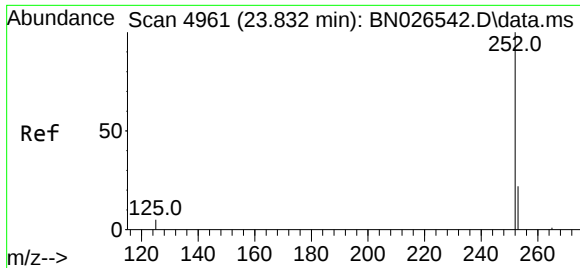

#26
 Benzo(a)pyrene
 Concen: 0.073 ng/ul
 RT: 23.764 min Scan# 4961
 Delta R.T. -0.062 min
 Lab File: BN026546.D
 Acq: 17 Jul 2023 20:53

Instrument :
 BNA_N
 ClientSampleId :
 A46L8

Tgt Ion:252	Resp:	2909
Ion Ratio	Lower	Upper
252	100	
253	65.3	32.6 49.0#
125	57.3	19.3 28.9#

