

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026557.D
 Acq On : 18 Jul 2023 03:39
 Operator : MA/JU
 Sample : 03458-26
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A46L6

Quant Time: Jul 18 04:24:46 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	561	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	1415	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.579	164	721	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.326	188	1369	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.523	240	1081	0.400	ng/ul	# 0.00
23) Perylene-d12	23.922	264	1728	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	3207	4.341	ng/ul	0.03
6) 2-Methylnaphthalene-d10	12.359	152	410	0.213	ng/ul	0.01
18) Fluoranthene-d10	19.358	212	1030	0.275	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.988	266	7	0.020	ng/ul#	Qvalue 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026557.D
Acq On : 18 Jul 2023 03:39
Operator : MA/JU
Sample : 03458-26
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A46L6


Quant Time: Jul 18 04:24:46 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

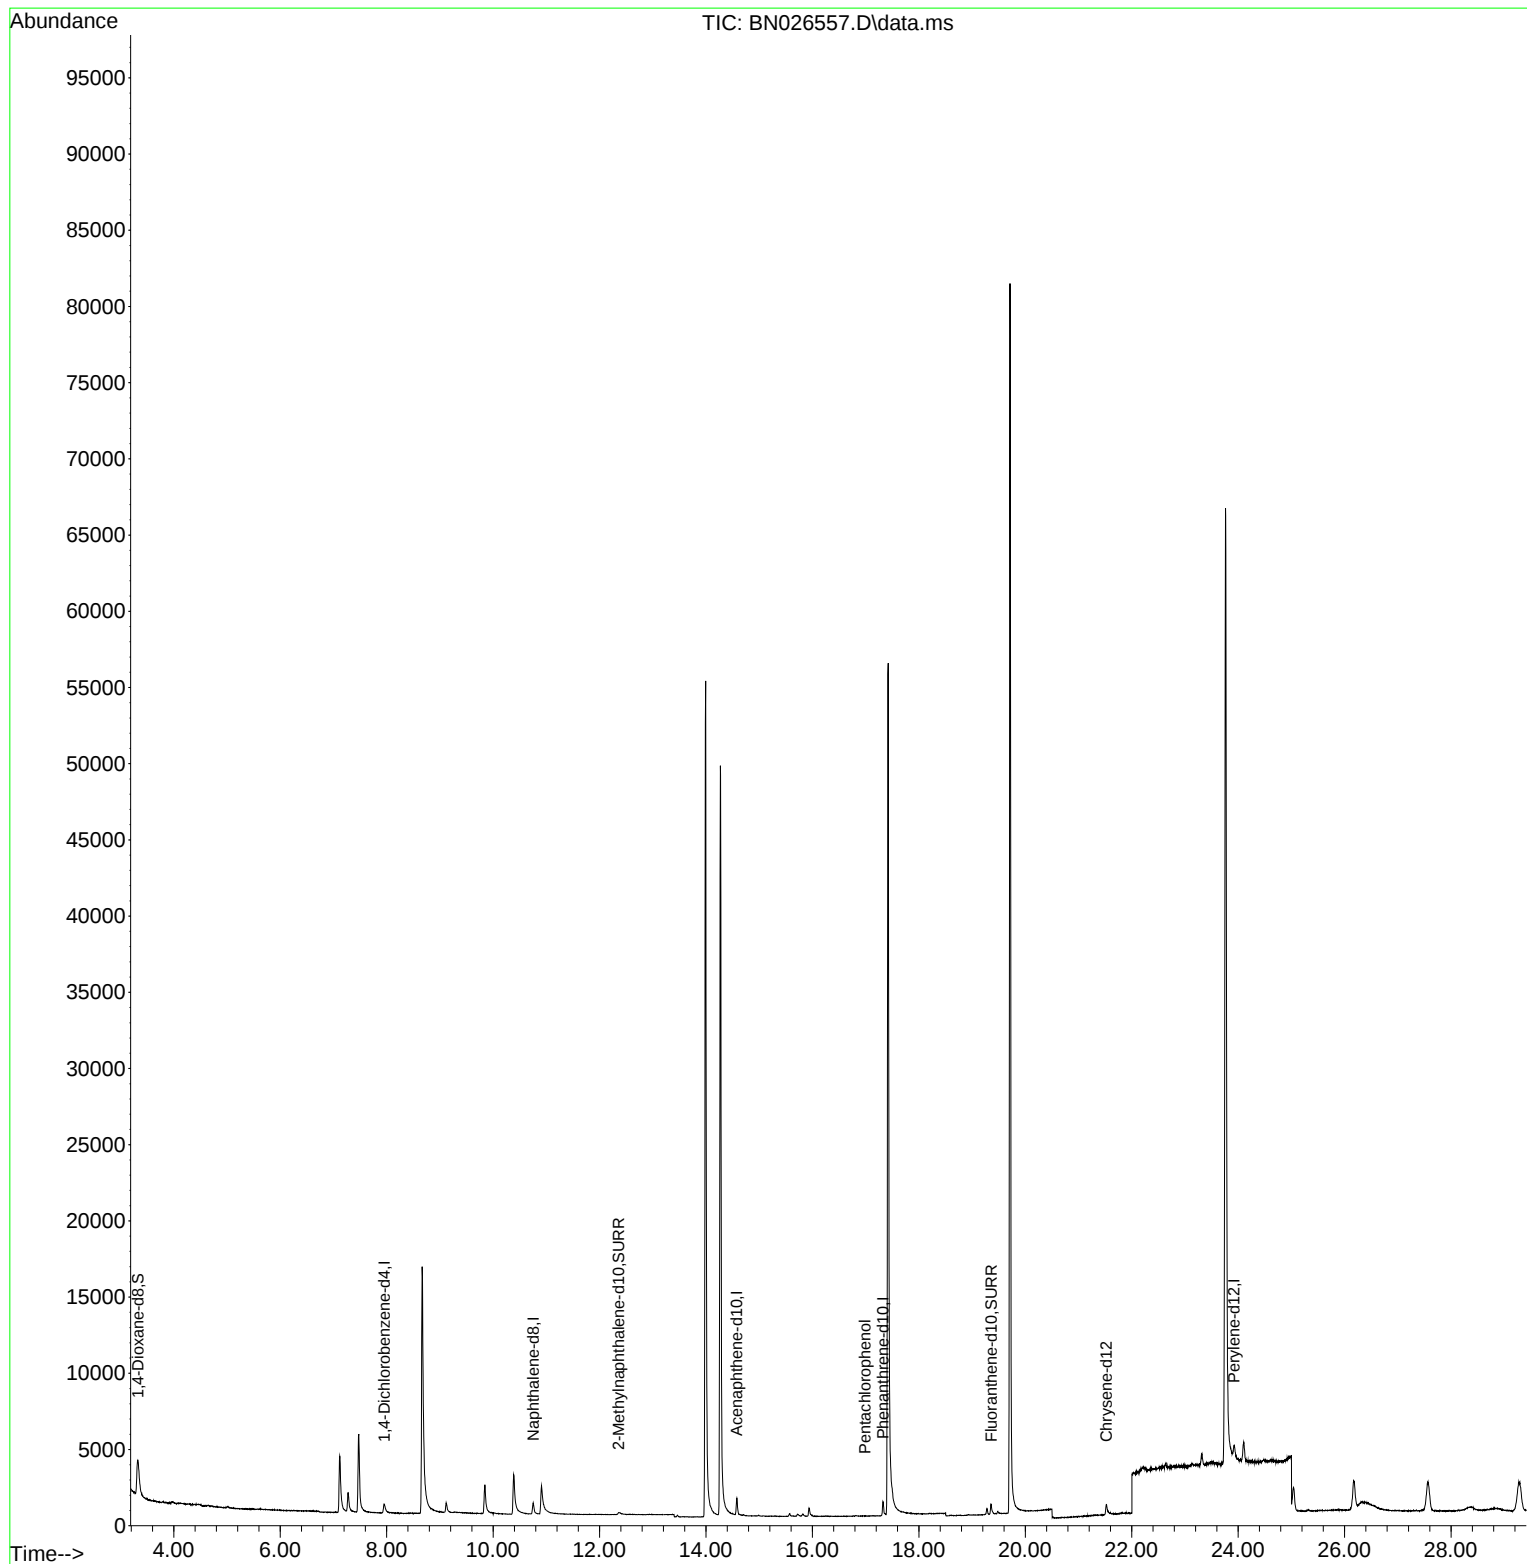

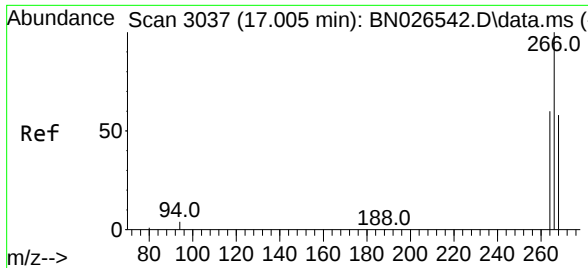

#14
 Pentachlorophenol
 Concen: 0.020 ng/ul
 RT: 16.988 min Scan# 30
 Delta R.T. -0.008 min
 Lab File: BN026557.D
 Acq: 18 Jul 2023 03:39

Instrument :
 BNA_N
 ClientSampleId :
 A46L6

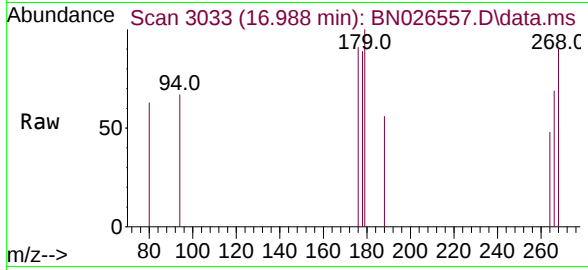

Tgt Ion:266 Resp: 7

Ion	Ratio	Lower	Upper
266	100		
264	0.0	52.0	78.0#
268	100.0	53.0	79.6#

