




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026527.D
 Acq On : 17 Jul 2023 09:06
 Operator : MA/JU
 Sample : PB153870BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK870

Manual IntegrationsAPPROVED

Quant Time: Jul 17 17:14:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :Sohil Jodhani 07/17/2023

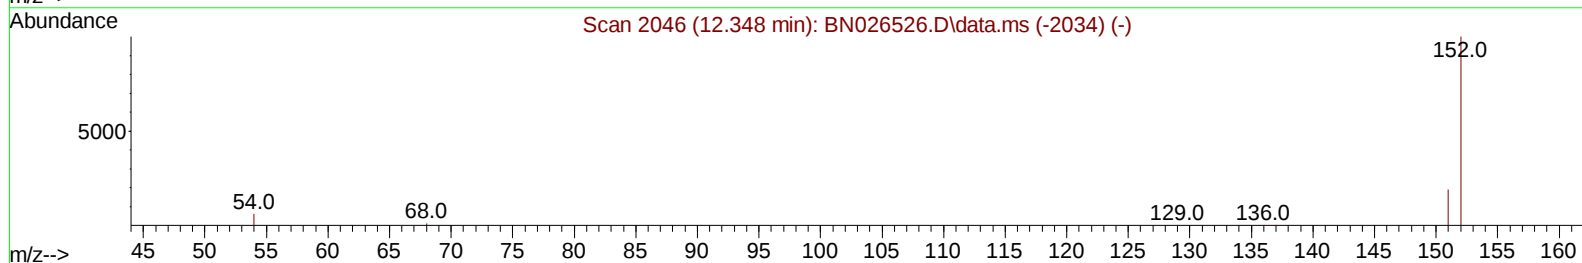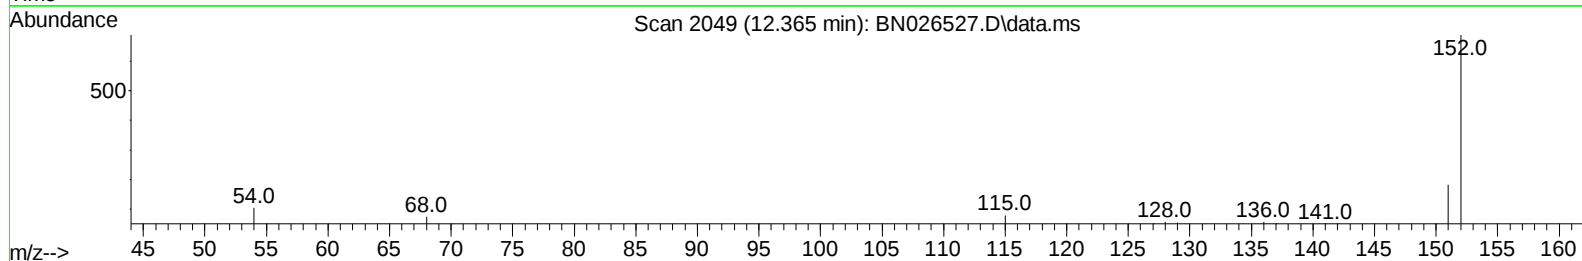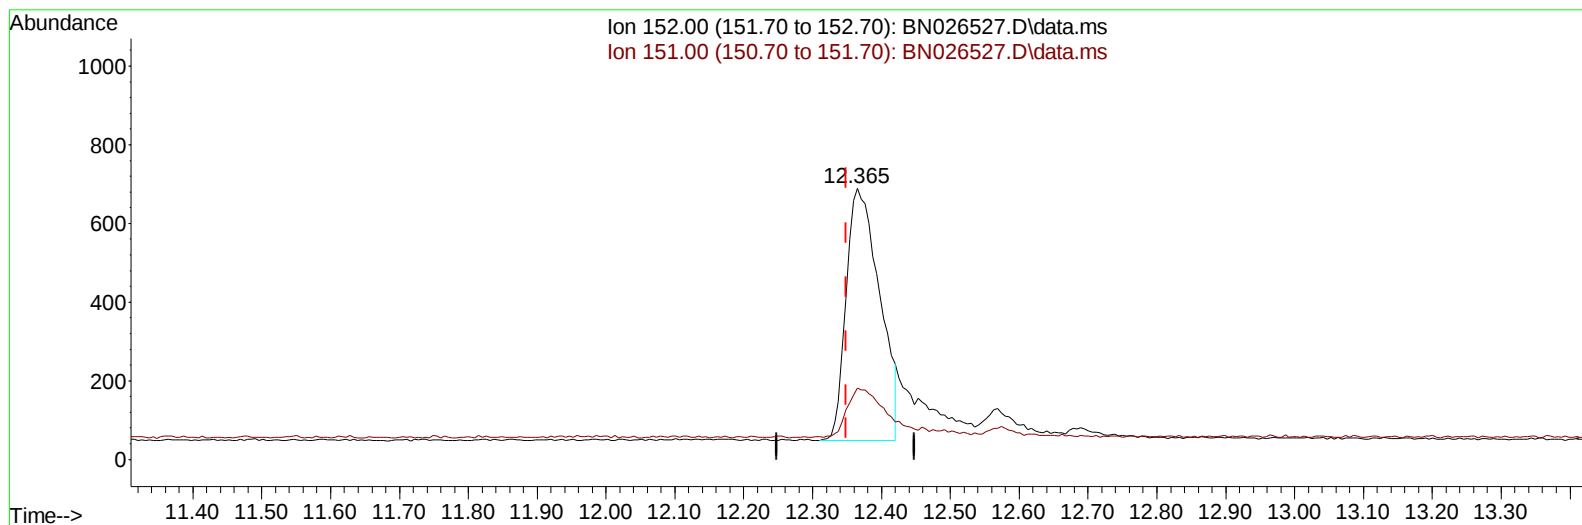

TIC: BN026527.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.365min (+ 0.017) 0.25 ng/u1

response 2162

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	20.12
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026527.D
 Acq On : 17 Jul 2023 09:06
 Operator : MA/JU
 Sample : PB153870BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK870

Manual IntegrationsAPPROVED

Quant Time: Jul 17 17:14:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :Sohil Jodhani 07/17/2023

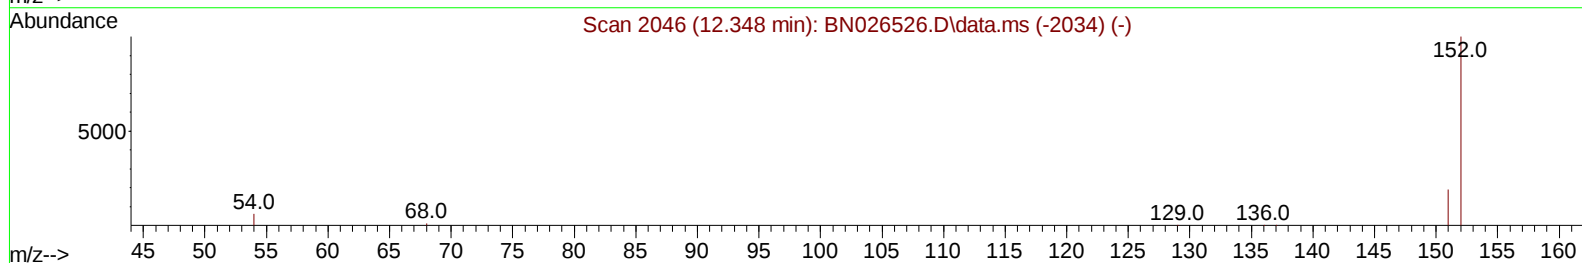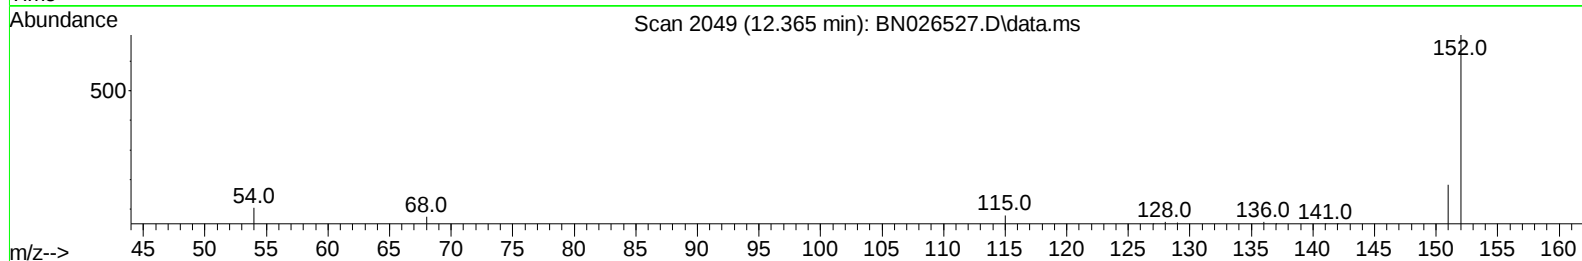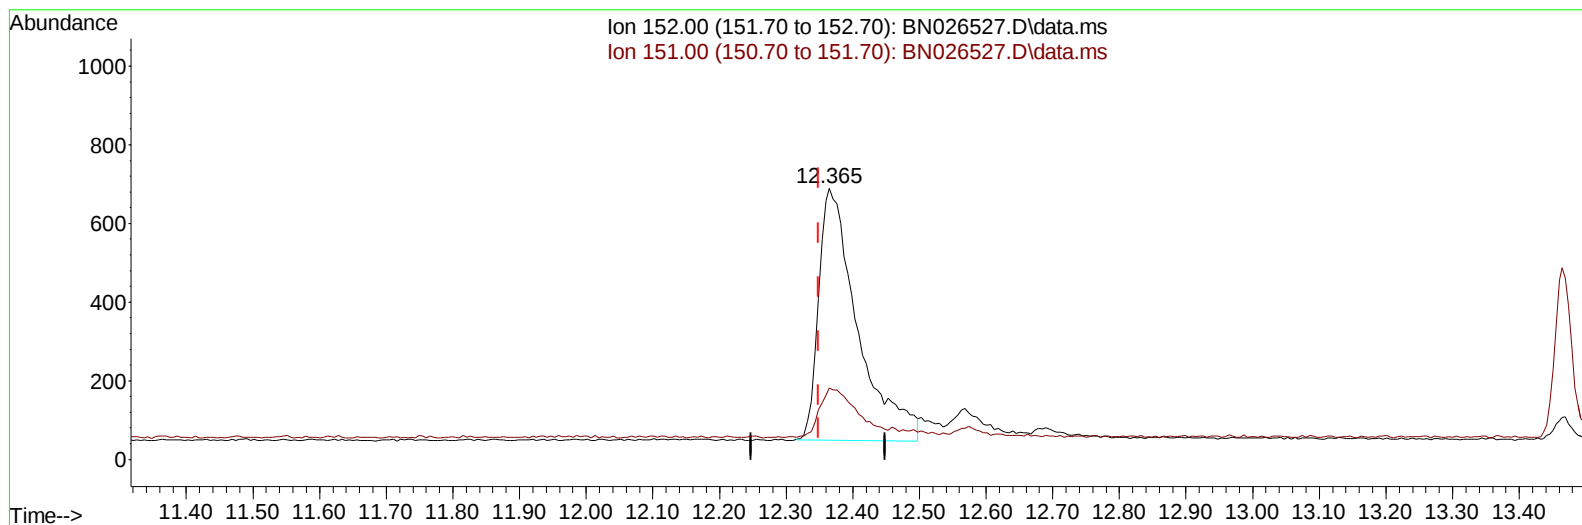

TIC: BN026527.D\data.ms

(6) 2-Methylnaphthalene-d10 (SURR)

12.365min (+ 0.017) 0.30 ng/ul m

response 2600

Ion	Exp%	Act%
152.00	100.00	100.00
151.00	20.90	16.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026527.D
 Acq On : 17 Jul 2023 09:06
 Operator : MA/JU
 Sample : PB153870BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK870

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :Sohil Jodhani 07/17/2023

Quant Time: Jul 17 17:14:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.951	152		2022	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136		6340	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164		4318	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188		9802	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.526	240		7487	0.400	ng/ul	# 0.00
23) Perylene-d12	23.929	264		8589	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.293	96		16066	6.033	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.365	152		2600m	0.302	ng/ul	0.02
18) Fluoranthene-d10	19.359	212		7641	0.294	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026527.D
Acq On : 17 Jul 2023 09:06
Operator : MA/JU
Sample : PB153870BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK870

Manual IntegrationsAPPROVED

Quant Time: Jul 17 17:14:40 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Sohil Jodhani 07/17/2023

