

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026532.D
 Acq On : 17 Jul 2023 12:10
 Operator : MA/JU
 Sample : 03457-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C54

Quant Time: Jul 18 03:03:54 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	2156	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	6627	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	4310	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	9726	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.517	240	8723	0.400	ng/ul	# 0.00
23) Perylene-d12	23.932	264	8767	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	12026	4.235	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	2850	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.354	212	10368	0.343	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.798	128	637	0.035	ng/ul#	69
12) Fluorene	15.630	166	659	0.039	ng/ul#	95
15) Phenanthrene	17.368	178	1650	0.053	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026532.D
Acq On : 17 Jul 2023 12:10
Operator : MA/JU
Sample : 03457-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C54


Quant Time: Jul 18 03:03:54 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

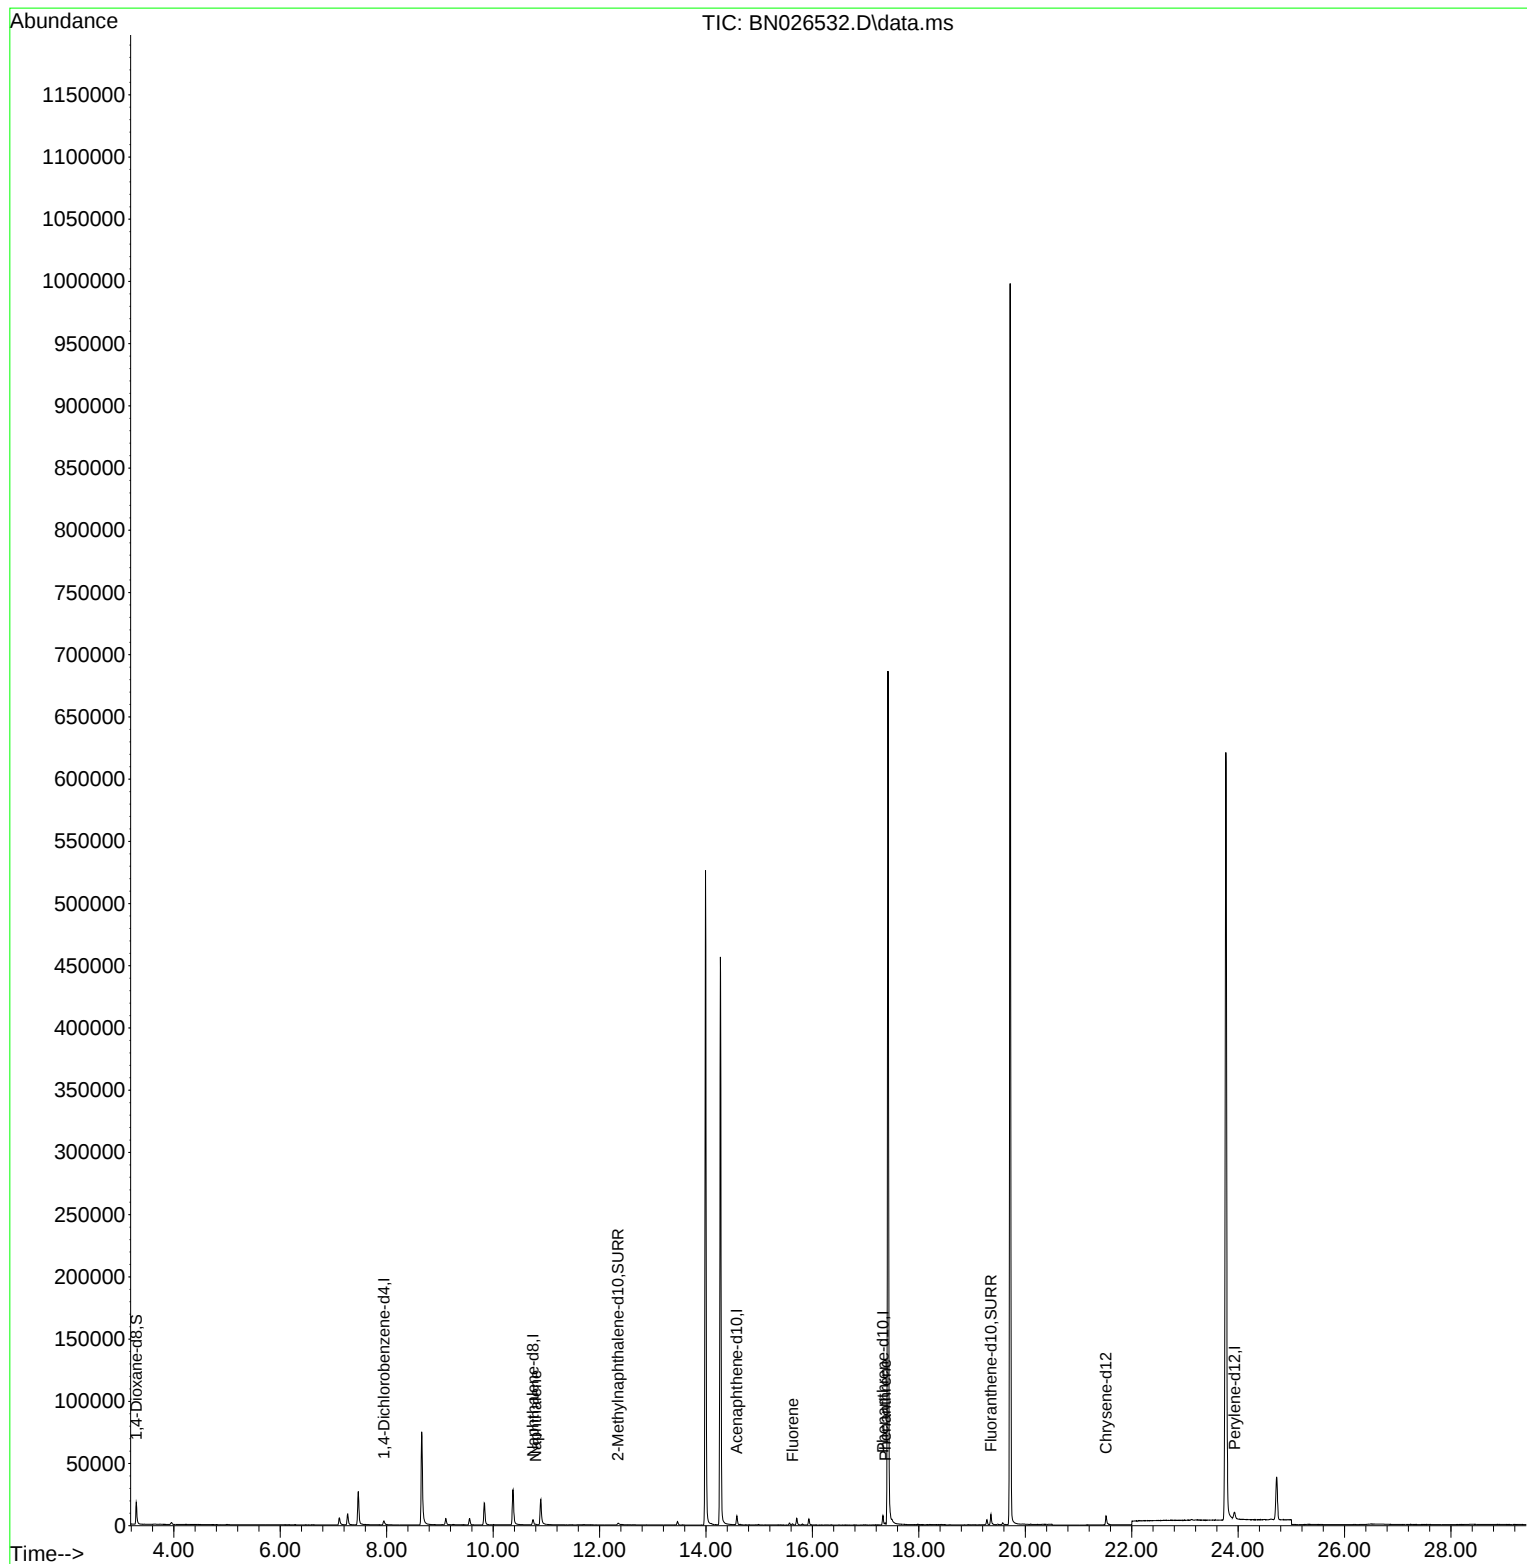



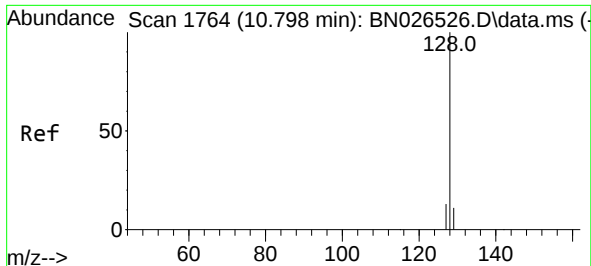


#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.798 min Scan# 1764
Delta R.T. -0.000 min
Lab File: BN026532.D
Acq: 17 Jul 2023 12:10

Instrument :
BNA_N
ClientSampleId :
C0C54



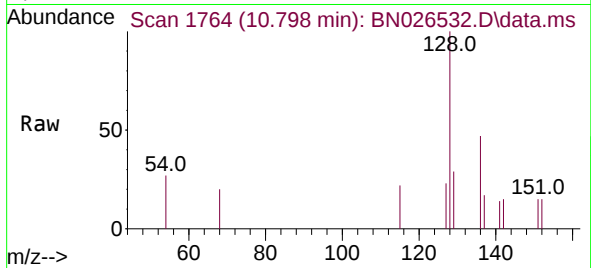



Tgt Ion:128 Resp: 637
Ion Ratio Lower Upper
128 100
129 28.8 10.2 15.2#
127 23.0 11.4 17.0#

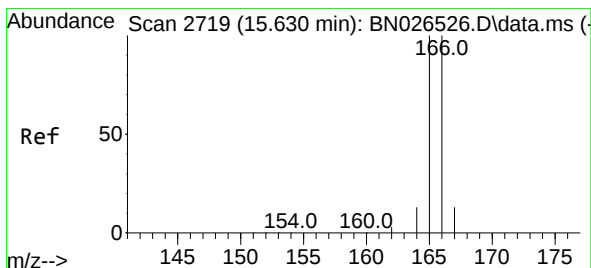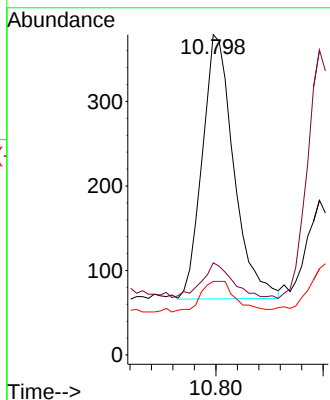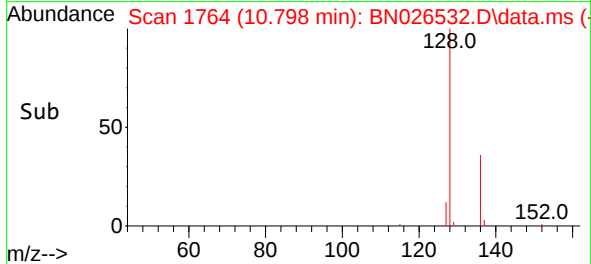

#12
Fluorene
Concen: 0.039 ng/ul
RT: 15.630 min Scan# 2719
Delta R.T. -0.000 min
Lab File: BN026532.D
Acq: 17 Jul 2023 12:10


Tgt Ion:166 Resp: 659
Ion Ratio Lower Upper
166 100
165 97.7 80.6 120.8
167 24.3 12.0 18.0#

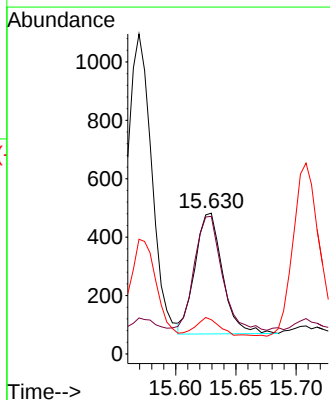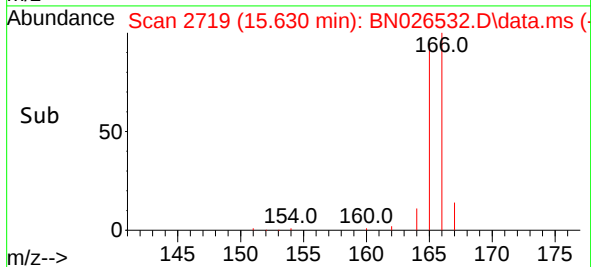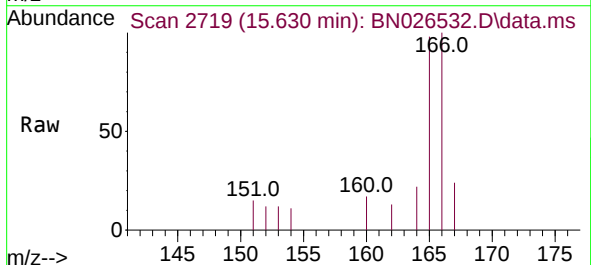

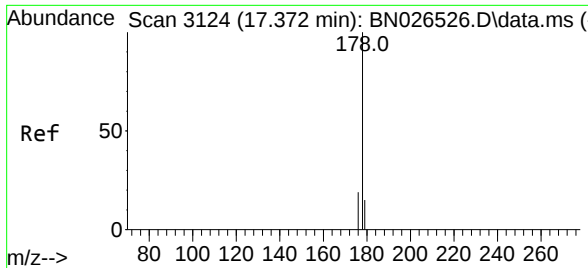

#15
 Phenanthrene
 Concen: 0.053 ng/ul
 RT: 17.368 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN026532.D
 Acq: 17 Jul 2023 12:10

Instrument :
 BNA_N
 ClientSampleId :
 C0C54

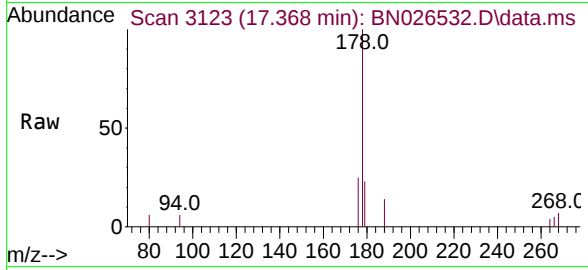

Tgt Ion:	178	Resp:	1650
Ion	Ratio	Lower	Upper
178	100		
179	22.8	13.7	20.5#
176	25.2	16.5	24.7#

