

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN071723\  
 Data File : BN026535.D  
 Acq On : 17 Jul 2023 14:02  
 Operator : MA/JU  
 Sample : 03457-09  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 C0C51

Quant Time: Jul 18 03:04:24 2023  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN071223.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jul 17 17:14:21 2023  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.946  | 152  | 2232     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.752 | 136  | 6822     | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.579 | 164  | 4510     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.325 | 188  | 10114    | 0.400 | ng/ul  | # 0.00   |
| 17) Chrysene-d12            | 21.525 | 240  | 8578     | 0.400 | ng/ul  | # 0.00   |
| 23) Perylene-d12            | 23.934 | 264  | 9247     | 0.400 | ng/ul  | # 0.00   |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.297  | 96   | 11753    | 3.998 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.353 | 152  | 2607     | 0.281 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.358 | 212  | 9680     | 0.326 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       |        | Qvalue   |
| 5) Naphthalene              | 10.802 | 128  | 415      | 0.022 | ng/ul# | 55       |
| -----                       |        |      |          |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN071723\  
Data File : BN026535.D  
Acq On : 17 Jul 2023 14:02  
Operator : MA/JU  
Sample : 03457-09  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
C0C51


Quant Time: Jul 18 03:04:24 2023  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN071223.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jul 17 17:14:21 2023  
Response via : Initial Calibration

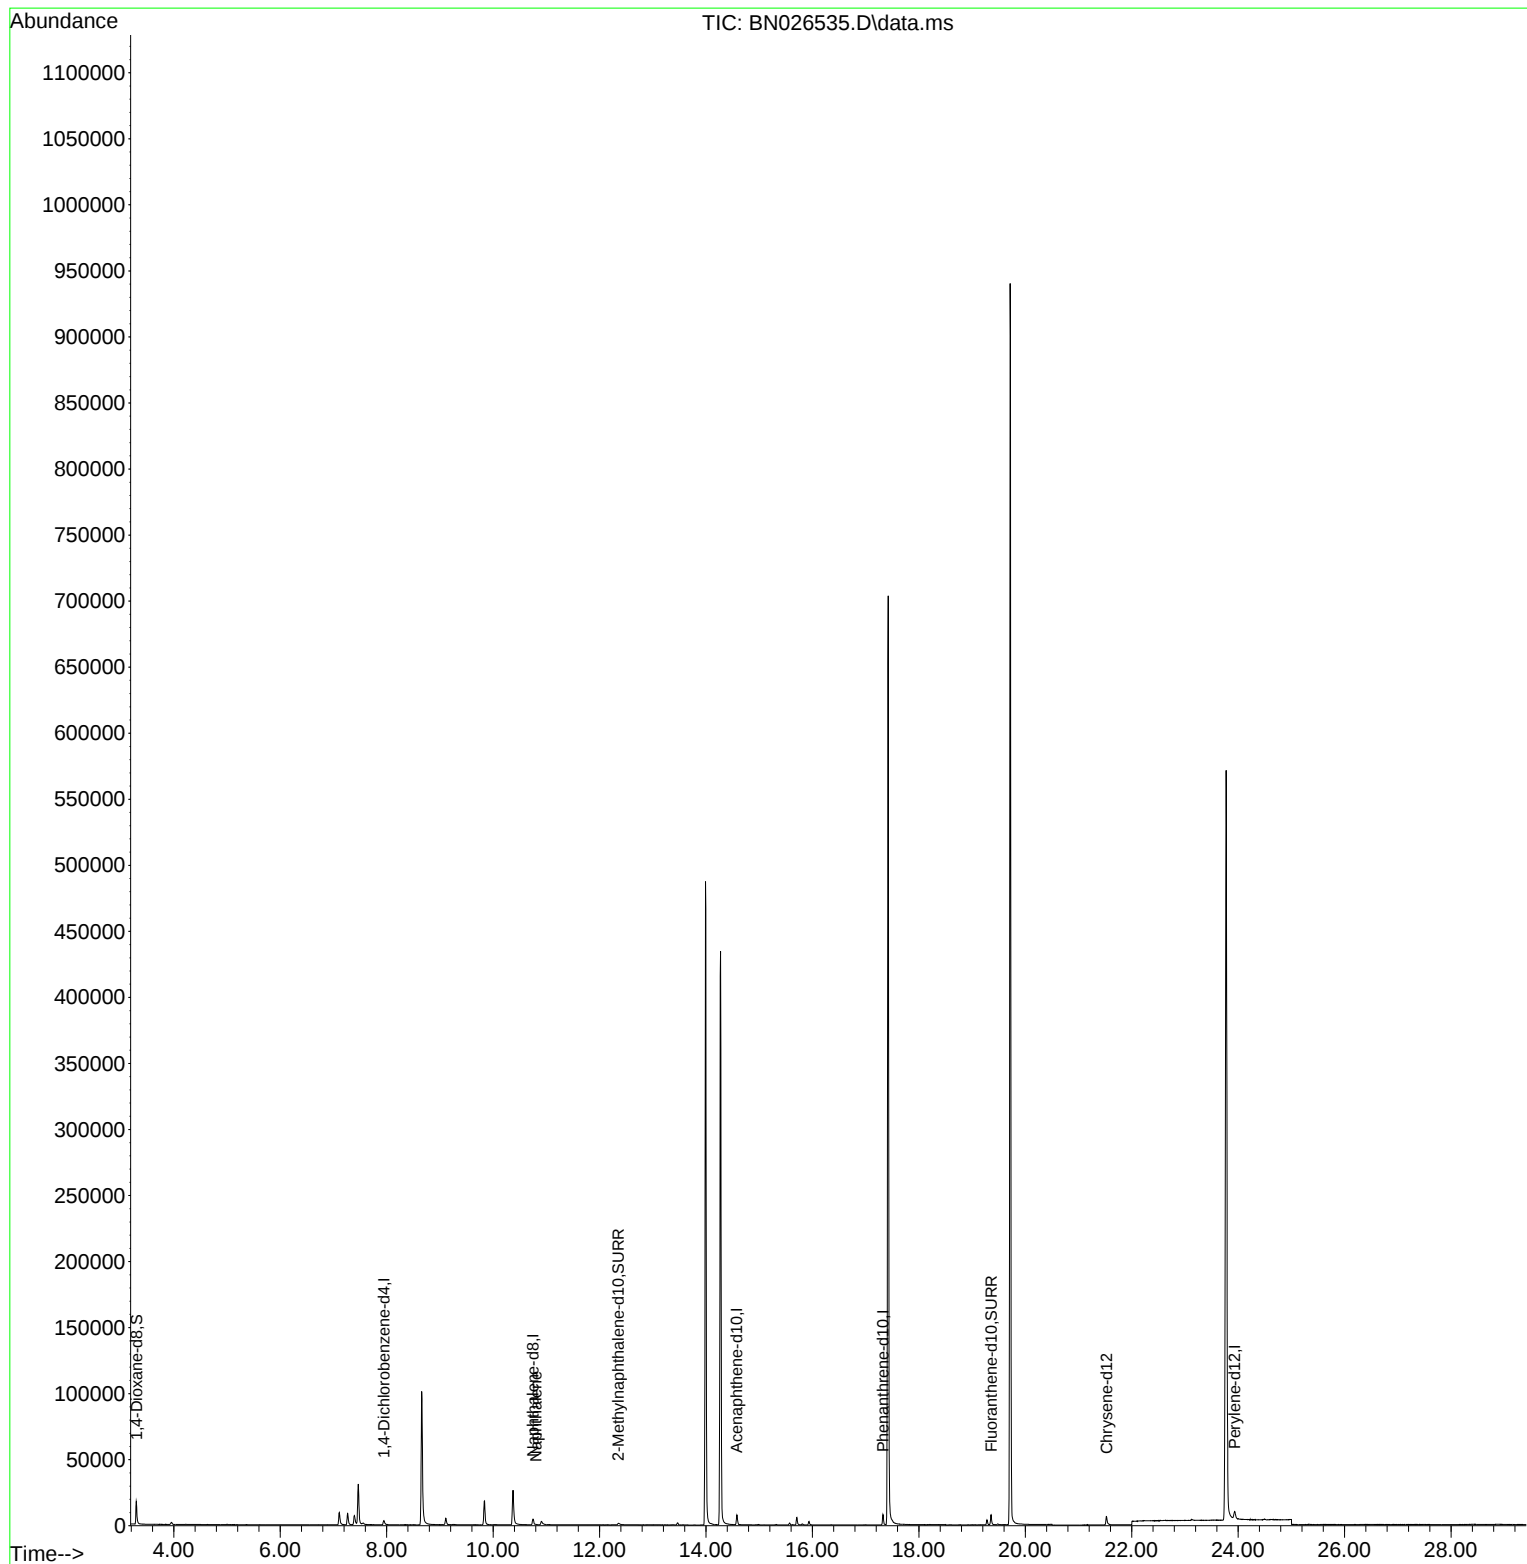

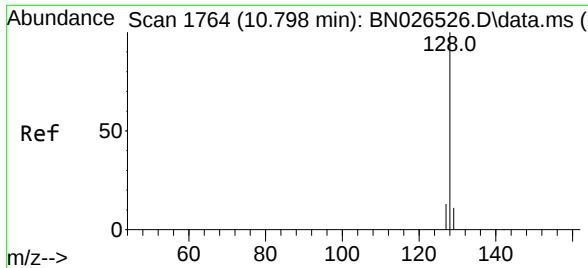

#5  
Naphthalene  
Concen: 0.022 ng/ul  
RT: 10.802 min Scan# 11  
Delta R.T. 0.004 min  
Lab File: BN026535.D  
Acq: 17 Jul 2023 14:02

Instrument :  
BNA\_N  
ClientSampleId :  
C0C51

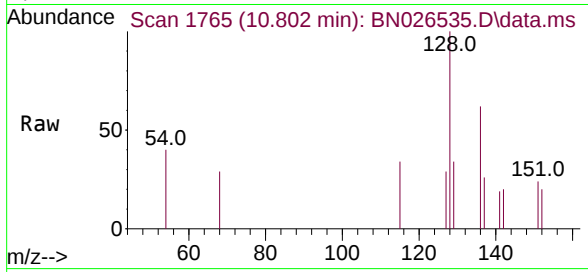

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 128   | Resp: | 415   |
| Ion      | Ratio | Lower | Upper |
| 128      | 100   |       |       |
| 129      | 34.2  | 10.2  | 15.2# |
| 127      | 29.2  | 11.4  | 17.0# |

