

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026537.D
 Acq On : 17 Jul 2023 15:16
 Operator : MA/JU
 Sample : 03457-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C56

Quant Time: Jul 18 03:04:44 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	2109	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	6483	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.580	164	4231	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.327	188	9619	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.524	240	8119	0.400	ng/ul	# 0.00
23) Perylene-d12	23.933	264	8734	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	12221	4.400	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	2590	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.355	212	9613	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.365	178	762	0.025	ng/ul#	73
24) Benzo(b)fluoranthene	23.199	252	685	0.020	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026537.D
Acq On : 17 Jul 2023 15:16
Operator : MA/JU
Sample : 03457-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C56

Quant Time: Jul 18 03:04:44 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration




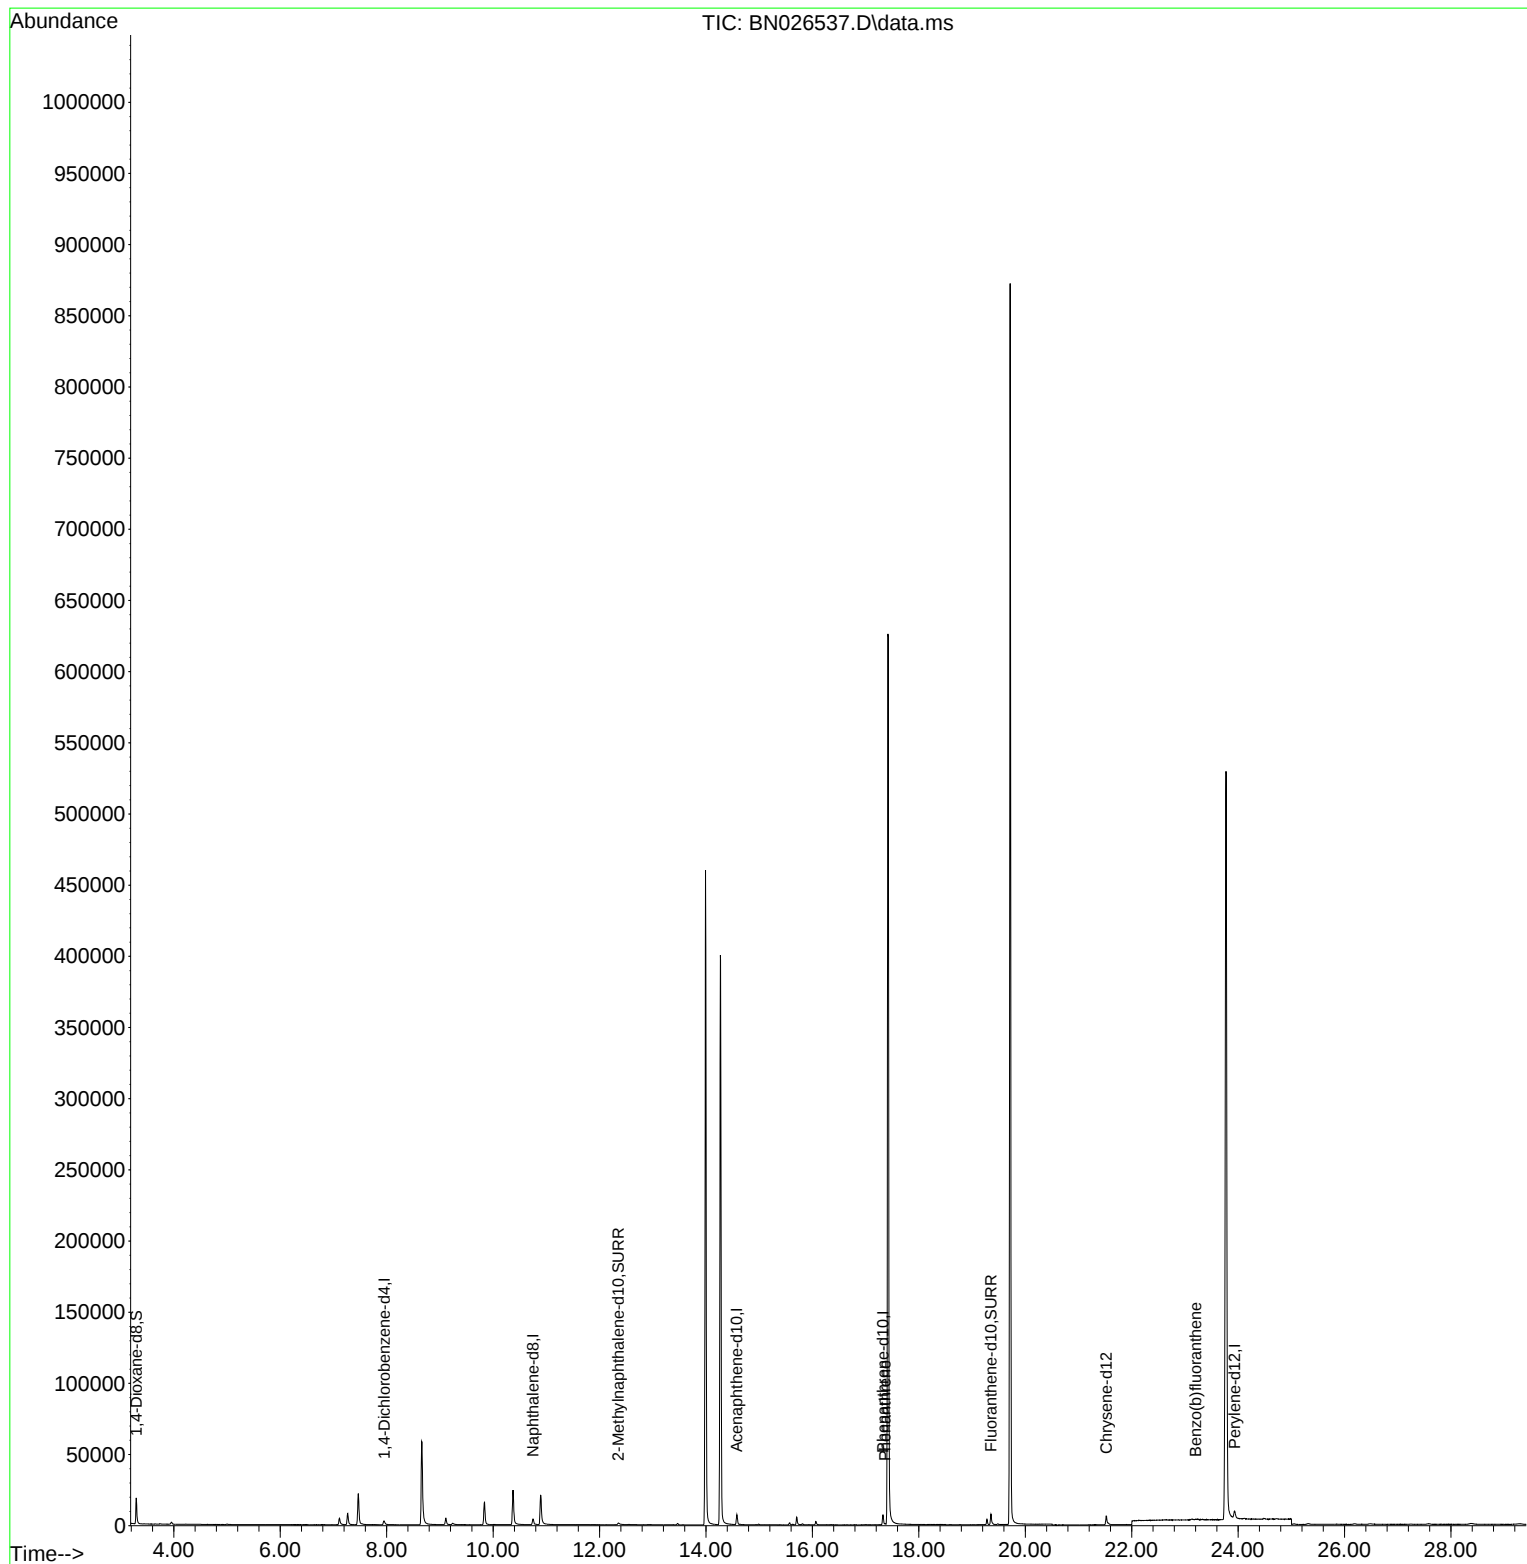


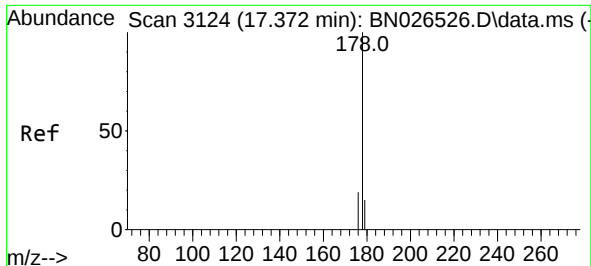

#15
Phenanthrene
Concen: 0.025 ng/ul
RT: 17.365 min Scan# 3122
Delta R.T. -0.007 min
Lab File: BN026537.D
Acq: 17 Jul 2023 15:16

Instrument :
BNA_N
ClientSampleId :
C0C56

Tgt Ion:178 Resp: 762
Ion Ratio Lower Upper
178 100
179 30.1 13.7 20.5#
176 32.1 16.5 24.7#

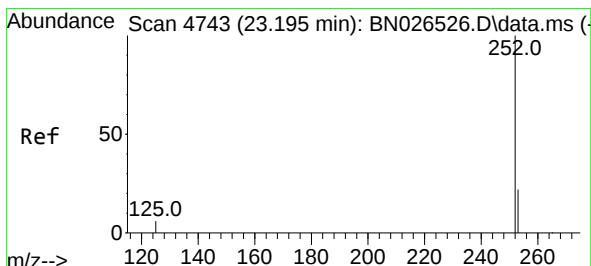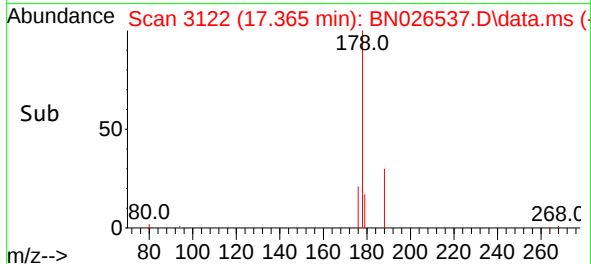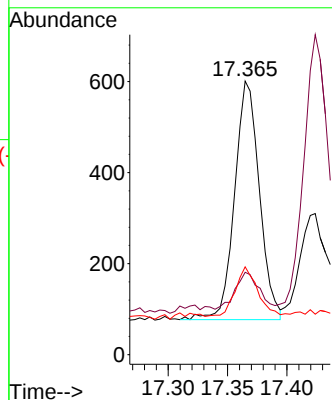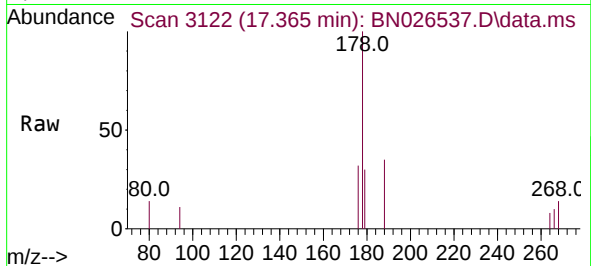

#24
Benzo(b)fluoranthene
Concen: 0.020 ng/ul
RT: 23.199 min Scan# 4744
Delta R.T. 0.004 min
Lab File: BN026537.D
Acq: 17 Jul 2023 15:16

Tgt Ion:252 Resp: 685
Ion Ratio Lower Upper
252 100
253 103.3 0.0 68.6#
125 66.8 0.0 34.0#

