

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
 Data File : BN026547.D
 Acq On : 17 Jul 2023 21:30
 Operator : MA/JU
 Sample : 03458-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A46L9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :mohammad ahmed 07/19/2023

Quant Time: Jul 18 04:22:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 17 17:14:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.938	152	3321	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.748	136	10442	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.579	164	6615	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.322	188	15950	0.400	ng/ul	0.00
17) Chrysene-d12	21.511	240	12239	0.400	ng/ul	# 0.00
23) Perylene-d12	23.923	264	11606	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	12440	2.844	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	3076	0.217	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	9156	0.216	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.798	128	8278	0.289	ng/ul	99
7) 2-Methylnaphthalene	12.414	142	724	0.045	ng/ul	100
8) 1-Methylnaphthalene	12.634	142	447	0.026	ng/ul	97
10) Acenaphthylene	14.297	152	1678	0.052	ng/ul#	80
11) Acenaphthene	14.640	153	955	0.039	ng/ul	94
12) Fluorene	15.625	166	700	0.027	ng/ul#	91
15) Phenanthrene	17.364	178	13733	0.270	ng/ul	99
16) Anthracene	17.457	178	3173	0.072	ng/ul#	94
19) Fluoranthene	19.382	202	35370	0.617	ng/ul#	96
20) Pyrene	19.740	202	41584	0.667	ng/ul	98
21) Benzo(a)anthracene	21.494	228	15370	0.342	ng/ul#	94
22) Chrysene	21.549	228	19125	0.374	ng/ul#	95
24) Benzo(b)fluoranthene	23.192	252	19219m	0.425	ng/ul	
25) Benzo(k)fluoranthene	23.236	252	6552m	0.138	ng/ul	
26) Benzo(a)pyrene	23.815	252	6515	0.162	ng/ul#	87
27) Indeno(1,2,3-cd)pyrene	26.437	276	6241	0.118	ng/ul#	83
28) Dibenzo(a,h)anthracene	26.450	278	2175	0.054	ng/ul#	19

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071723\
Data File : BN026547.D
Acq On : 17 Jul 2023 21:30
Operator : MA/JU
Sample : 03458-06
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A46L9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023


Quant Time: Jul 18 04:22:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 17 17:14:21 2023
Response via : Initial Calibration

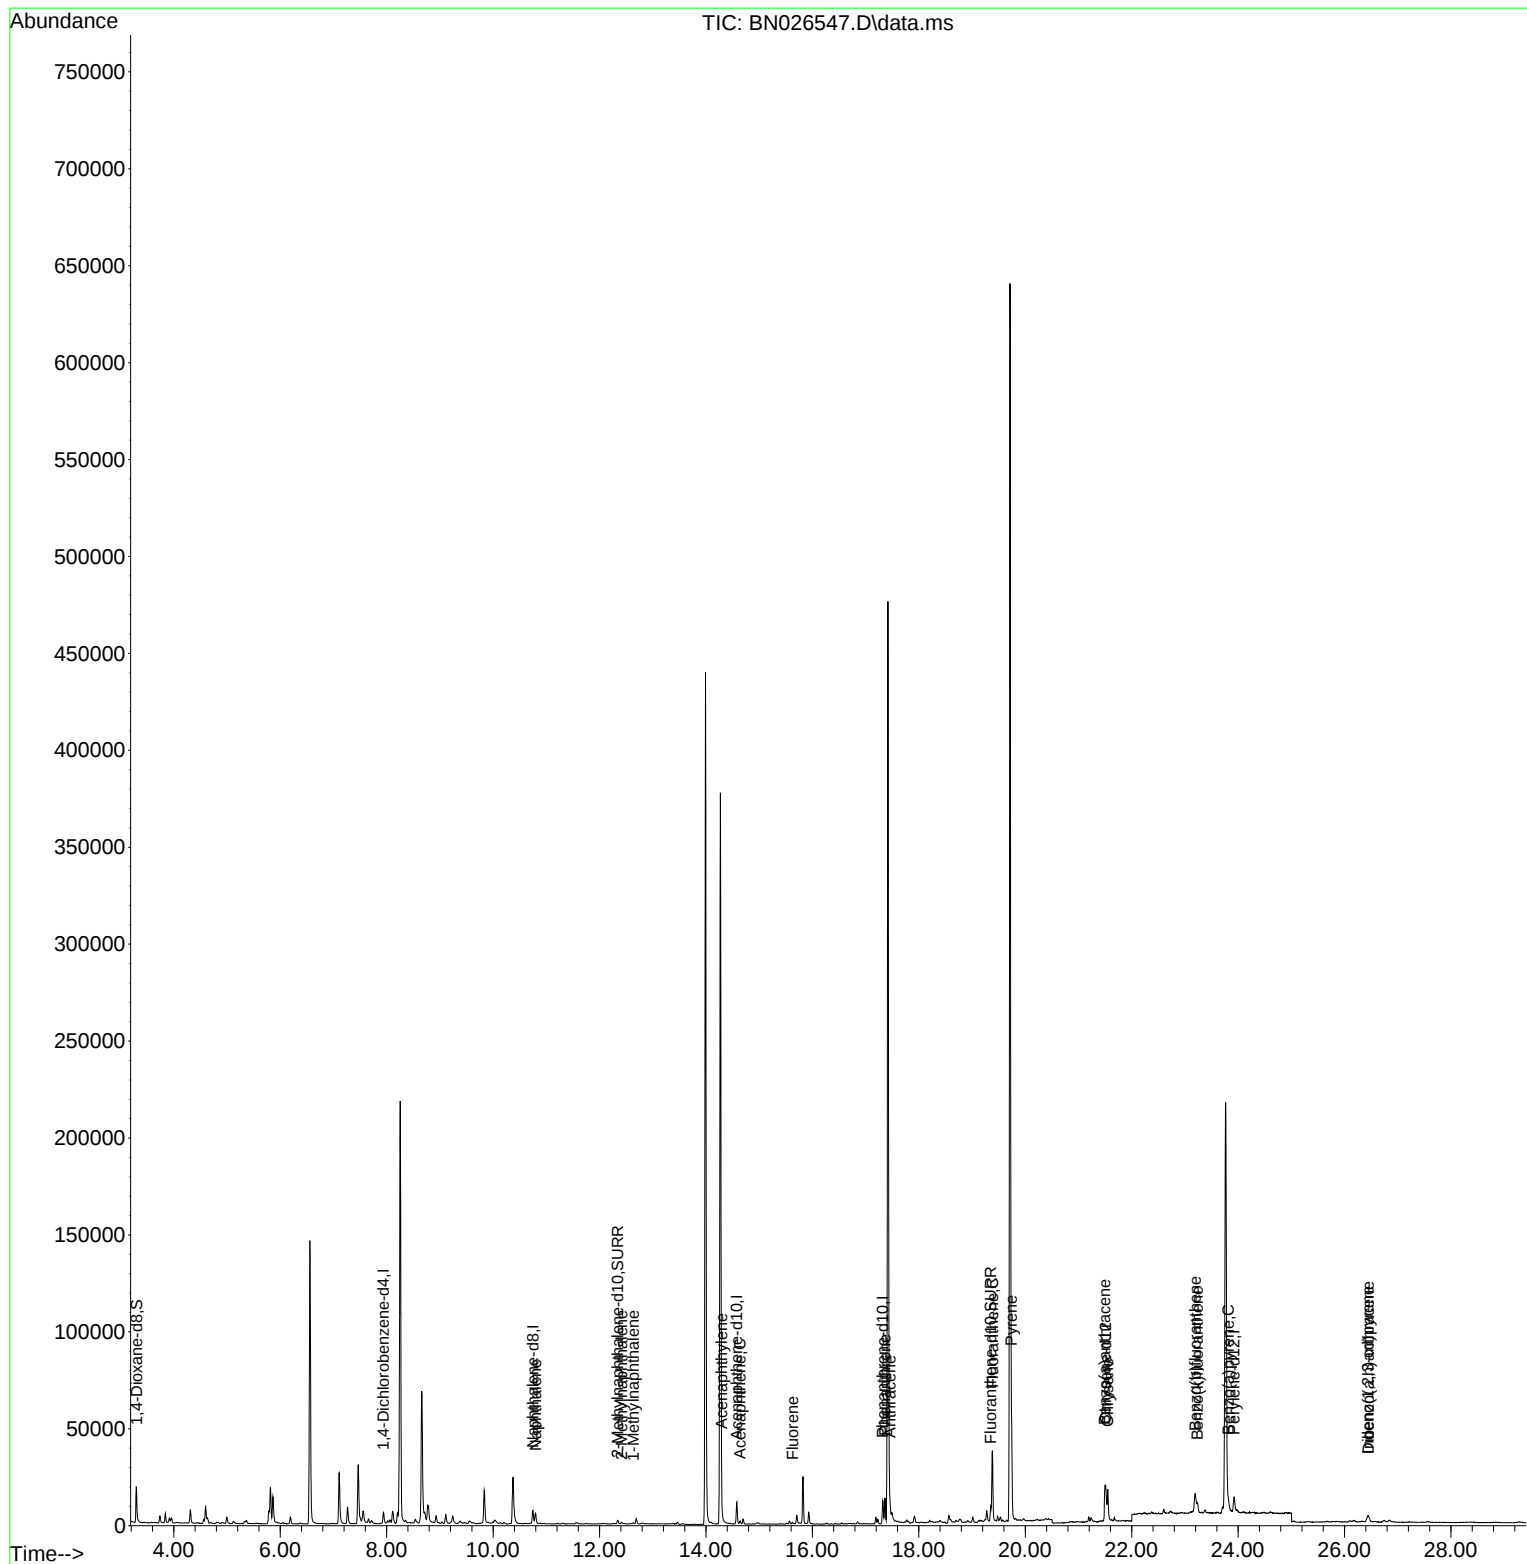



#5
Naphthalene
Concen: 0.289 ng/ul
RT: 10.798 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9




Tgt Ion:128 Resp: 8278
Ion Ratio Lower Upper
128 100
129 12.7 10.2 15.2
127 14.7 11.4 17.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

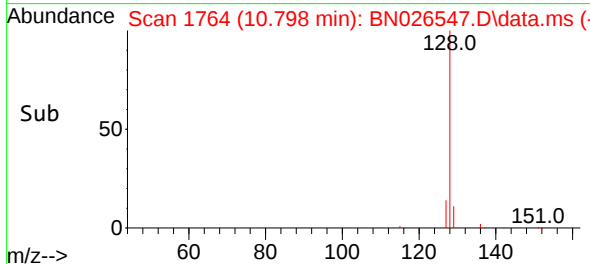


#7
2-Methylnaphthalene
Concen: 0.045 ng/ul
RT: 12.414 min Scan# 2058
Delta R.T. -0.005 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30

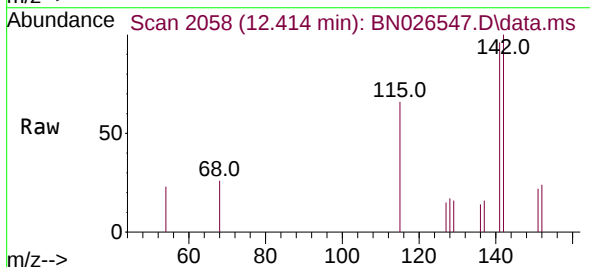


Tgt Ion:142 Resp: 724
Ion Ratio Lower Upper
142 100
141 90.5 72.3 108.5

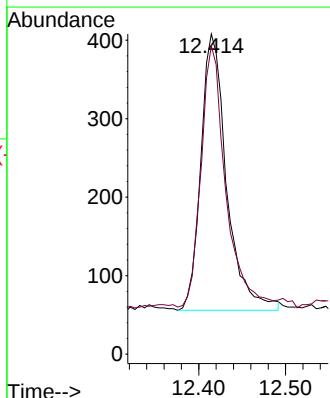



#8
1-Methylnaphthalene
Concen: 0.026 ng/ul
RT: 12.634 min Scan# 2099
Delta R.T. 0.006 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9



Tgt Ion:142 Resp: 44
Ion Ratio Lower Upper
142 100
141 95.7 74.5 111.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

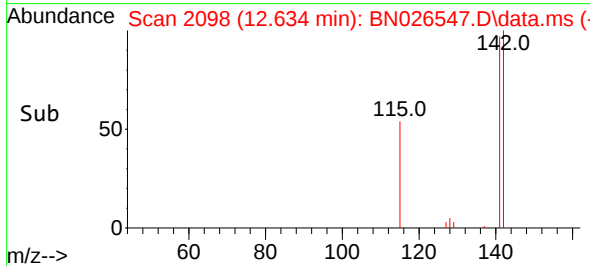

#10
Acenaphthylene
Concen: 0.052 ng/ul
RT: 14.297 min Scan# 2431
Delta R.T. -0.005 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30


Tgt Ion:152 Resp: 1678
Ion Ratio Lower Upper
152 100
151 31.0 17.0 25.6#
153 21.6 11.4 17.2#

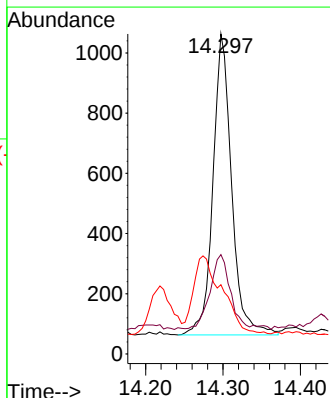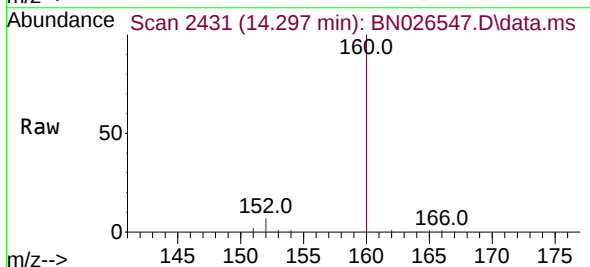

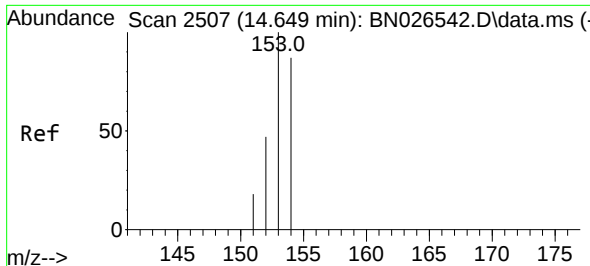

#11
Acenaphthene
Concen: 0.039 ng/u1
RT: 14.640 min Scan# 2118
Delta R.T. 0.000 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9



Tgt Ion:153 Resp: 95
Ion Ratio Lower Upper
153 100
152 55.6 40.2 60.4
154 91.5 69.3 103.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

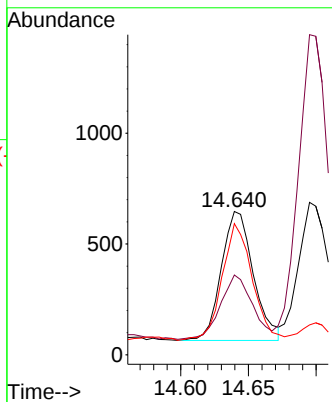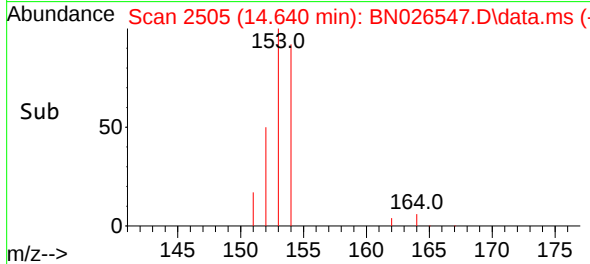

#12
Fluorene
Concen: 0.027 ng/u1
RT: 15.625 min Scan# 2718
Delta R.T. -0.005 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30


Tgt Ion:166 Resp: 700
Ion Ratio Lower Upper
166 100
165 105.3 80.6 120.8
167 30.7 12.0 18.0#

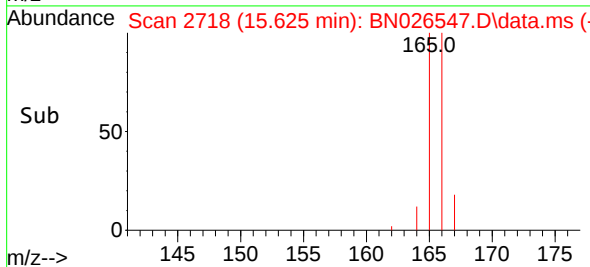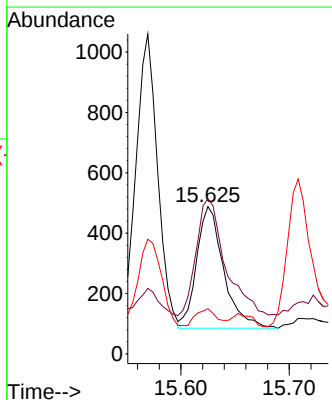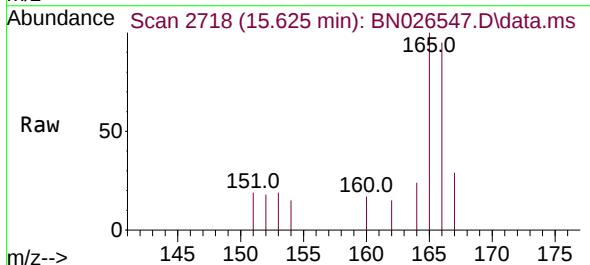



#15
Phenanthrene
Concen: 0.270 ng/u1
RT: 17.364 min Scan# 3122
Delta R.T. -0.008 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9



Tgt Ion:178 Resp: 1373
Ion Ratio Lower Upper
178 100
179 17.1 13.7 20.5
176 20.1 16.5 24.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

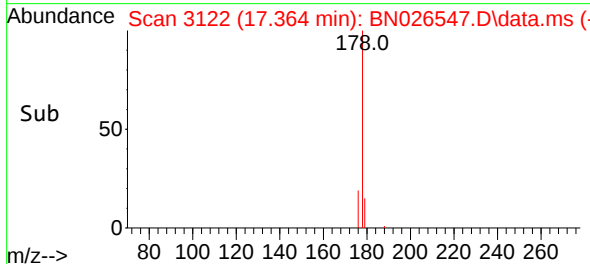

#16
Anthracene
Concen: 0.072 ng/u1
RT: 17.457 min Scan# 3144
Delta R.T. -0.008 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30


Tgt Ion:178 Resp: 3173
Ion Ratio Lower Upper
178 100
179 22.4 14.8 22.2#
176 22.5 16.6 25.0

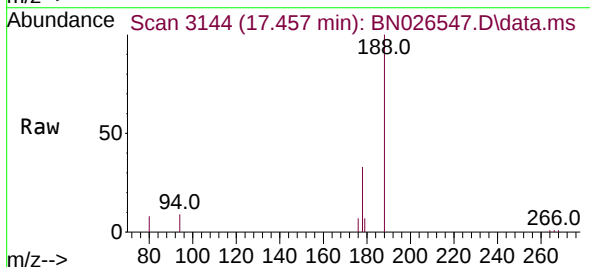



#19
Fluoranthene
Concen: 0.617 ng/ul
RT: 19.382 min Scan# 3583
Delta R.T. -0.005 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9




Tgt Ion:202 Resp: 35370
Ion Ratio Lower Upper
202 100
101 7.8 7.0 10.4
100 5.8 6.0 9.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

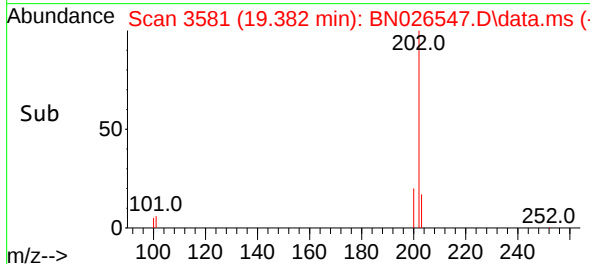


#20
Pyrene
Concen: 0.667 ng/ul
RT: 19.740 min Scan# 3658
Delta R.T. -0.009 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30

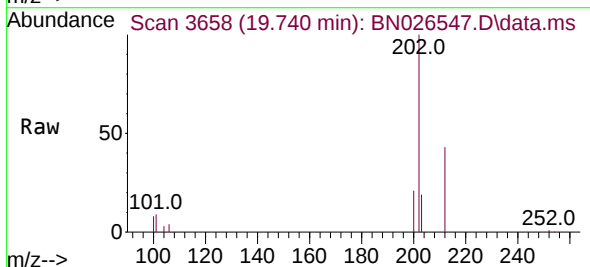


Tgt Ion:202 Resp: 41584
Ion Ratio Lower Upper
202 100
101 9.3 8.0 12.0
100 8.4 6.2 9.2

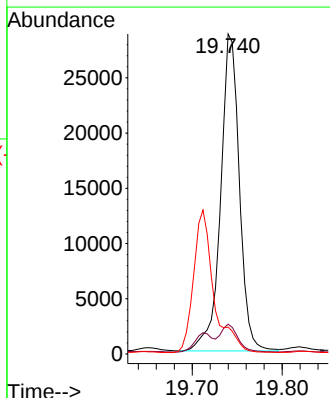



#21
Benzo(a)anthracene
Concen: 0.342 ng/ul
RT: 21.494 min Scan# 4165
Delta R.T. -0.009 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9



Tgt Ion:228 Resp: 15370
Ion Ratio Lower Upper
228 100
229 25.5 16.7 25.1
226 30.9 23.5 35.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

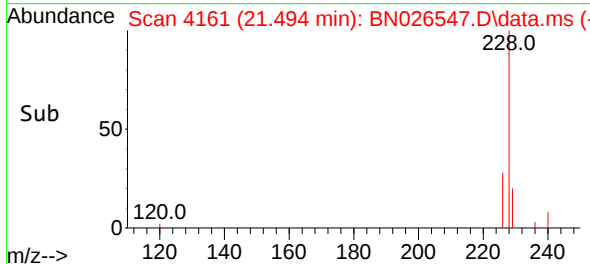

#22
Chrysene
Concen: 0.374 ng/ul
RT: 21.549 min Scan# 4180
Delta R.T. -0.009 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30


Tgt Ion:228 Resp: 19125
Ion Ratio Lower Upper
228 100
226 32.8 25.2 37.8
229 25.2 16.4 24.6

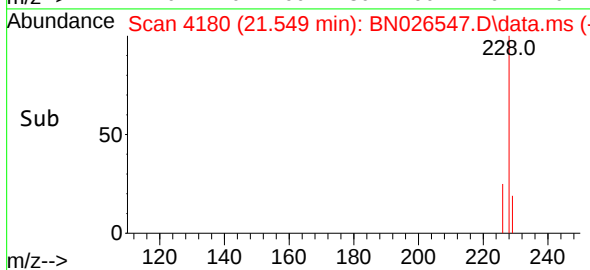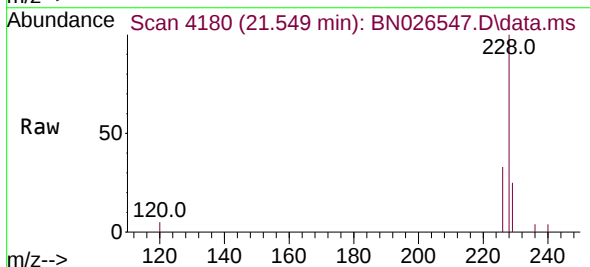

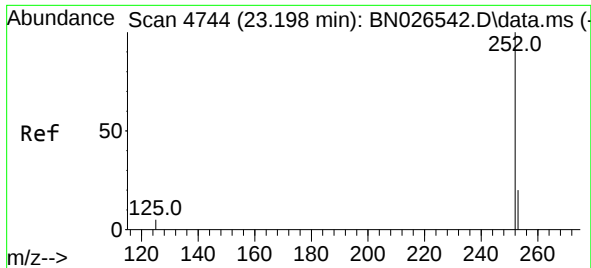

#24
Benzo(b)fluoranthene
Concen: 0.425 ng/ul m
RT: 23.192 min Scan# 4741
Delta R.T. -0.003 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9

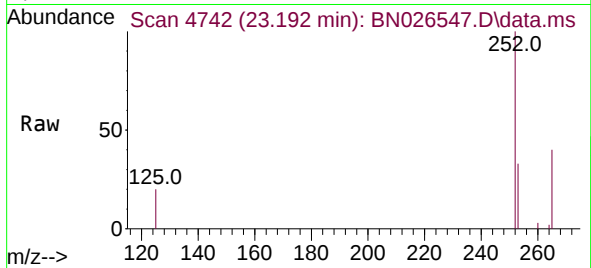

Tgt Ion:252 Resp: 19219
Ion Ratio Lower Upper
252 100
253 33.3 0.0 68.6
125 20.3 0.0 34.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

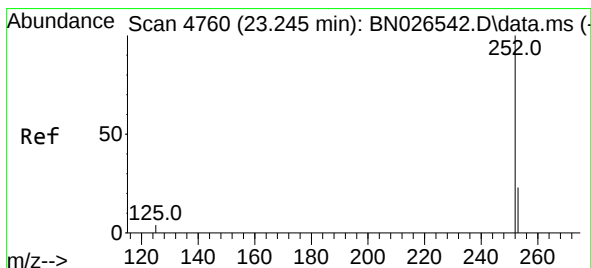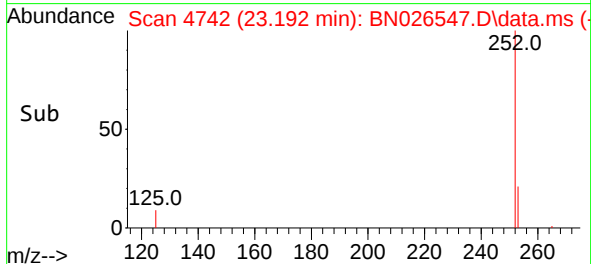

#25
Benzo(k)fluoranthene
Concen: 0.138 ng/ul m
RT: 23.236 min Scan# 4757
Delta R.T. -0.009 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30


Tgt Ion:252 Resp: 6552
Ion Ratio Lower Upper
252 100
253 44.7 27.2 40.8#
125 28.3 13.4 20.2#

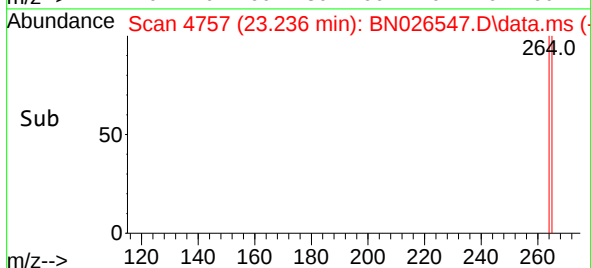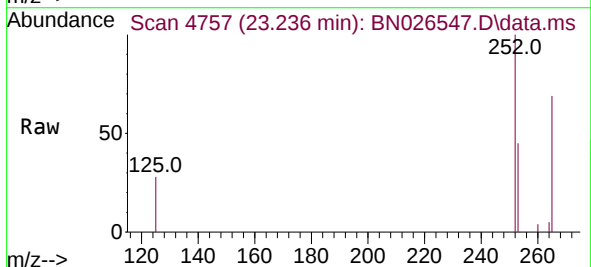

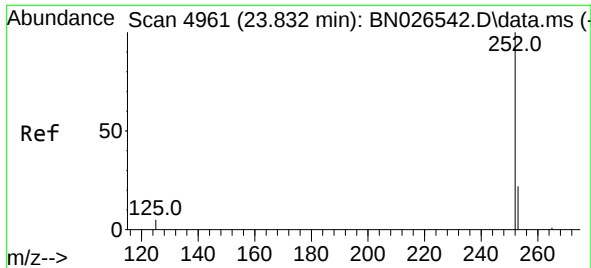

#26
Benzo(a)pyrene
Concen: 0.162 ng/ul
RT: 23.815 min Scan# 4961
Delta R.T. -0.012 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30




Instrument :
BNA_N
ClientSampleId :
A46L9

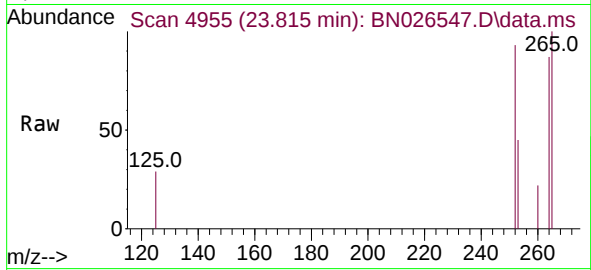


Tgt Ion:252 Resp: 651
Ion Ratio Lower Upper
252 100
253 48.4 32.6 49.0
125 31.1 19.3 28.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/19/2023
Supervised By :mohammad ahmed 07/19/2023

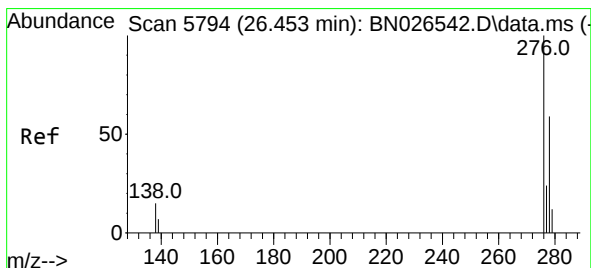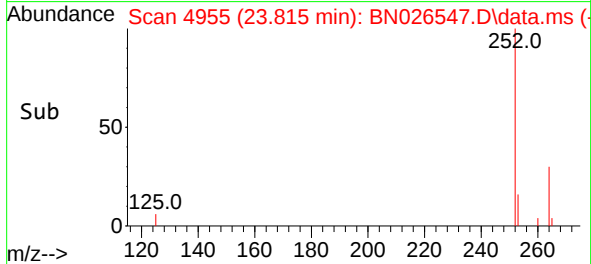


#27
Indeno(1,2,3-cd)pyrene
Concen: 0.118 ng/ul
RT: 26.437 min Scan# 5789
Delta R.T. -0.017 min
Lab File: BN026547.D
Acq: 17 Jul 2023 21:30

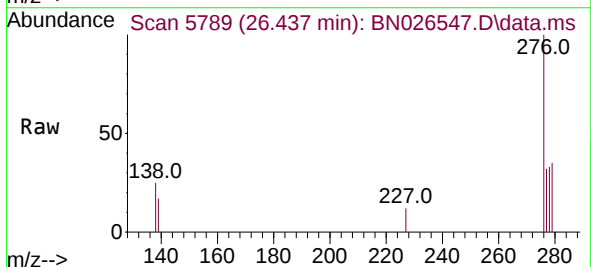


Tgt Ion:276 Resp: 6241
Ion Ratio Lower Upper
276 100
138 18.9 22.2 33.4
227 0.1 0.1 0.1

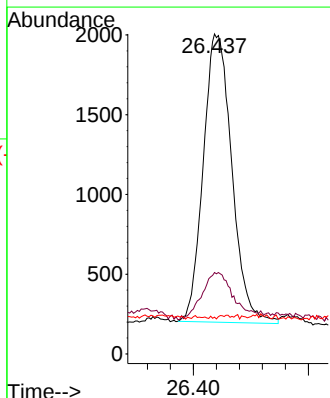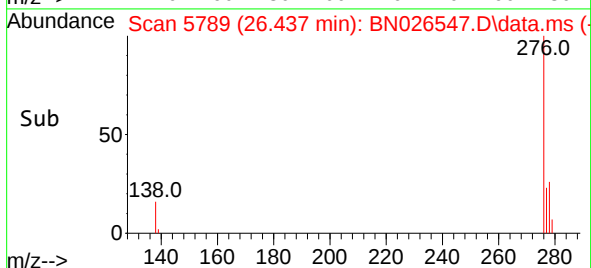

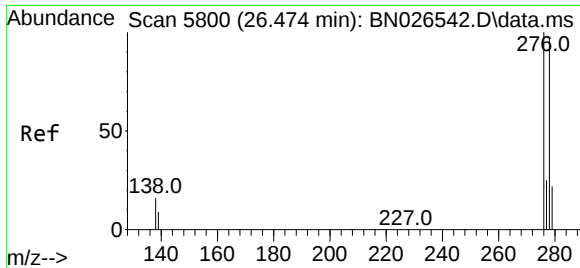

#28
 Dibenzo(a,h)anthracene
 Concen: 0.054 ng/ul
 RT: 26.450 min Scan# 51
 Delta R.T. -0.017 min
 Lab File: BN026547.D
 Acq: 17 Jul 2023 21:30

Instrument :
 BNA_N
 ClientSampleId :
 A46L9

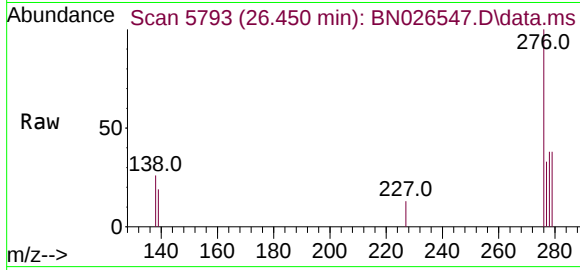

Tgt Ion: 278 Resp: 2175

Ion	Ratio	Lower	Upper
278	100		
139	48.8	18.9	28.3
279	99.9	31.3	46.9

Manual Integrations
 APPROVED

Reviewed By : Yogesh Patel 07/19/2023
 Supervised By : mohammad ahmed 07/19/2023

