

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006900.D
 Acq On : 18 Jul 2019 20:11
 Operator : HP/JU
 Sample : K3822-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 03:41:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	3011	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	11008	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5738	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	934527	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	897800	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	4254	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.40	128	2015	0.064	ng/ul#	Ovalue 85




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006900.D
Acq On : 18 Jul 2019 20:11
Operator : HP/JU
Sample : K3822-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 03:41:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

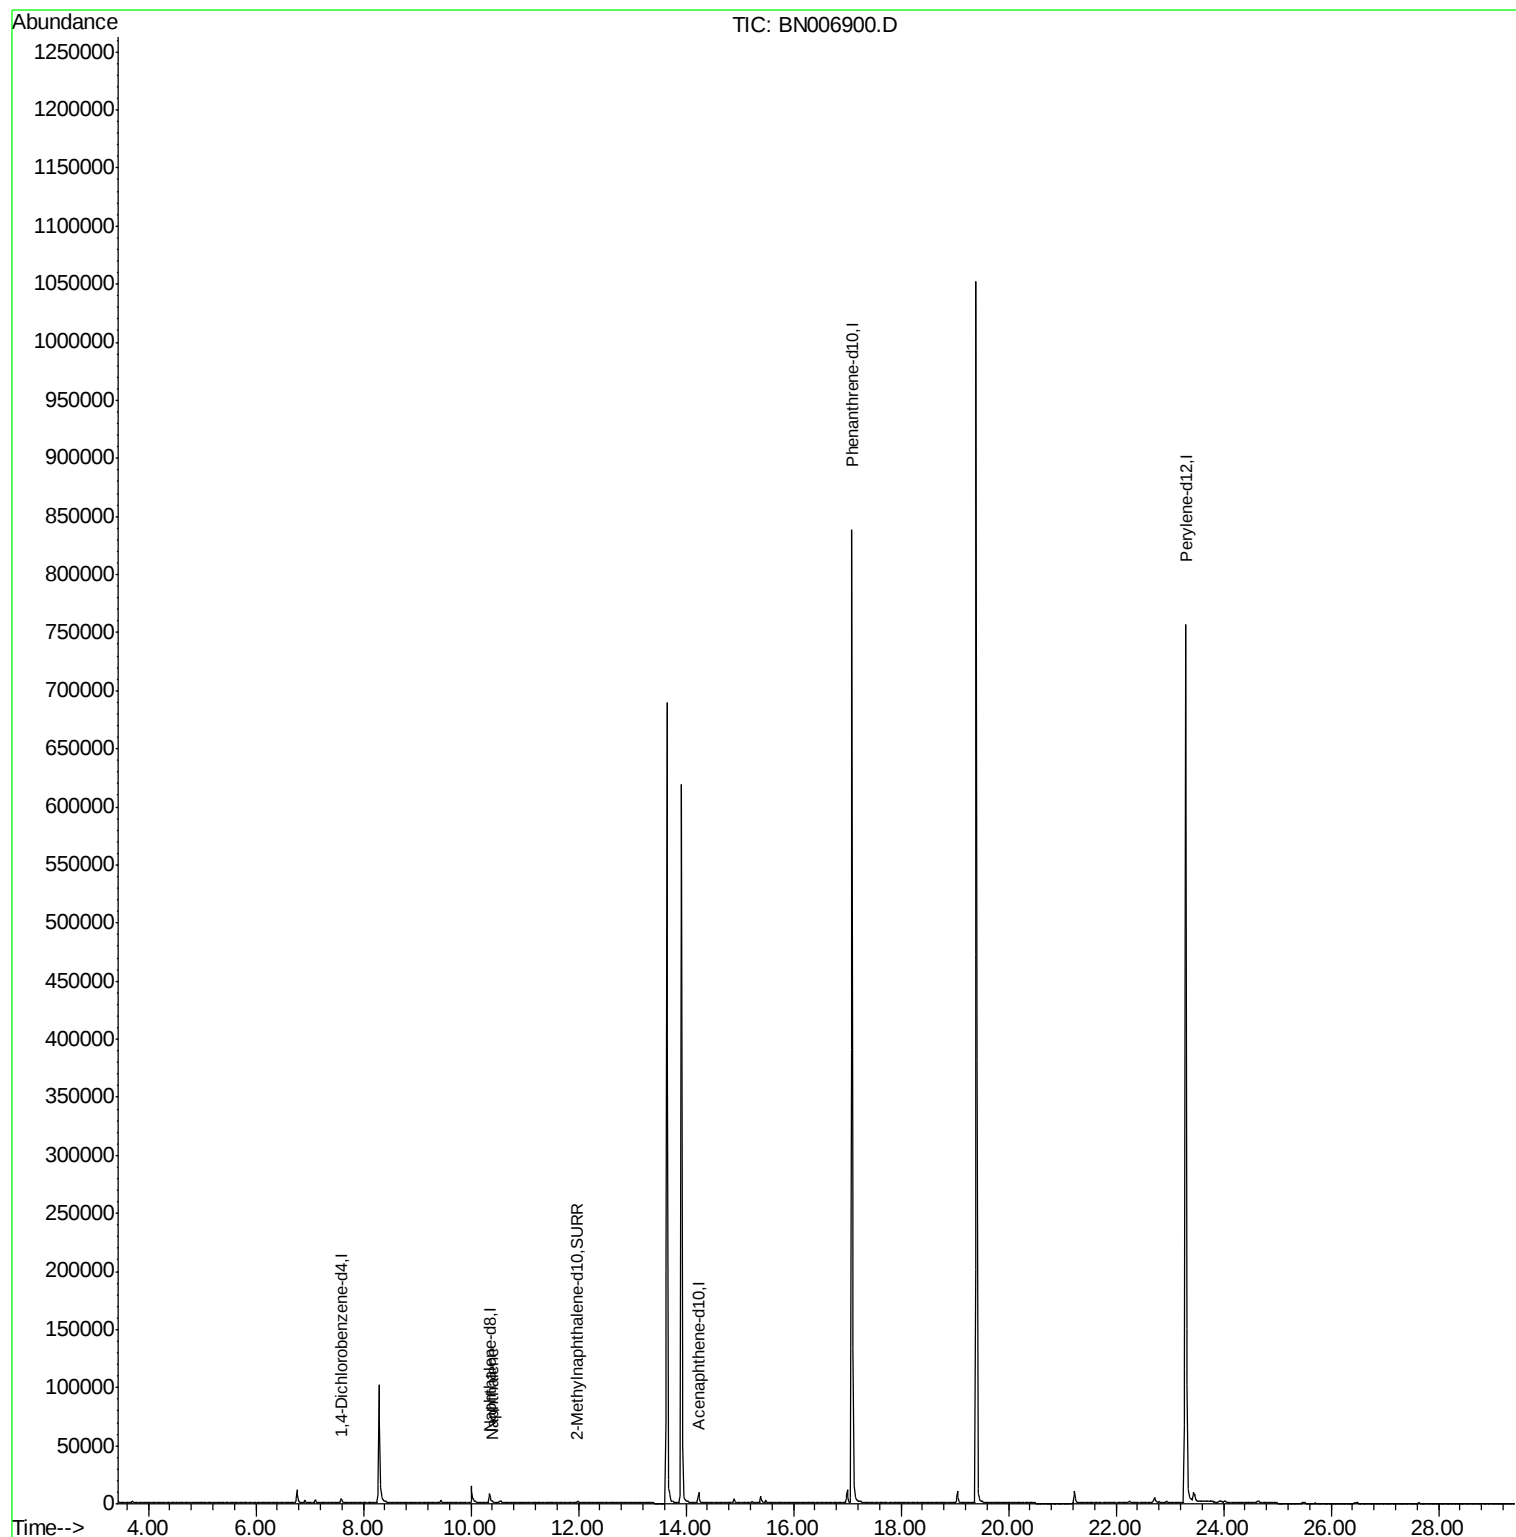

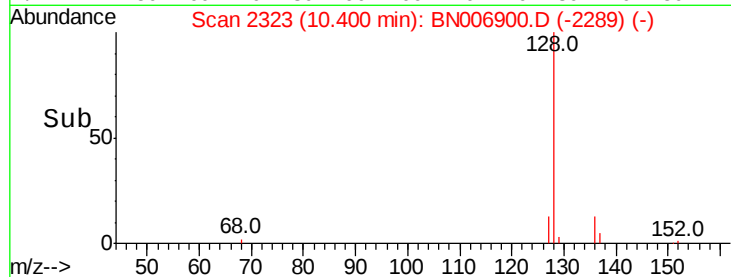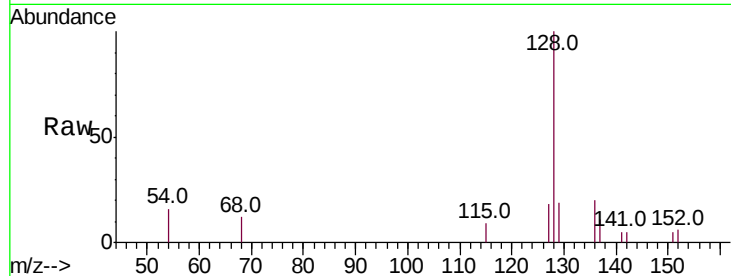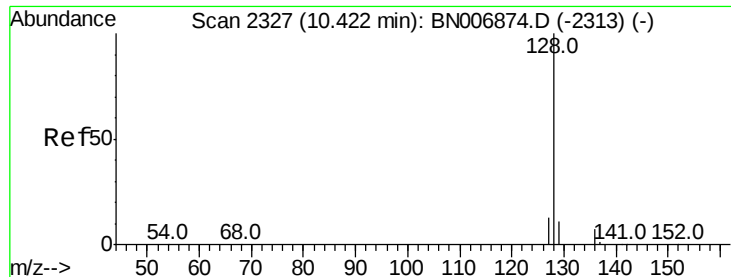

#3

Naphthalene

Concen: 0.064 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.01 min

Lab File: BN006900.D

Acq: 18 Jul 2019 20:11

Instrument :

BNA_N

ClientSampleId :

Tot Ion:128 Resp: 2015

Ion Ratio Lower Upper

128 100

129 18.8 9.4 14.0#

127 17.8 10.6 16.0#

