

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006908.D
 Acq On : 19 Jul 2019 01:58
 Operator : HP/JU
 Sample : K3764-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 05:29:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 03:57:16 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3441	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	12622	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	6421	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	666879	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.45	264	15310	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	3120	0.16	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.29	252	2665	0.043	ng/ul#	Ovalue 33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006908.D
Acq On : 19 Jul 2019 01:58
Operator : HP/JU
Sample : K3764-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 05:29:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 03:57:16 2019
Response via : Initial Calibration

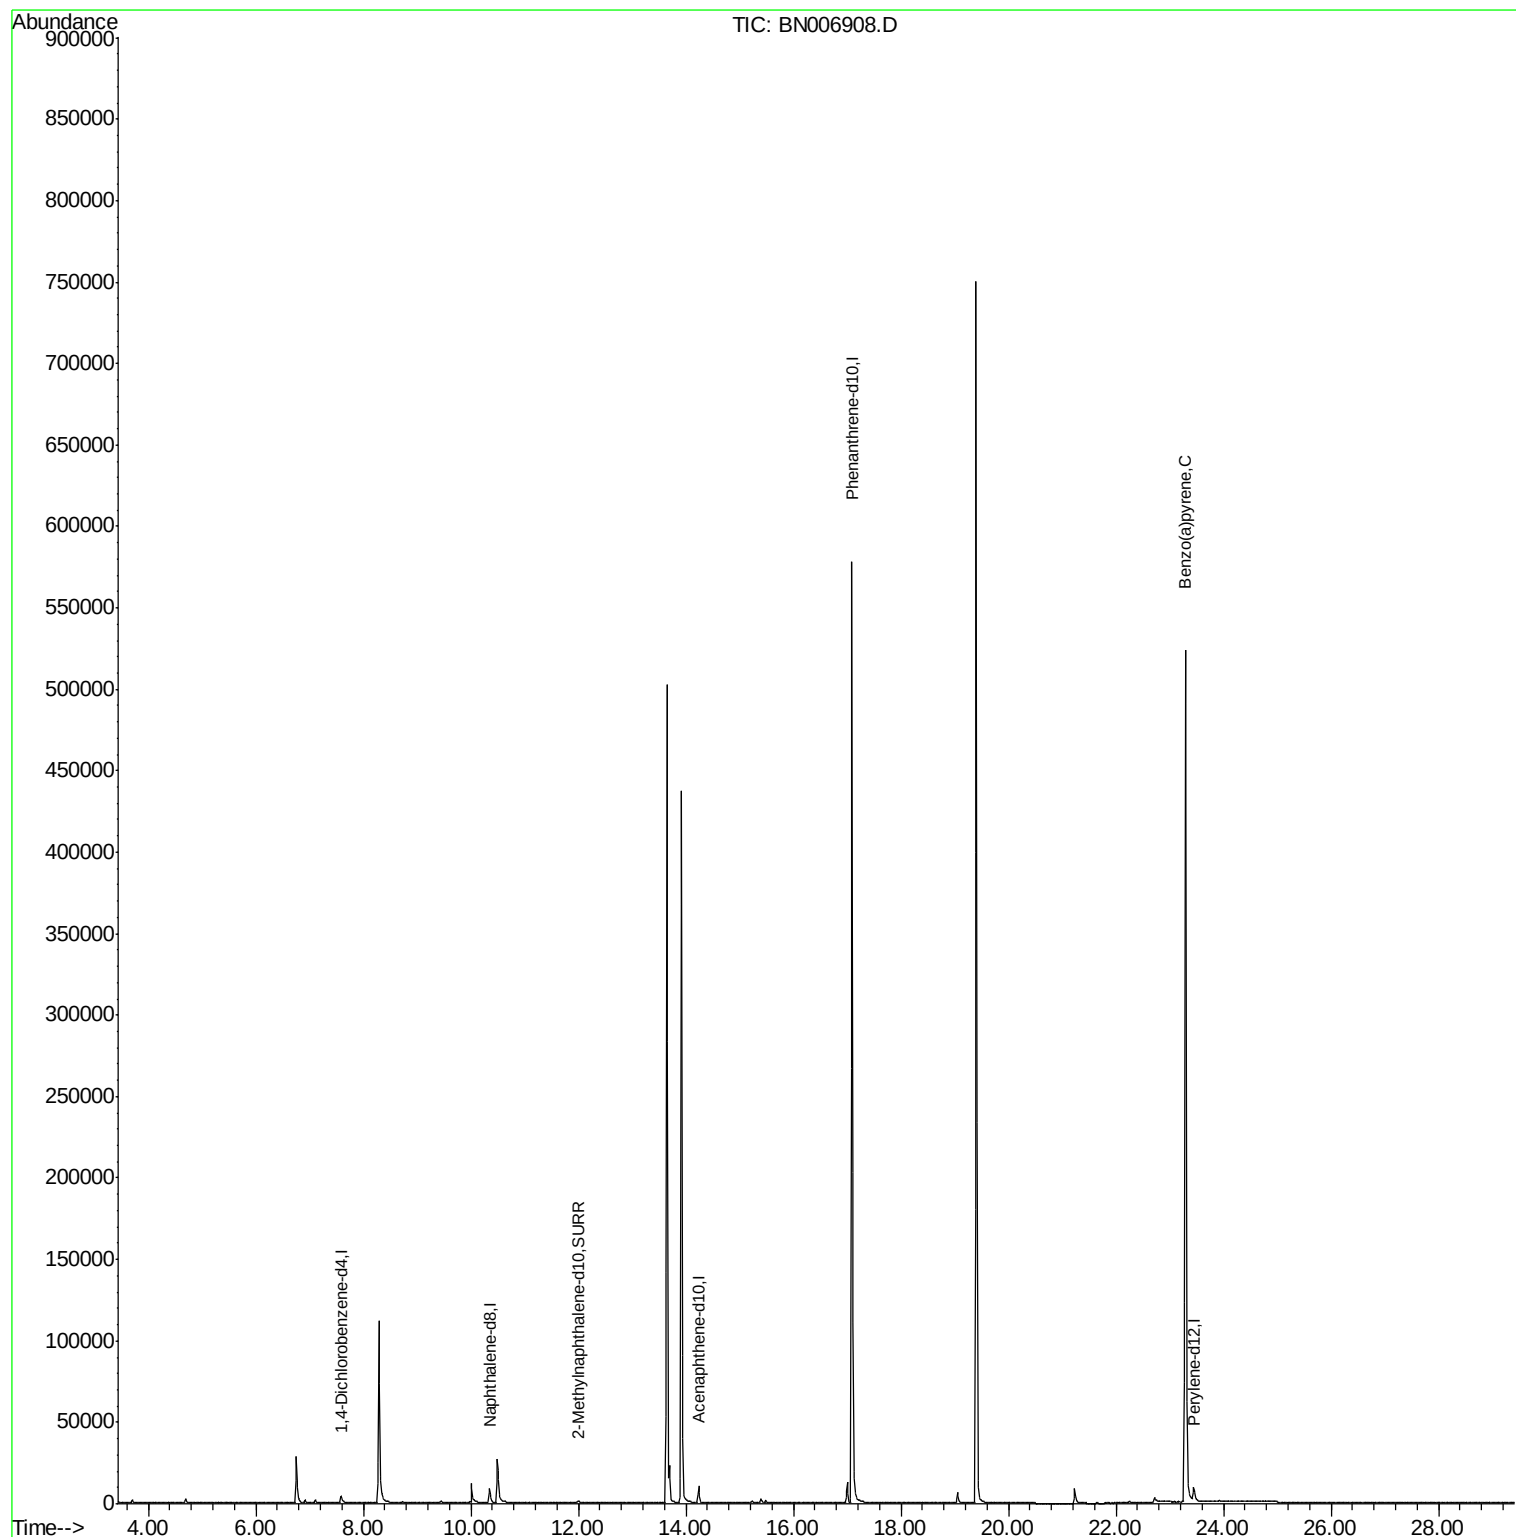

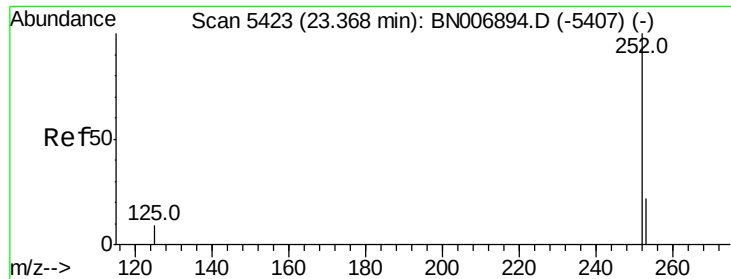

#23

Benzo(a)pyrene

Concen: 0.043 ng/ul

RT: 23.29 min Scan# 5397

Delta R.T. -0.10 min

Lab File: BN006908.D

Acq: 19 Jul 2019 01:58

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 2665

Ion Ratio Lower Upper

252 100

253 42.5 19.4 29.2#

125 63.8 12.6 19.0#

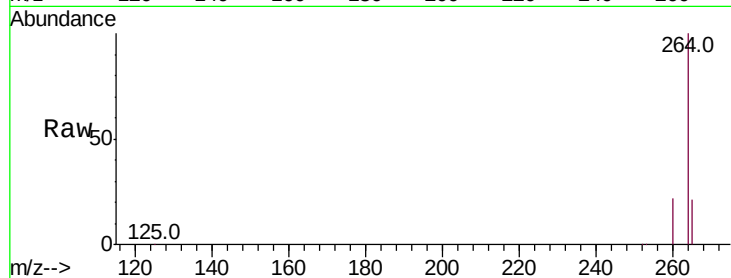

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

