

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006914.D
 Acq On : 19 Jul 2019 05:26
 Operator : HP/JU
 Sample : K3764-21
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 06:33:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 03:57:16 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3571	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	12950	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.23	164	6558	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.09	188	730304	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.45	264	15951	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	3705	0.19	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.29	252	3104	0.048	ng/ul#	Ovalue 36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006914.D
Acq On : 19 Jul 2019 05:26
Operator : HP/JU
Sample : K3764-21
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 06:33:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 03:57:16 2019
Response via : Initial Calibration

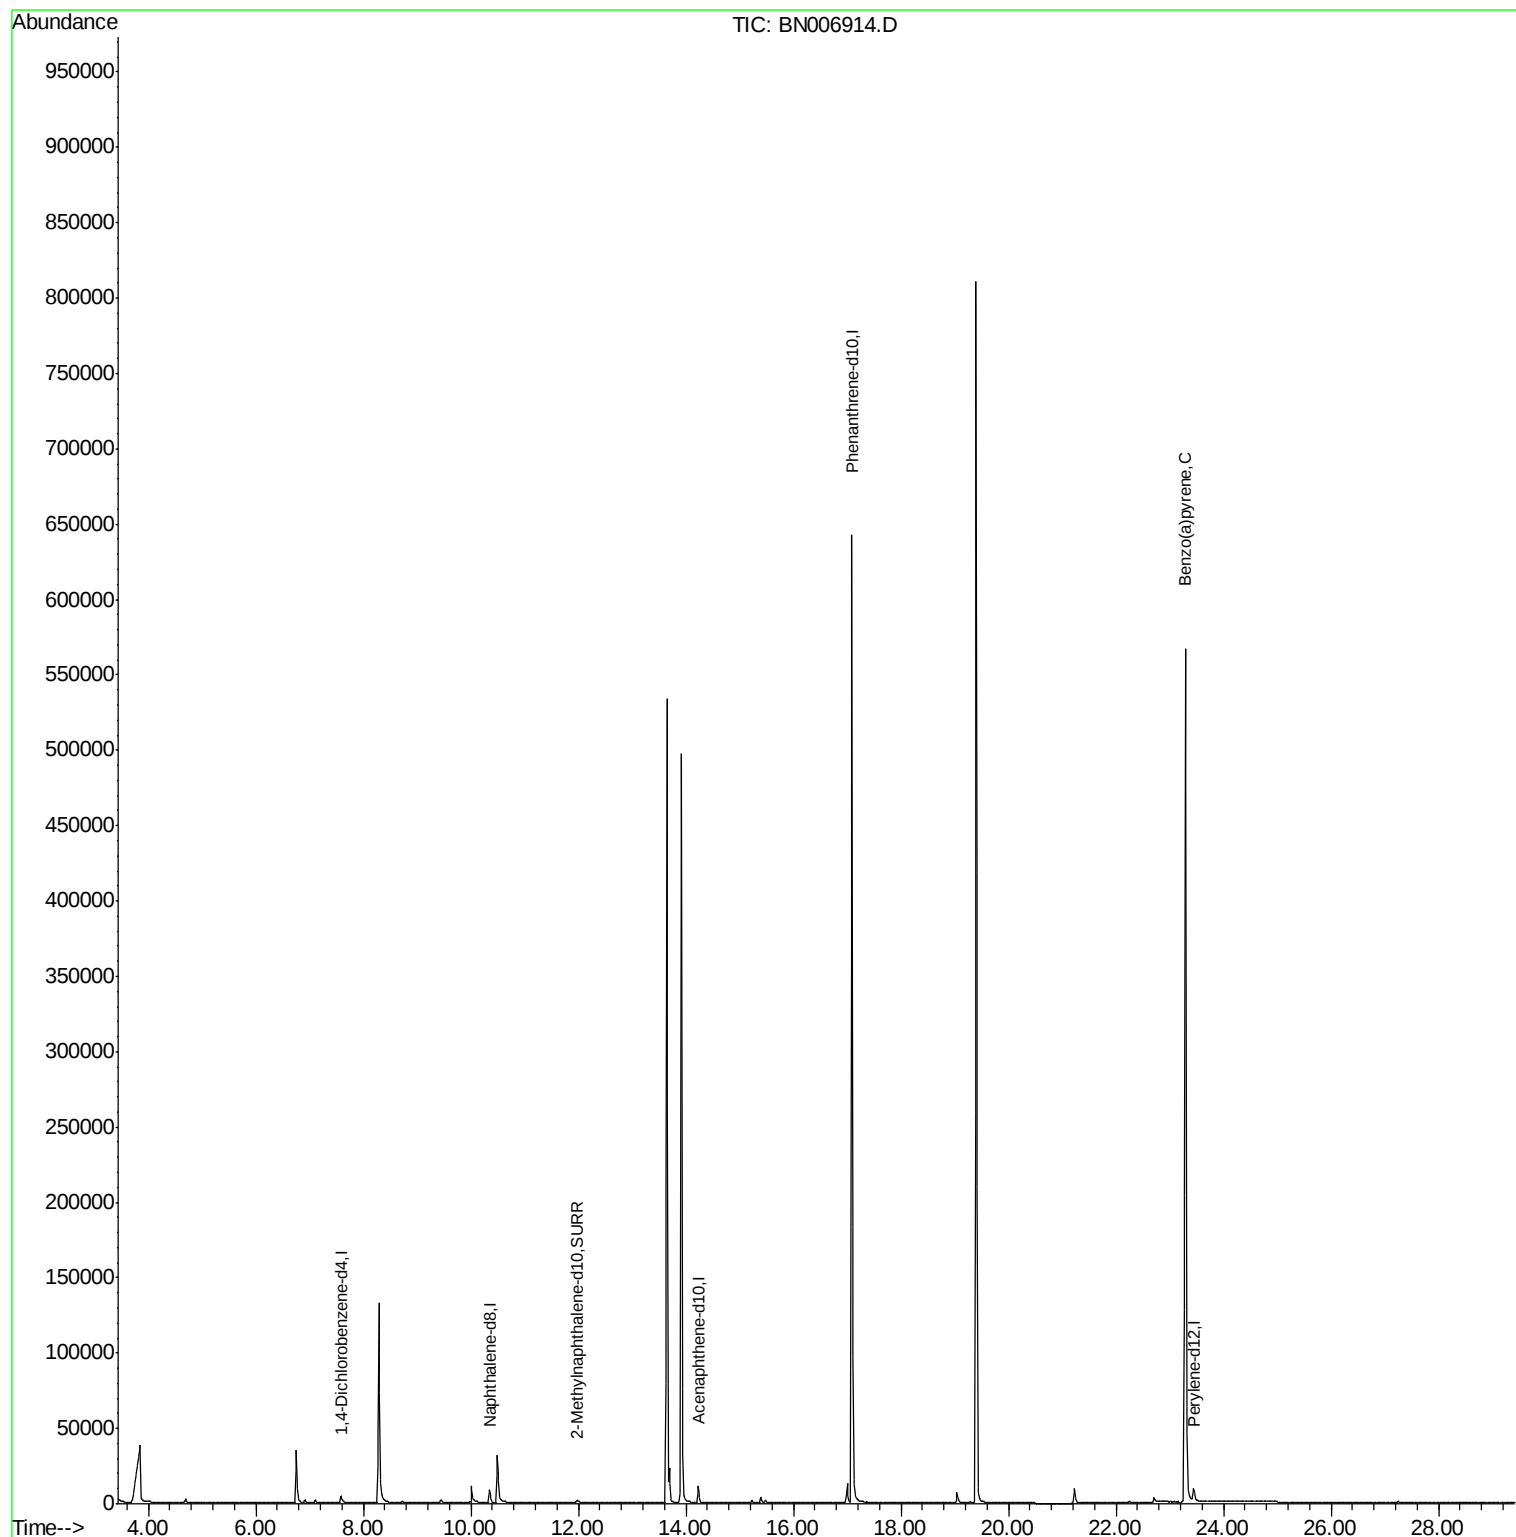

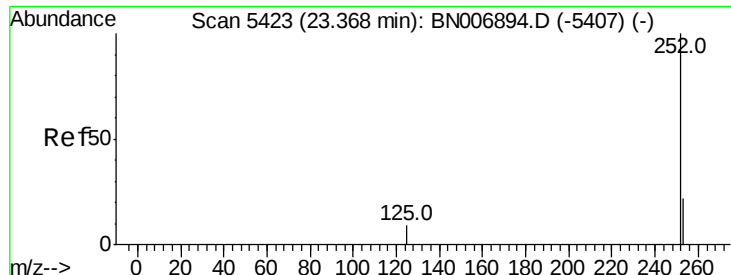

#23

Benzo(a)pyrene

Concen: 0.048 ng/ul

RT: 23.29 min Scan# 5396

Delta R.T. -0.10 min


Lab File: BN006914.D

Acq: 19 Jul 2019 05:26

Instrument :

BNA_N

ClientSampleId :

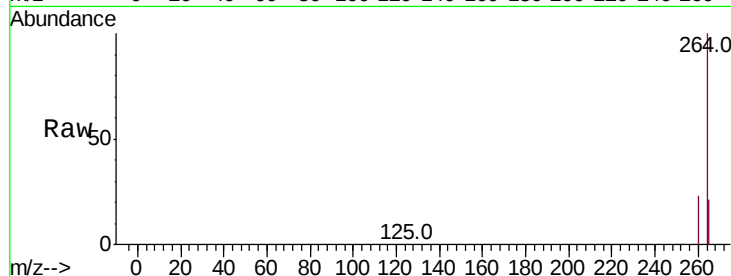

Tot Ion: 252 Resp: 3104

Ion Ratio Lower Upper

252 100

253 41.8 19.4 29.2#

125 61.0 12.6 19.0#

