

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006891.D
 Acq On : 18 Jul 2019 14:58
 Operator : HP/JU
 Sample : K3822-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4C6

Manual Integrations
 APPROVED

mohammad
 7/19/2019 3:59:23 PM

Quant Time: Jul 18 15:58:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3087	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10955	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5860	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	12612m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.24	240	10374m	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	9429m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	3864	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	9626m	0.26	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.40	128	6856	0.218	ng/ul	Ovalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006891.D
Acq On : 18 Jul 2019 14:58
Operator : HP/JU
Sample : K3822-12
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BF4C6

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:23 PM

Quant Time: Jul 18 15:58:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

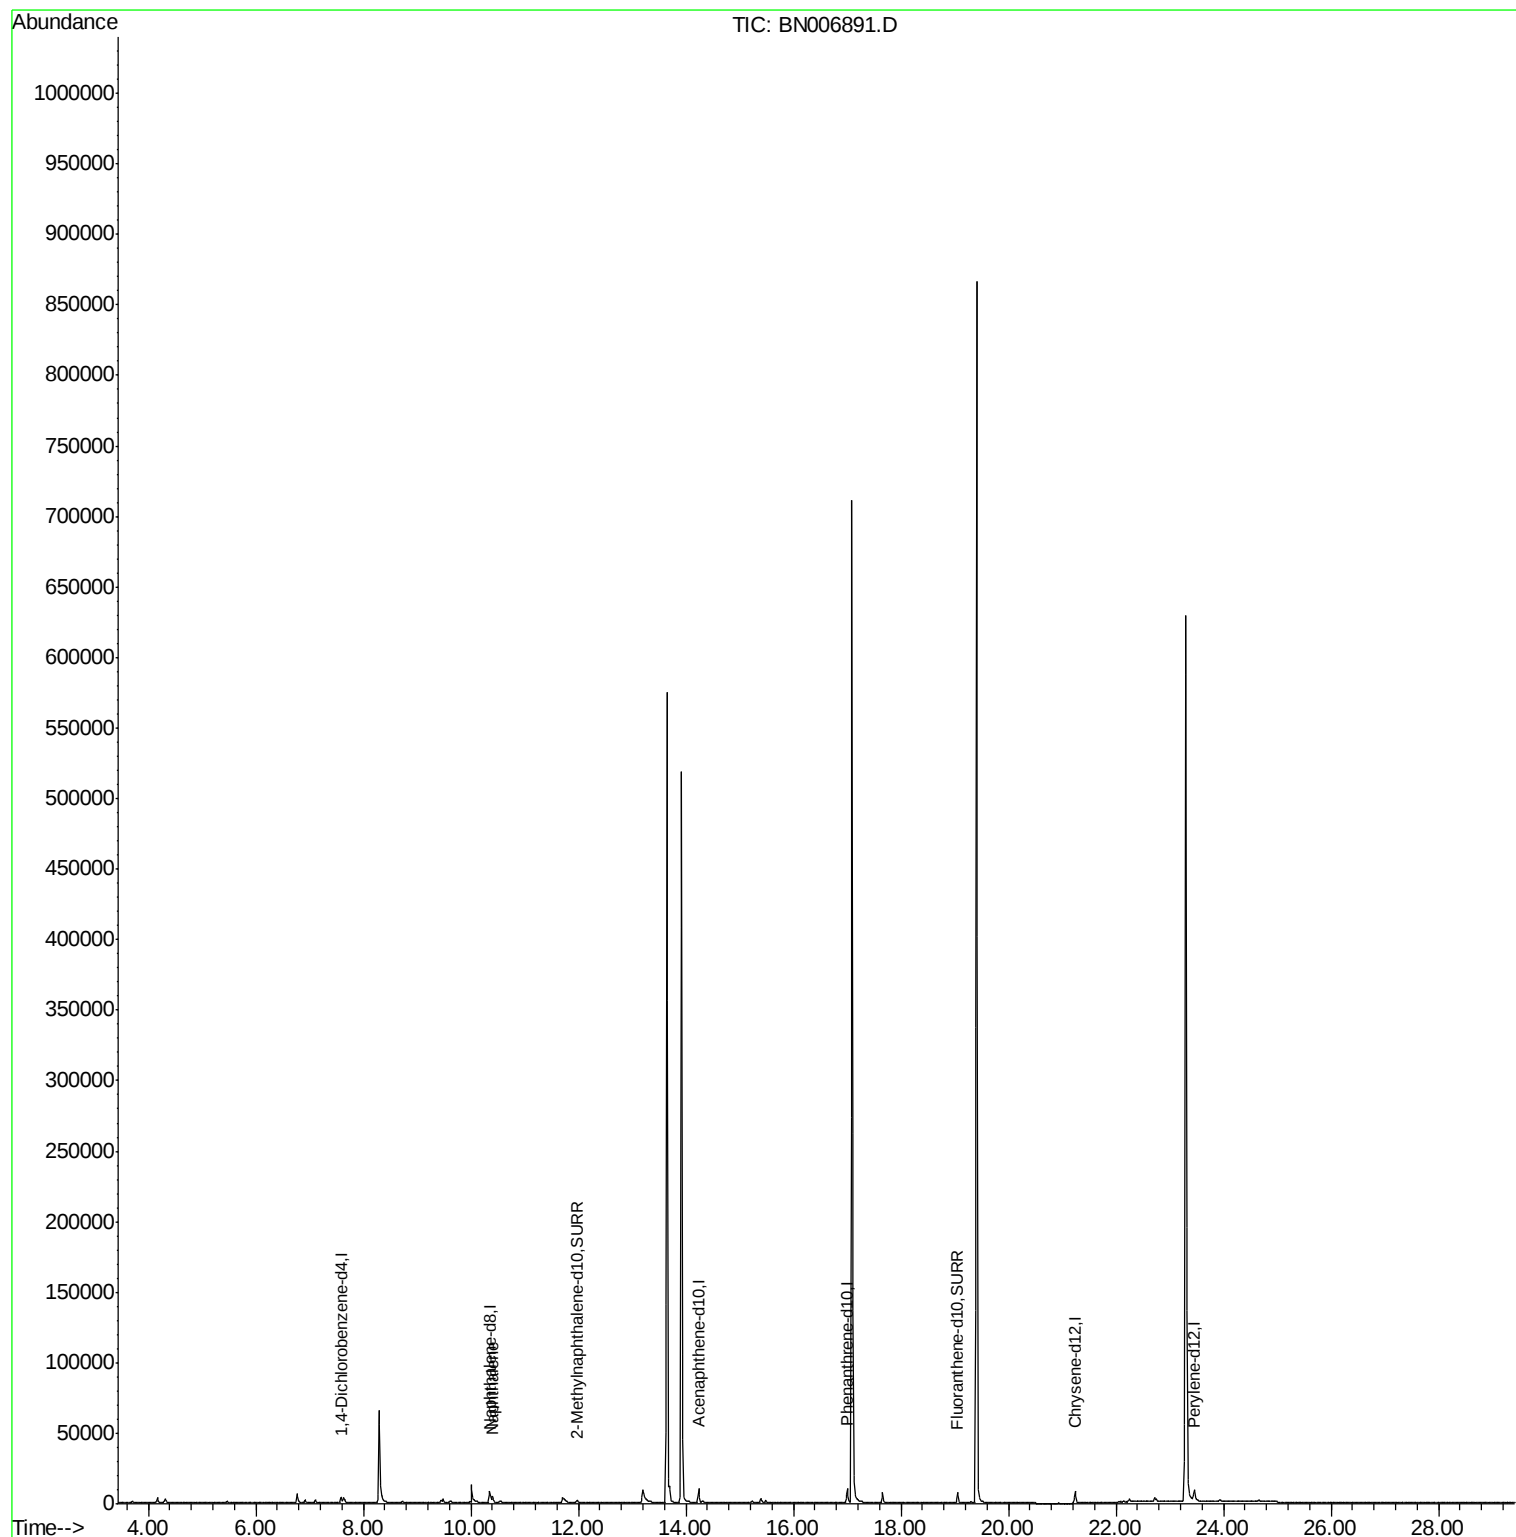

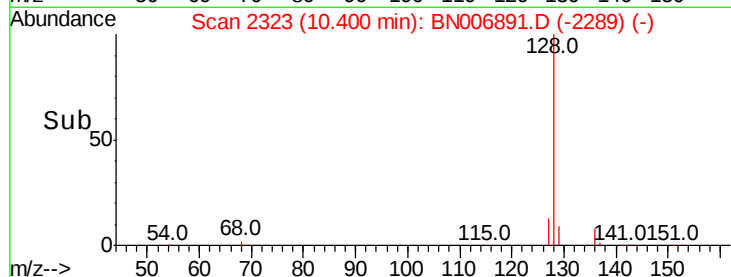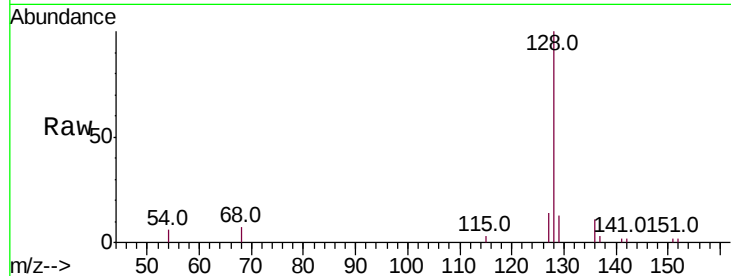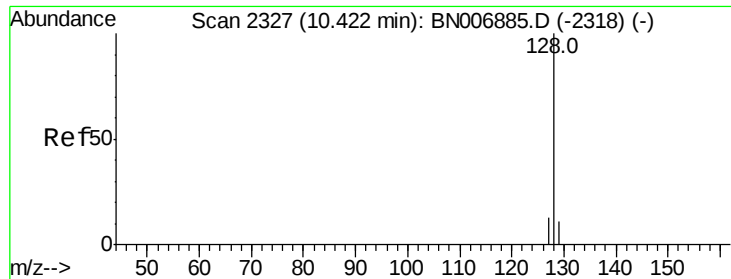

#3

Naphthalene

Concen: 0.218 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.01 min

Lab File: BN006891.D

Acq: 18 Jul 2019 14:58

Tot Ion:	128	Resp:	6856
Ion Ratio	Lower	Upper	
128	100		
129	13.3	9.4	14.0
127	14.2	10.6	16.0

Instrument :

BNA_N

ClientSampleId :

BF4C6

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:23 PM

