

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006892.D
 Acq On : 18 Jul 2019 15:32
 Operator : HP/JU
 Sample : K3822-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4C8

Manual Integrations
 APPROVED

mohammad
 7/19/2019 3:59:28 PM

Quant Time: Jul 18 16:15:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3371	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	12005	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	6371	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	13749m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.24	240	10664m	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	9771m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	4153	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	9537m	0.24	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.40	128	5063	0.147	ng/ul#	Ovalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006892.D
Acq On : 18 Jul 2019 15:32
Operator : HP/JU
Sample : K3822-13
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BF4C8

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:28 PM

Quant Time: Jul 18 16:15:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration



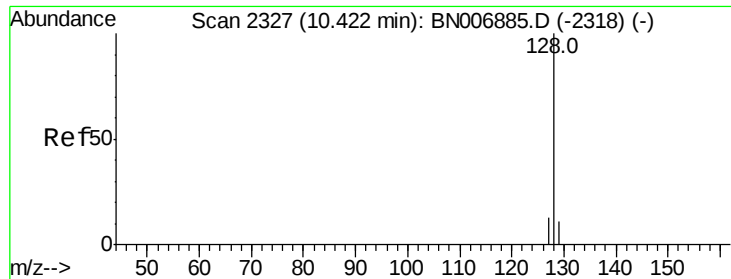

#3

Naphthalene

Concen: 0.147 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.01 min

Lab File: BN006892.D

Acq: 18 Jul 2019 15:32

Instrument :

BNA_N

ClientSampleId :

BF4C8

Tot Ion	Ratio	Lower	Upper
128	100		
129	14.0	9.4	14.0#
127	15.2	10.6	16.0

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:28 PM

