

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006893.D
 Acq On : 18 Jul 2019 16:07
 Operator : HP/JU
 Sample : K3822-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF485

Manual Integrations
 APPROVED

mohammad
 7/19/2019 3:59:26 PM

Quant Time: Jul 18 16:49:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2791	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10173	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5245	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	11584m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.24	240	9304m	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	8067m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	3165	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	8624m	0.25	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.30	153	1737	0.083	ng/ul	Ovalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006893.D
Acq On : 18 Jul 2019 16:07
Operator : HP/JU
Sample : K3822-01
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BF485

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:26 PM

Quant Time: Jul 18 16:49:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

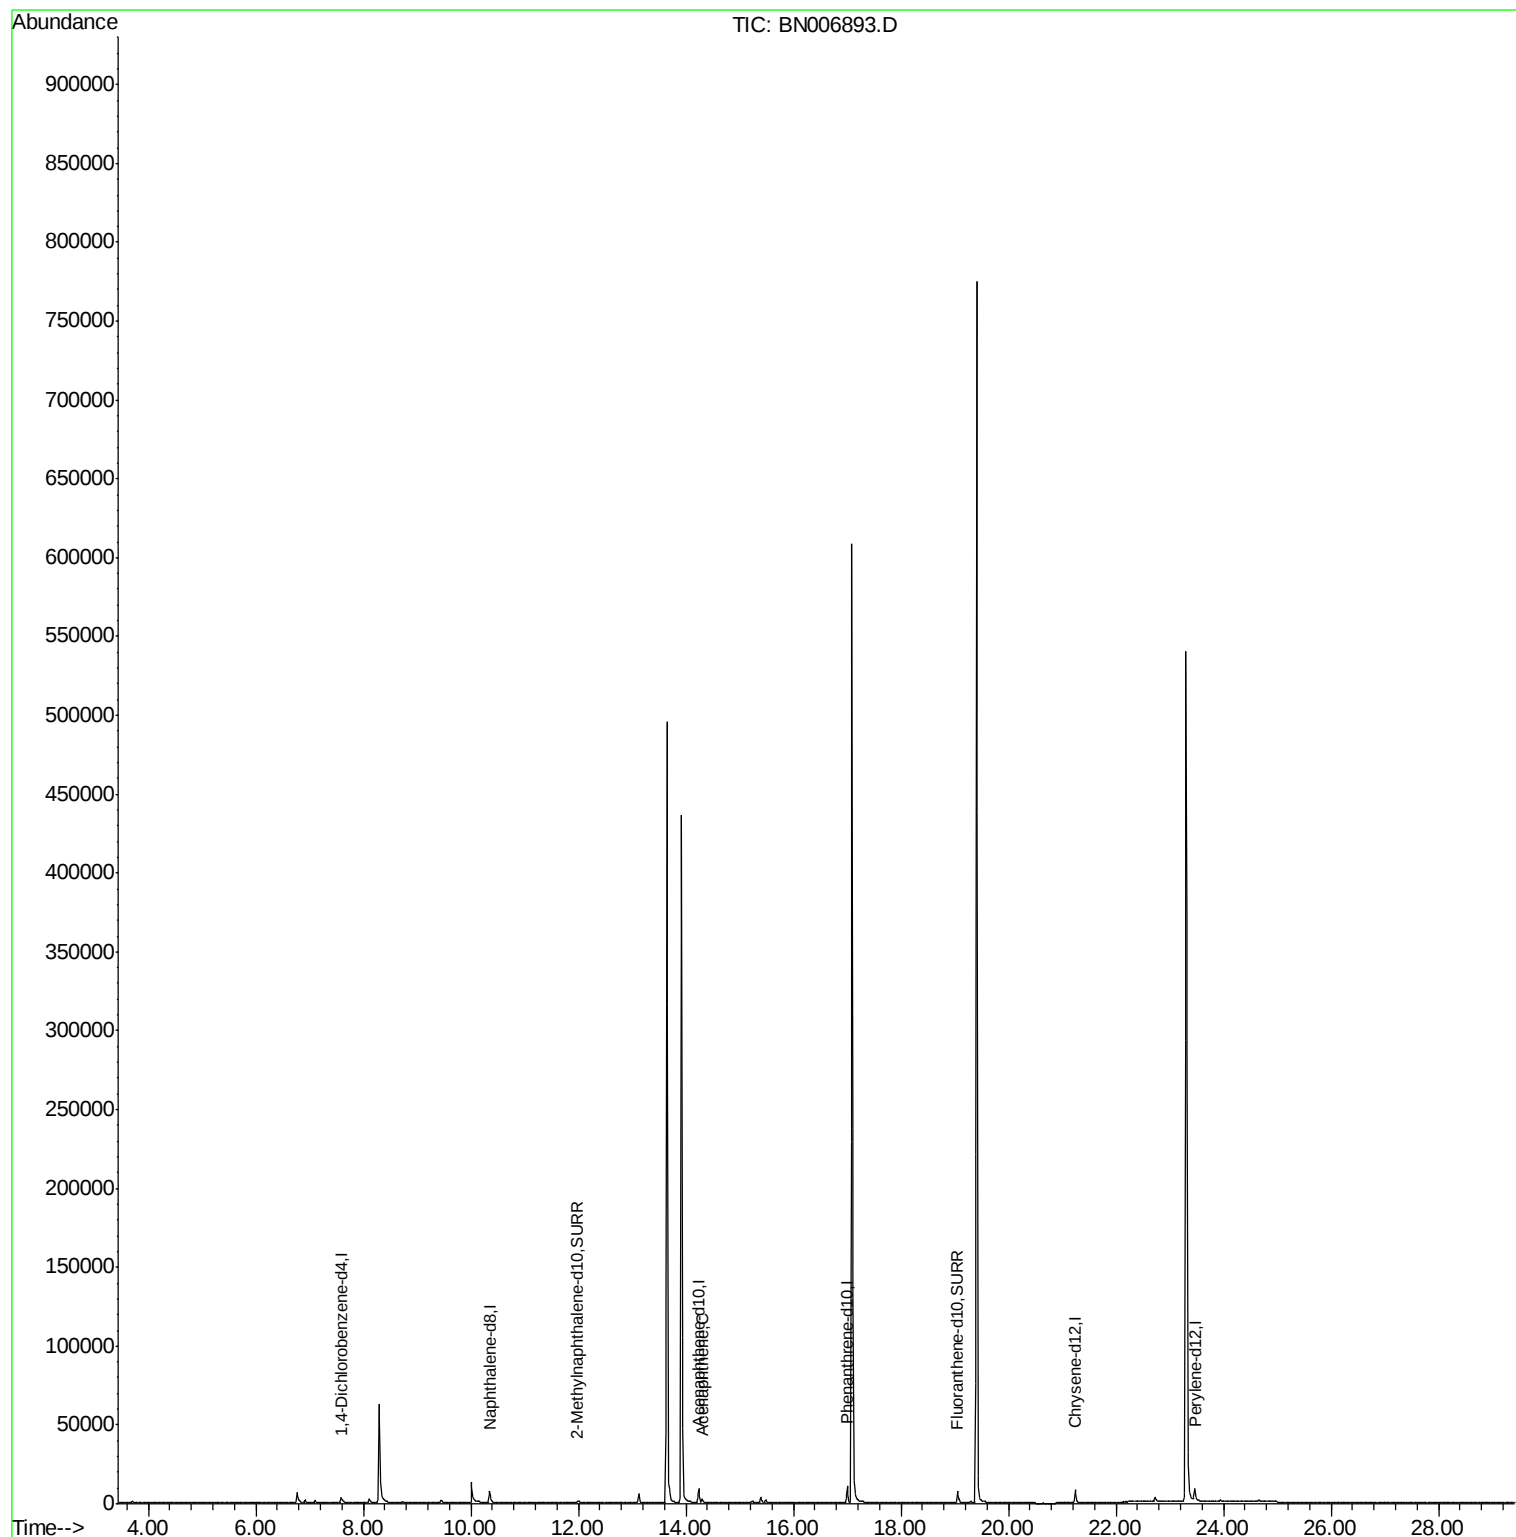

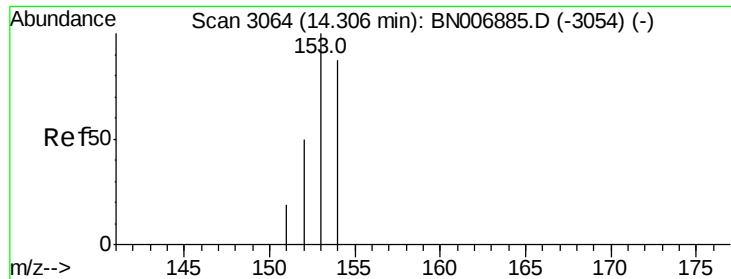

#8

Acenaphthene

Concen: 0.083 ng/ul

RT: 14.30 min Scan# 3063

Delta R.T. -0.00 min

Lab File: BN006893.D

Acq: 18 Jul 2019 16:07

Instrument :

BNA_N


ClientSampleId :

BF485

Tot Ion:	153	Resp:	1737
Ion Ratio	Lower	Upper	
153	100		
152	53.7	39.3	58.9
154	90.5	70.6	105.8

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:26 PM

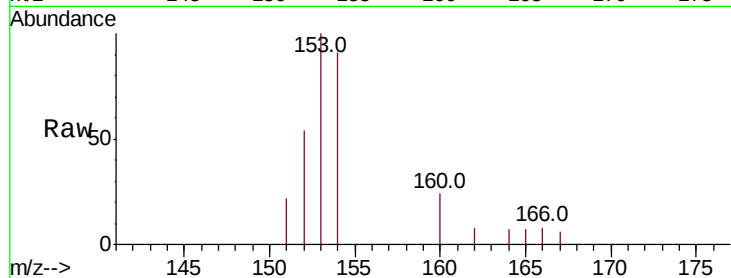

Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

