

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
 Data File : BN006899.D
 Acq On : 18 Jul 2019 19:36
 Operator : HP/JU
 Sample : K3822-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF483

Manual Integrations
 APPROVED

mohammad
 7/19/2019 3:59:40 PM

Quant Time: Jul 19 04:08:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	3145	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	11500	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	6129	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	13340m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.23	240	11094m	0.40	ng/ul	-0.01
20) Perylene-d12	23.44	264	9969m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	4097	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.04	212	11070m	0.28	ng/ul	0.00
Target Compounds						
13) Anthracene	17.13	178	1477m	0.040	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071819\
Data File : BN006899.D
Acq On : 18 Jul 2019 19:36
Operator : HP/JU
Sample : K3822-05
Misc :
ALS Vial : 15 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
BF483

Manual Integrations
APPROVED

mohammad
7/19/2019 3:59:40 PM

Quant Time: Jul 19 04:08:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

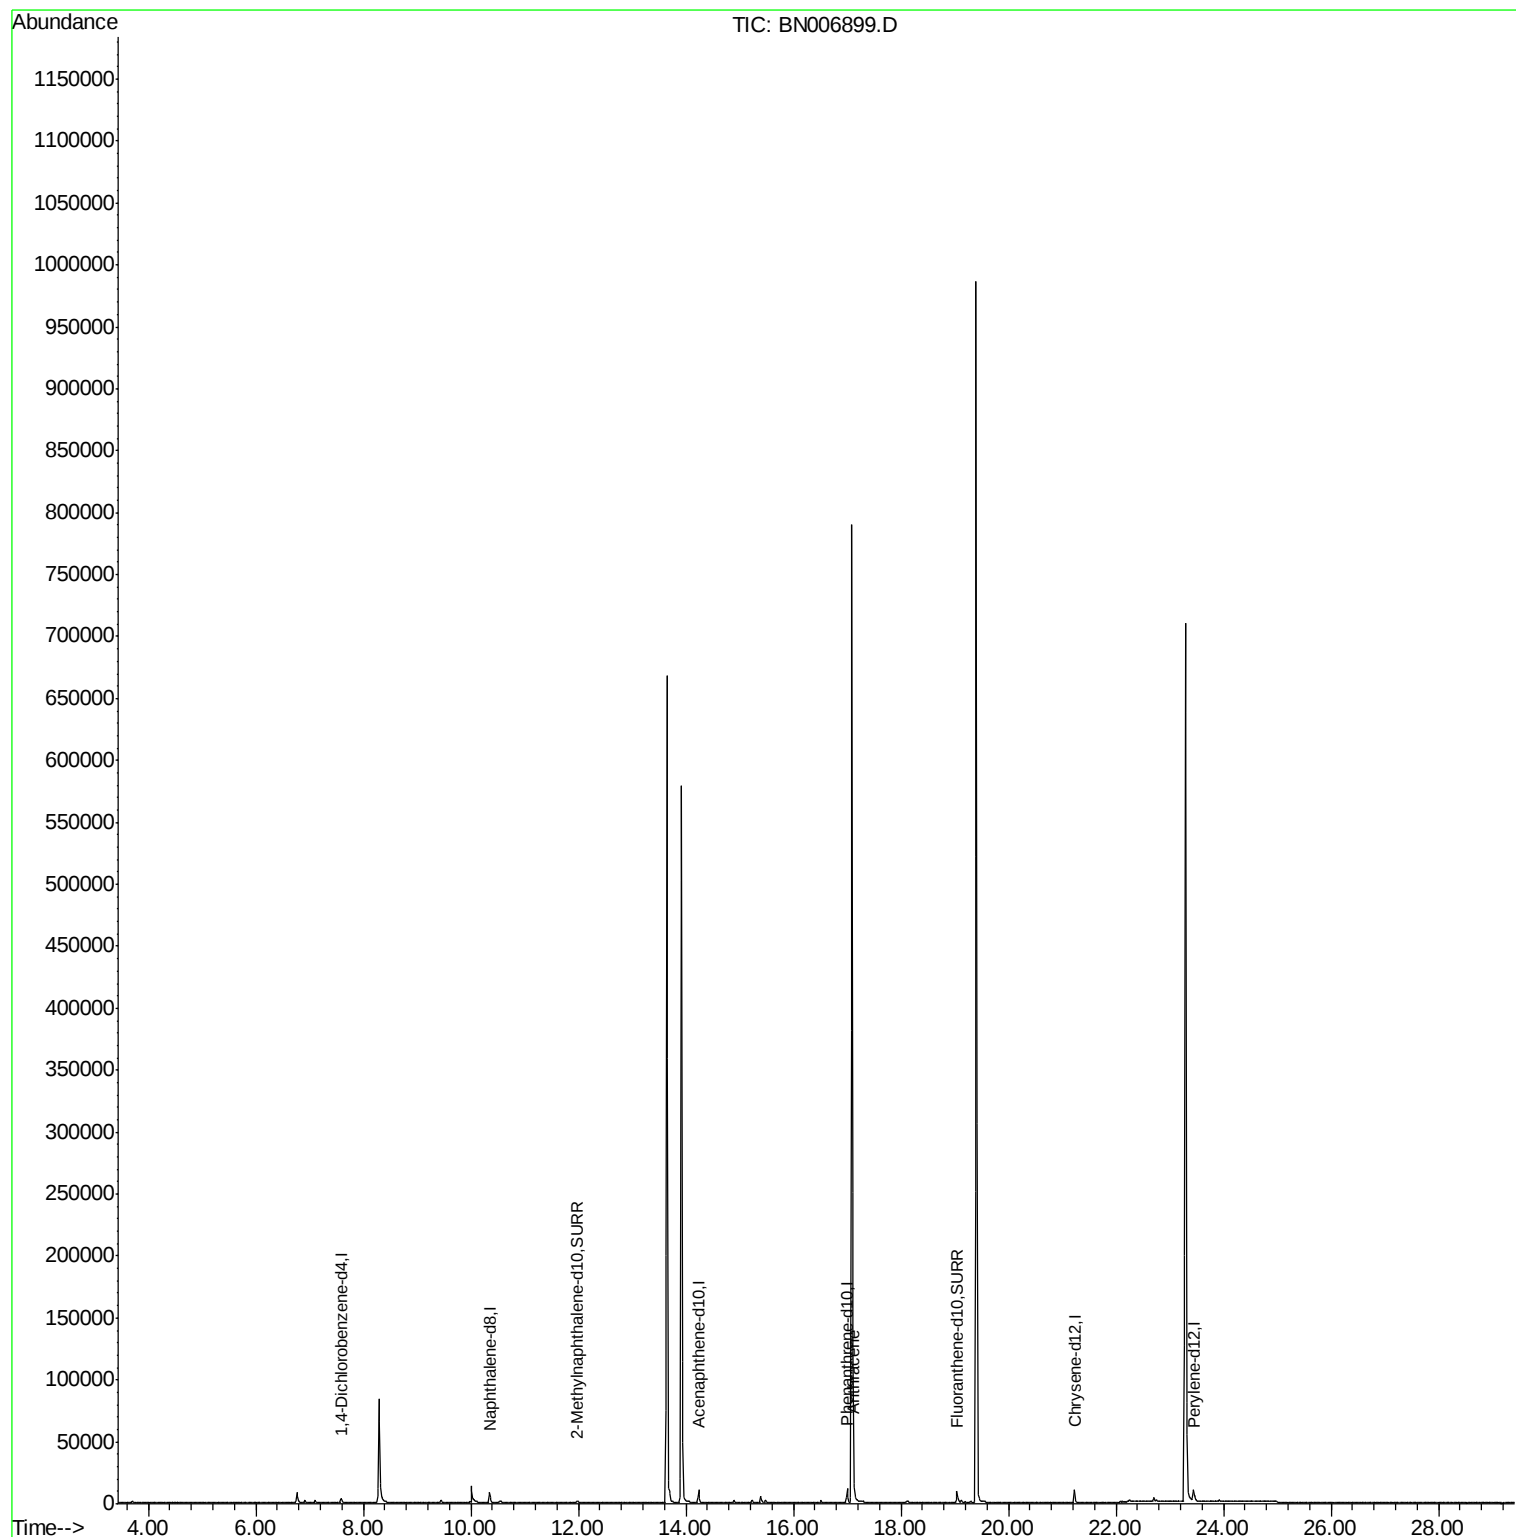

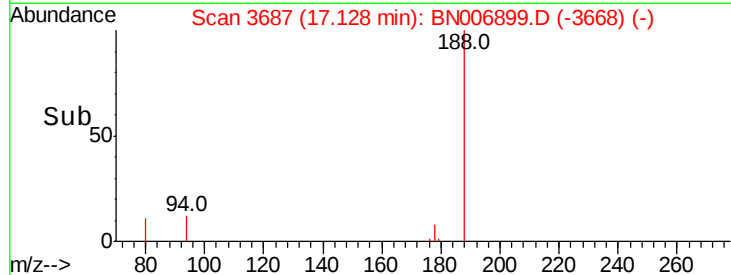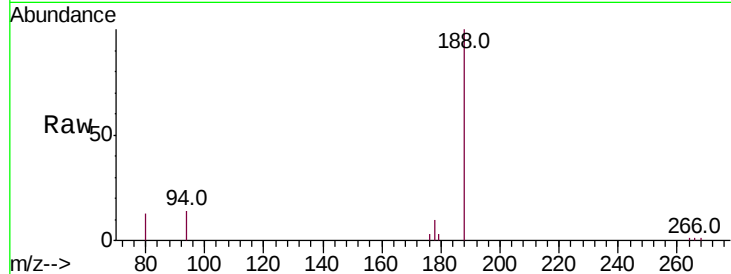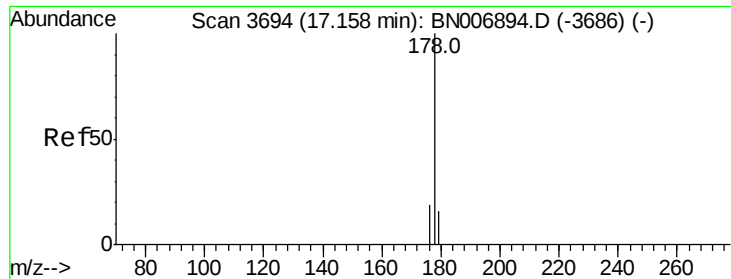

#13

Anthracene

Concen: 0.040 ng/ul m

RT: 17.13 min Scan# 3687

Delta R.T. -0.02 min

Lab File: BN006899.D

Acq: 18 Jul 2019 19:36

Instrument :

BNA_N

ClientSampleId :

BF483

Tot Ion:178 Resp: 1477

Ion Ratio Lower Upper

178 100

179 28.8 12.7 19.1#

176 27.9 15.8 23.6#

Manual Integrations

APPROVED

mohammad

7/19/2019 3:59:40 PM

