
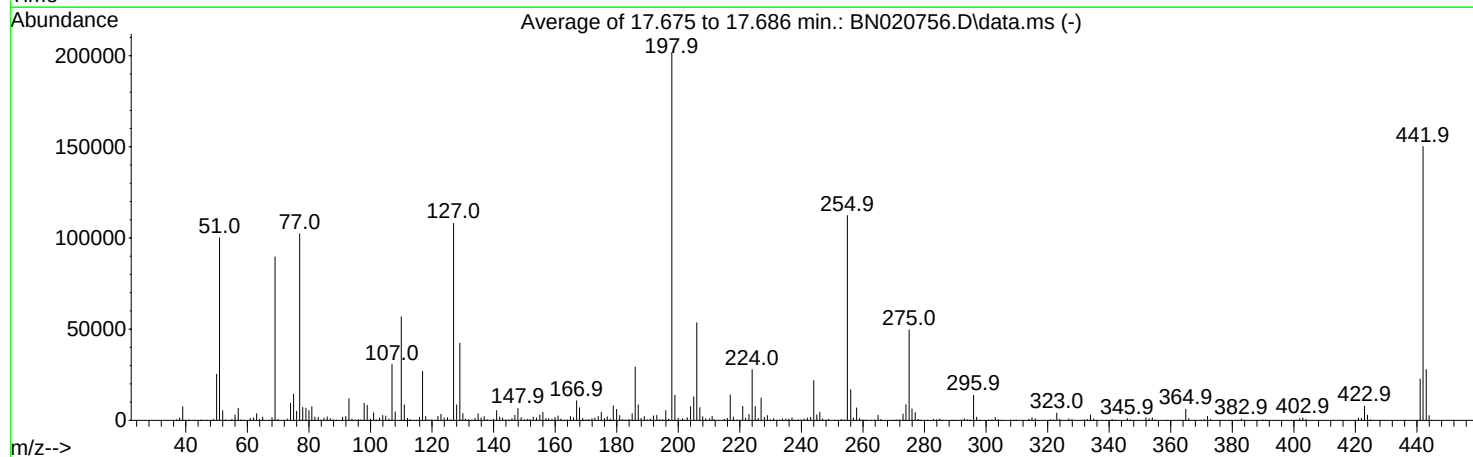


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071822\
 Data File : BN020756.D
 Acq On : 18 Jul 2022 12:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 16 03:21:59 2022

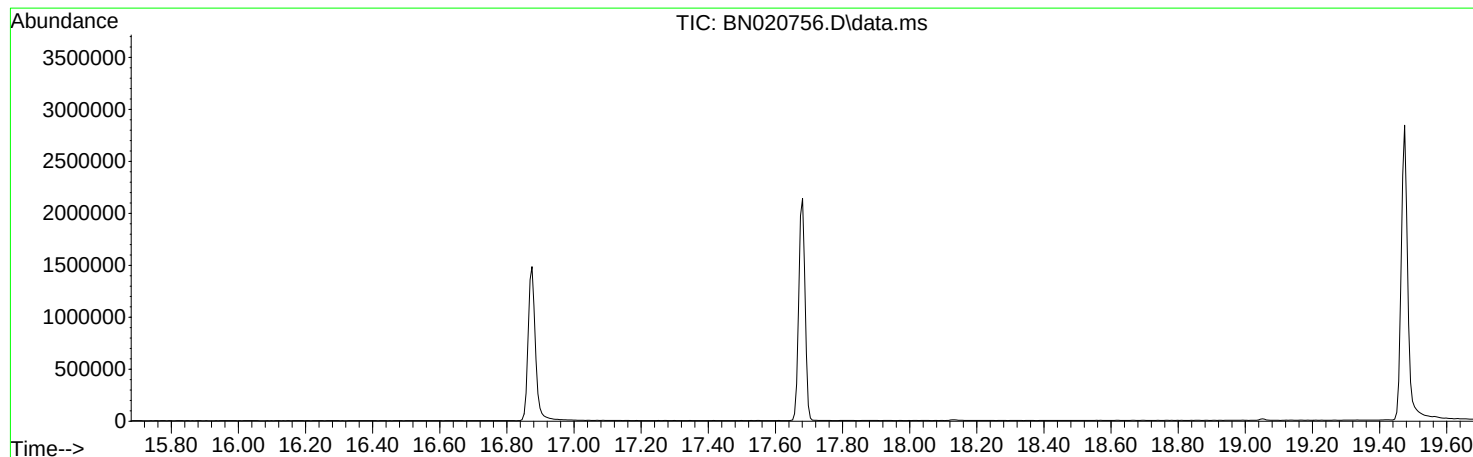




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.6	100087	PASS
68	69	0.00	2	1.8	1607	PASS
69	198	0.00	100	44.4	89573	PASS
70	69	0.00	2	0.5	446	PASS
127	198	10	80	53.5	108024	PASS
197	198	0.00	2	0.4	738	PASS
198	198	100	100	100.0	201728	PASS
199	198	5	9	6.8	13815	PASS
275	198	10	60	24.6	49680	PASS
365	198	1	100	3.1	6176	PASS
441	198	0.01	100	11.2	22664	PASS
442	442	50	100	100.0	150173	PASS
443	442	15	24	18.6	27928	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071822\
 Data File : BN020756.D
 Acq On : 18 Jul 2022 12:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 19 05:50:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 19 05:50:52 2022
 Response via : Initial Calibration

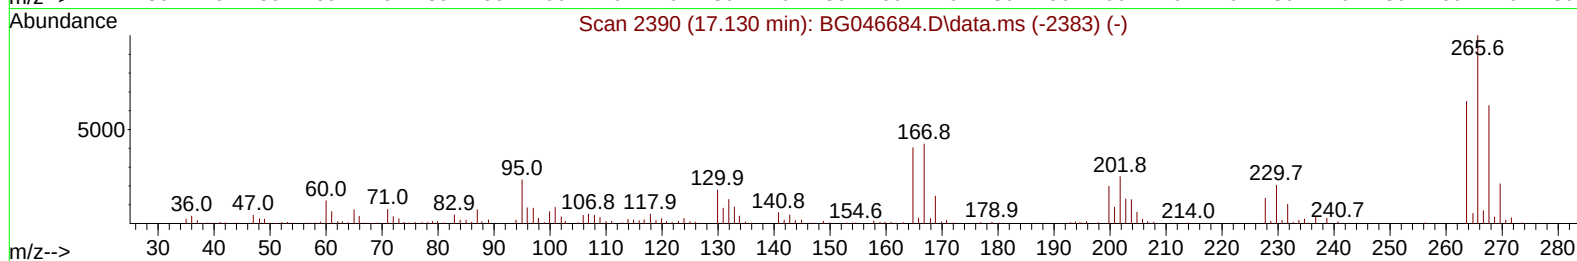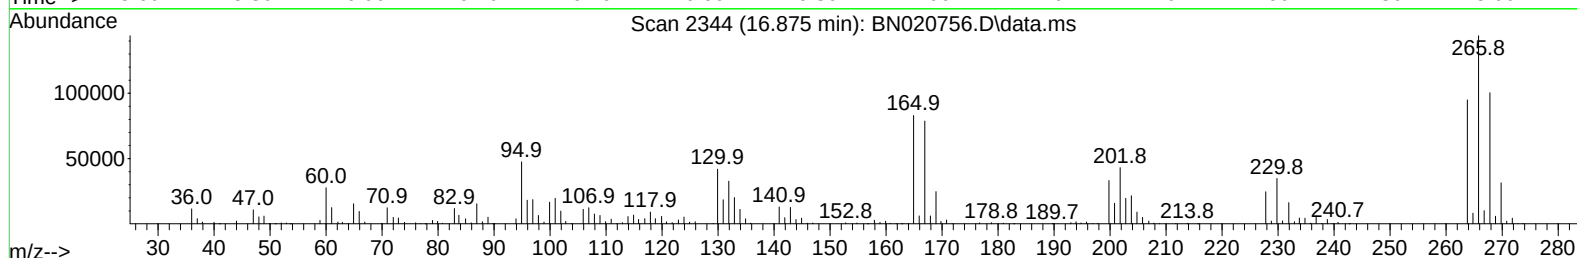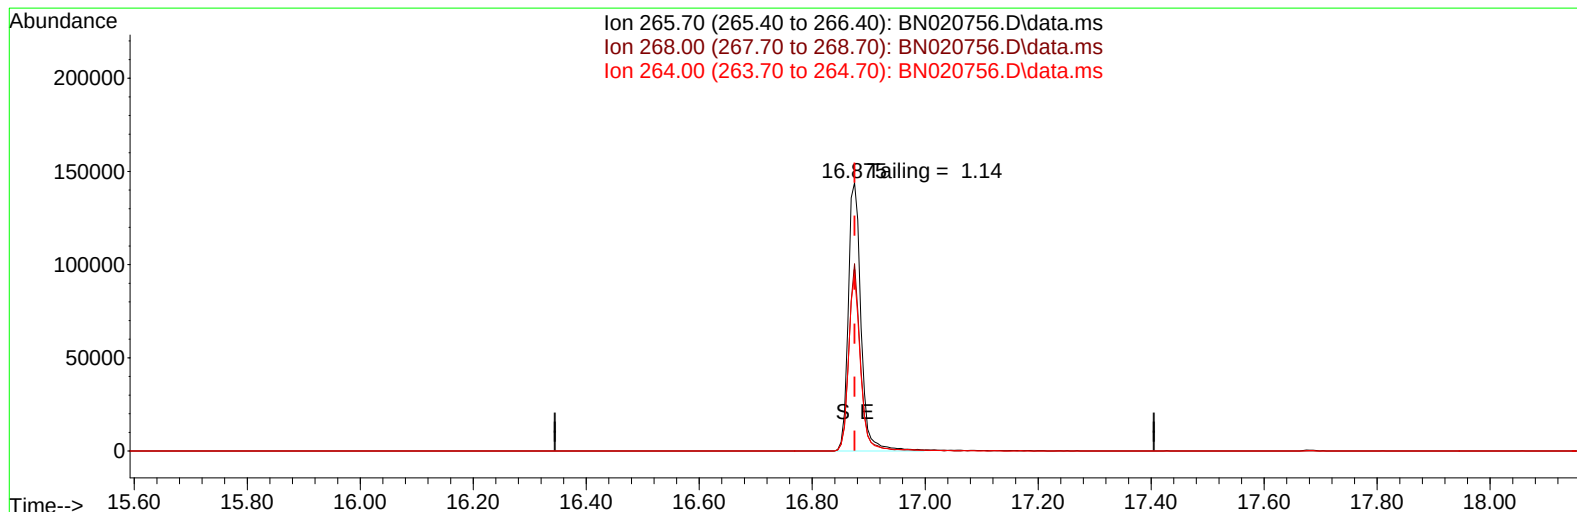

TIC: BN020756.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 18144.25 ng




response 228396

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.73
264.00	61.60	65.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071822\
Data File : BN020756.D
Acq On : 18 Jul 2022 12:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 19 05:50:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 19 05:50:52 2022
Response via : Initial Calibration

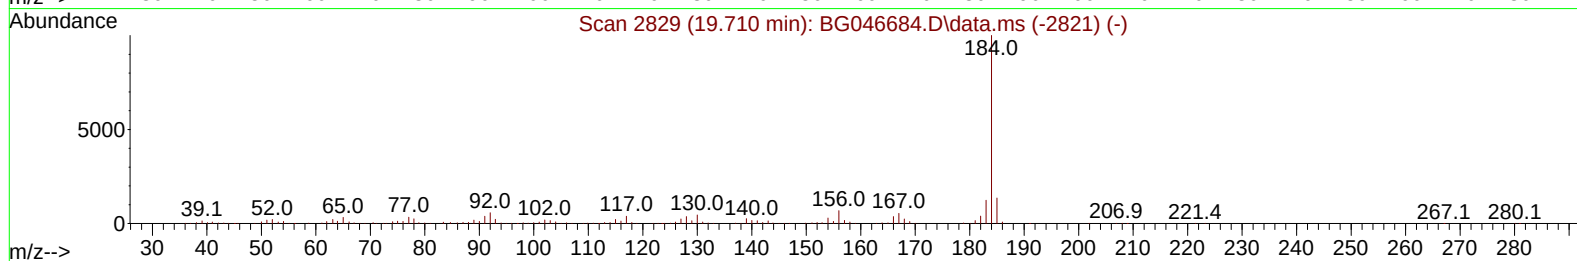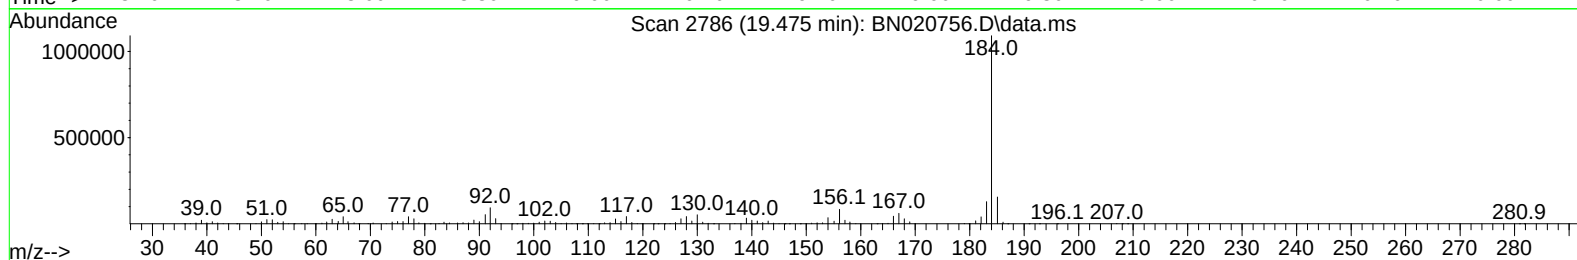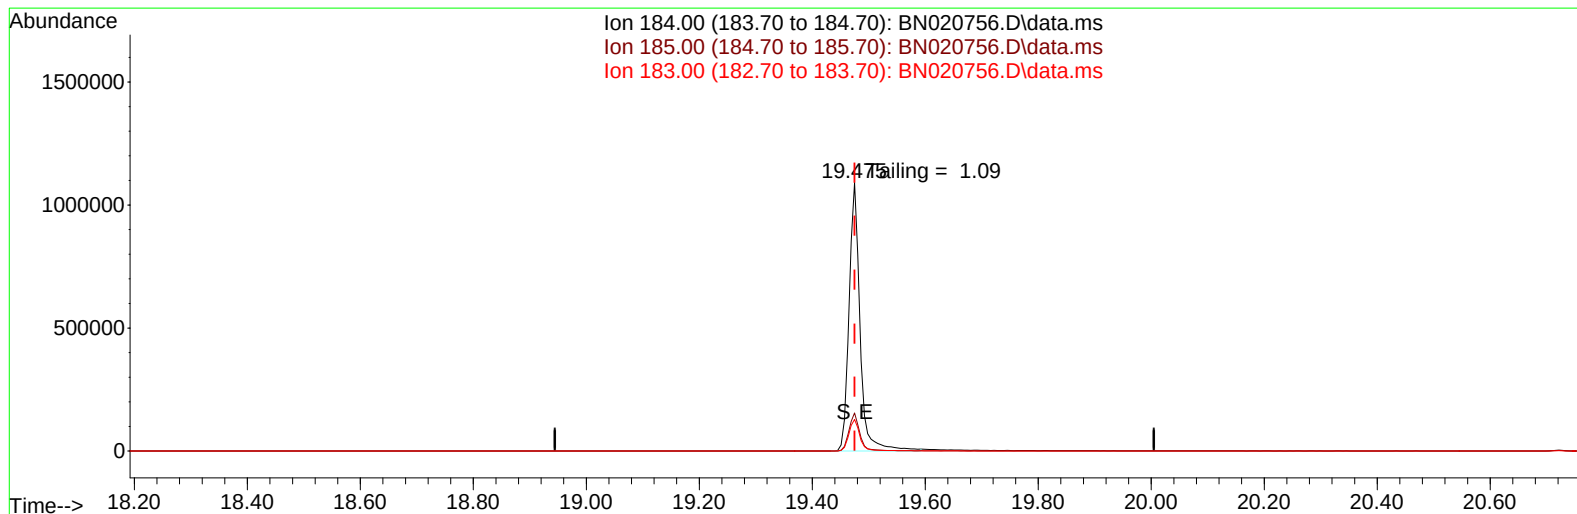

TIC: BN020756.D\data.ms

(77) Benzidine

19.475min (0.000) 0.00 ng

response 1508590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/18/2022	BNA_N	<u>BN020756.D</u>
Compound Name	Response	Retention Time
DDT	777361	20.722
DDD	13416	20.28
DDE	2048	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15464	792825	1.95

Instrument :
BNA_N
ClientSampleId :
DFTPP