

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071823\
 Data File : BN026561.D
 Acq On : 18 Jul 2023 13:02
 Operator : MA/JU
 Sample : PB154018BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 00:16:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 19 00:15:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	2310	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.737	136	7286	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.575	164	4992	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	11859	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.540	240	11263	0.400	ng/ul	# 0.00
23) Perylene-d12	23.966	264	13666	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	22572	7.419	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	4224	0.426	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	15590	0.399	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.725	202	2474	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.808	252	5702	0.120	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071823\
Data File : BN026561.D
Acq On : 18 Jul 2023 13:02
Operator : MA/JU
Sample : PB154018BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 19 00:16:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 19 00:15:47 2023
Response via : Initial Calibration

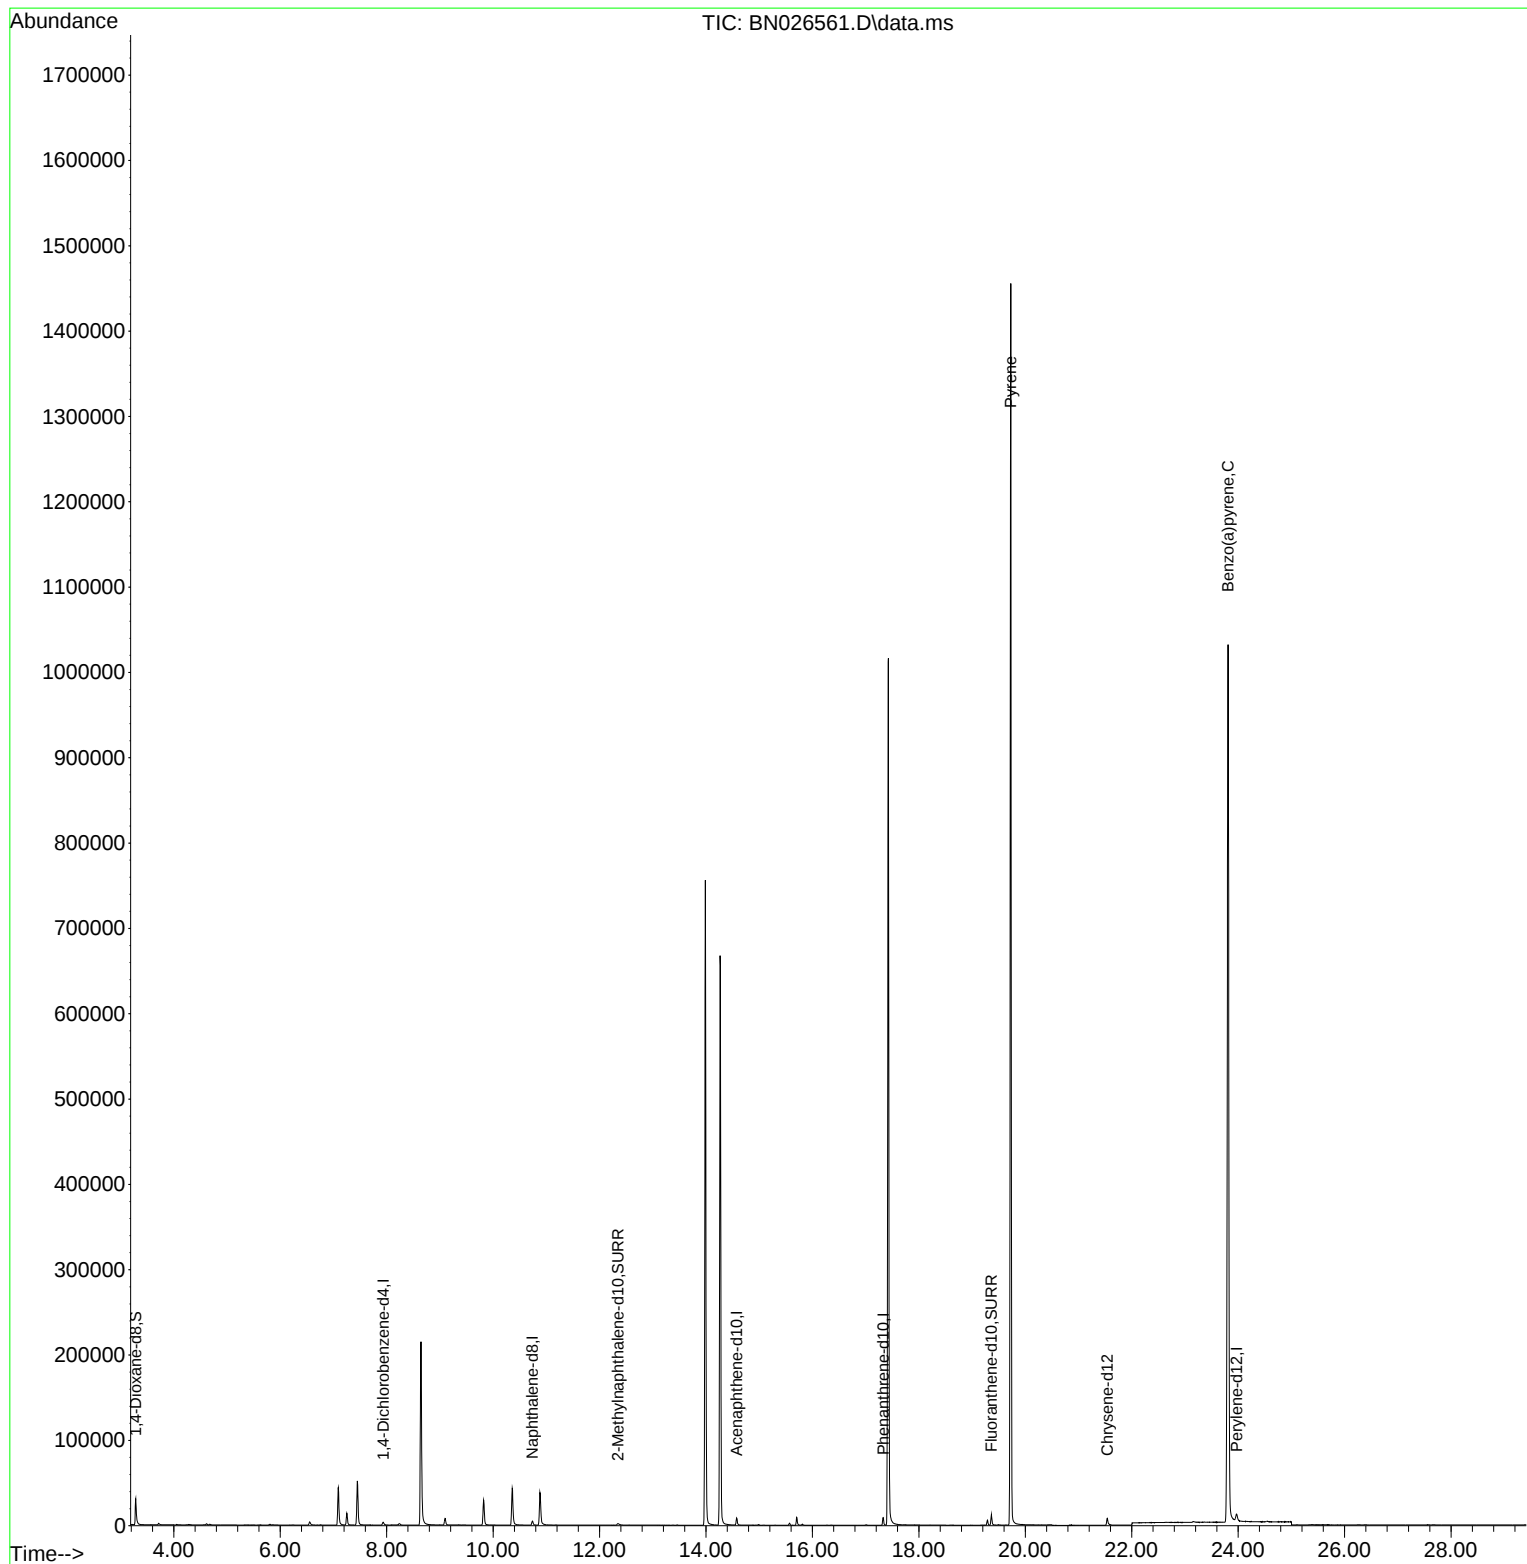



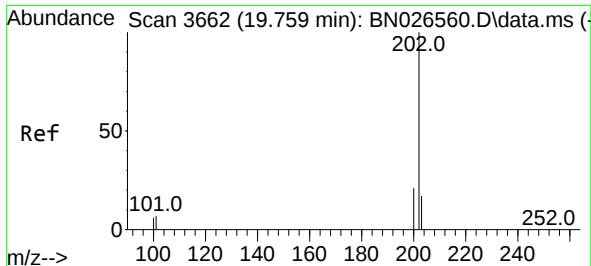


#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.725 min Scan# 30
Delta R.T. -0.033 min
Lab File: BN026561.D
Acq: 18 Jul 2023 13:02

Instrument :
BNA_N
ClientSampleId :

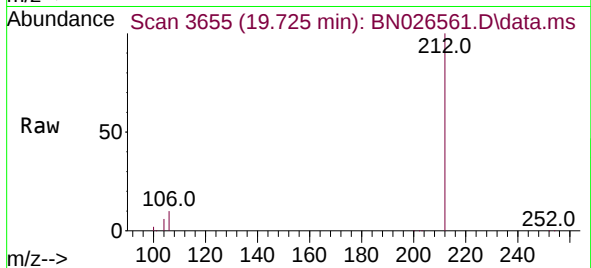

Tgt Ion:202 Resp: 2474
Ion Ratio Lower Upper
202 100
101 199.5 8.0 12.0#
100 1624.6 6.2 9.2#

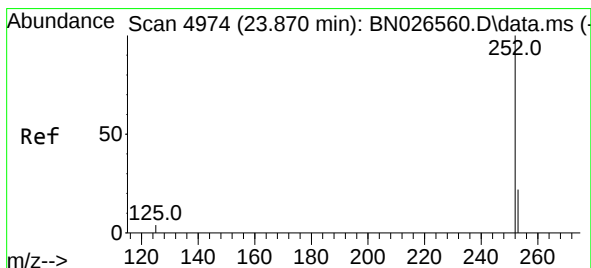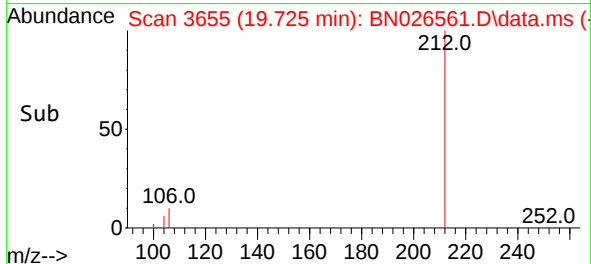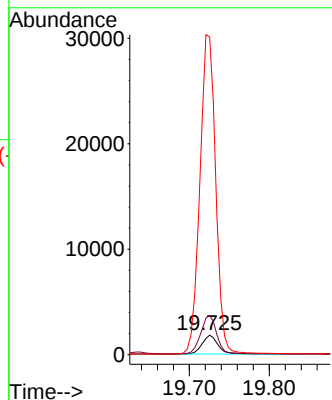

#26
Benzo(a)pyrene
Concen: 0.120 ng/ul
RT: 23.808 min Scan# 4953
Delta R.T. -0.062 min
Lab File: BN026561.D
Acq: 18 Jul 2023 13:02

Tgt Ion:252 Resp: 5702
Ion Ratio Lower Upper
252 100
253 47.7 32.6 49.0
125 48.7 19.3 28.9#

