

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071823\
 Data File : BN026563.D
 Acq On : 18 Jul 2023 14:16
 Operator : MA/JU
 Sample : 03458-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 00:16:47 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 19 00:15:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	2626	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.737	136	8399	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.575	164	5405	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	12455	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.535	240	11719	0.400	ng/ul	# 0.00
23) Perylene-d12	23.964	264	12481	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	13380	3.869	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	2614	0.229	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	8821	0.217	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.569	166	1305	0.062	ng/ul#	16
26) Benzo(a)pyrene	23.803	252	3154	0.073	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071823\
Data File : BN026563.D
Acq On : 18 Jul 2023 14:16
Operator : MA/JU
Sample : 03458-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 19 00:16:47 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 19 00:15:47 2023
Response via : Initial Calibration

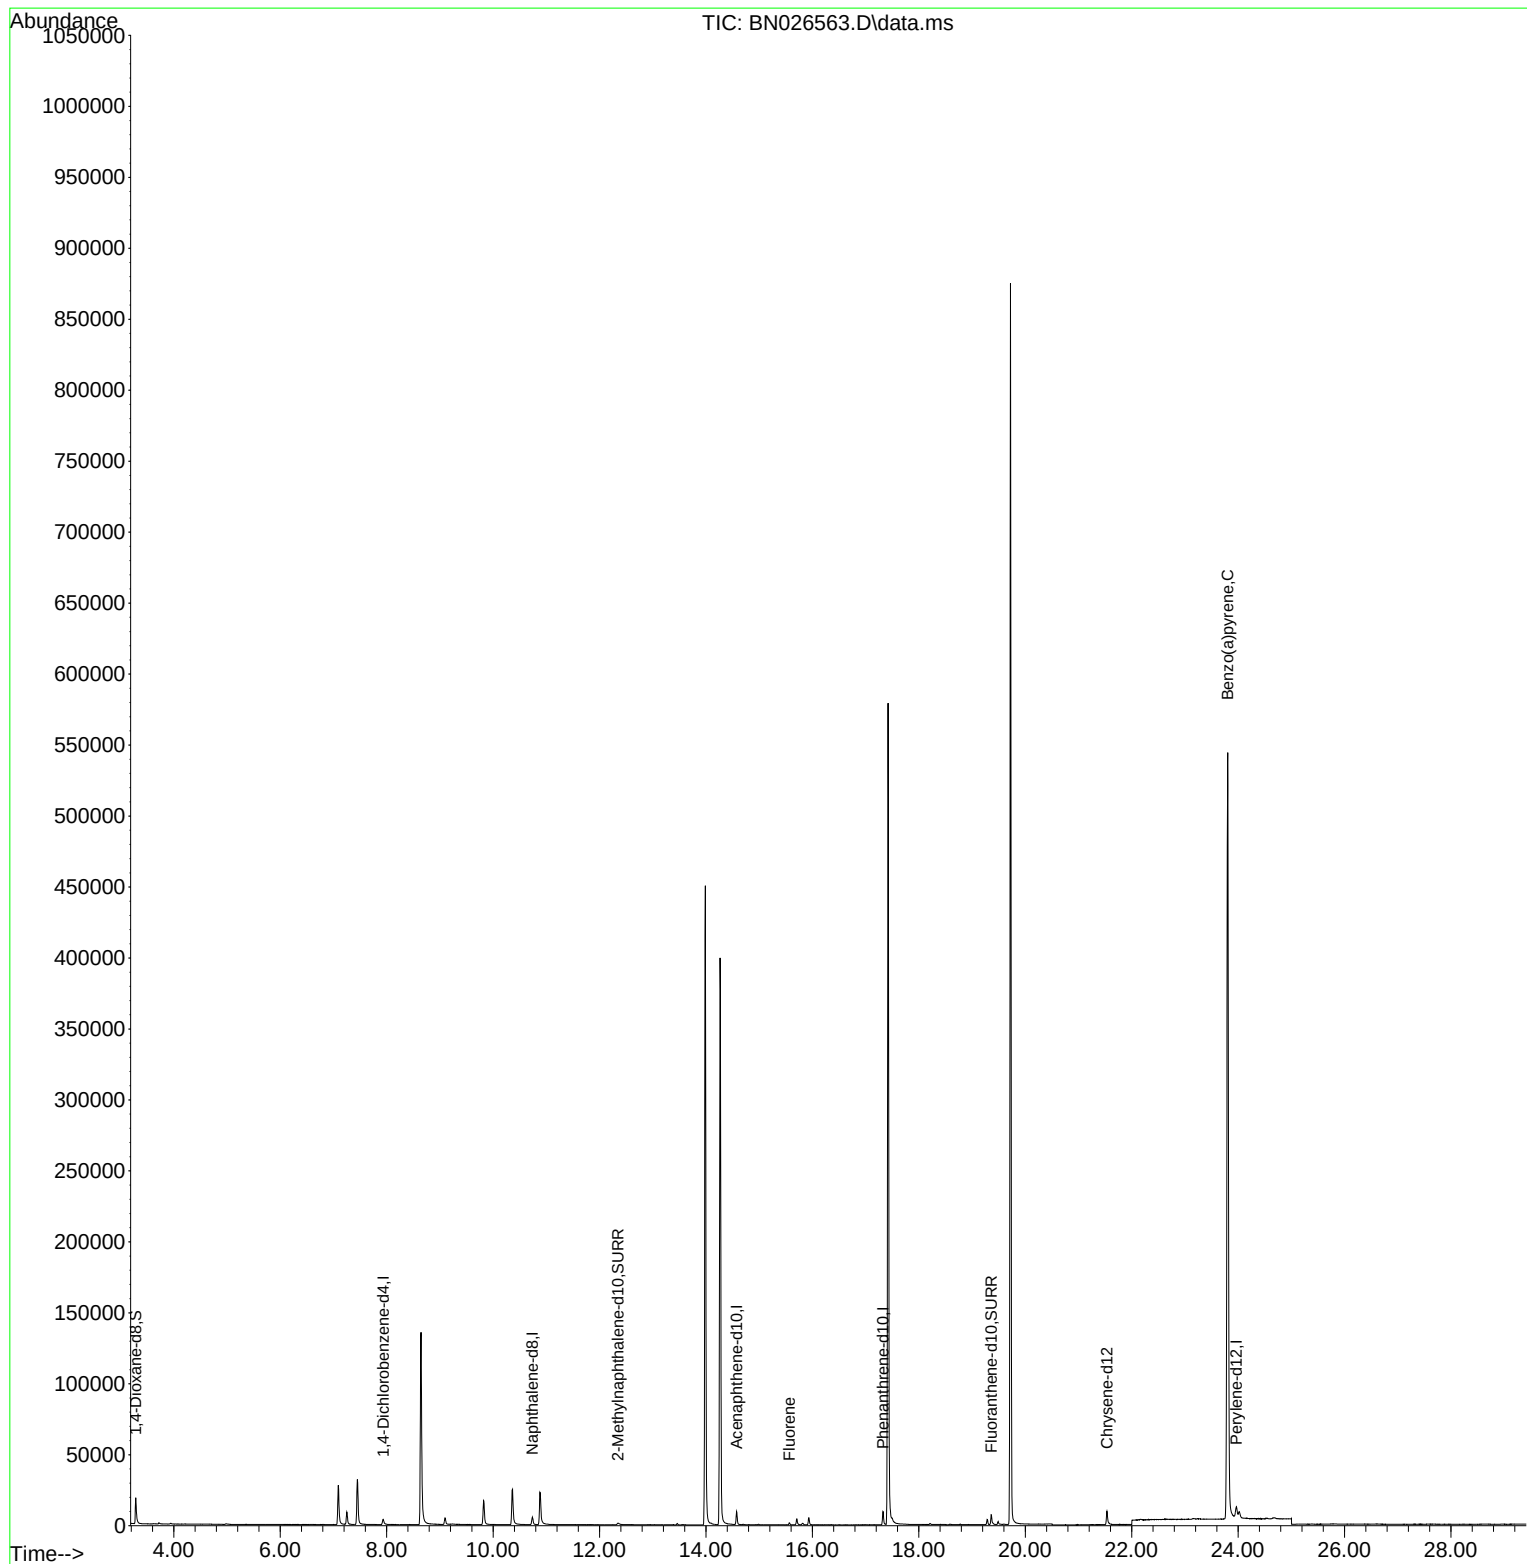



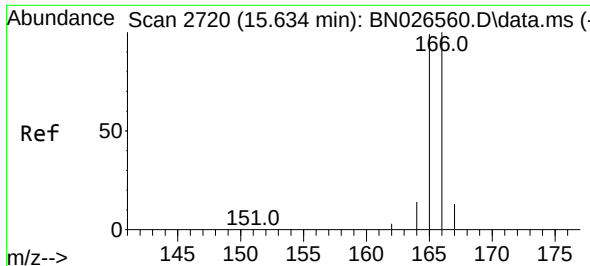


#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.569 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN026563.D
Acq: 18 Jul 2023 14:16

Instrument :
BNA_N
ClientSampleId :

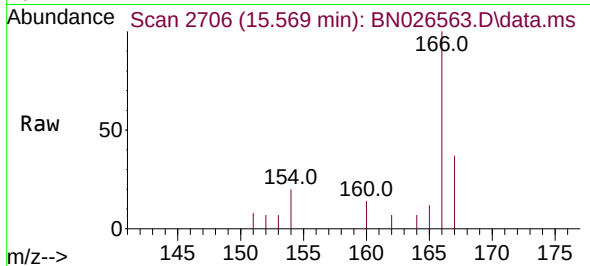

Tgt Ion:166 Resp: 1305
Ion Ratio Lower Upper
166 100
165 11.7 80.6 120.8#
167 36.9 12.0 18.0#

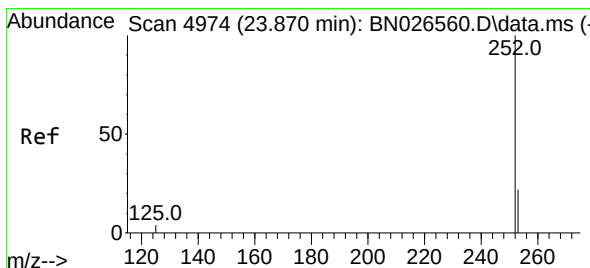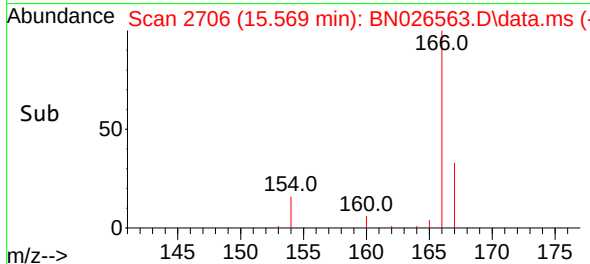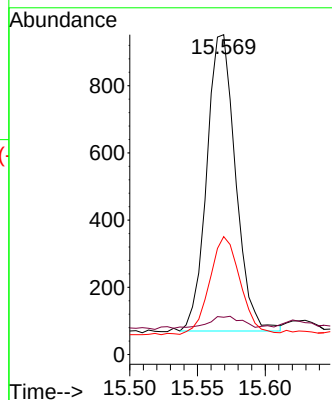

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.803 min Scan# 4951
Delta R.T. -0.067 min
Lab File: BN026563.D
Acq: 18 Jul 2023 14:16

Tgt Ion:252 Resp: 3154
Ion Ratio Lower Upper
252 100
253 66.6 32.6 49.0#
125 60.4 19.3 28.9#

