

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071823\
 Data File : BN026574.D
 Acq On : 18 Jul 2023 21:06
 Operator : MA/JU
 Sample : 03458-26
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 00:19:08 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 19 00:15:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	2194	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.736	136	6879	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.574	164	4589	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	10659	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.525	240	10379	0.400	ng/ul	# 0.00
23) Perylene-d12	23.954	264	11513	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	11328	3.920	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.347	152	2381	0.255	ng/ul	0.00
18) Fluoranthene-d10	19.358	212	9092	0.253	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.716	202	1834	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.788	252	2773	0.069	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071823\
Data File : BN026574.D
Acq On : 18 Jul 2023 21:06
Operator : MA/JU
Sample : 03458-26
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 00:19:08 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN071223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 19 00:15:47 2023
Response via : Initial Calibration

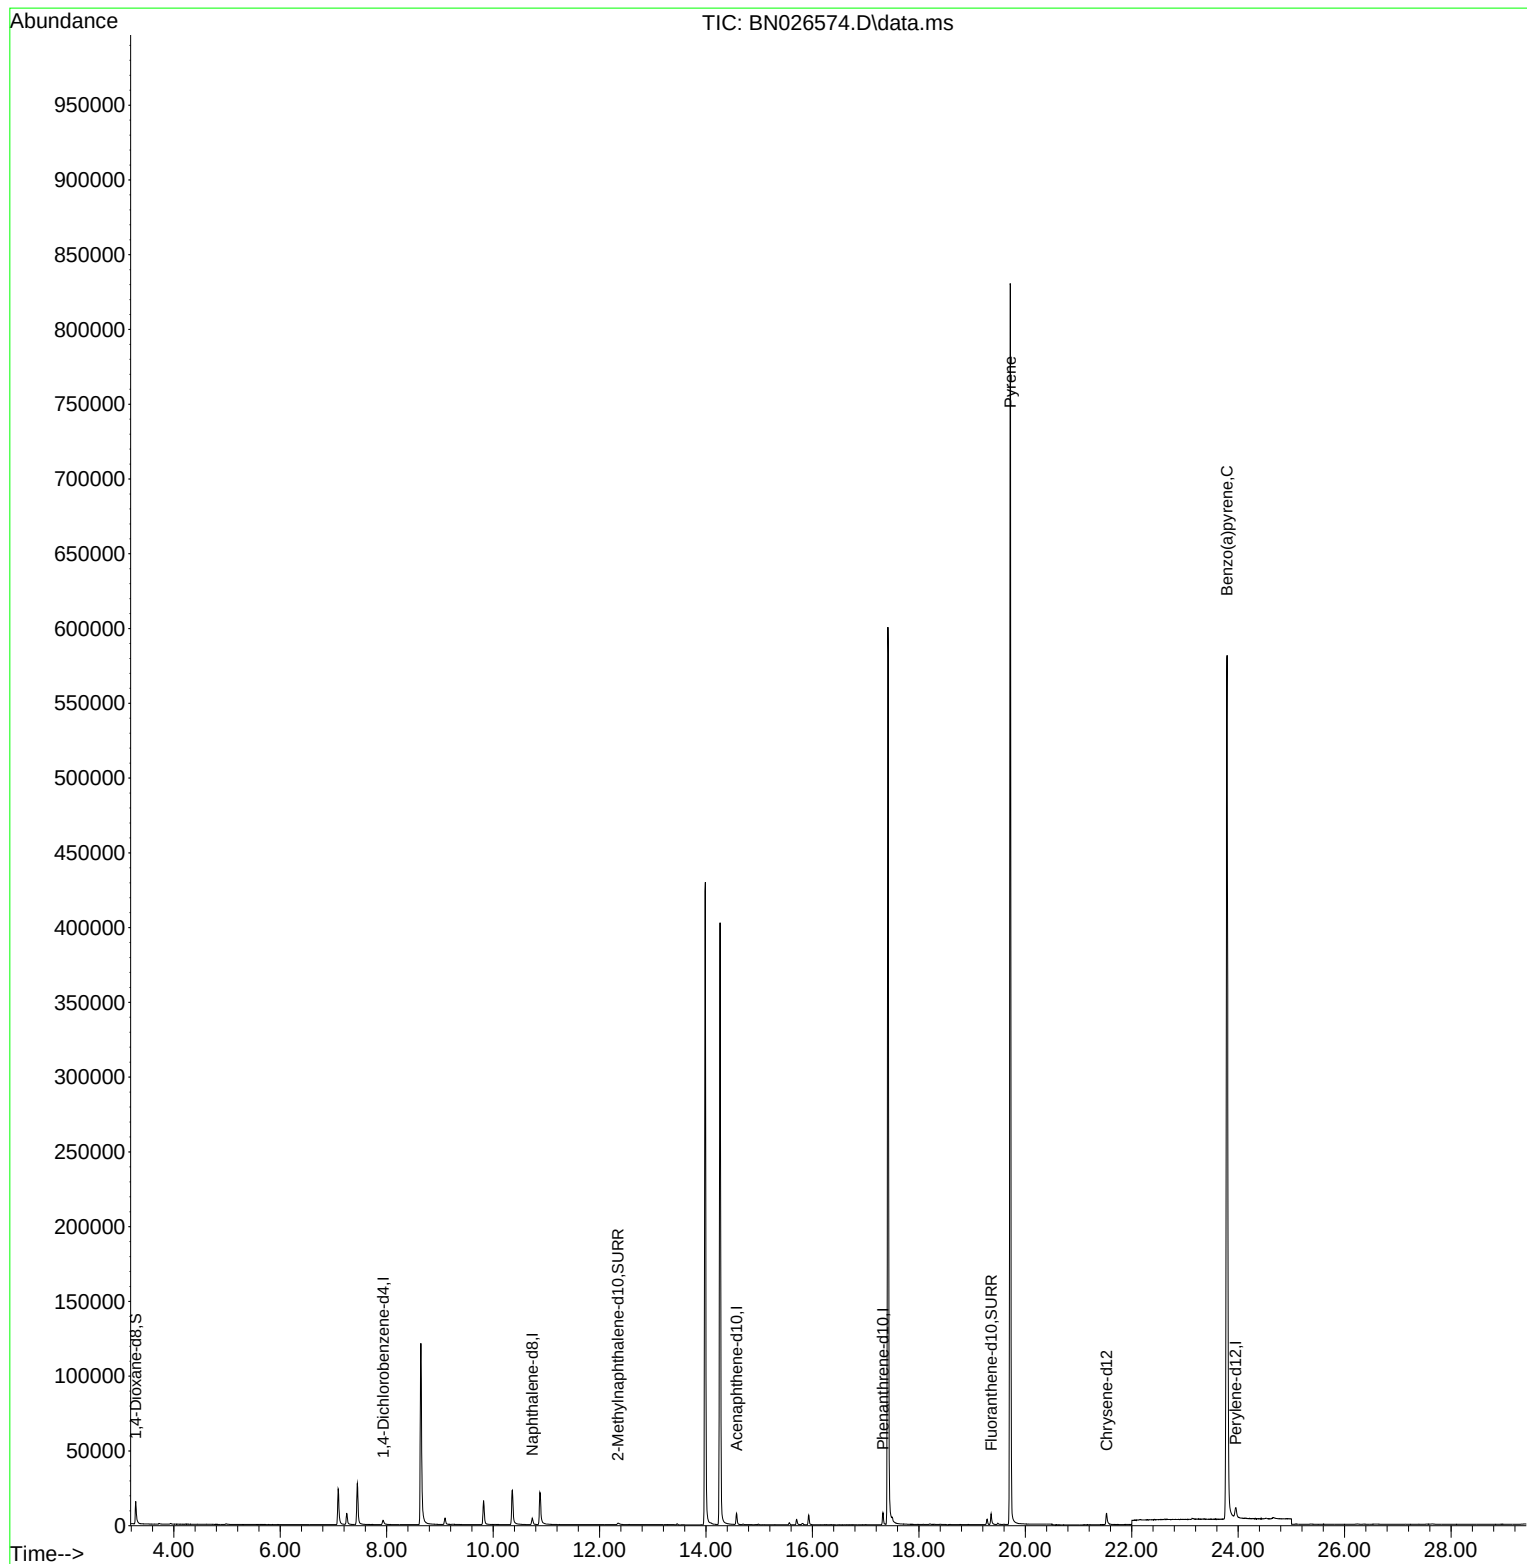

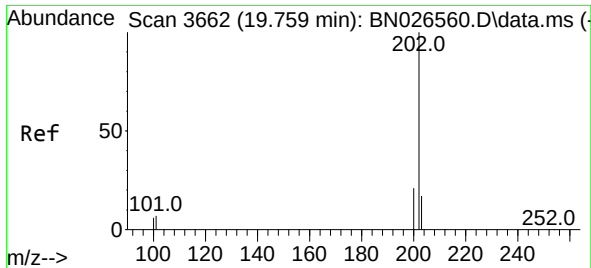

#20

Pyrene

Concen: 0.035 ng/ul

RT: 19.716 min Scan# 3

Delta R.T. -0.043 min


Lab File: BN026574.D

Acq: 18 Jul 2023 21:06




Instrument :

BNA_N

ClientSampleId :

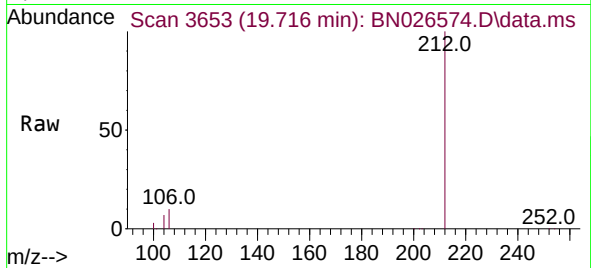

Tgt Ion:	202	Resp:	1834
Ion Ratio	Lower	Upper	
202	100		
101	212.9	8.0	12.0#
100	1765.5	6.2	9.2#

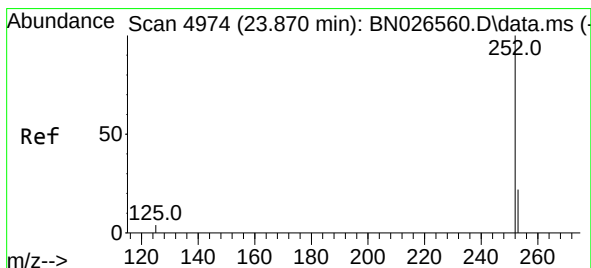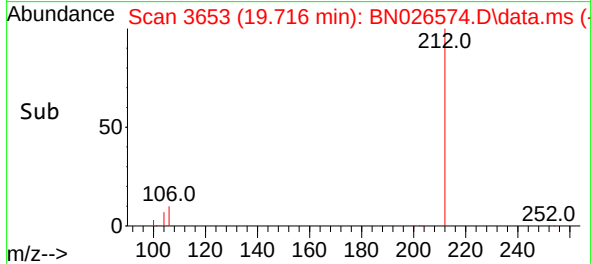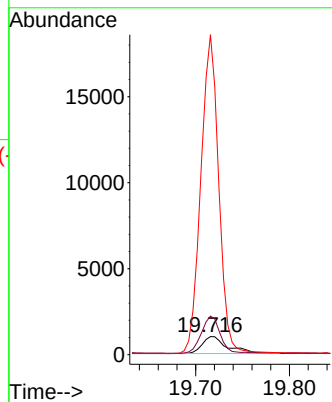

#26

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.788 min Scan# 4946

Delta R.T. -0.083 min

Lab File: BN026574.D

Acq: 18 Jul 2023 21:06

Tgt Ion:	252	Resp:	2773
Ion Ratio	Lower	Upper	
252	100		
253	62.7	32.6	49.0#
125	54.7	19.3	28.9#

