

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071825\
 Data File : BN037527.D
 Acq On : 18 Jul 2025 17:54
 Operator : RC/JU
 Sample : PB166542BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK542

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	16	19	28	rVB	24894	32337	1.67%	0.155%
2	3.605	83	88	106	rBV	347802	484538	25.03%	2.330%
3	3.940	140	145	150	rVB	6349	8406	0.43%	0.040%
4	6.881	639	645	652	rBV	385000	583764	30.16%	2.807%
5	7.052	668	674	683	rBV	297532	447963	23.14%	2.154%
6	7.252	701	708	718	rVB	399280	602072	31.11%	2.895%
7	7.716	781	787	795	rBV	316023	503702	26.02%	2.422%
8	8.346	889	894	899	rBV3	1502	3091	0.16%	0.015%
9	8.416	899	906	917	rVV	458276	717055	37.05%	3.448%
10	8.863	974	982	991	rBV	344293	542081	28.01%	2.607%
11	8.981	998	1002	1008	rVB3	2793	4069	0.21%	0.020%
12	9.587	1098	1105	1112	rBV	256270	404050	20.88%	1.943%
13	10.122	1186	1196	1205	rBV	429944	702238	36.28%	3.377%
14	10.504	1253	1261	1268	rBV	421815	679876	35.13%	3.269%
15	10.634	1276	1283	1293	rBV	426914	710285	36.70%	3.415%
16	12.098	1526	1532	1539	rBV2	5130	8799	0.45%	0.042%
17	13.769	1810	1816	1822	rBV	731168	1000155	51.67%	4.809%
18	14.045	1856	1863	1871	rBV2	868575	1256983	64.94%	6.044%
19	14.351	1909	1915	1924	rVB	592103	885823	45.77%	4.259%
20	14.534	1938	1946	1958	rBV	333039	475655	24.58%	2.287%
21	14.610	1958	1959	1964	rVB3	2167	2079	0.11%	0.010%
22	15.345	2078	2084	2092	rBV	1067392	1507489	77.89%	7.249%
23	15.457	2097	2103	2112	rBV	252271	348240	17.99%	1.674%
24	15.586	2119	2125	2128	rBV4	3428	4482	0.23%	0.022%
25	16.881	2341	2345	2349	rVB3	2480	3333	0.17%	0.016%
26	17.092	2375	2381	2387	rBV2	710392	992532	51.28%	4.772%
27	17.192	2391	2398	2406	rBV	1166378	1612919	83.33%	7.756%
28	17.516	2449	2453	2456	rBV3	1463	2046	0.11%	0.010%
29	18.004	2533	2536	2541	rVB6	3192	4501	0.23%	0.022%
30	18.845	2676	2679	2682	rBV4	1478	2307	0.12%	0.011%
31	19.051	2710	2714	2719	rBV2	11256	14237	0.74%	0.068%
32	19.122	2722	2726	2729	rBV2	10918	13415	0.69%	0.065%
33	19.292	2751	2755	2757	rBV3	3407	4013	0.21%	0.019%
34	19.333	2759	2762	2770	rVB	15578	22542	1.16%	0.108%
35	19.486	2782	2788	2796	rBV	1376477	1844268	95.29%	8.868%
36	20.163	2897	2903	2910	rBV10	7058	21298	1.10%	0.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071825\
Data File : BN037527.D
Acq On : 18 Jul 2025 17:54
Operator : RC/JU
Sample : PB166542BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK542

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
Title : SVOA CALIBRATION

37	21.321	3094	3100	3107	rBV	827622	1145672	59.19%	5.509%
38	24.063	3556	3566	3576	rBV2	846868	1935489	100.00%	9.307%
39	24.262	3591	3600	3610	rBV	508935	1199997	62.00%	5.770%
40	24.357	3613	3616	3625	rVB4	28412	63155	3.26%	0.304%




Sum of corrected areas: 20796956

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071825\
Data File : BN037527.D
Acq On : 18 Jul 2025 17:54
Operator : RC/JU
Sample : PB166542BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK542

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

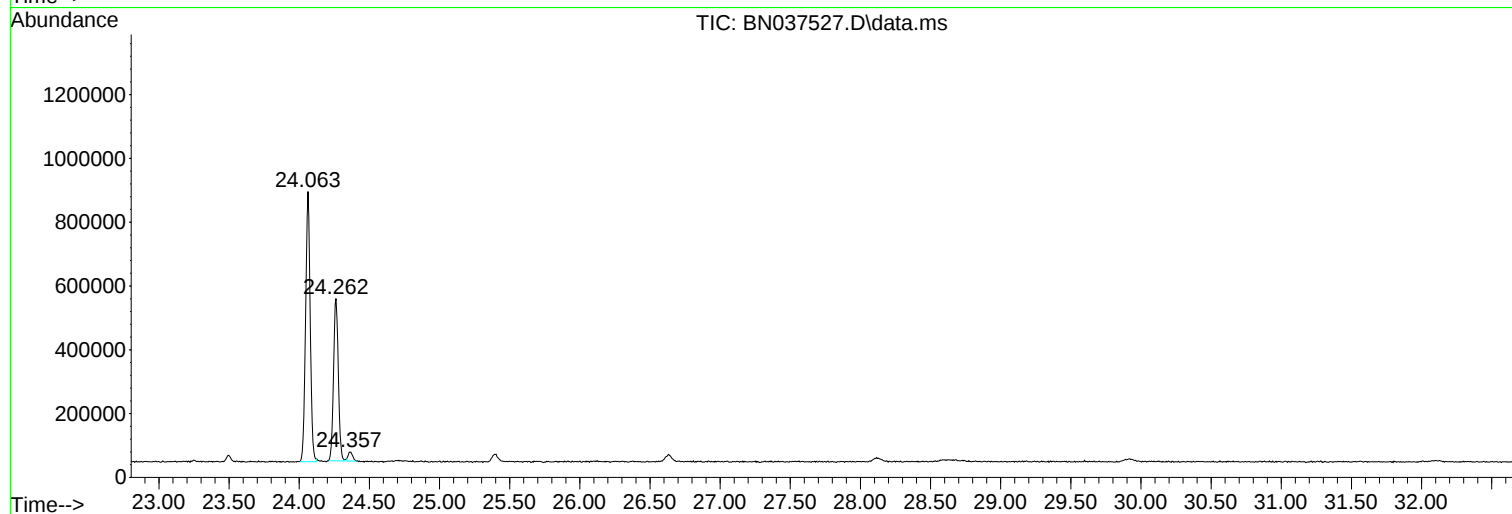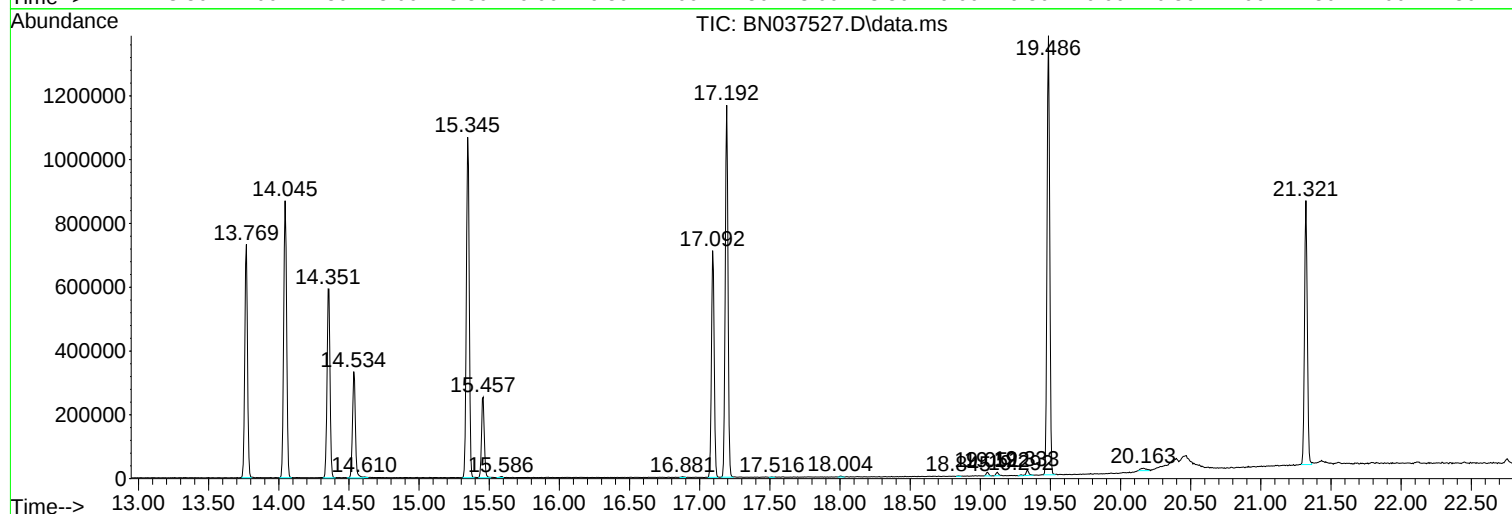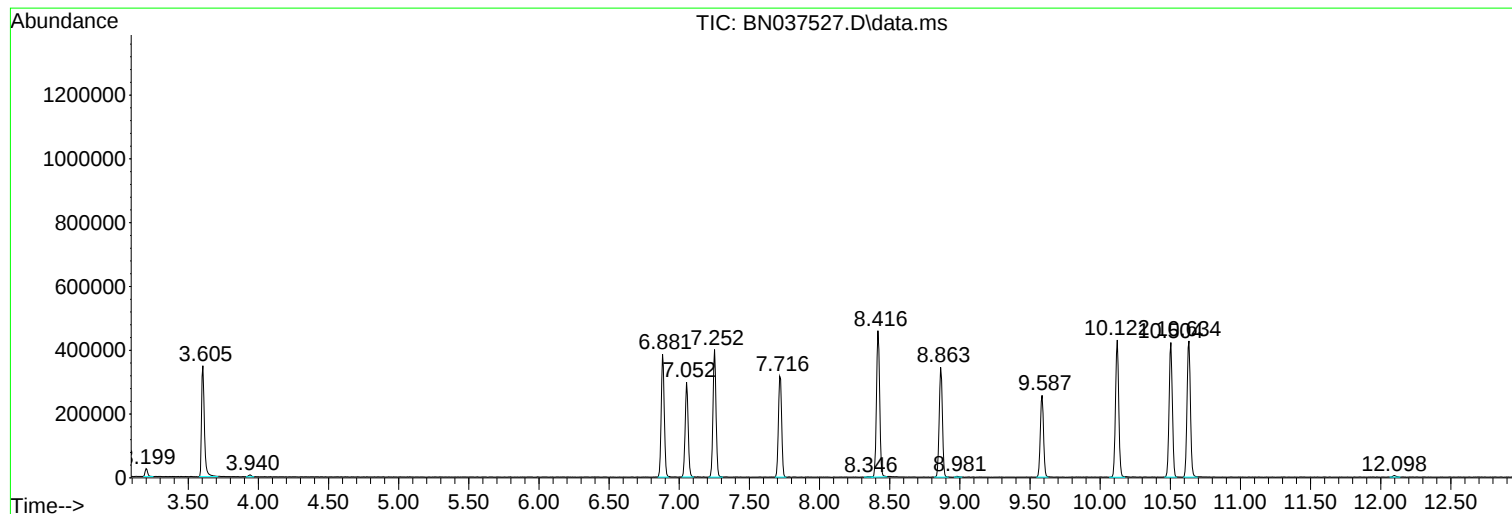

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071825\
Data File : BN037527.D
Acq On : 18 Jul 2025 17:54
Operator : RC/JU
Sample : PB166542BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK542

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071825\
Data File : BN037527.D
Acq On : 18 Jul 2025 17:54
Operator : RC/JU
Sample : PB166542BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK542

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN071825.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc