

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071918\
 Data File : BN002072.D
 Acq On : 19 Jul 2018 14:42
 Operator : JU/SJ
 Sample : J4024-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 19 16:48:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 17 00:49:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	287874	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	1332349	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	819702	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	1871489	20.00	ng/ul	0.00
77) Chrysene-d12	21.28	240	1932595	20.00	ng/ul	0.00
85) Perylene-d12	23.52	264	1790637	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	34432	5.40	ng/uL	0.00
5) Phenol-d5	6.88	99	158505	5.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	458597	27.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	476340	22.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	305745	14.00	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	318120	28.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	361463	28.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	589140	26.07	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	48987	1.89	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	2195914	31.60	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	2605231	30.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	75720	5.70	ng/ul	0.00
57) Fluorene-d10	15.33	176	1856986	31.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	358088	29.38	ng/ul	0.00
70) Anthracene-d10	17.18	188	2962852	32.47	ng/ul	0.00
78) Pyrene-d10	19.48	212	3262546	32.47	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.38	264	3228851	33.39	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	13.79	163	465599	6.841	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071918\
Data File : BN002072.D
Acq On : 19 Jul 2018 14:42
Operator : JU/SJ
Sample : J4024-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 19 16:48:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 17 00:49:33 2018
Response via : Initial Calibration

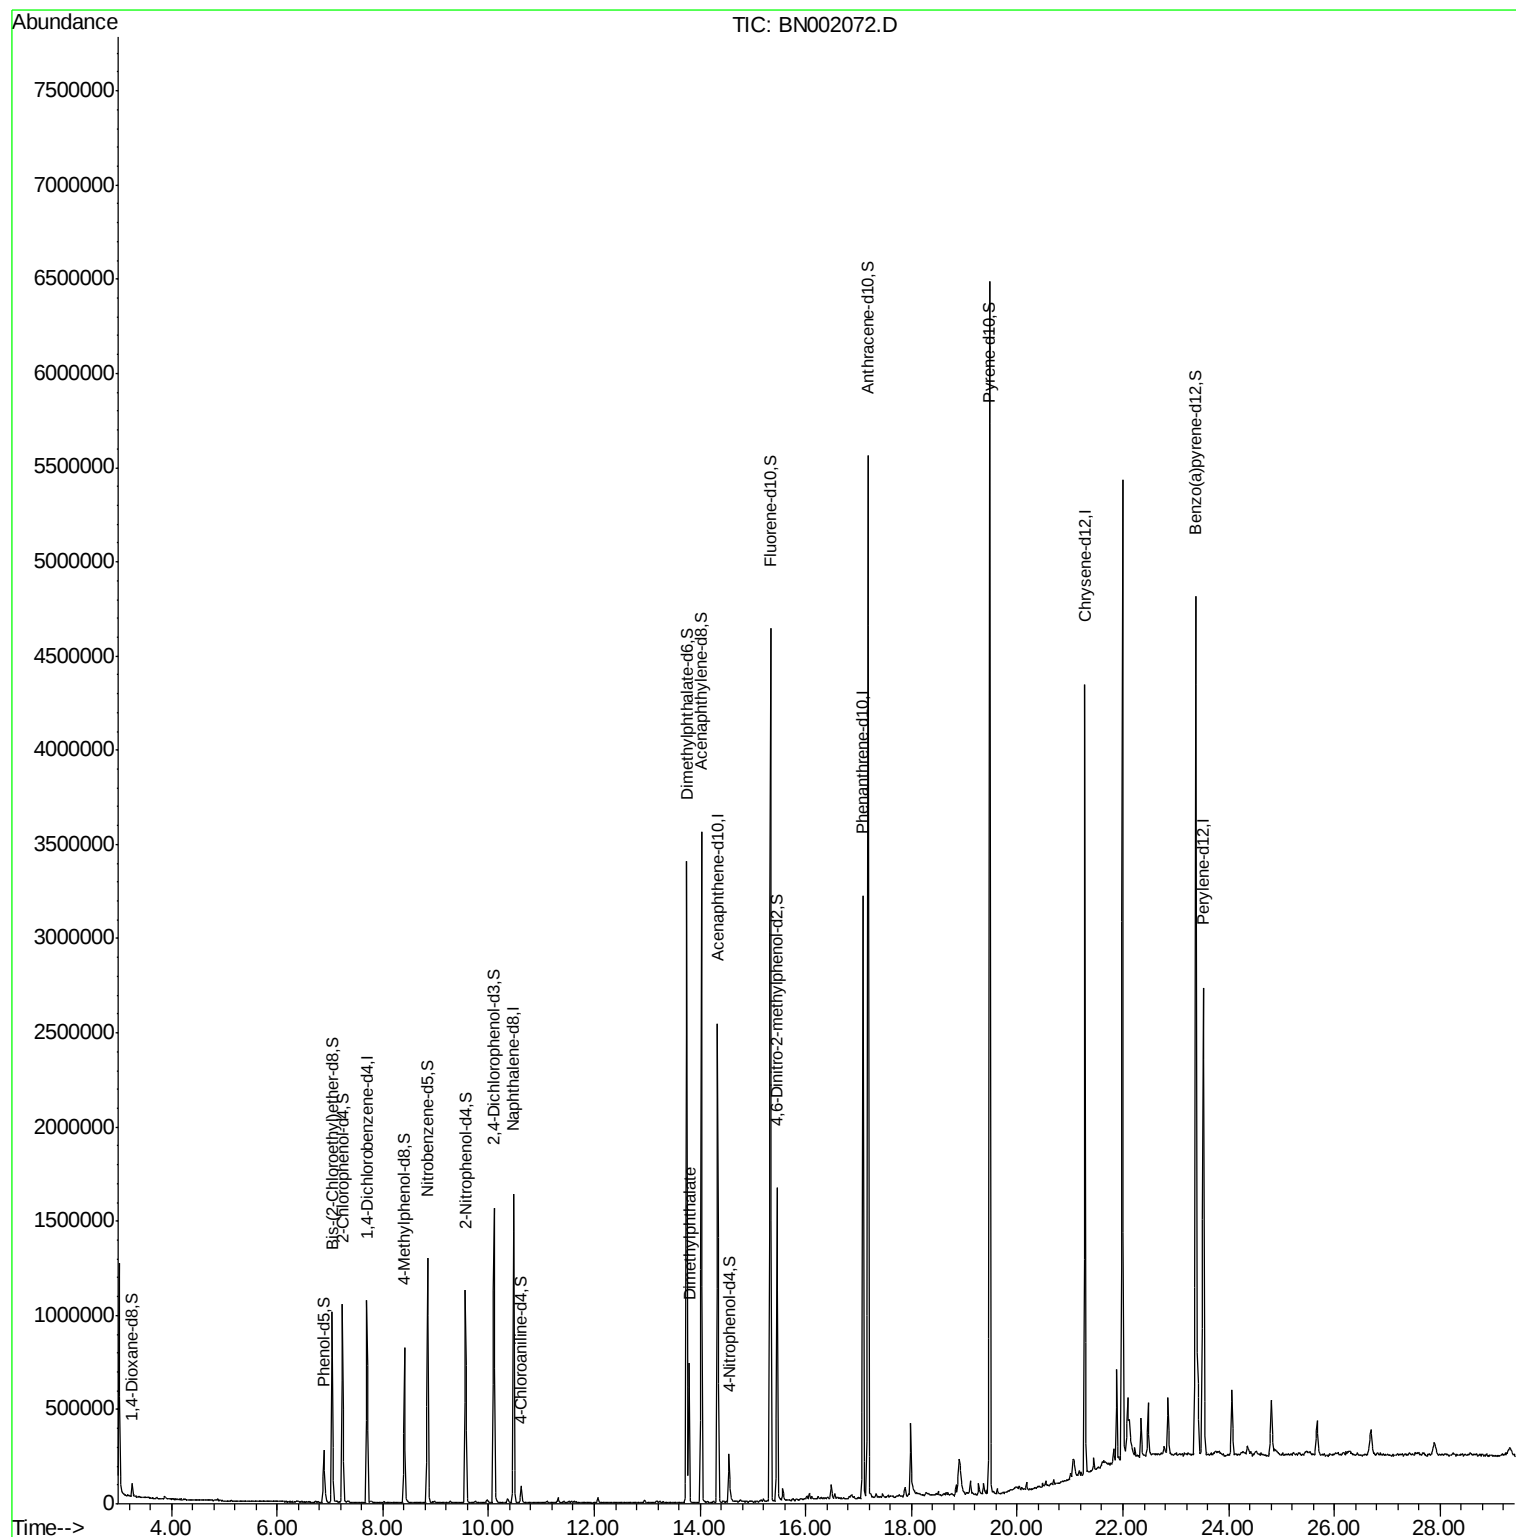

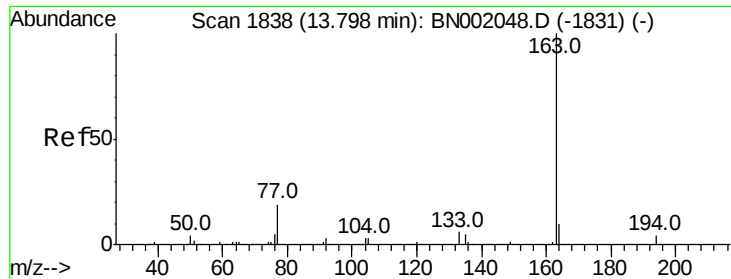

#44

Dimethylphthalate

Concen: 6.841 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BN002072.D

Acq: 19 Jul 2018 14:42

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 465599

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.4 7.8 11.8

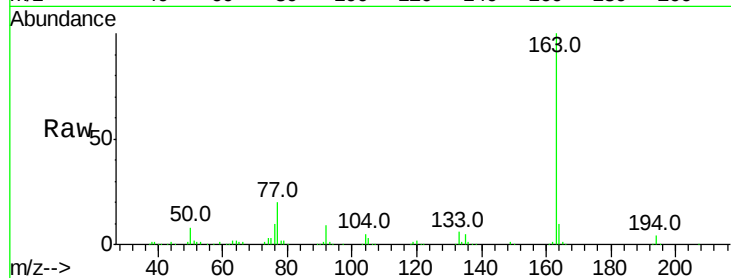

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

