

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071918\
 Data File : BN002076.D
 Acq On : 19 Jul 2018 17:45
 Operator : JU/SJ
 Sample : J4023-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB1K2

Quant Time: Jul 20 02:58:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 20 02:57:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	249467	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	1155257	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	729832	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	1705925	20.00	ng/ul	0.00
77) Chrysene-d12	21.28	240	1819074	20.00	ng/ul	0.00
85) Perylene-d12	23.52	264	1744671	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	4533	0.82	ng/uL	0.00
5) Phenol-d5	6.88	99	101861	4.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	65770	4.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	80605	4.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	80886	4.27	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	41834	4.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	43293	4.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	81388	4.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	106307	4.72	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	313862	5.07	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	355621	4.62	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	41087	3.48	ng/ul	0.00
57) Fluorene-d10	15.33	176	270272	5.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	31432	2.83	ng/ul	0.00
70) Anthracene-d10	17.18	188	432586	5.20	ng/ul	0.00
78) Pyrene-d10	19.48	212	521338	5.51	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.37	264	521346	5.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.79	163	137827	2.275	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071918\
Data File : BN002076.D
Acq On : 19 Jul 2018 17:45
Operator : JU/SJ
Sample : J4023-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB1K2

Quant Time: Jul 20 02:58:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 20 02:57:55 2018
Response via : Initial Calibration

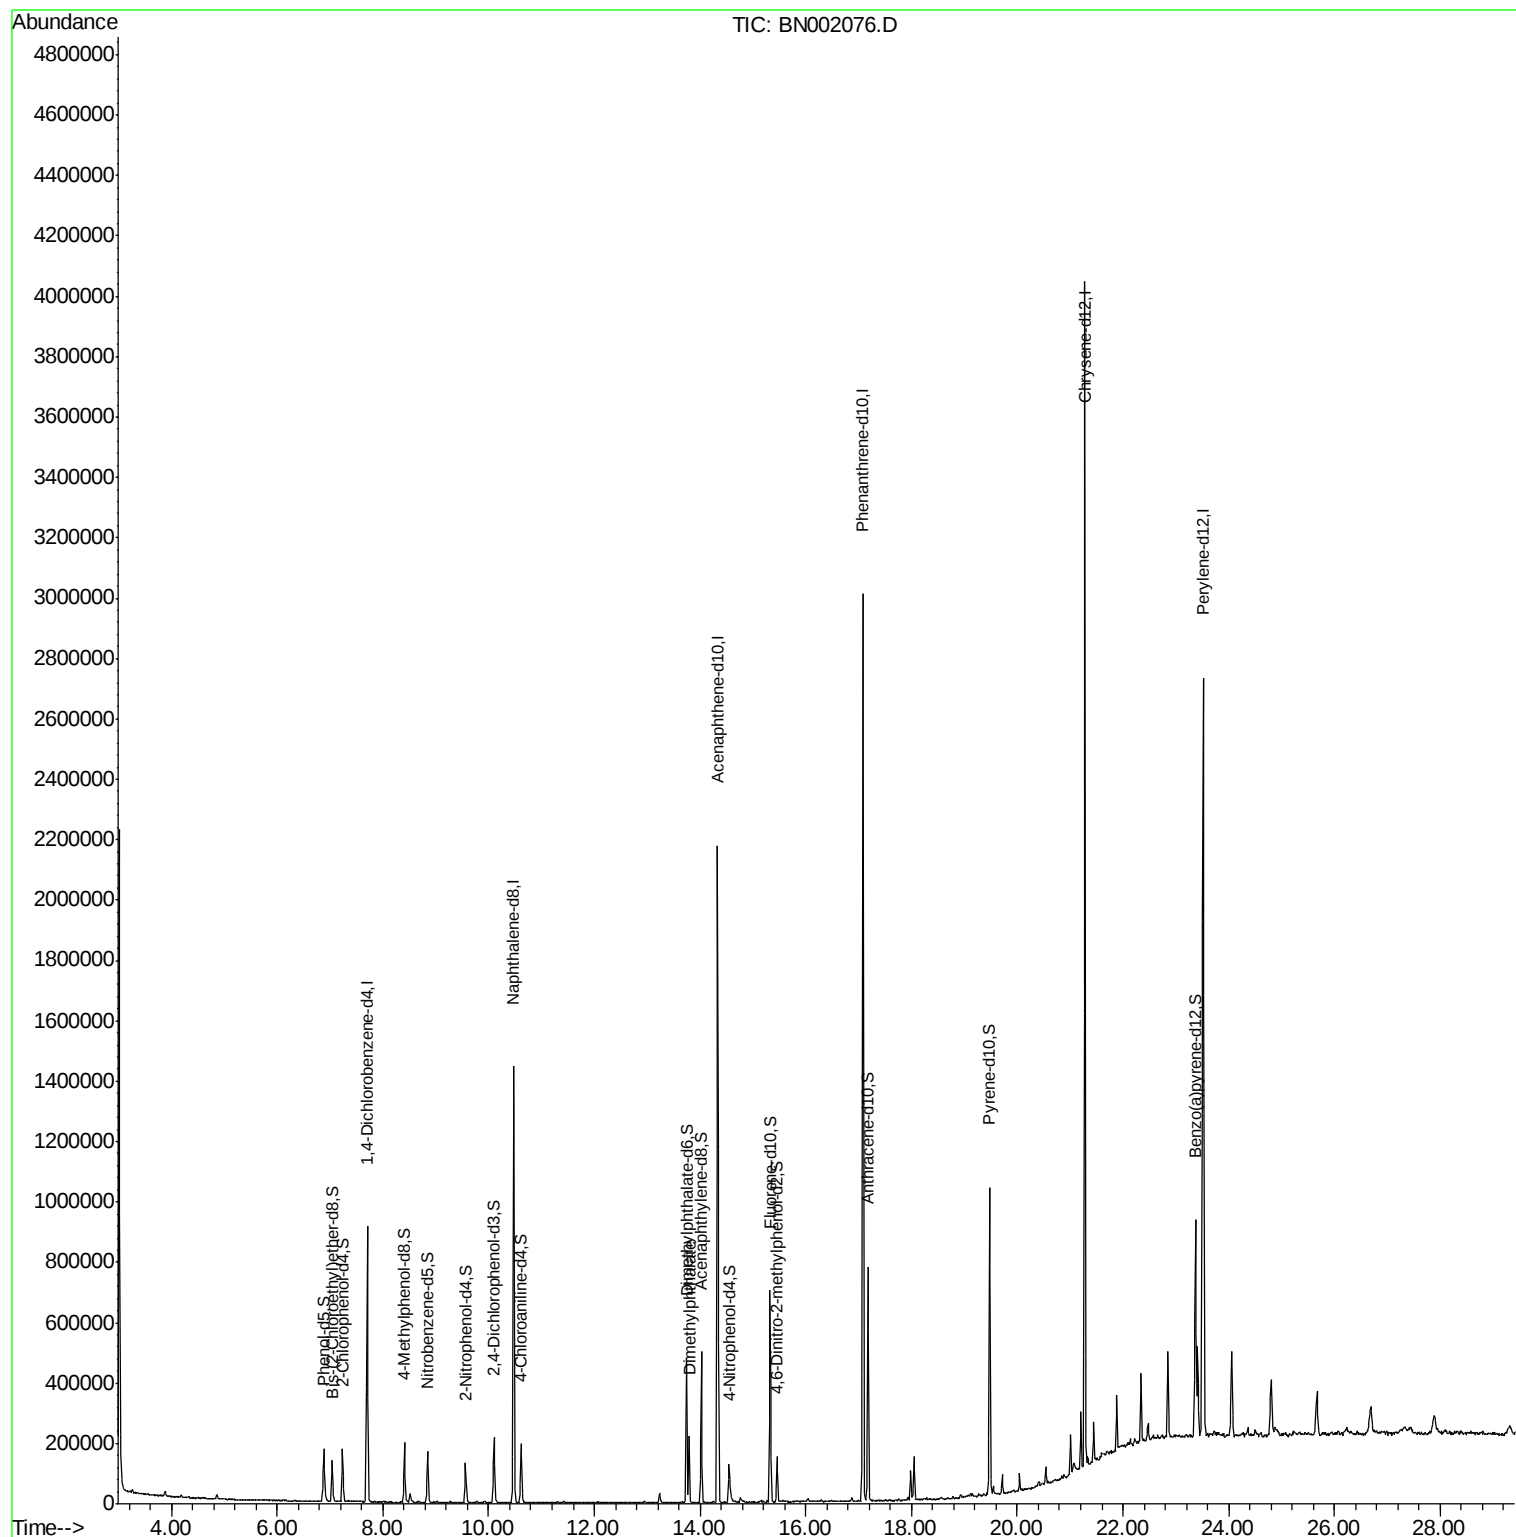

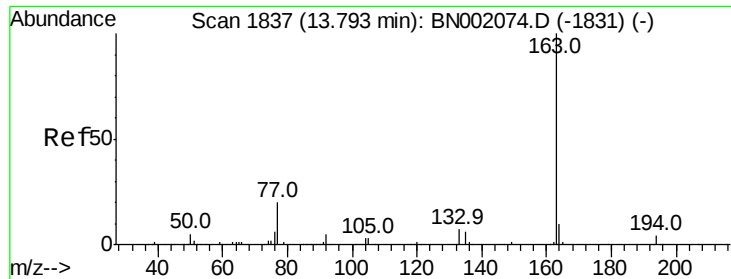

#44

Dimethylphthalate

Concen: 2.275 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.00 min

Lab File: BN002076.D

Acq: 19 Jul 2018 17:45

Instrument :

BNA_N

ClientSampleId :

DB1K2


Tot Ion:163 Resp: 137827

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 11.0 7.8 11.8

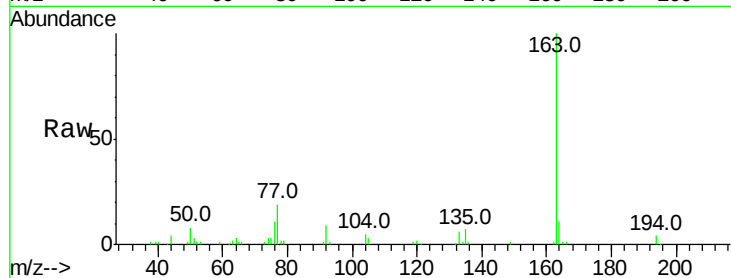

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

