

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071918\
 Data File : BN002077.D
 Acq On : 19 Jul 2018 18:20
 Operator : JU/SJ
 Sample : J4023-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB1K3

Quant Time: Jul 20 02:58:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 20 02:57:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	265367	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	1219955	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	761637	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	1763027	20.00	ng/ul	0.00
77) Chrysene-d12	21.28	240	1853658	20.00	ng/ul	0.00
85) Perylene-d12	23.52	264	1805539	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.26	96	8923	1.52	ng/uL	0.00
5) Phenol-d5	6.88	99	263367	10.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.04	67	171536	11.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	198903	10.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	265044	13.17	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	127379	12.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	147393	12.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	280287	13.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	448456	18.85	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	1393090	21.58	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1539657	19.17	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	217313	17.62	ng/ul	0.00
57) Fluorene-d10	15.33	176	1179422	21.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	193146	16.82	ng/ul	0.00
70) Anthracene-d10	17.18	188	1922925	22.37	ng/ul	0.00
78) Pyrene-d10	19.48	212	2126969	22.07	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.37	264	2208354	22.65	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.79	163	589680	9.325	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN071918\
Data File : BN002077.D
Acq On : 19 Jul 2018 18:20
Operator : JU/SJ
Sample : J4023-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB1K3

Quant Time: Jul 20 02:58:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 20 02:57:55 2018
Response via : Initial Calibration

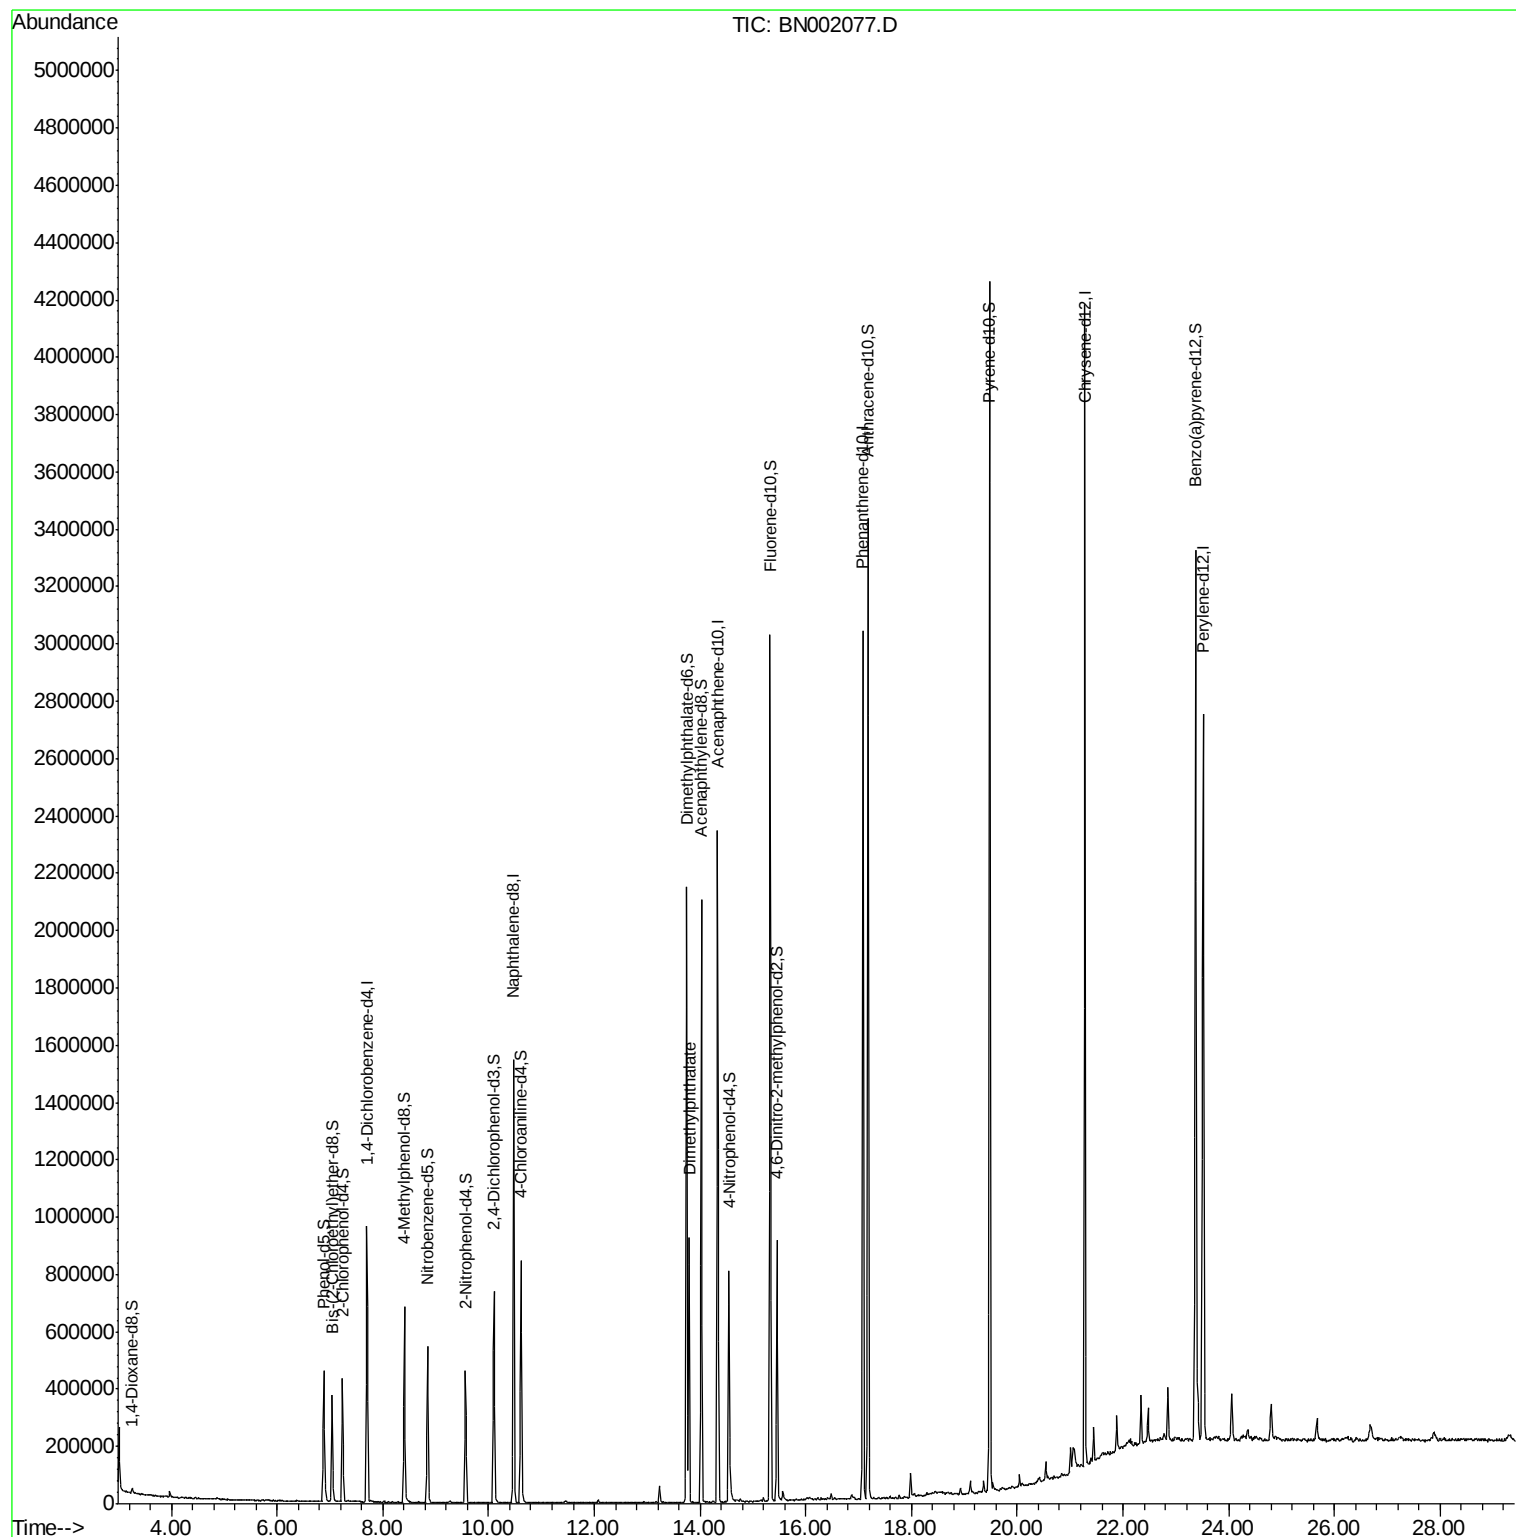

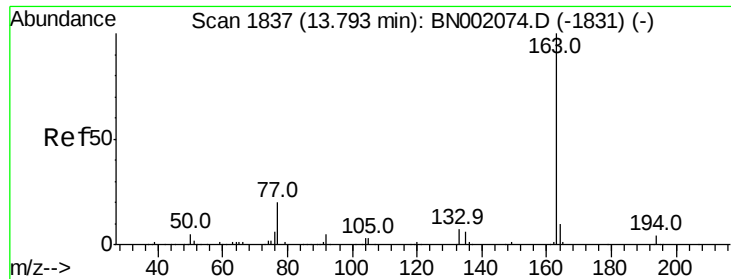

#44

Dimethylphthalate

Concen: 9.325 ng/ul

RT: 13.79 min Scan# 1837

Delta R.T. -0.00 min

Lab File: BN002077.D

Acq: 19 Jul 2018 18:20

Instrument :

BNA_N

ClientSampleId :

DB1K3


Tot Ion:163 Resp: 589680

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.4 7.8 11.8

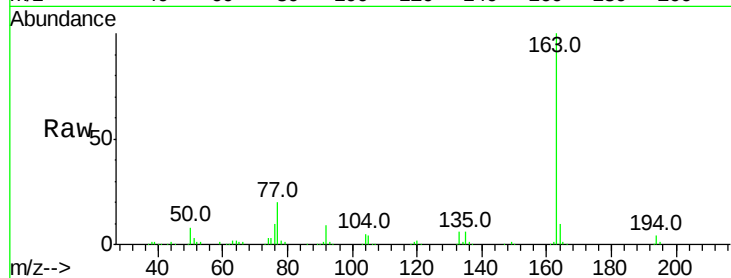

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

